
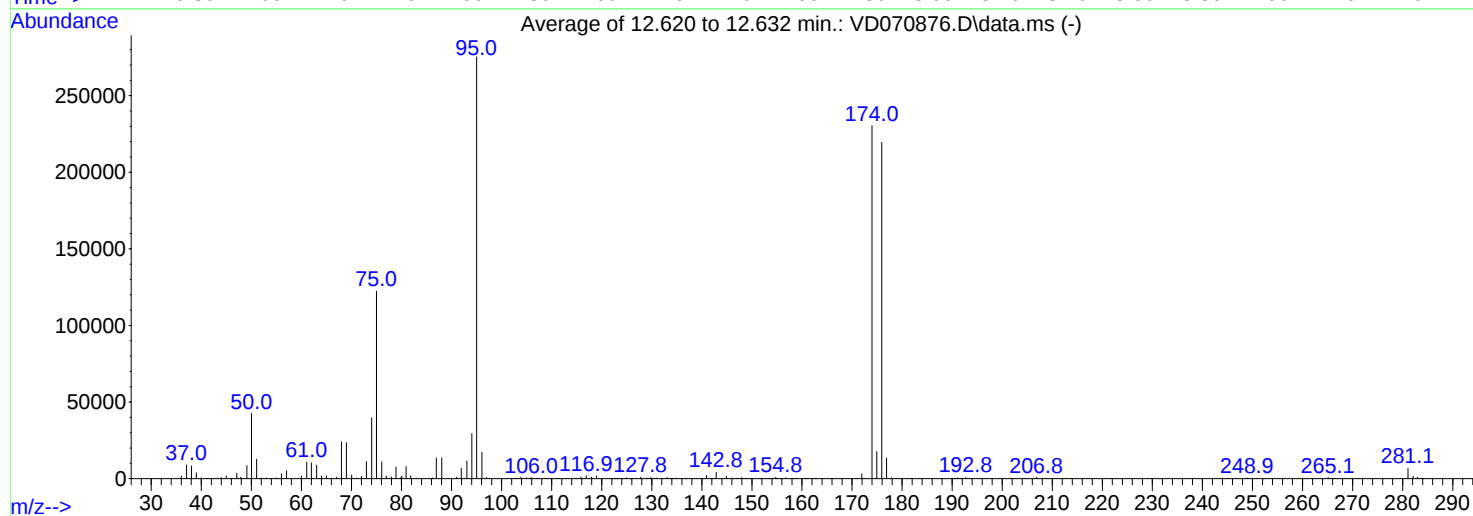


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102721\
Data File : VD070876.D
Acq On : 27 Oct 2021 21:27
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D102621S.M
Title : SW846 8260
Last Update : Wed Oct 27 05:34:47 2021

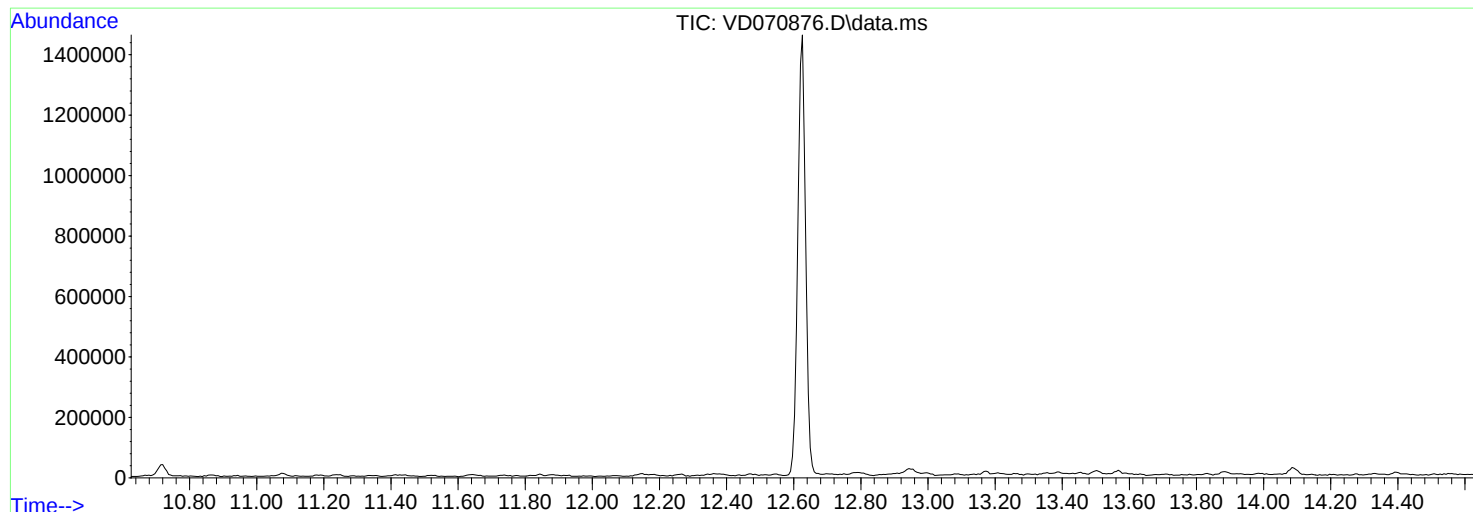

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	42523	PASS
75	95	30	60	44.4	122320	PASS
95	95	100	100	100.0	275329	PASS
96	95	5	9	6.3	17259	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.7	230379	PASS
175	174	5	9	7.7	17699	PASS
176	174	95	101	95.3	219520	PASS
177	176	5	9	6.1	13370	PASS