
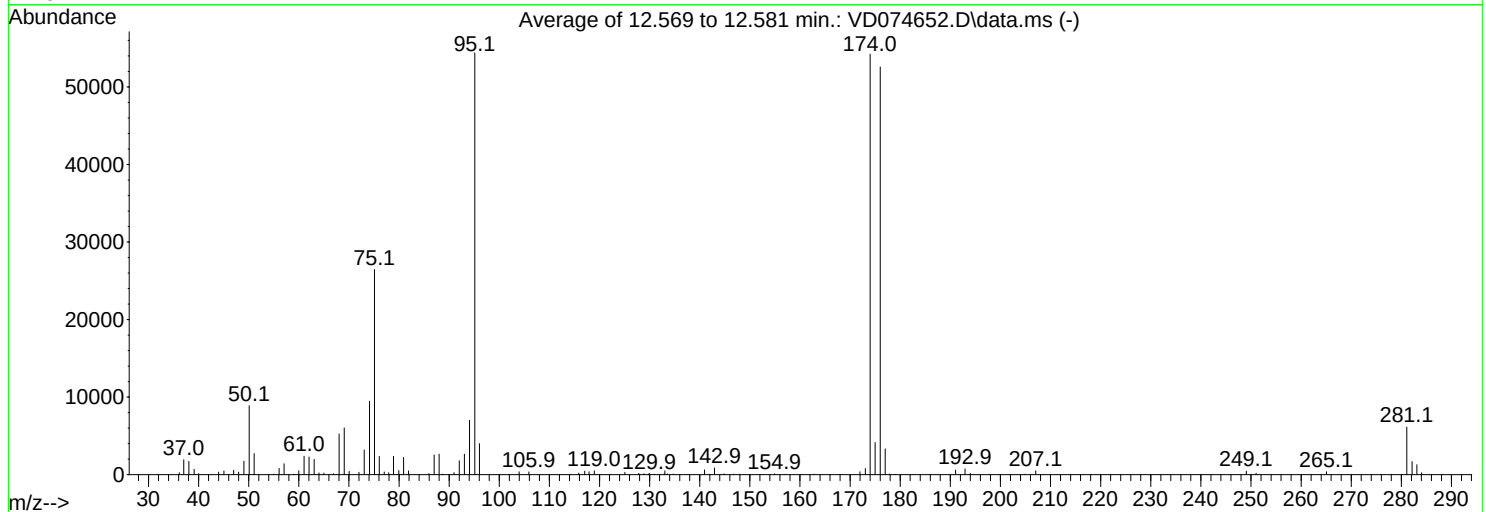


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102722\
 Data File : VD074652.D
 Acq On : 27 Oct 2022 10:40
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D102722S.M
 Title : SW846 8260
 Last Update : Fri Oct 28 00:18:17 2022

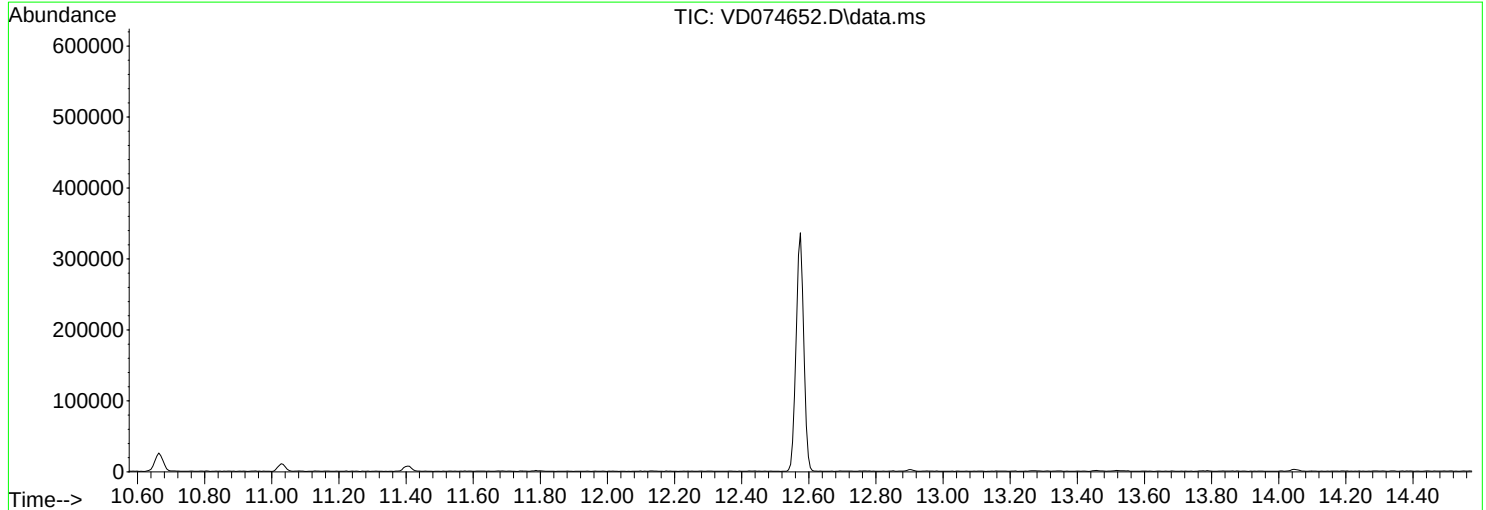

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	8894	PASS
75	95	30	60	48.6	26451	PASS
95	95	100	100	100.0	54405	PASS
96	95	5	9	7.3	3996	PASS
173	174	0.00	2	1.5	789	PASS
174	95	50	100	99.7	54237	PASS
175	174	5	9	7.6	4143	PASS
176	174	95	101	97.0	52595	PASS
177	176	5	9	6.3	3320	PASS