


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110119\
Data File : VD064145.D
Acq On : 01 Nov 2019 11:11
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D102919S.M
Title : SW846 8260
Last Update : Wed Oct 30 08:00:10 2019

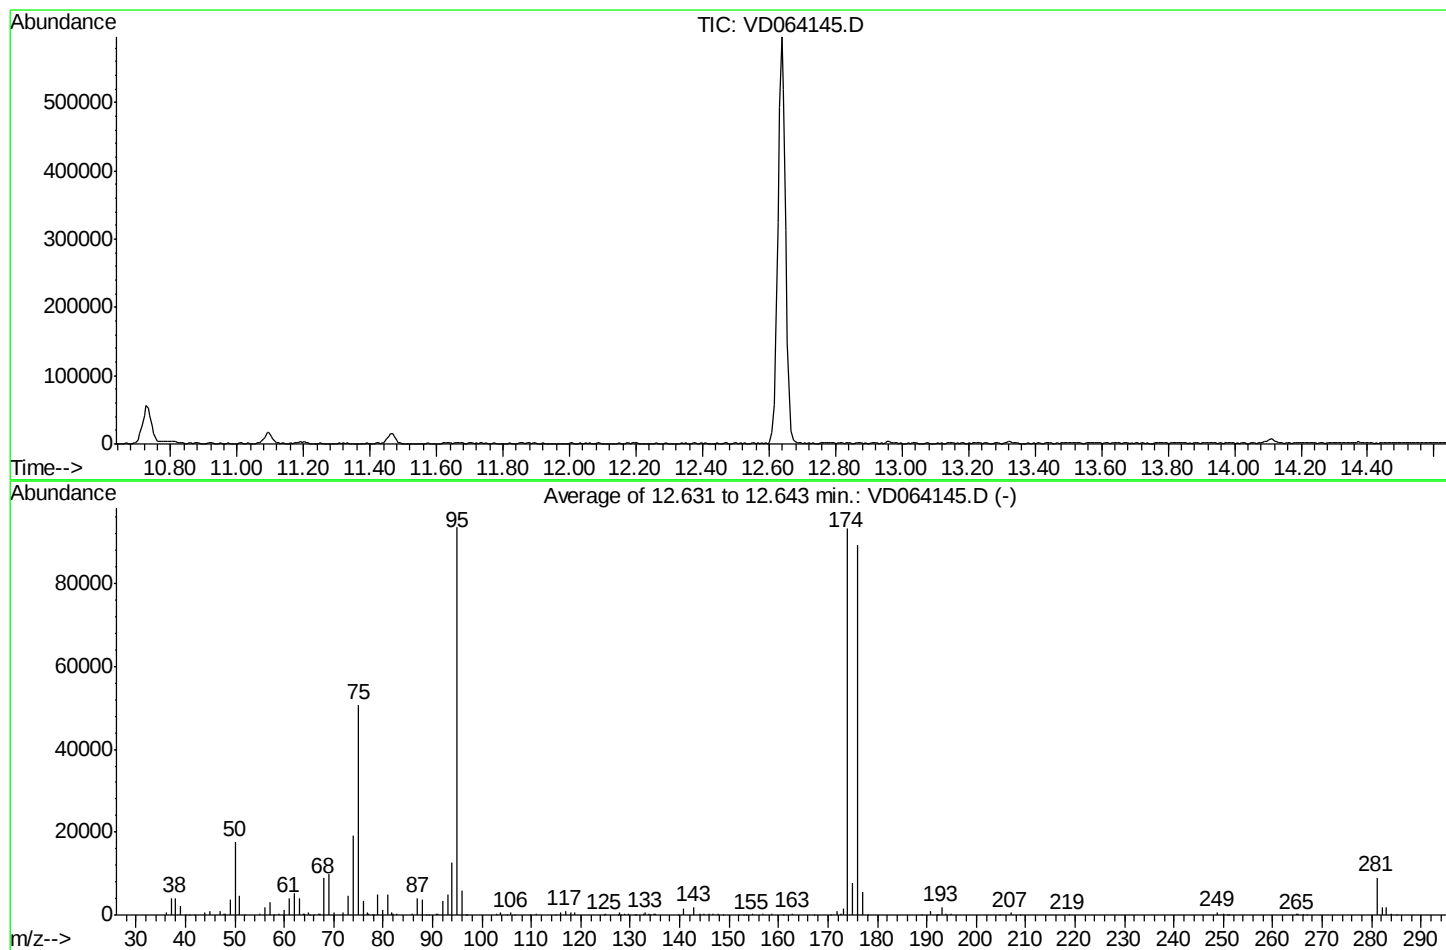

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	17737	PASS
75	95	30	60	54.3	50776	PASS
95	95	100	100	100.0	93584	PASS
96	95	5	9	6.2	5775	PASS
173	174	0.00	2	1.5	1430	PASS
174	95	50	100	99.6	93200	PASS
175	174	5	9	8.3	7741	PASS
176	174	95	101	95.8	89245	PASS
177	176	5	9	6.4	5712	PASS