

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110822\
 Data File : VD074814.D
 Acq On : 08 Nov 2022 20:11
 Operator : VA/SY
 Sample : N5494-17
 Misc : 5.03G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-20

Quant Time: Nov 08 23:40:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110222S.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 03 02:30:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.875	168	82923	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	131620	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	124681	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	52538	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	52653	80.170	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 160.340%	
35) Dibromofluoromethane	7.804	113	65450	84.063	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 168.120%#	
50) Toluene-d8	10.269	98	174370	61.397	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 122.800%	
62) 4-Bromofluorobenzene	12.575	95	52041	63.464	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 126.920%	
Target Compounds						
16) Acetone	4.022	43	3045	22.217	ug/l	Qvalue # 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110822\
Data File : VD074814.D
Acq On : 08 Nov 2022 20:11
Operator : VA/SY
Sample : N5494-17
Misc : 5.03G/5.00ml/MSVOA_D/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-20

Quant Time: Nov 08 23:40:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110222S.M
Quant Title : SW846 8260
QLast Update : Thu Nov 03 02:30:45 2022
Response via : Initial Calibration




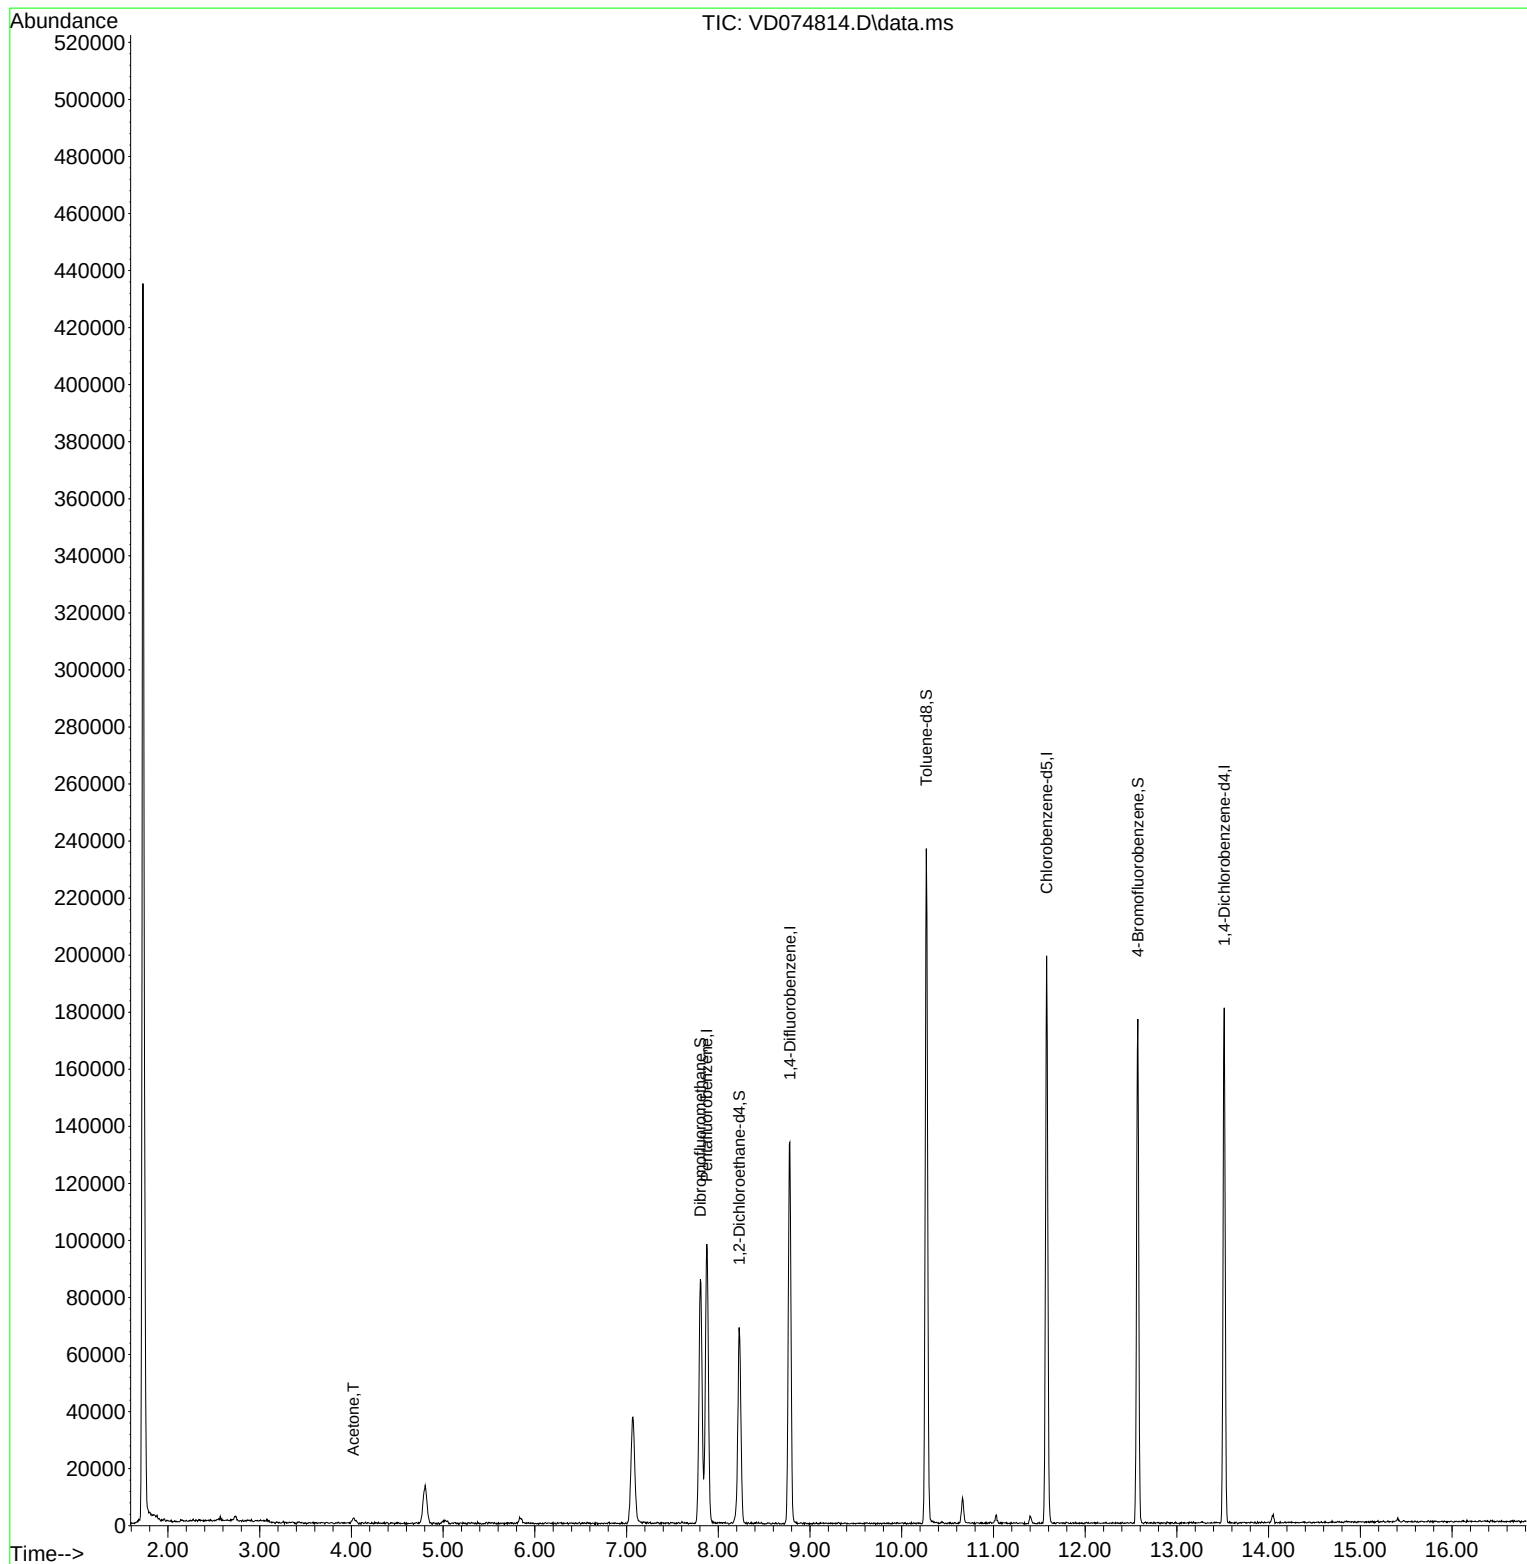


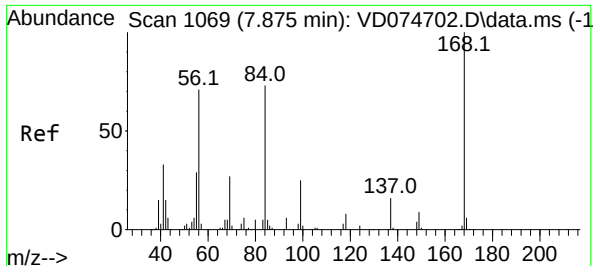

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD074814.D
Acq: 08 Nov 2022 20:11




Instrument :
MSVOA_D
ClientSampleId :
SB-20


Tgt Ion:168 Resp: 82923
Ion Ratio Lower Upper
168 100
99 47.0 40.9 61.3

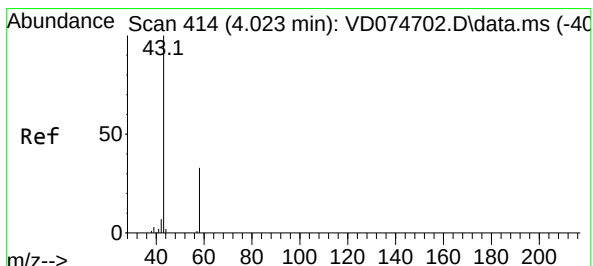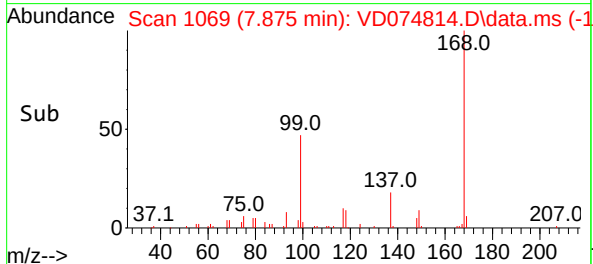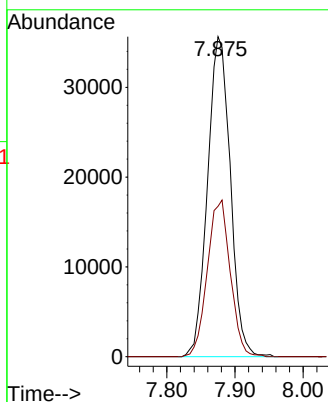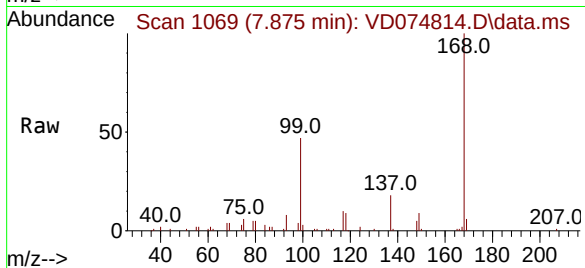

#16
Acetone
Concen: 22.217 ug/l
RT: 4.022 min Scan# 414
Delta R.T. -0.001 min
Lab File: VD074814.D
Acq: 08 Nov 2022 20:11

Tgt Ion: 43 Resp: 3045
Ion Ratio Lower Upper
43 100
58 51.2 30.2 45.2#

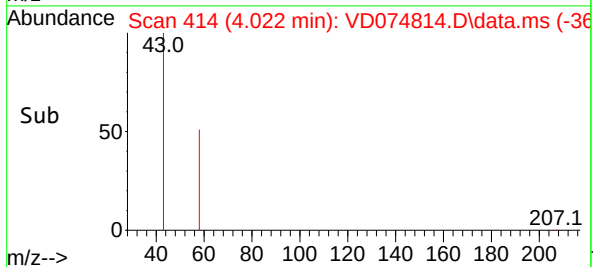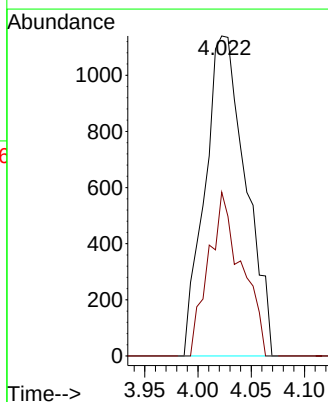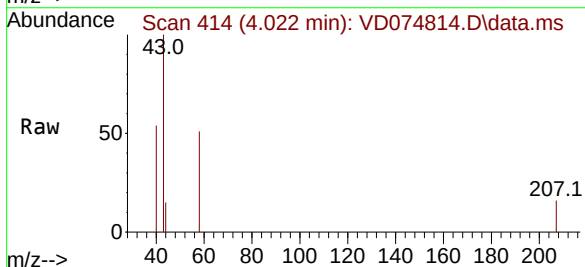

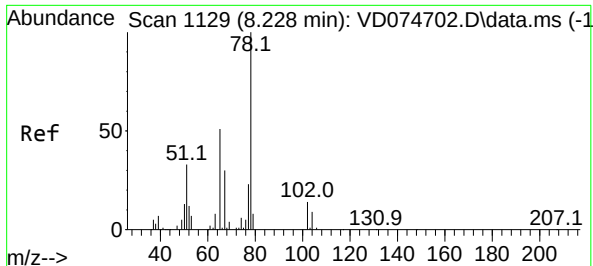

#33

1,2-Dichloroethane-d4

Concen: 80.170 ug/l

RT: 8.228 min Scan# 1129

Delta R.T. -0.000 min

Lab File: VD074814.D

Acq: 08 Nov 2022 20:11

Instrument :

MSVOA_D

ClientSampleId :





SB-20

Tgt Ion: 65 Resp: 52653

Ion Ratio Lower Upper

65 100

67 54.8 0.0 110.2

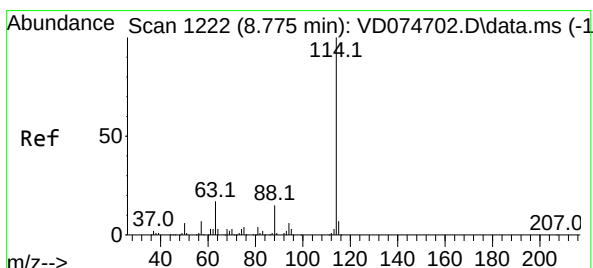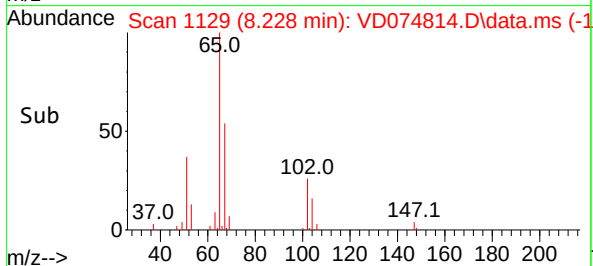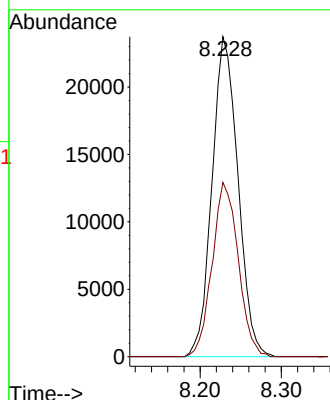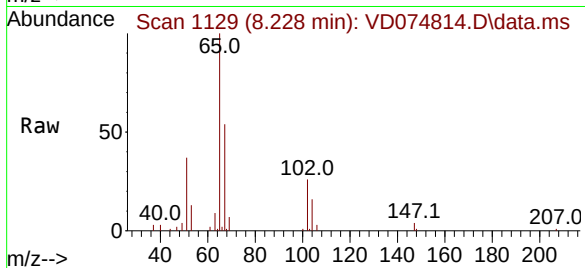

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1223

Delta R.T. 0.006 min

Lab File: VD074814.D

Acq: 08 Nov 2022 20:11




Tgt Ion: 114 Resp: 131620


Ion Ratio Lower Upper

114 100

63 16.4 0.0 33.2

88 14.3 0.0 28.2

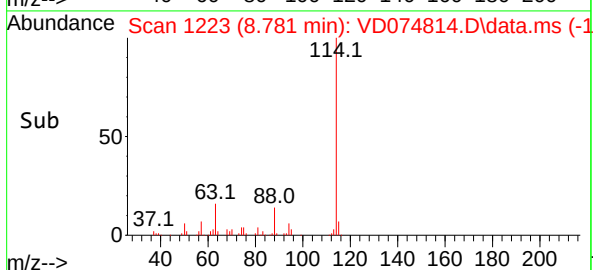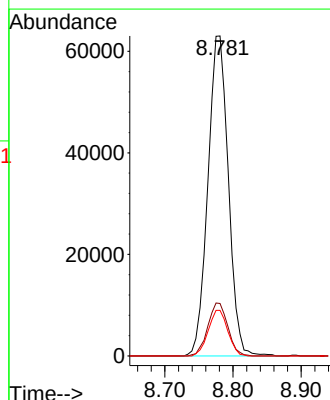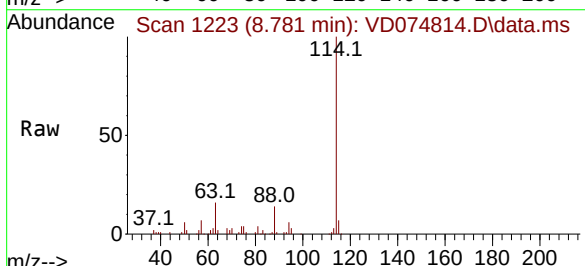

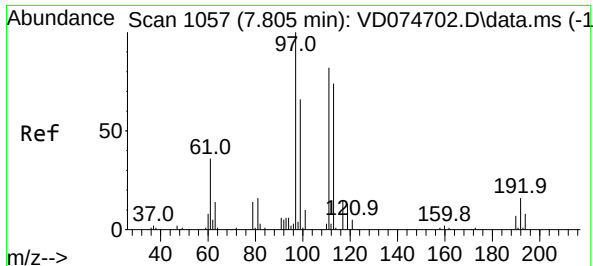

#35

Dibromofluoromethane

Concen: 84.063 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.001 min

Lab File: VD074814.D

Acq: 08 Nov 2022 20:11

Instrument :

MSVOA_D

ClientSampleId :

SB-20





Tgt Ion:113 Resp: 65450

Ion Ratio Lower Upper

113 100

111 100.2 82.3 123.5

192 19.0 16.4 24.6

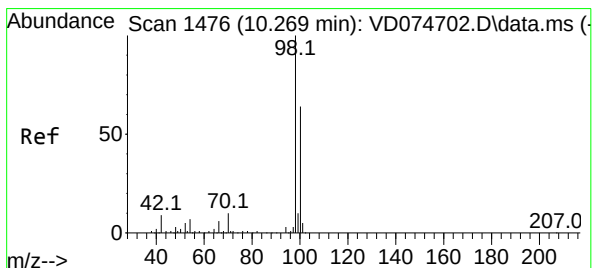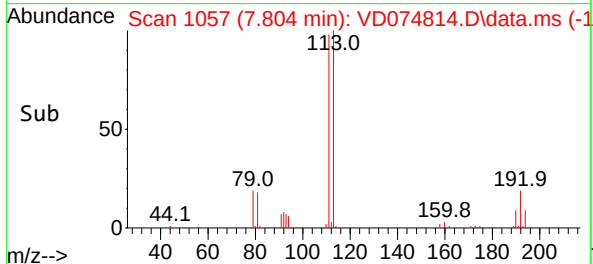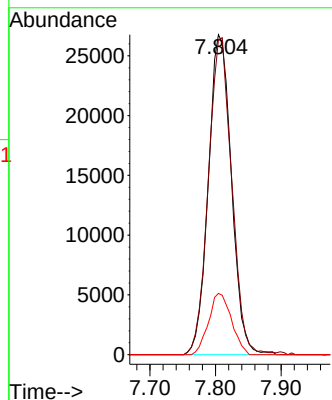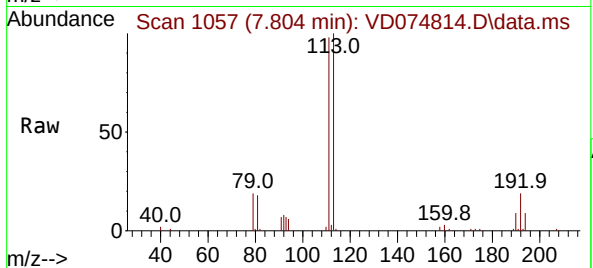

#50

Toluene-d8

Concen: 61.397 ug/l

RT: 10.269 min Scan# 1476

Delta R.T. 0.000 min

Lab File: VD074814.D




Acq: 08 Nov 2022 20:11


Tgt Ion: 98 Resp: 174370

Ion Ratio Lower Upper

98 100

100 63.2 51.4 77.0


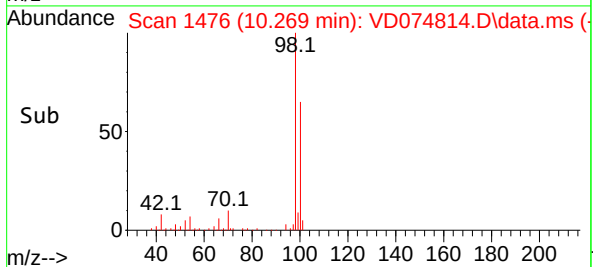
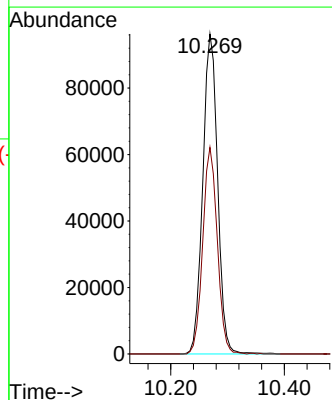
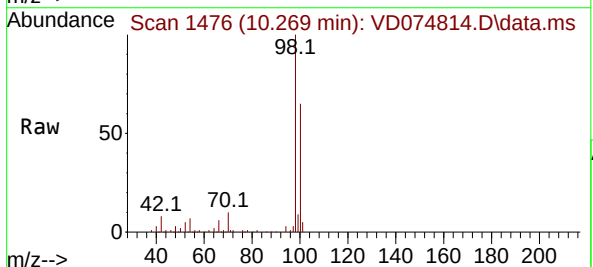


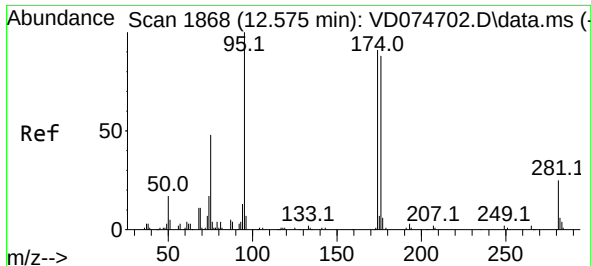

#62
4-Bromofluorobenzene
Concen: 63.464 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD074814.D
Acq: 08 Nov 2022 20:11




Instrument :
MSVOA_D
ClientSampleId :
SB-20


Tgt Ion: 95 Resp: 52041
Ion Ratio Lower Upper
95 100
174 96.8 0.0 197.0
176 93.6 0.0 182.6

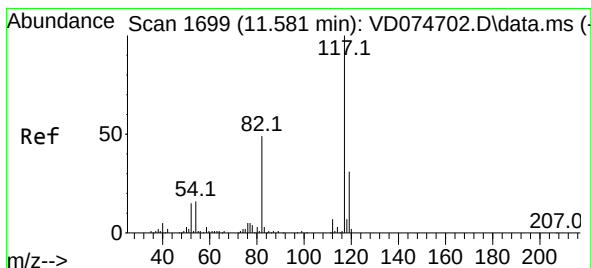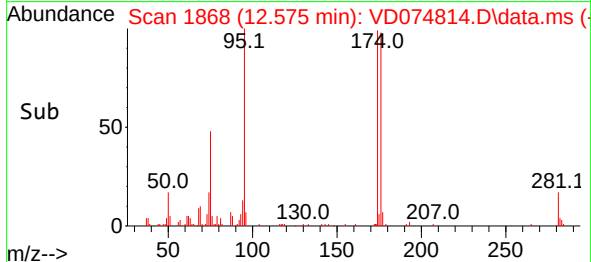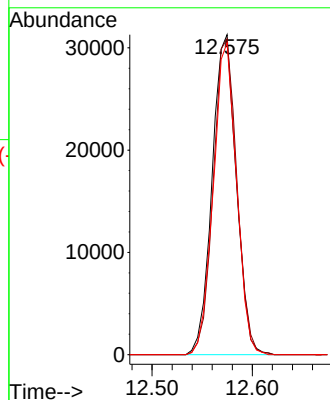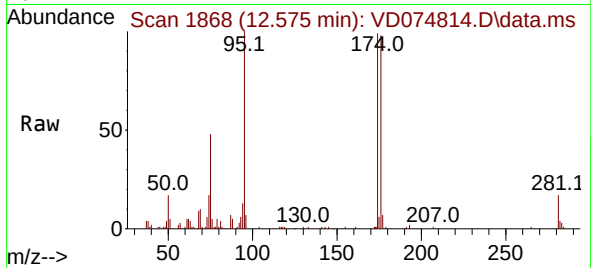

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD074814.D
Acq: 08 Nov 2022 20:11


Tgt Ion: 117 Resp: 124681
Ion Ratio Lower Upper
117 100
82 47.9 41.6 62.4
119 30.7 25.2 37.8

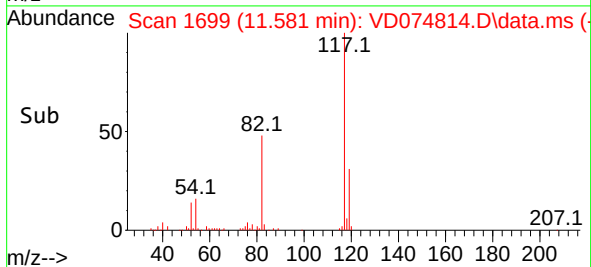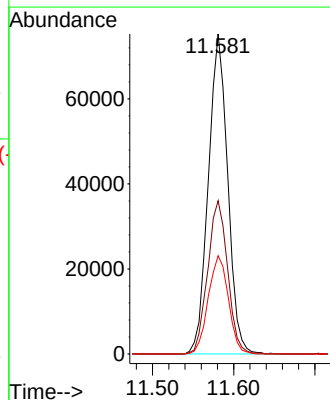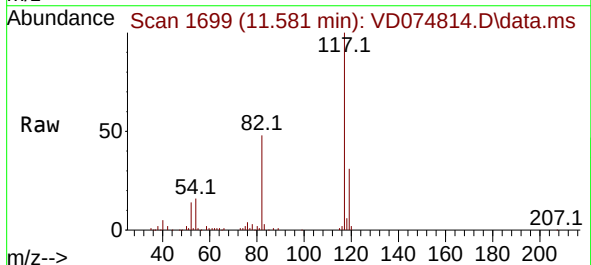

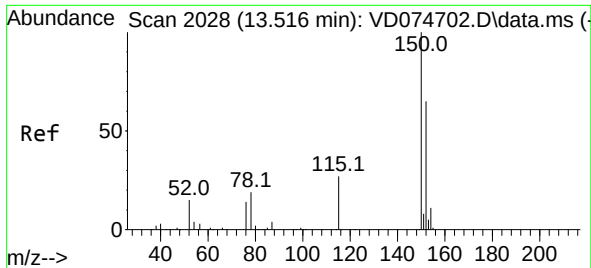

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.516 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VD074814.D
 Acq: 08 Nov 2022 20:11

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-20

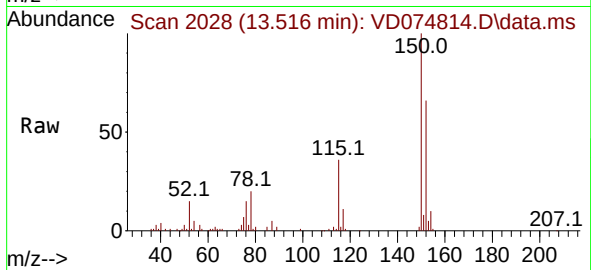

Tgt Ion:152 Resp: 52538
 Ion Ratio Lower Upper
 152 100
 115 54.4 26.8 80.4
 150 154.4 0.0 348.2

