
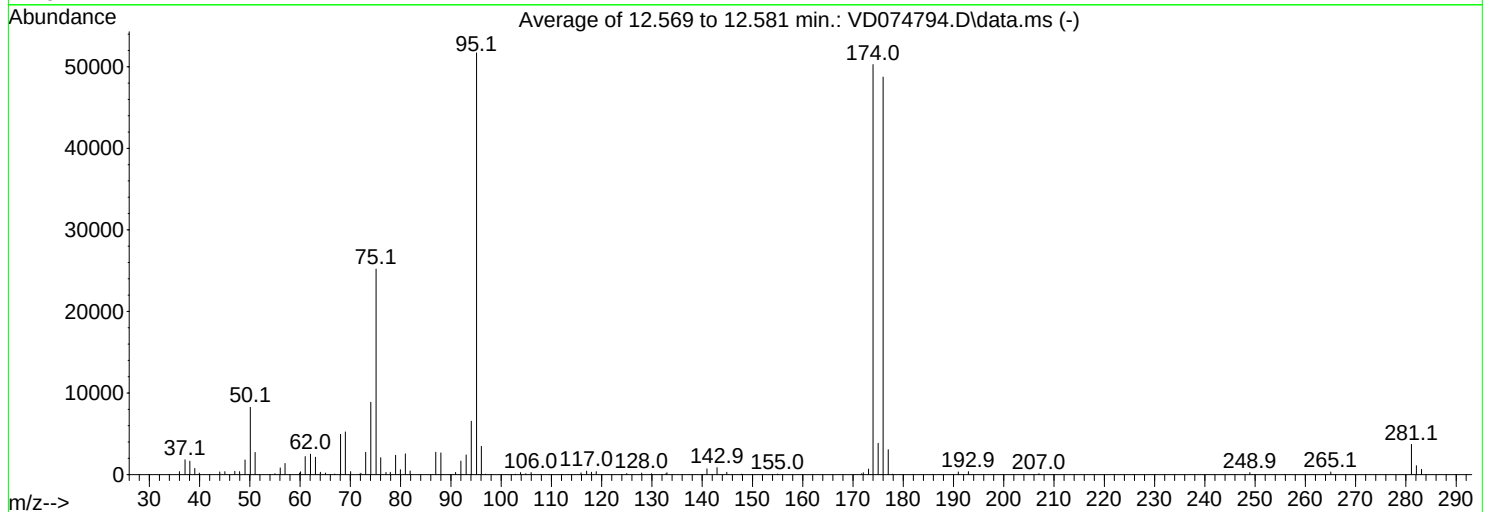


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110822\
Data File : VD074794.D
Acq On : 08 Nov 2022 09:49
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110222S.M
Title : SW846 8260
Last Update : Thu Nov 03 02:30:45 2022

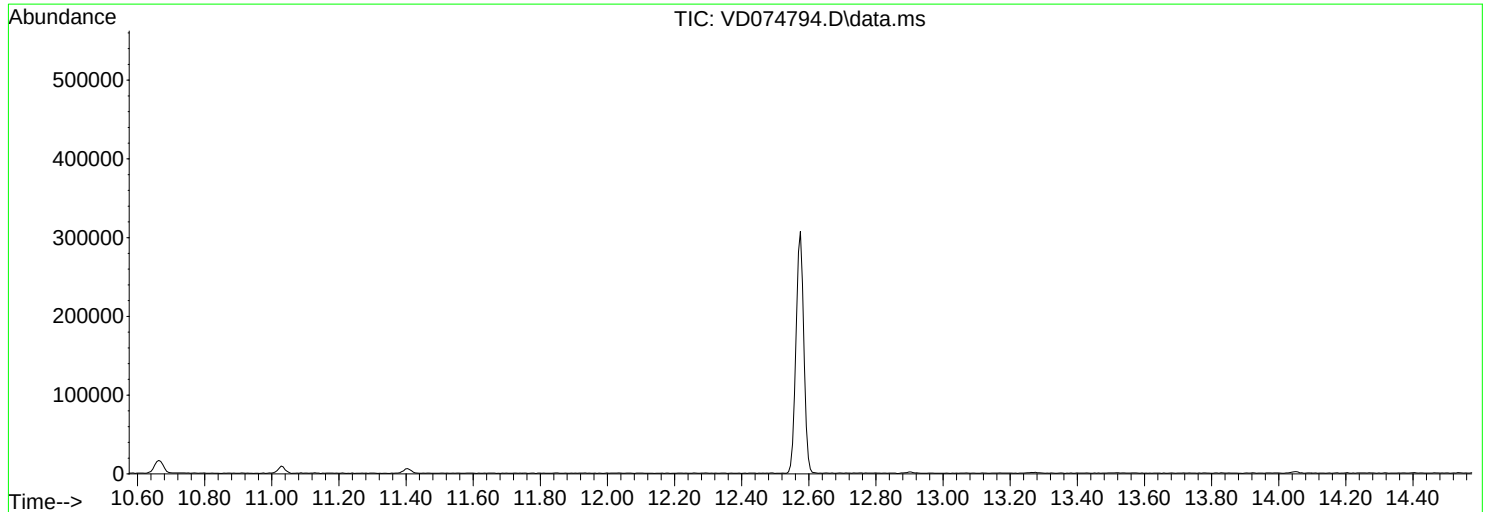

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	8259	PASS
75	95	30	60	48.7	25203	PASS
95	95	100	100	100.0	51704	PASS
96	95	5	9	6.7	3467	PASS
173	174	0.00	2	1.4	690	PASS
174	95	50	100	97.2	50277	PASS
175	174	5	9	7.7	3849	PASS
176	174	95	101	96.9	48736	PASS
177	176	5	9	6.3	3053	PASS