

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110922\
 Data File : VD074829.D
 Acq On : 09 Nov 2022 15:43
 Operator : VA/SY
 Sample : N5520-03
 Misc : 5.07G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 124037

Quant Time: Nov 10 00:36:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110222S.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 03 02:30:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	160792	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	289583	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	257893	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	108325	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	57472	45.129	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	90.260%
35) Dibromofluoromethane	7.810	113	83814	48.928	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.860%
50) Toluene-d8	10.269	98	239944	38.400	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	76.800%
62) 4-Bromofluorobenzene	12.575	95	72822	40.364	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	80.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110922\
Data File : VD074829.D
Acq On : 09 Nov 2022 15:43
Operator : VA/SY
Sample : N5520-03
Misc : 5.07G/5.00ml/MSVOA_D/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
124037

Quant Time: Nov 10 00:36:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110222S.M
Quant Title : SW846 8260
QLast Update : Thu Nov 03 02:30:45 2022
Response via : Initial Calibration




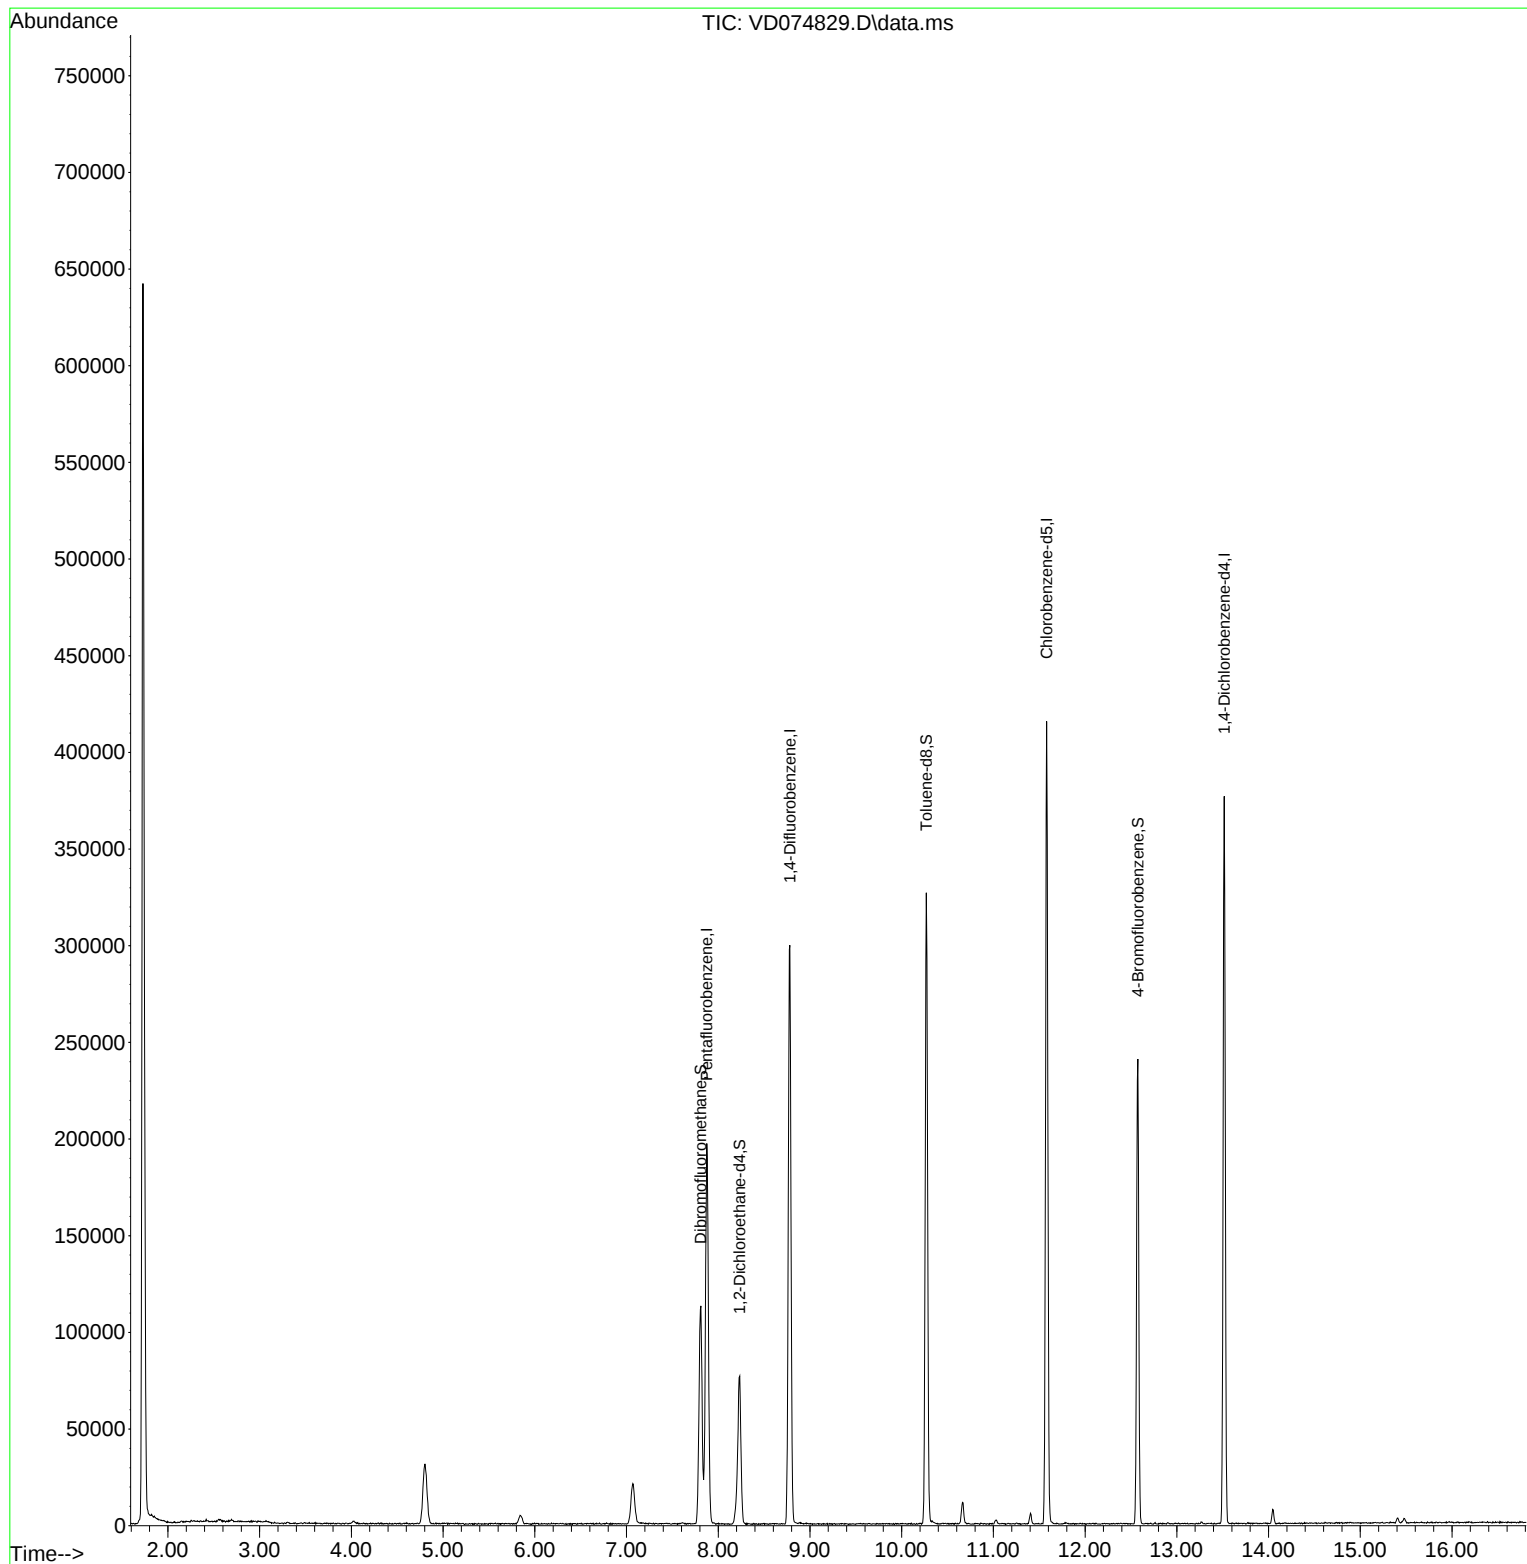


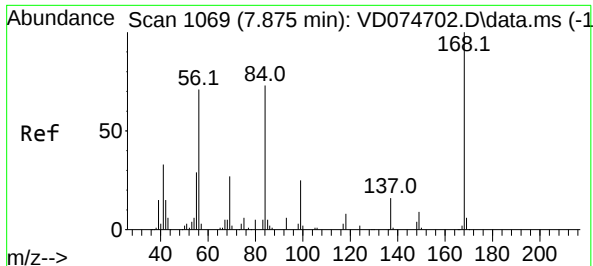

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 110
Delta R.T. 0.000 min
Lab File: VD074829.D
Acq: 09 Nov 2022 15:43




Instrument :
MSVOA_D
ClientSampleId :
124037

Tgt Ion:168 Resp: 160792
Ion Ratio Lower Upper
168 100
99 50.6 40.9 61.3

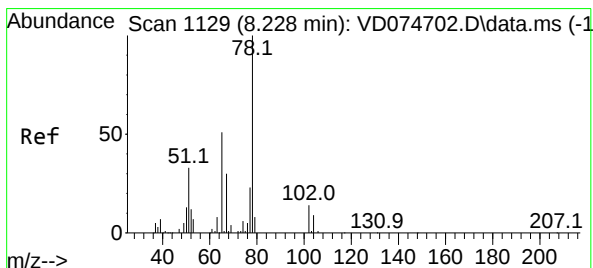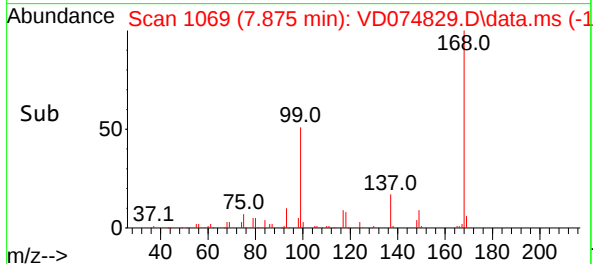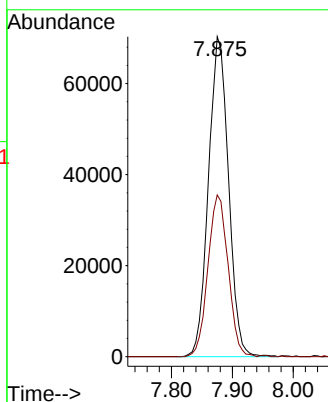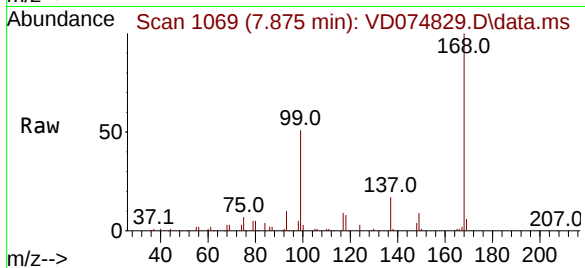

#33
1,2-Dichloroethane-d4
Concen: 45.129 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD074829.D
Acq: 09 Nov 2022 15:43

Tgt Ion: 65 Resp: 57472
Ion Ratio Lower Upper
65 100
67 54.9 0.0 110.2

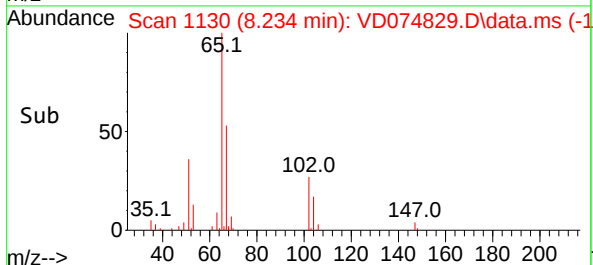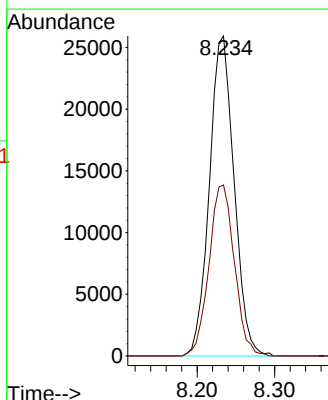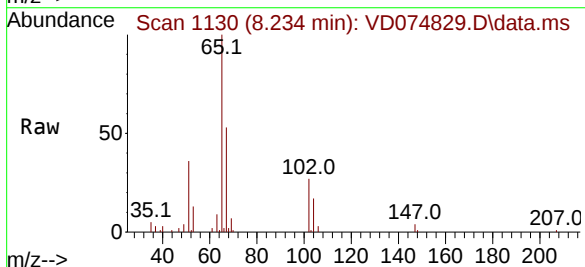



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD074829.D

Acq: 09 Nov 2022 15:43

Instrument :

MSVOA_D

ClientSampleId :

124037





Tgt Ion:114 Resp: 289583

Ion Ratio Lower Upper

114 100

63 16.7 0.0 33.2

88 14.8 0.0 28.2

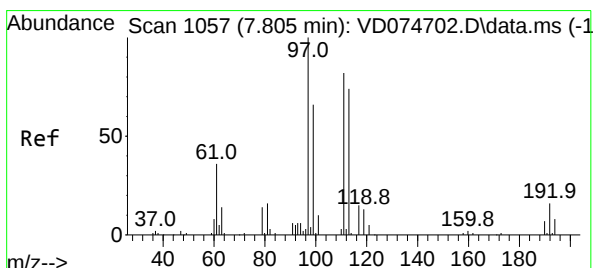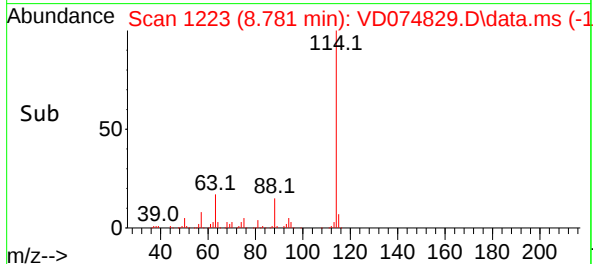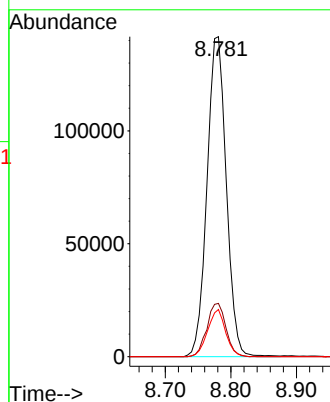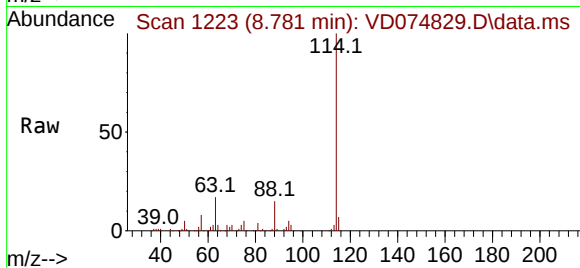

#35

Dibromofluoromethane

Concen: 48.928 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.005 min

Lab File: VD074829.D

Acq: 09 Nov 2022 15:43




Tgt Ion:113 Resp: 83814

Ion Ratio Lower Upper

113 100

111 102.3 82.3 123.5

192 19.5 16.4 24.6


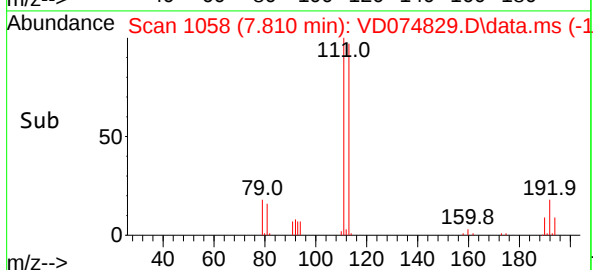
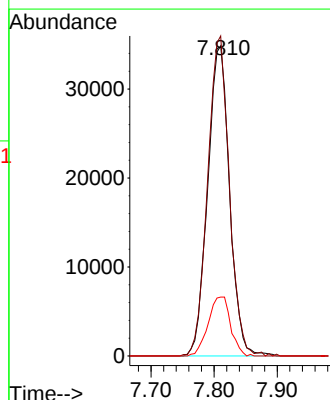
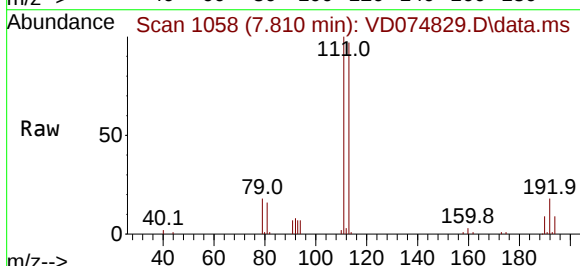




#50
Toluene-d8
Concen: 38.400 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD074829.D
Acq: 09 Nov 2022 15:43




Instrument :
MSVOA_D
ClientSampleId :
124037


Tgt Ion: 98 Resp: 239944
Ion Ratio Lower Upper
98 100
100 63.8 51.4 77.0

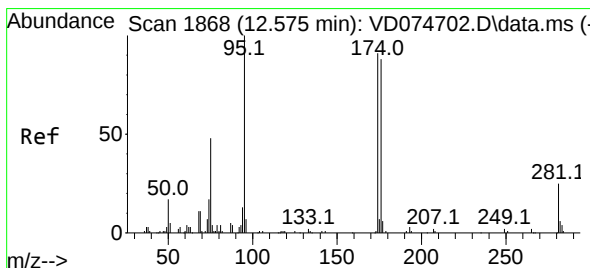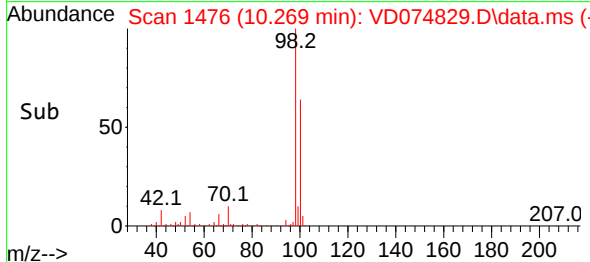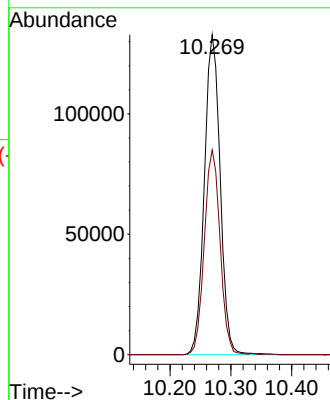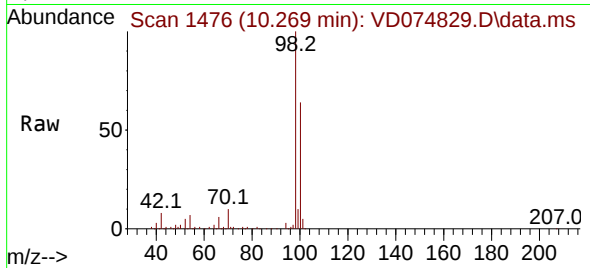

#62
4-Bromofluorobenzene
Concen: 40.364 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD074829.D
Acq: 09 Nov 2022 15:43


Tgt Ion: 95 Resp: 72822
Ion Ratio Lower Upper
95 100
174 97.6 0.0 197.0
176 92.2 0.0 182.6

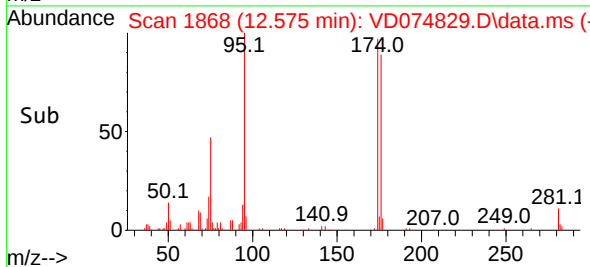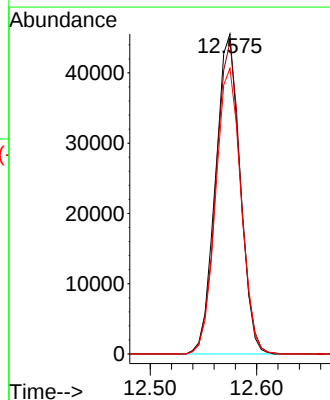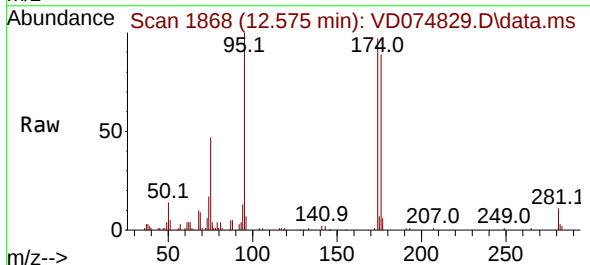



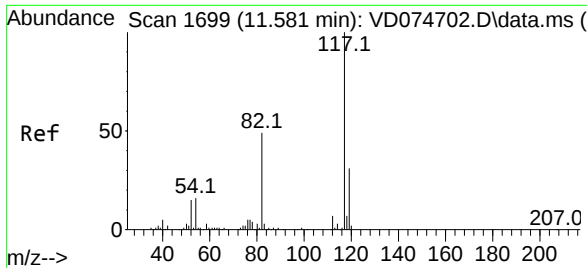


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD074829.D
Acq: 09 Nov 2022 15:43


Instrument :
MSVOA_D
ClientSampleId :
124037

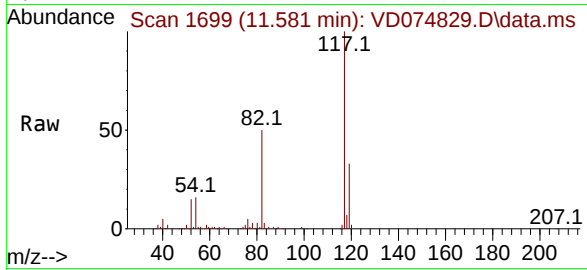

Tgt Ion:117 Resp: 257893
Ion Ratio Lower Upper
117 100
82 50.0 41.6 62.4
119 32.6 25.2 37.8

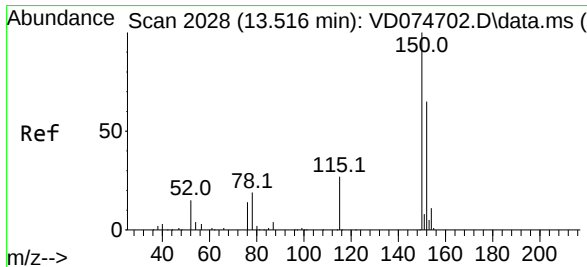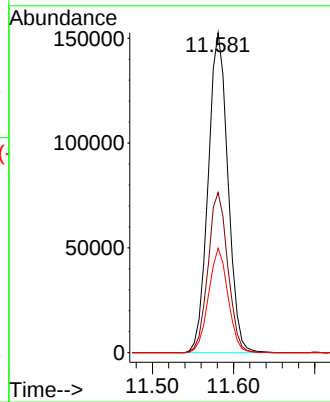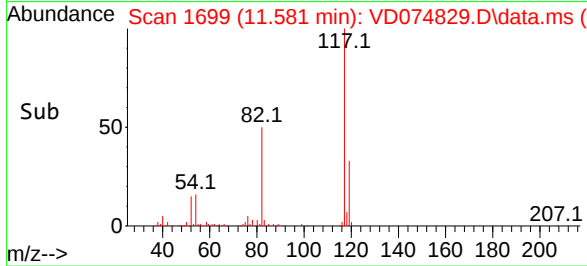

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. 0.000 min
Lab File: VD074829.D
Acq: 09 Nov 2022 15:43

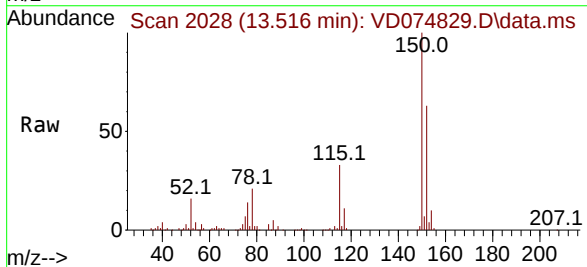

Tgt Ion:152 Resp: 108325
Ion Ratio Lower Upper
152 100
115 54.3 26.8 80.4
150 156.9 0.0 348.2

