
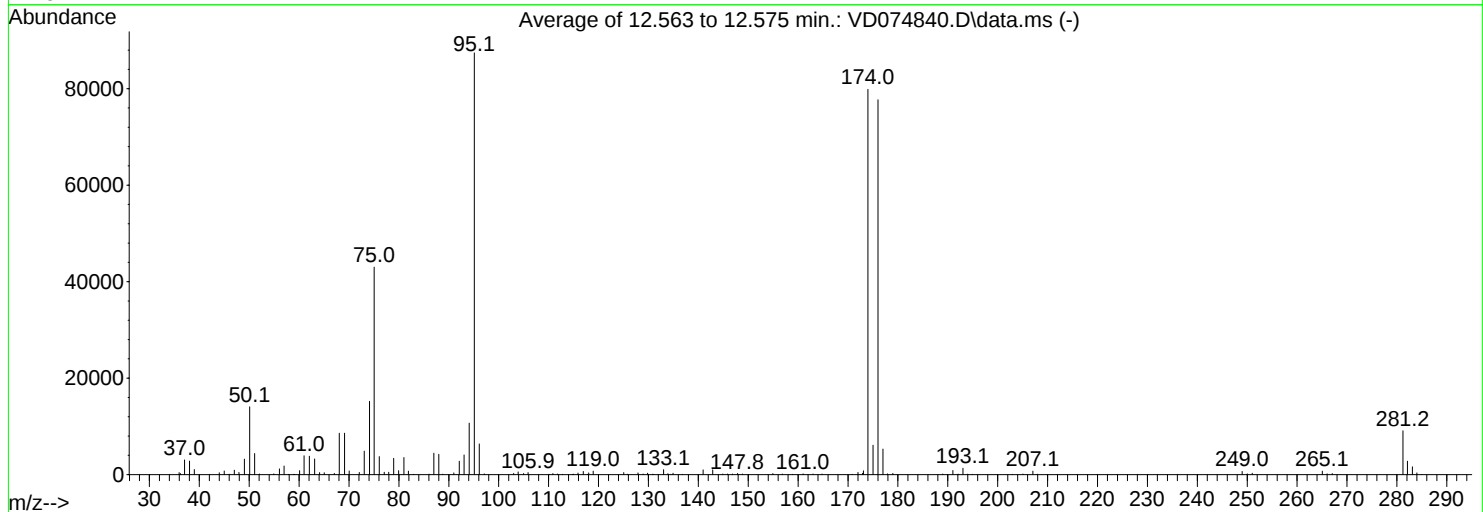


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110922\
 Data File : VD074840.D
 Acq On : 09 Nov 2022 21:13
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110222S.M
 Title : SW846 8260
 Last Update : Thu Nov 03 02:30:45 2022

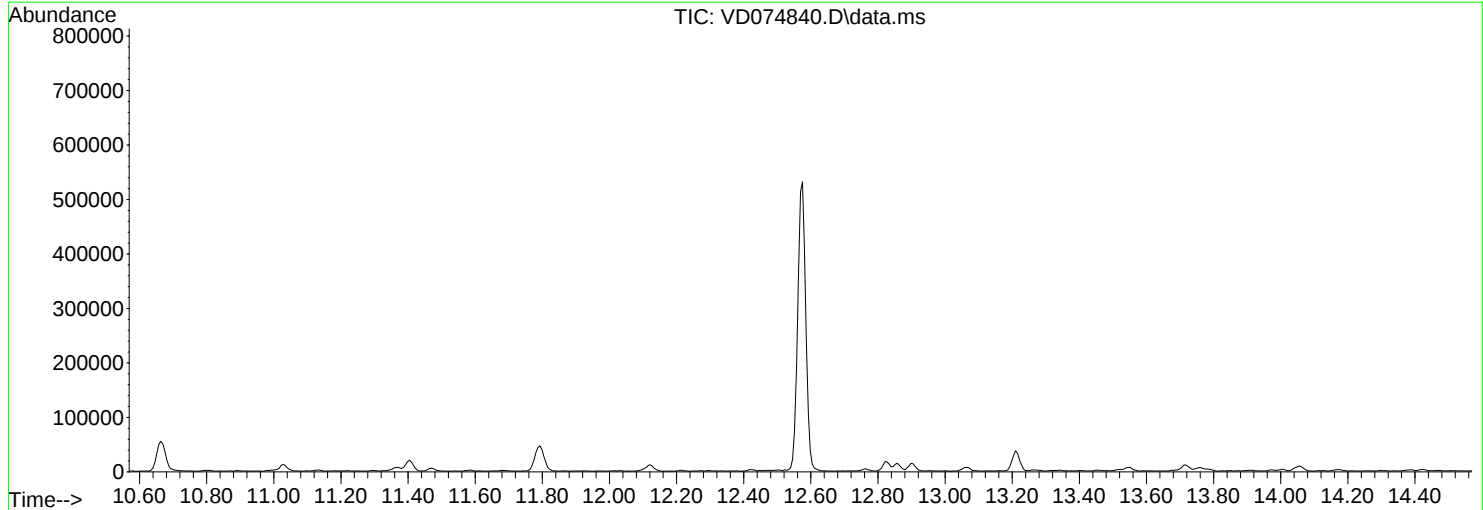

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	14056	PASS
75	95	30	60	49.2	43003	PASS
95	95	100	100	100.0	87429	PASS
96	95	5	9	7.3	6367	PASS
173	174	0.00	2	1.0	805	PASS
174	95	50	100	91.4	79872	PASS
175	174	5	9	7.6	6107	PASS
176	174	95	101	97.3	77709	PASS
177	176	5	9	6.8	5296	PASS