
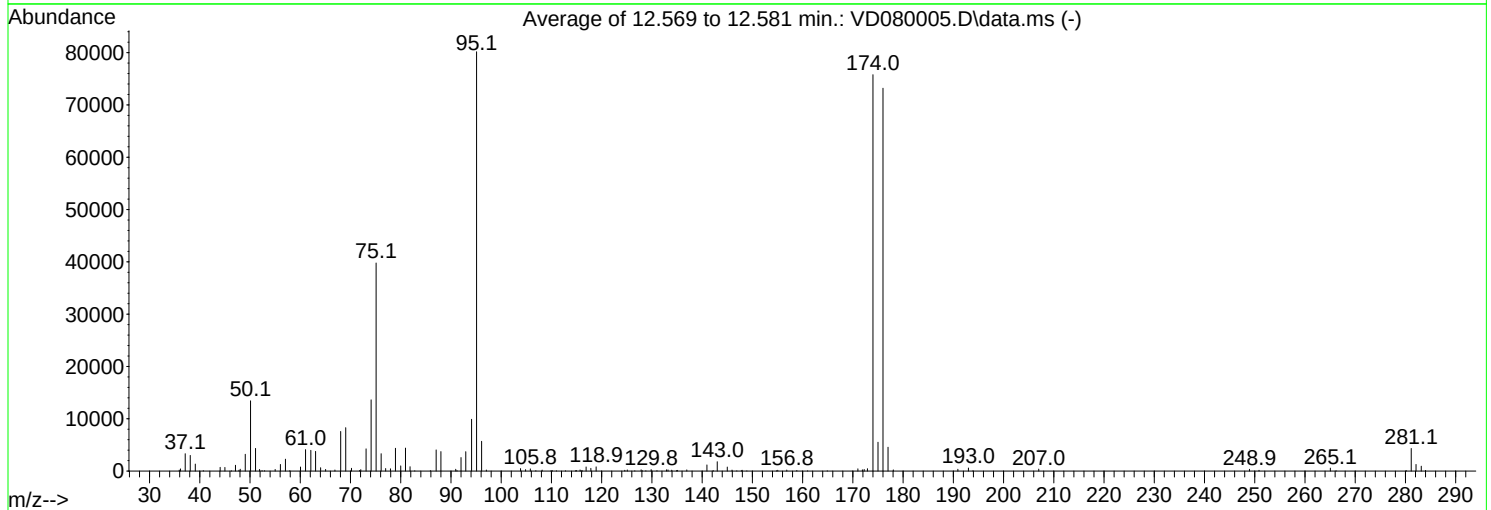


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111424\
Data File : VD080005.D
Acq On : 14 Nov 2024 09:33
Operator : RP/MD
Sample : BFB838
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB838

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM111224SMA.M
Title : SFAM01.0
Last Update : Fri Nov 15 03:41:03 2024

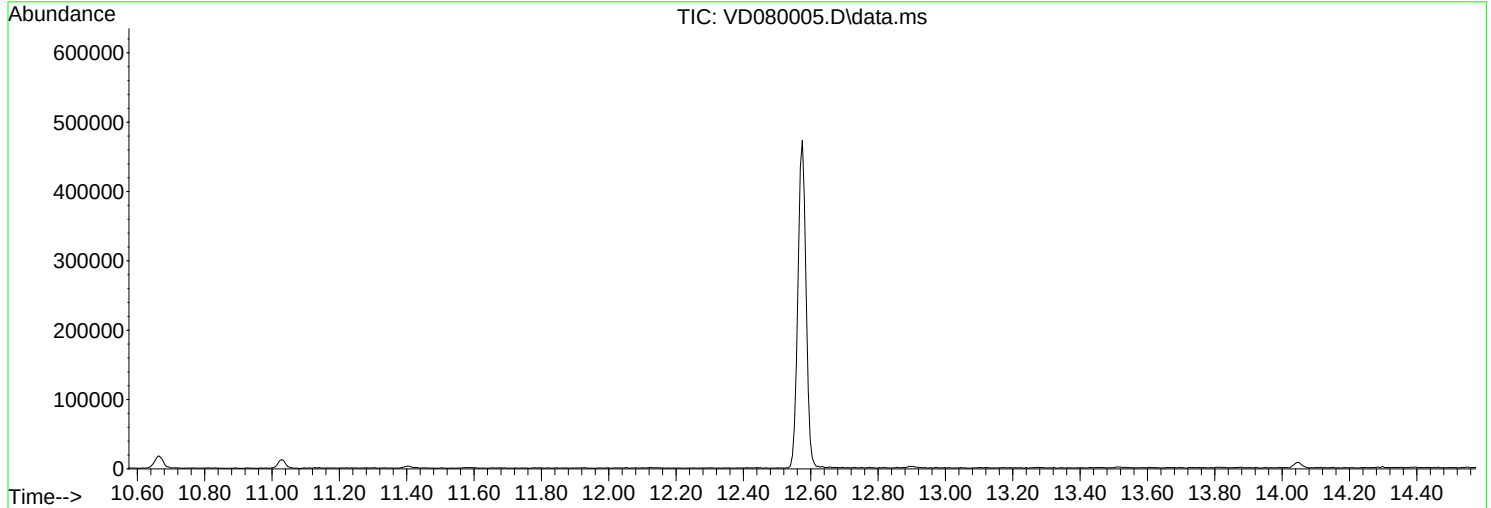

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	13434	PASS
75	95	30	80	49.6	39781	PASS
95	95	100	100	100.0	80171	PASS
96	95	5	9	7.1	5691	PASS
173	174	0.00	2	0.6	460	PASS
174	95	50	120	94.5	75781	PASS
175	174	5	9	7.3	5512	PASS
176	174	95	105	96.6	73192	PASS
177	176	5	10	6.2	4561	PASS

Scan 1859 (12.522 min): VD080005.D\data.ms
BFB838

m/z	Abundance
40.00	960.0
44.10	183.0

Instrument :
MSVOA_D
ClientSampleId :
BFB838

m/z	Abundance
36.10	641.0
37.10	3445.0
38.10	3319.0
39.10	1519.0
40.00	917.0
40.70	262.0
44.00	838.0
45.10	950.0
47.00	1579.0
47.80	504.0
49.00	3377.0
50.10	14901.0
51.10	4123.0
51.90	186.0
52.40	246.0
52.90	236.0
55.10	276.0
56.10	1349.0
57.10	2034.0
60.10	679.0
61.10	3786.0
62.10	4900.0
63.10	3664.0
64.10	742.0
65.10	200.0
67.00	322.0
68.00	7982.0
69.10	8946.0
70.20	675.0
71.80	344.0
73.10	4080.0
74.10	13635.0
75.10	41184.0
76.10	3476.0
76.90	478.0
78.10	328.0
79.00	4428.0
80.00	1008.0
80.90	4652.0
81.80	753.0
87.10	3902.0
88.00	3592.0
91.00	606.0
92.00	2537.0
93.00	3594.0
94.10	9633.0
95.10	80504.0
96.10	5528.0
97.10	165.0
103.80	420.0
104.90	449.0
105.80	479.0
106.90	243.0
108.10	197.0
109.90	171.0
112.80	170.0
114.80	229.0
115.70	316.0
116.90	739.0
117.80	488.0
118.90	1041.0
124.60	152.0
126.60	169.0
127.90	503.0
128.80	203.0
129.90	356.0
131.00	296.0
132.90	311.0
134.00	275.0
134.90	312.0
137.00	216.0
141.00	1178.0
143.00	2075.0
144.90	580.0
147.80	188.0
155.10	217.0
158.80	175.0
171.10	666.0
172.20	517.0
172.90	1381.0
174.00	75312.0
175.00	5339.0
176.00	69088.0
177.00	4445.0
178.00	277.0
191.00	265.0
193.00	559.0
207.00	376.0
249.10	355.0
265.10	507.0
281.10	3805.0
282.10	1221.0

Instrument :
MSVOA_D
ClientSampleId :
BFB838

283.10937.0

284.00339.0

Instrument :
MSVOA_D
ClientSampleId :
BFB838

m/z	Abundance
36.20	629.0
37.10	3546.0
38.10	3432.0
39.10	1243.0
39.90	980.0
44.00	1119.0
45.00	626.0
46.30	175.0
47.10	982.0
48.00	681.0
49.00	3303.0
50.10	14220.0
51.10	4878.0
52.00	371.0
55.10	271.0
56.00	1326.0
57.10	2297.0
57.90	173.0
60.00	1030.0
61.00	4514.0
62.10	4024.0
63.00	4525.0
64.00	681.0
65.00	325.0
68.10	7267.0
69.10	9004.0
70.20	489.0
72.00	378.0
73.10	4479.0
74.10	15731.0
75.10	43112.0
76.10	3518.0
77.00	619.0
77.90	627.0
78.90	4955.0
80.00	1107.0
81.00	4474.0
81.90	985.0
82.80	155.0
85.90	225.0
87.10	4035.0
88.00	4105.0
90.90	437.0
92.00	3020.0
92.90	3533.0
94.10	10534.0
95.10	90152.0
96.10	5996.0
97.00	272.0
103.90	556.0
104.90	243.0
105.80	534.0
108.20	217.0
115.00	340.0
115.90	337.0
116.90	849.0
117.90	430.0
118.90	876.0
124.60	308.0
125.10	414.0
127.80	250.0
129.80	212.0
133.20	690.0
135.10	221.0
137.00	167.0
140.90	1427.0
142.20	278.0
143.00	1997.0
145.00	1193.0
146.00	327.0
148.00	291.0
148.90	153.0
154.80	184.0
156.90	326.0
158.90	201.0
161.00	178.0
170.90	373.0
171.90	375.0
172.30	421.0
174.00	81976.0
175.00	5790.0
176.00	82408.0
177.00	4961.0
178.10	261.0
190.80	204.0
193.00	500.0
193.90	176.0
206.90	386.0
248.90	359.0
251.00	157.0
265.00	772.0
266.20	157.0

Instrument :
MSVOA_D
ClientSampleId :
BFB838

280.20	203.0
281.20	4721.0
282.10	1370.0
283.20	892.0

Instrument :
MSVOA_D
ClientSampleId :
BFB838

m/z	Abundance
35.90	554.0
37.10	2977.0
38.00	2218.0
39.10	1265.0
40.10	951.0
44.10	736.0
44.90	531.0
47.20	777.0
48.10	402.0
49.10	2952.0
50.10	11182.0
51.10	4004.0
51.80	401.0
54.90	393.0
56.00	1135.0
57.00	2501.0
60.10	653.0
61.10	4009.0
62.10	2976.0
63.10	3109.0
64.10	515.0
65.00	398.0
66.80	315.0
68.00	7455.0
69.00	6936.0
70.20	445.0
72.10	462.0
73.10	4205.0
74.10	11483.0
75.10	35048.0
76.10	2981.0
77.10	360.0
78.00	367.0
79.00	3694.0
80.00	864.0
81.00	4074.0
81.90	772.0
87.00	4214.0
88.00	3493.0
91.20	310.0
92.00	2218.0
93.00	4011.0
94.10	9541.0
95.10	69856.0
96.10	5550.0
97.10	183.0
103.90	462.0
104.70	157.0
105.80	252.0
108.10	167.0
110.20	181.0
111.00	175.0
115.70	360.0
116.20	155.0
116.90	785.0
117.90	663.0
118.90	524.0
125.10	253.0
128.10	201.0
129.80	301.0
132.90	445.0
133.90	242.0
135.10	187.0
136.90	301.0
141.00	923.0
143.00	1314.0
145.10	538.0
145.90	256.0
146.90	160.0
147.90	217.0
155.00	262.0
156.80	285.0
164.90	174.0
170.90	246.0
171.90	366.0
174.00	70056.0
175.00	5406.0
176.00	68080.0
177.00	4278.0
178.00	161.0
190.90	579.0
193.00	697.0
207.10	364.0
248.90	309.0
250.80	315.0
265.10	434.0
281.10	4439.0
282.10	1202.0
283.10	986.0

Instrument :
MSVOA_D
ClientSampleId :
BFB838