

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111924\
 Data File : VD080092.D
 Acq On : 19 Nov 2024 19:13
 Operator : RP/MD
 Sample : P4833-07
 Misc : 5.23G/5ml/MSVOA_D/SOIL/B
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-2-VOC

Quant Time: Nov 20 03:58:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 15 16:25:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	115861	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	209582	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	198863	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	90585	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	80940	67.851	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	135.700%
35) Dibromofluoromethane	7.805	113	83220	59.663	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	119.320%
50) Toluene-d8	10.269	98	278333	52.944	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	105.880%
62) 4-Bromofluorobenzene	12.569	95	85180	49.385	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	98.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111924\
Data File : VD080092.D
Acq On : 19 Nov 2024 19:13
Operator : RP/MD
Sample : P4833-07
Misc : 5.23G/5ml/MSVOA_D/SOIL/B
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-2-VOC


Quant Time: Nov 20 03:58:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111524S.M
Quant Title : SW846 8260
QLast Update : Fri Nov 15 16:25:47 2024
Response via : Initial Calibration

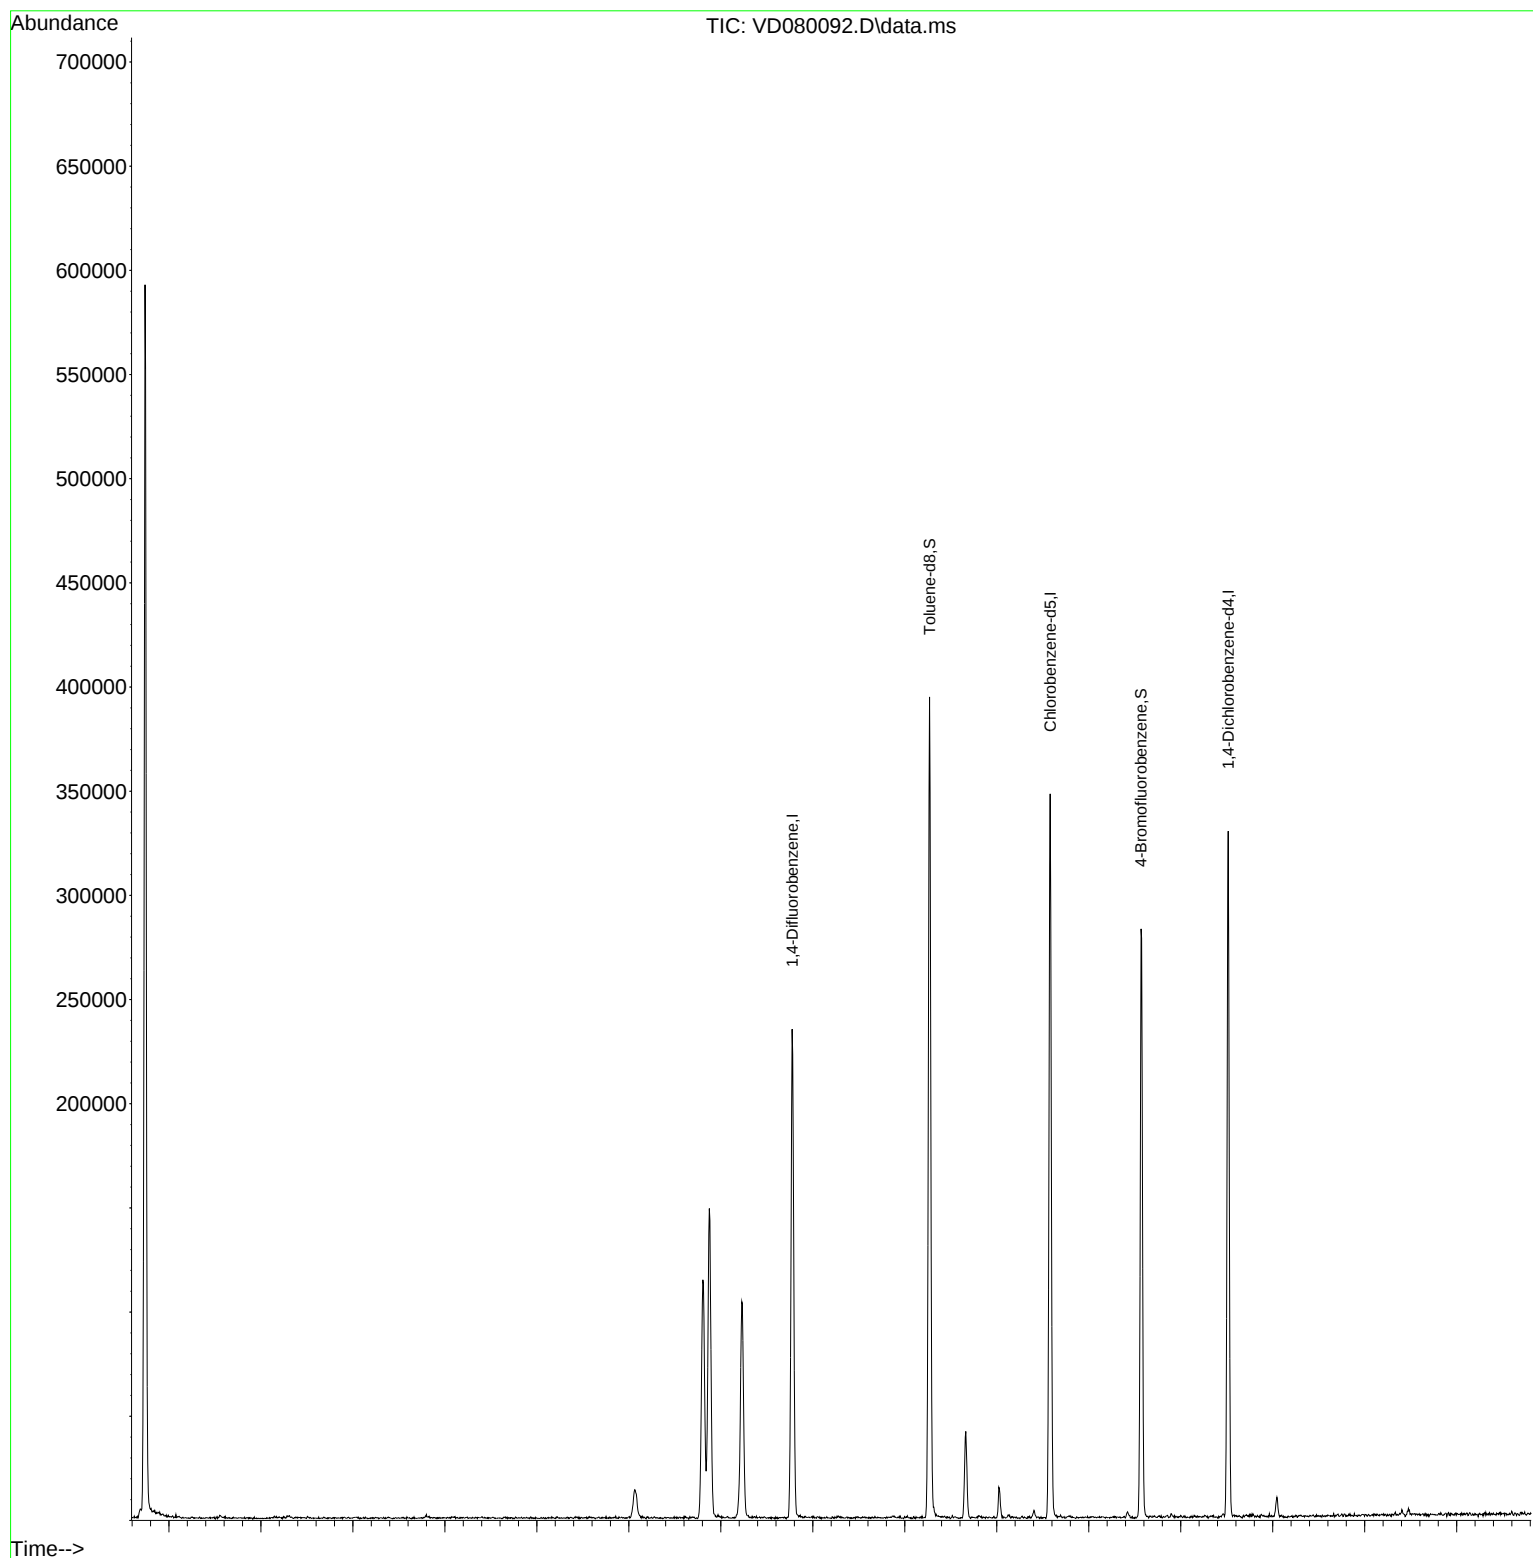



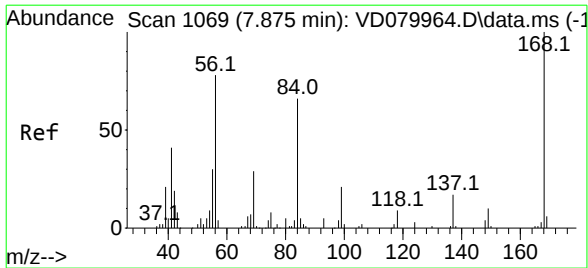


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD080092.D
Acq: 19 Nov 2024 19:13


Instrument :
MSVOA_D
ClientSampleId :
TP-2-VOC

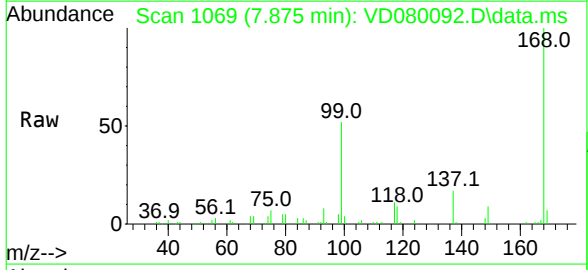



Tgt Ion:168 Resp: 115861
Ion Ratio Lower Upper
168 100
99 52.1 46.0 69.0

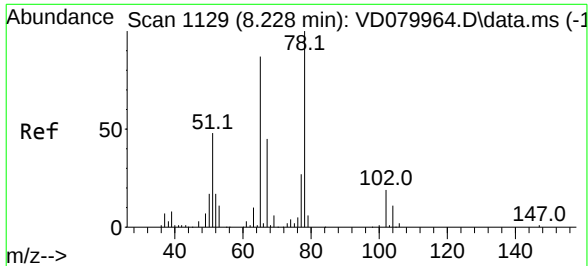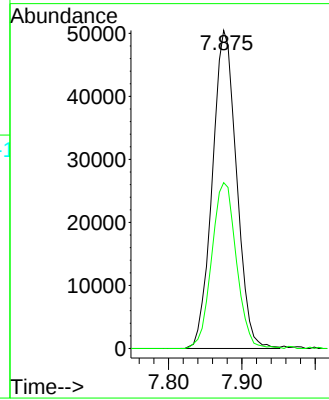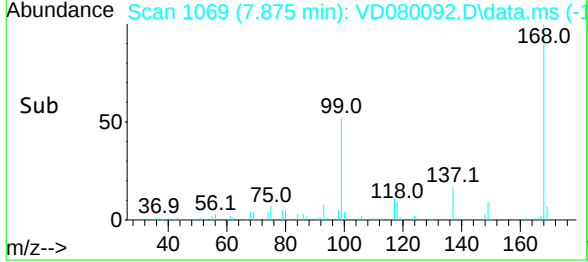


#33
1,2-Dichloroethane-d4
Concen: 67.851 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VD080092.D
Acq: 19 Nov 2024 19:13

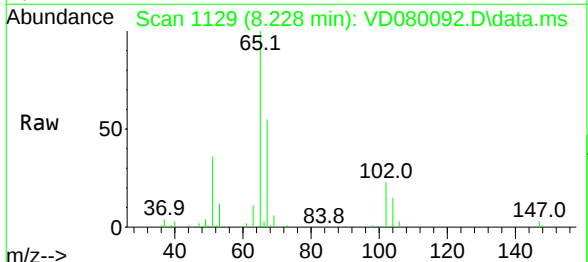

Tgt Ion: 65 Resp: 80940
Ion Ratio Lower Upper
65 100
67 54.5 0.0 109.2



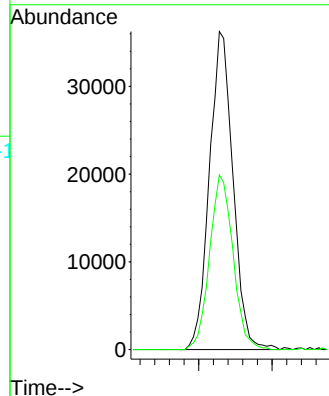
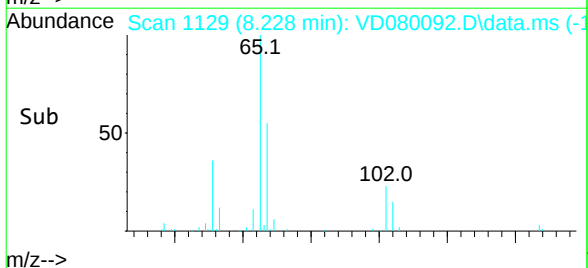


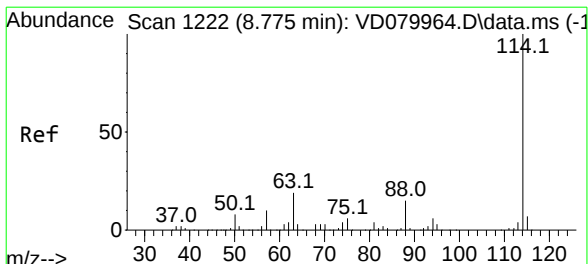

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.775 min Scan# 12
 Delta R.T. 0.000 min
 Lab File: VD080092.D
 Acq: 19 Nov 2024 19:13




Instrument :
 MSVOA_D
 ClientSampleId :
 TP-2-VOC


Tgt Ion:	114	Resp:	209582
Ion	Ratio	Lower	Upper
114	100		
63	18.1	0.0	38.8
88	14.9	0.0	30.6

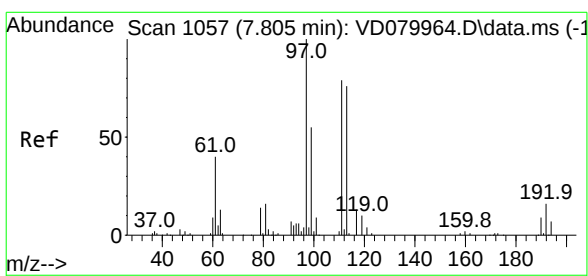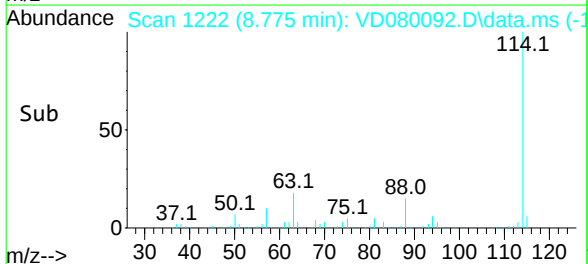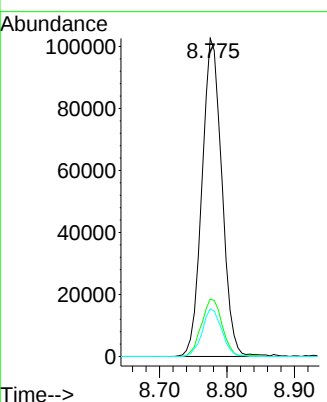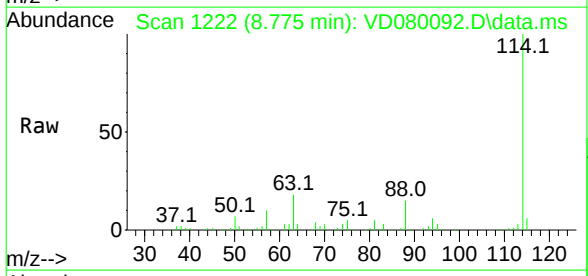

#35
 Dibromofluoromethane
 Concen: 59.663 ug/l
 RT: 7.805 min Scan# 1057
 Delta R.T. -0.000 min
 Lab File: VD080092.D
 Acq: 19 Nov 2024 19:13

Tgt Ion:	113	Resp:	83220
Ion	Ratio	Lower	Upper
113	100		
111	102.9	82.5	123.7
192	20.0	16.6	25.0

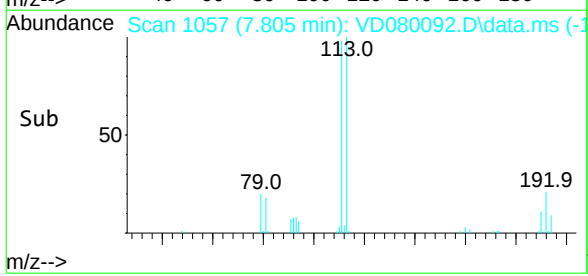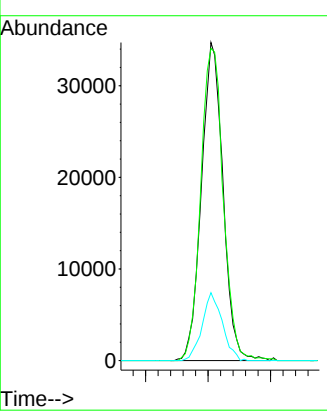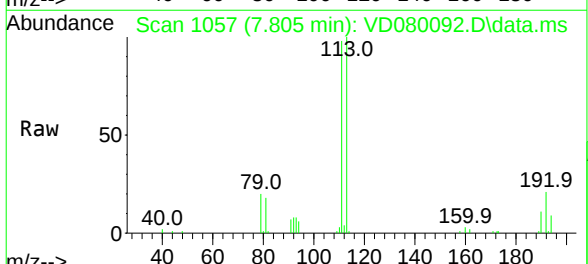

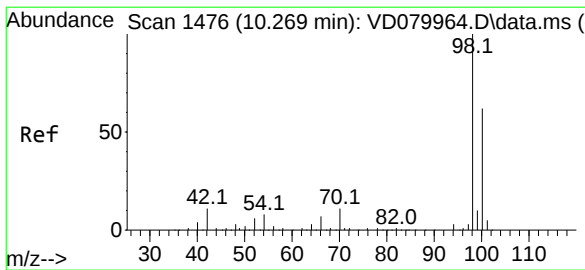

#50

Toluene-d8

Concen: 52.944 ug/l

RT: 10.269 min Scan# 14

Delta R.T. 0.000 min

Lab File: VD080092.D

Acq: 19 Nov 2024 19:13

Instrument :

MSVOA_D

ClientSampleId :





TP-2-VOC

Tgt Ion: 98 Resp: 278333

Ion Ratio Lower Upper

98 100

100 61.6 50.2 75.4

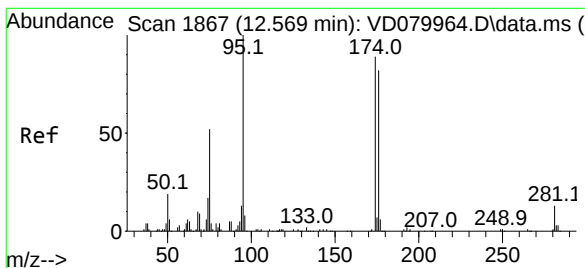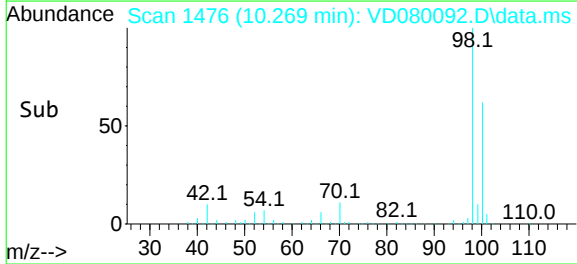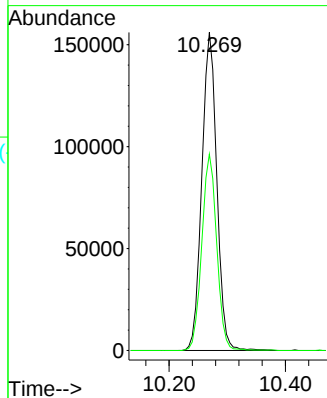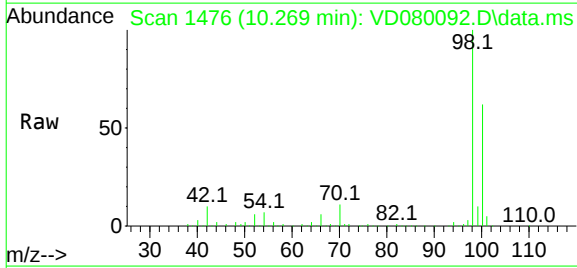

#62

4-Bromofluorobenzene

Concen: 49.385 ug/l

RT: 12.569 min Scan# 1867

Delta R.T. 0.000 min

Lab File: VD080092.D

Acq: 19 Nov 2024 19:13




Tgt Ion: 95 Resp: 85180


Ion Ratio Lower Upper

95 100

174 91.0 0.0 173.4

176 88.3 0.0 166.6


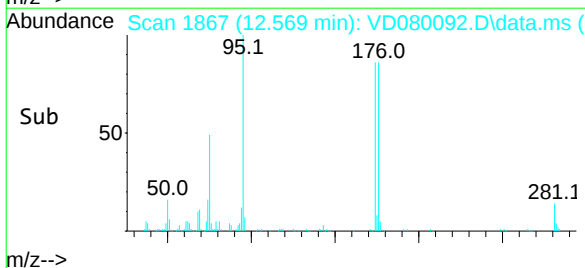
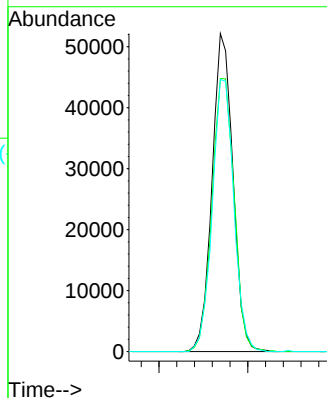
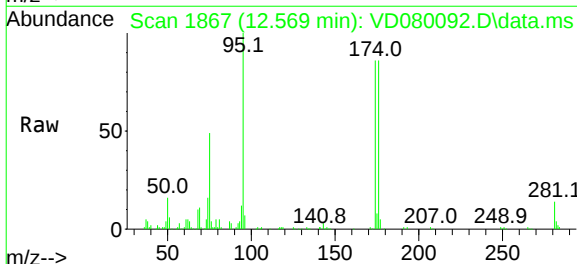


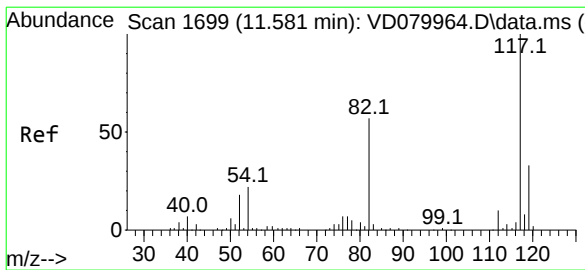

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD080092.D
Acq: 19 Nov 2024 19:13

Instrument :
MSVOA_D
ClientSampleId :
TP-2-VOC

Tgt Ion:117 Resp: 198863
Ion Ratio Lower Upper
117 100
82 55.7 45.8 68.6
119 32.7 26.2 39.2

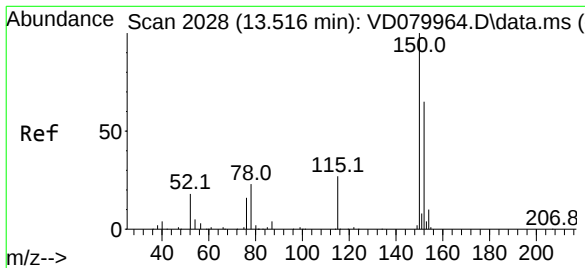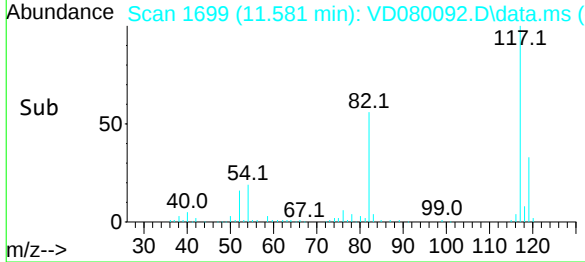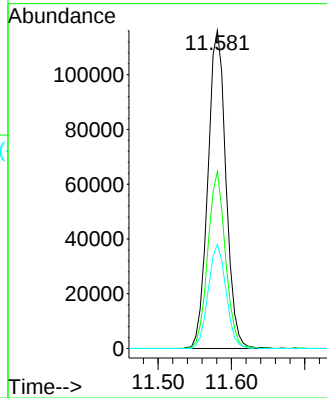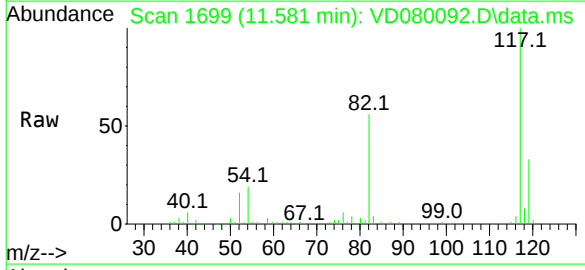

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. 0.000 min
Lab File: VD080092.D
Acq: 19 Nov 2024 19:13

Tgt Ion:152 Resp: 90585
Ion Ratio Lower Upper
152 100
115 58.7 28.9 86.8
150 157.9 0.0 354.8

