
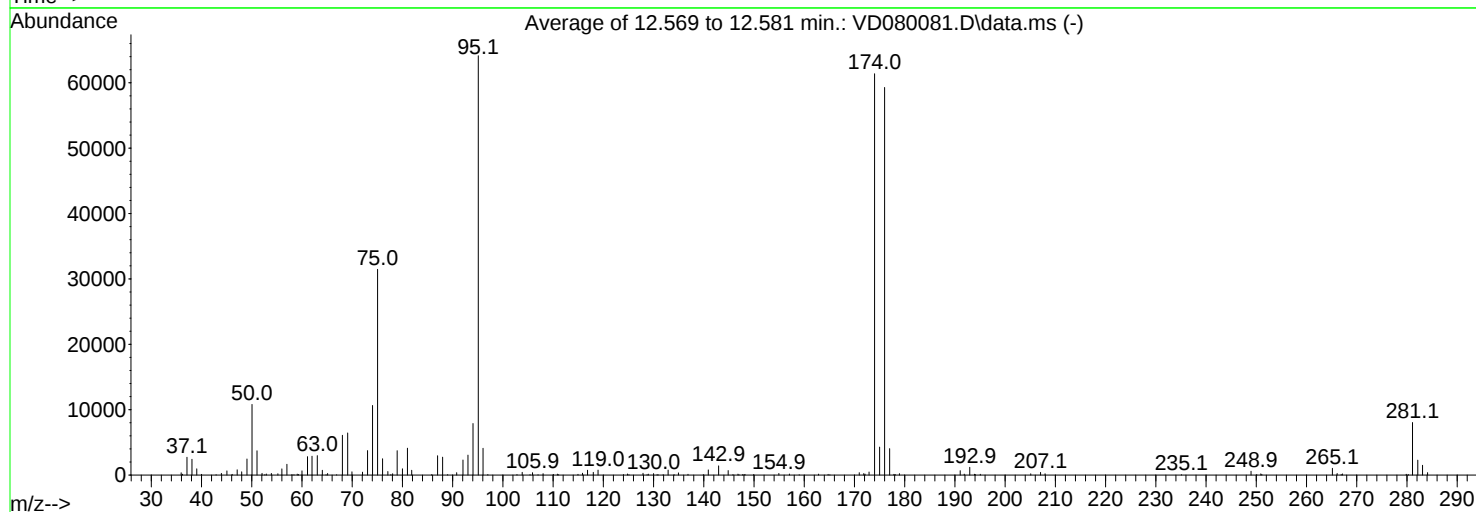


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111924\
Data File : VD080081.D
Acq On : 19 Nov 2024 12:34
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111524S.M
Title : SW846 8260
Last Update : Fri Nov 15 16:25:47 2024

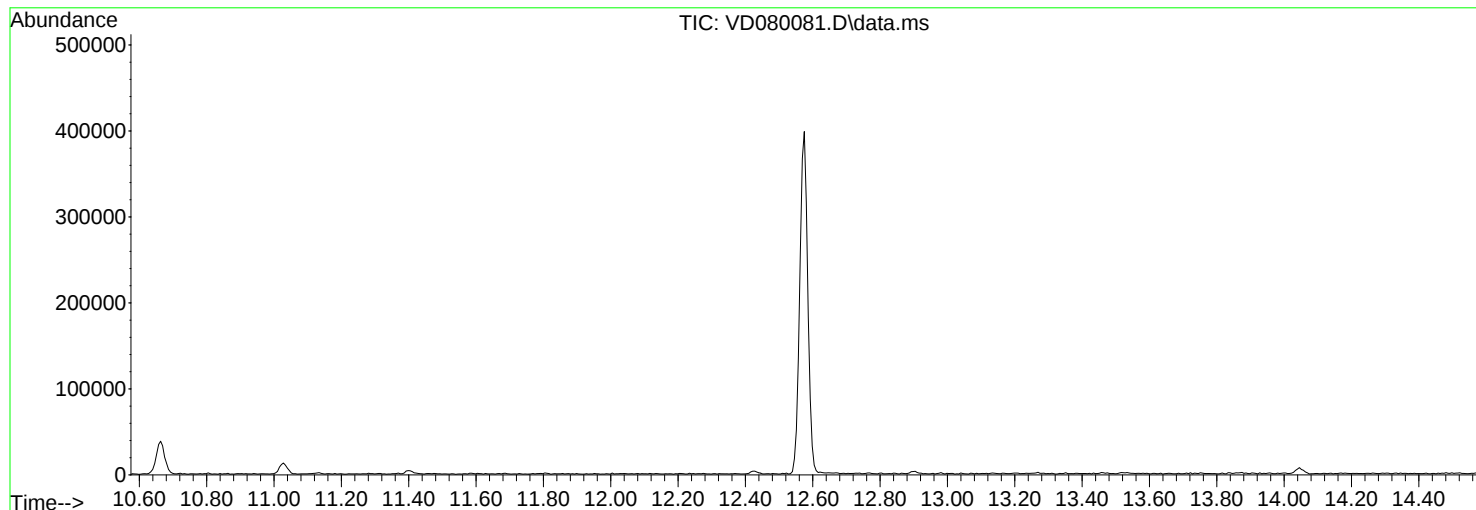

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	10808	PASS
75	95	30	60	49.1	31467	PASS
95	95	100	100	100.0	64139	PASS
96	95	5	9	6.4	4100	PASS
173	174	0.00	2	0.8	469	PASS
174	95	50	100	95.7	61384	PASS
175	174	5	9	7.0	4282	PASS
176	174	95	101	96.6	59280	PASS
177	176	5	9	6.8	4047	PASS