

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120421\
 Data File : VD071145.D
 Acq On : 04 Dec 2021 15:56
 Operator : VA/SY
 Sample : M4927-01
 Misc : 5.09G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 PH1-BOT-3

Quant Time: Dec 06 03:43:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 29 17:54:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	319894	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	562293	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.637	117	580568	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	275880	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	166931	44.472	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	88.940%
35) Dibromofluoromethane	7.914	113	173484	48.451	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.900%
50) Toluene-d8	10.337	98	714281	52.420	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.840%
62) 4-Bromofluorobenzene	12.626	95	273956	58.001	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	116.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120421\
Data File : VD071145.D
Acq On : 04 Dec 2021 15:56
Operator : VA/SY
Sample : M4927-01
Misc : 5.09G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PH1-BOT-3

Quant Time: Dec 06 03:43:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 29 17:54:09 2021
Response via : Initial Calibration




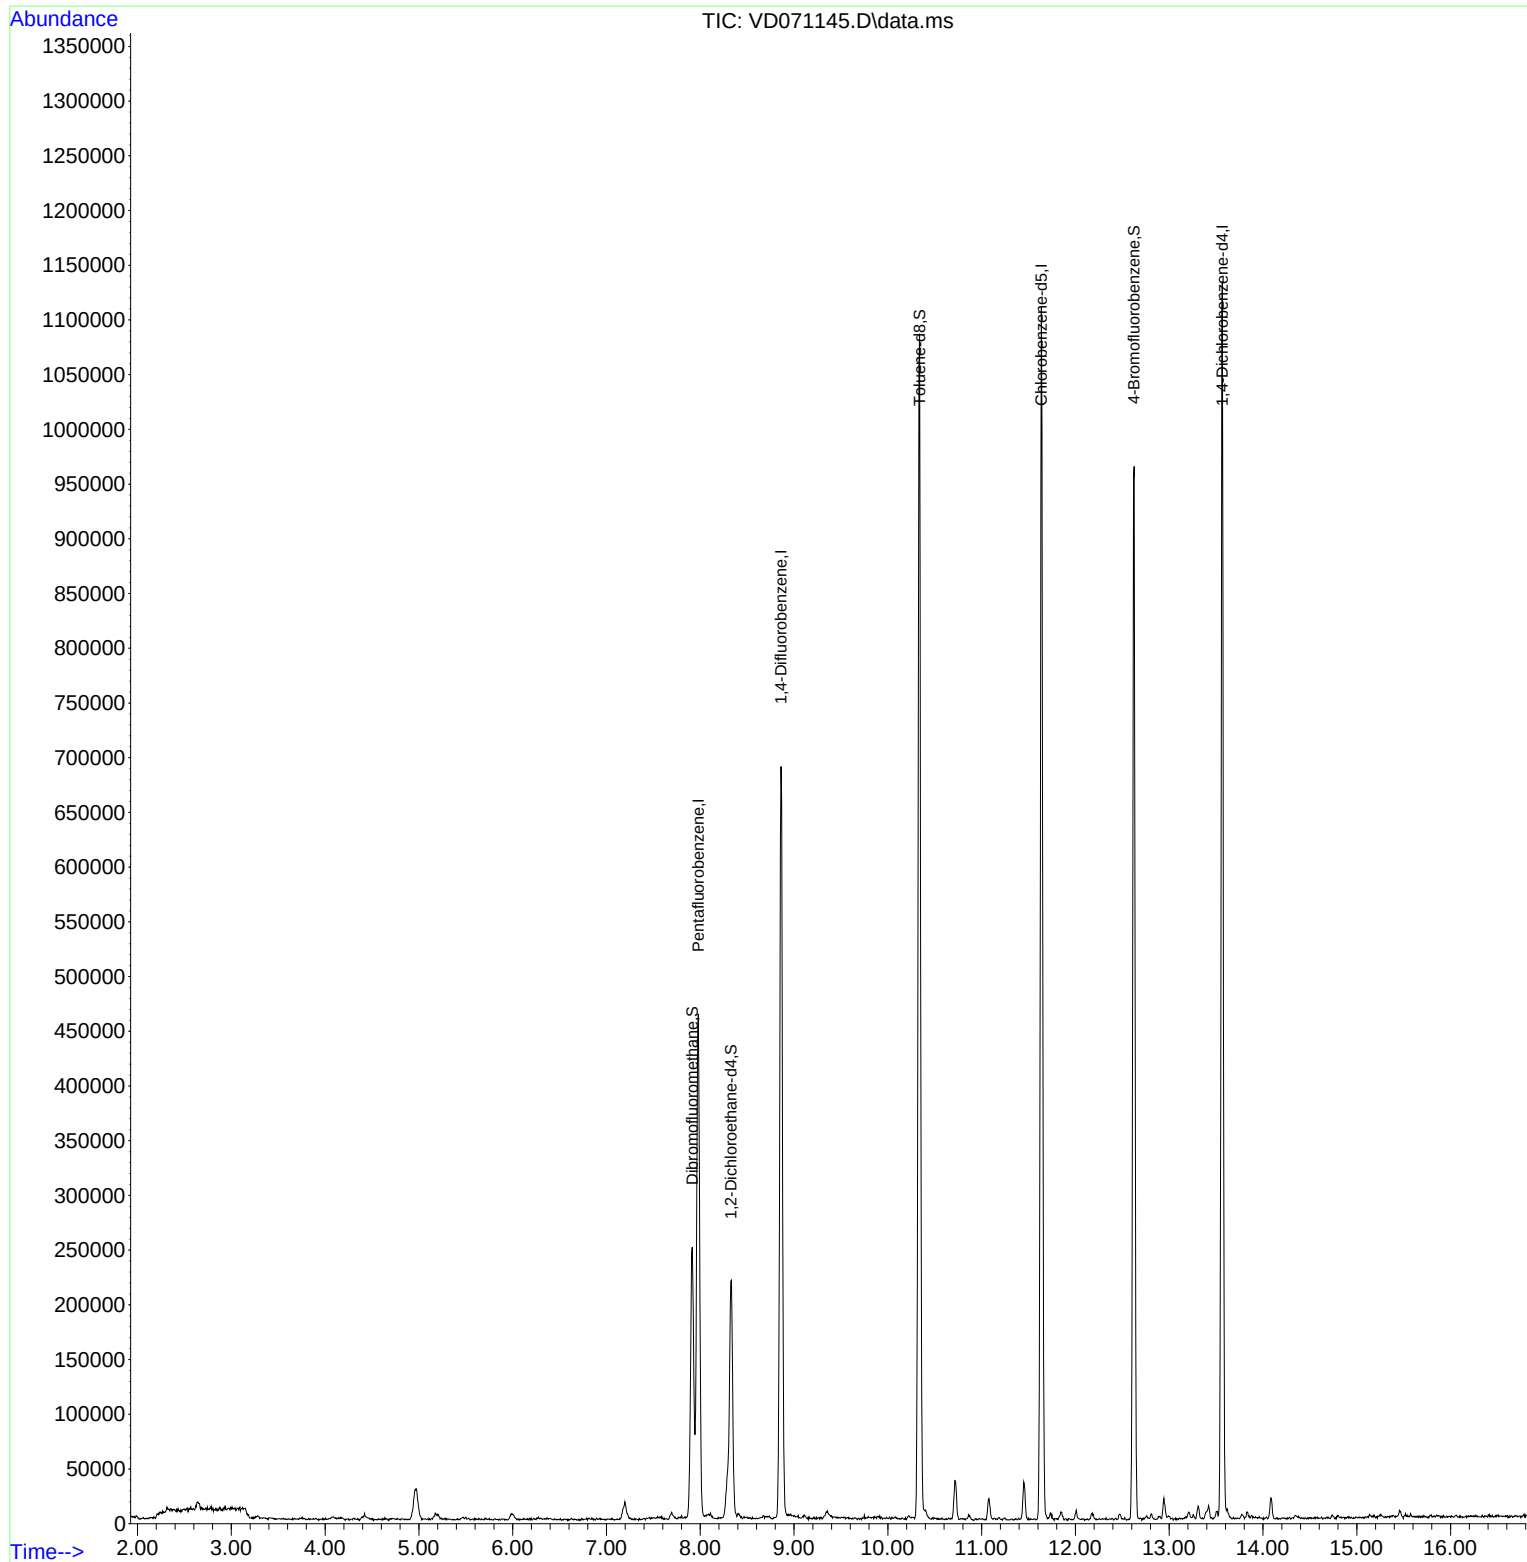


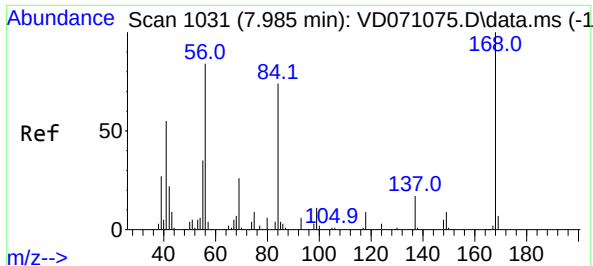

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD071145.D
Acq: 04 Dec 2021 15:56




Instrument :
MSVOA_D
ClientSampleId :
PH1-BOT-3


Tgt Ion:168 Resp: 319894
Ion Ratio Lower Upper
168 100
99 66.2 46.6 69.8

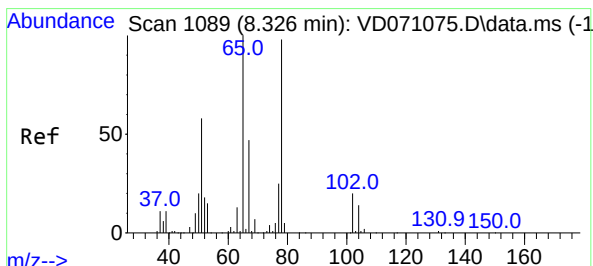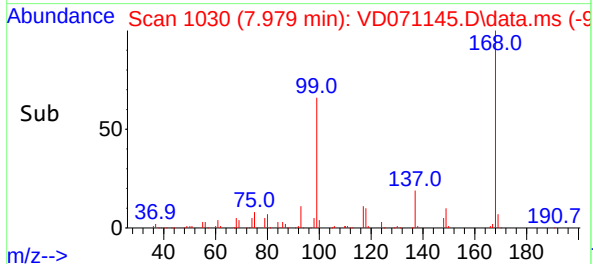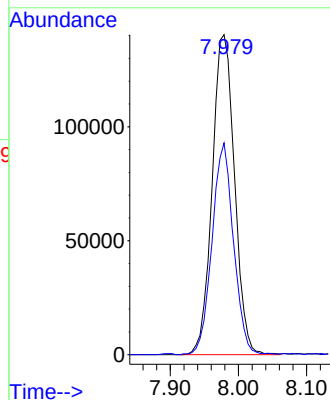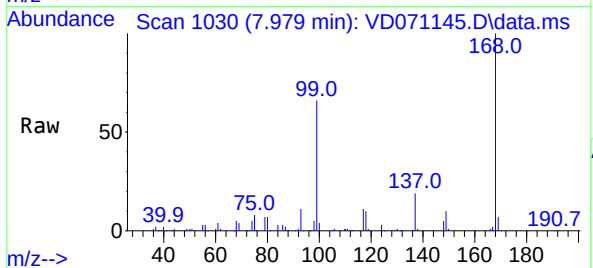

#33
1,2-Dichloroethane-d4
Concen: 44.472 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD071145.D
Acq: 04 Dec 2021 15:56

Tgt Ion: 65 Resp: 166931
Ion Ratio Lower Upper
65 100
67 51.8 0.0 112.2

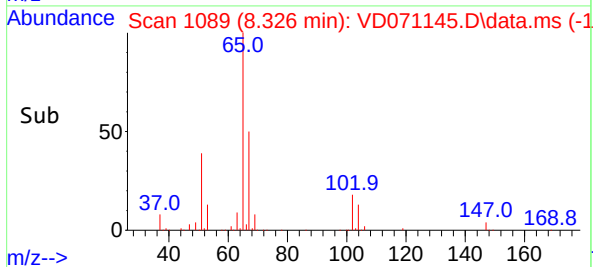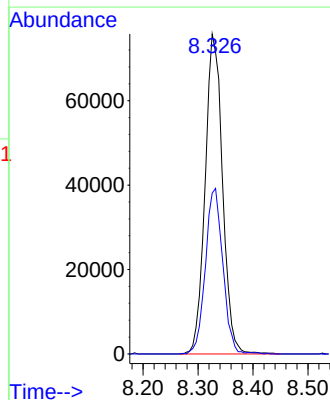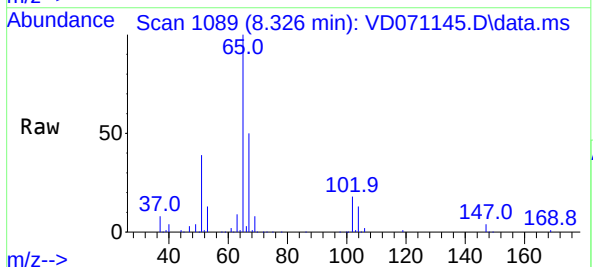

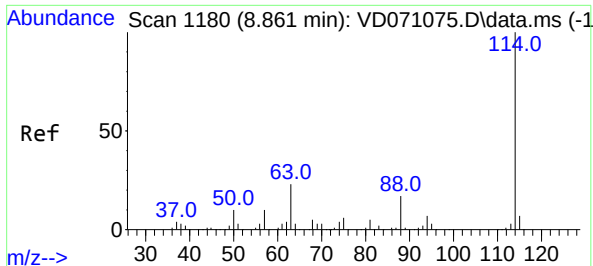

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD071145.D

Acq: 04 Dec 2021 15:56

Instrument :

MSVOA_D

ClientSampleId :

PH1-BOT-3





Tgt Ion:114 Resp: 562293

Ion Ratio Lower Upper

114 100

63 22.3 0.0 41.8

88 15.2 0.0 32.8

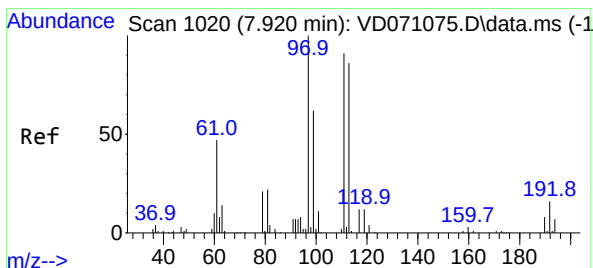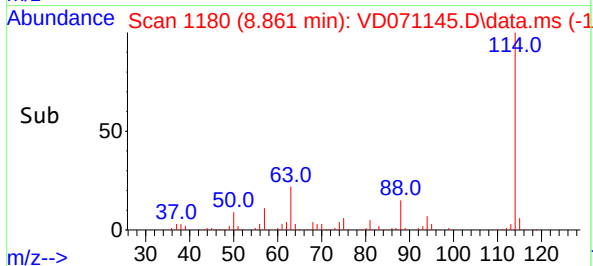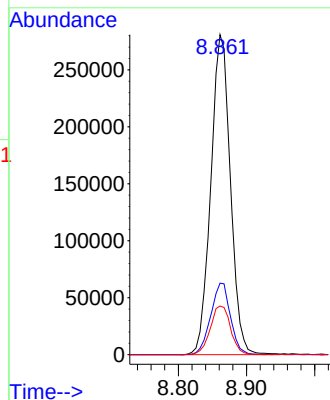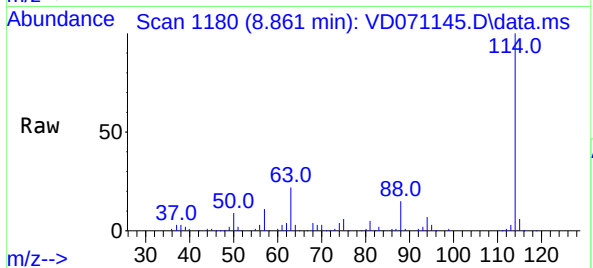

#35

Dibromofluoromethane

Concen: 48.451 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. -0.006 min

Lab File: VD071145.D

Acq: 04 Dec 2021 15:56




Tgt Ion:113 Resp: 173484


Ion Ratio Lower Upper

113 100

111 102.6 82.0 123.0

192 17.7 15.2 22.8


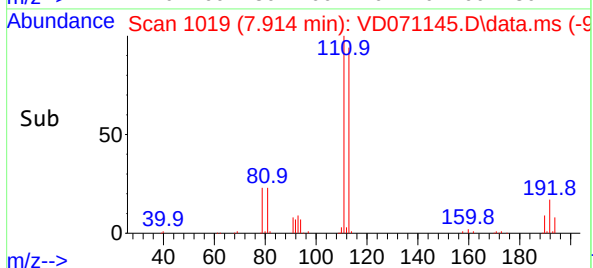
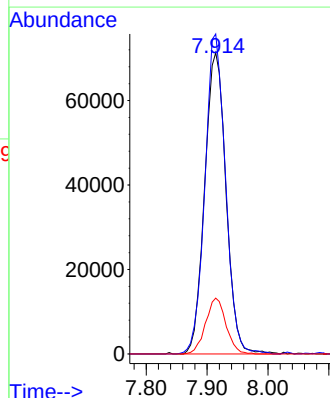
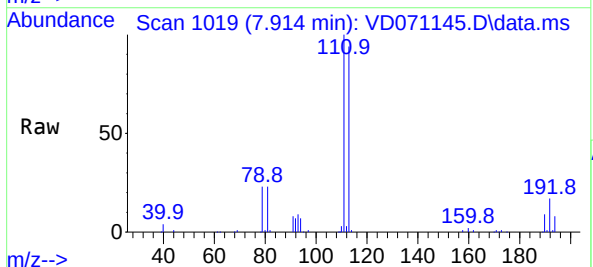


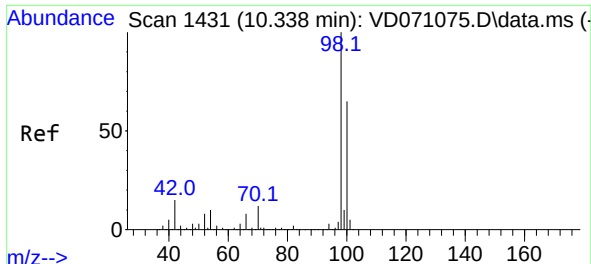

#50
Toluene-d8
Concen: 52.420 ug/l
RT: 10.337 min Scan# 1431
Delta R.T. -0.001 min
Lab File: VD071145.D
Acq: 04 Dec 2021 15:56




Instrument :
MSVOA_D
ClientSampleId :
PH1-BOT-3


Tgt Ion: 98 Resp: 714281
Ion Ratio Lower Upper
98 100
100 65.6 51.8 77.6

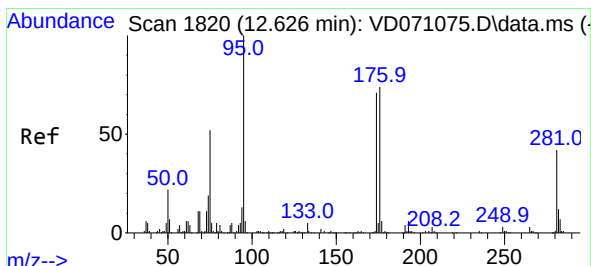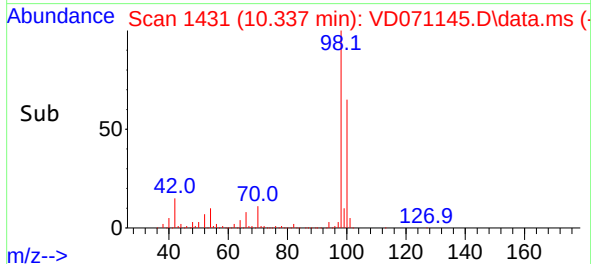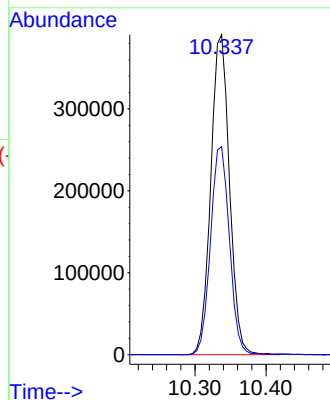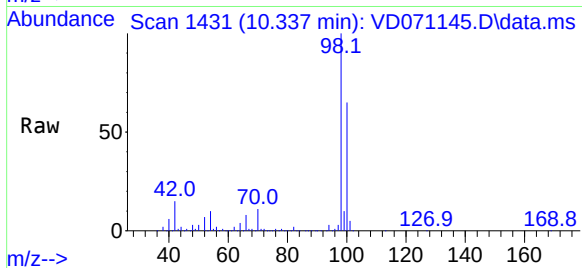

#62
4-Bromofluorobenzene
Concen: 58.001 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD071145.D
Acq: 04 Dec 2021 15:56

Tgt Ion: 95 Resp: 273956
Ion Ratio Lower Upper
95 100
174 78.9 0.0 159.4
176 74.7 0.0 154.0


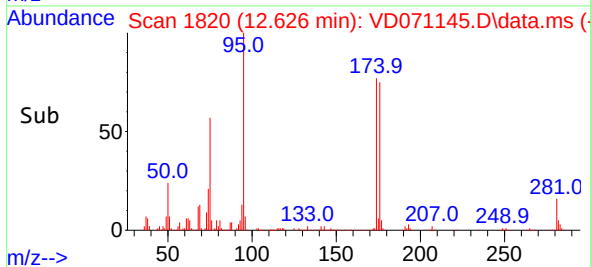
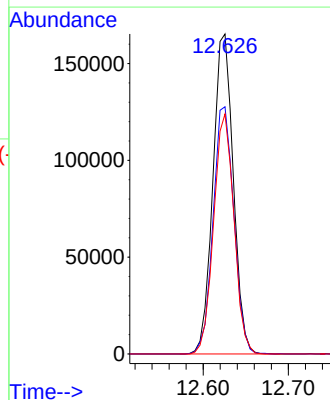
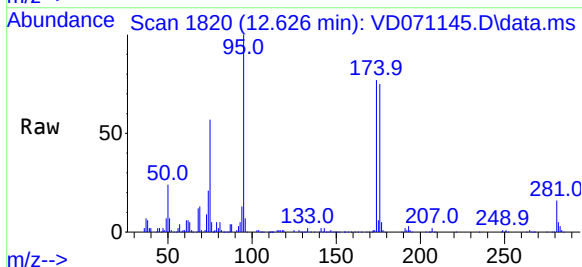


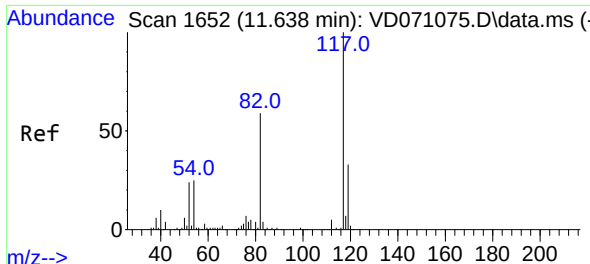

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.637 min Scan# 1170
Delta R.T. -0.001 min
Lab File: VD071145.D
Acq: 04 Dec 2021 15:56

Instrument :
MSVOA_D
ClientSampleId :
PH1-BOT-3

Tgt Ion:117 Resp: 580568
Ion Ratio Lower Upper
117 100
82 56.9 44.7 67.1
119 30.6 26.2 39.4

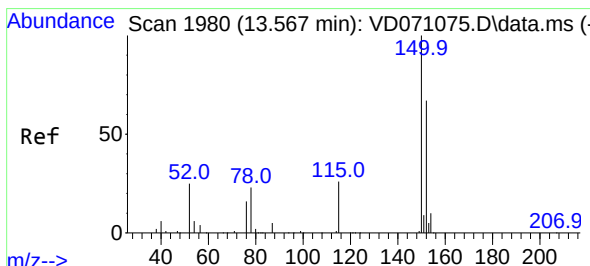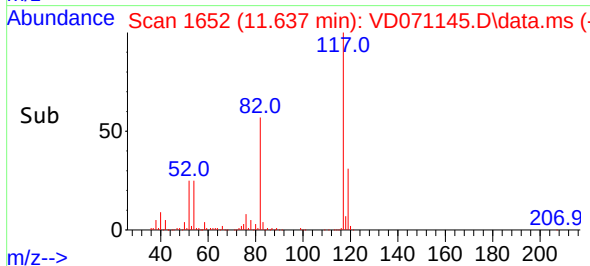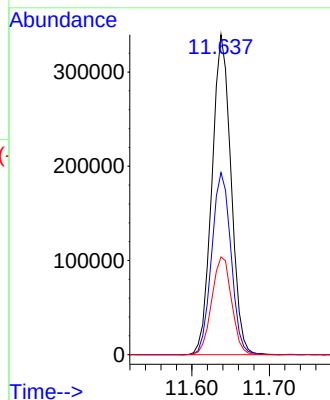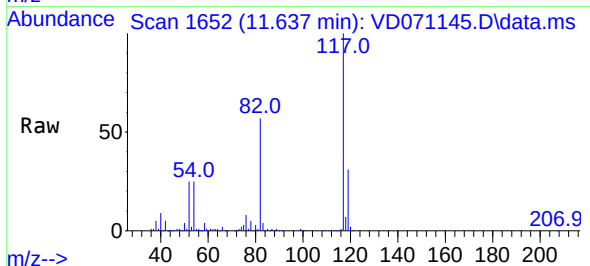

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD071145.D
Acq: 04 Dec 2021 15:56

Tgt Ion:152 Resp: 275880
Ion Ratio Lower Upper
152 100
115 60.2 29.8 89.3
150 154.9 0.0 349.2

