


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120524\
Data File : VD080099.D
Acq On : 05 Dec 2024 09:35
Operator : RP/MD
Sample : BFB839
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB839

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM120524SMA.M
Title : SFAM01.0
Last Update : Fri Dec 06 01:10:30 2024

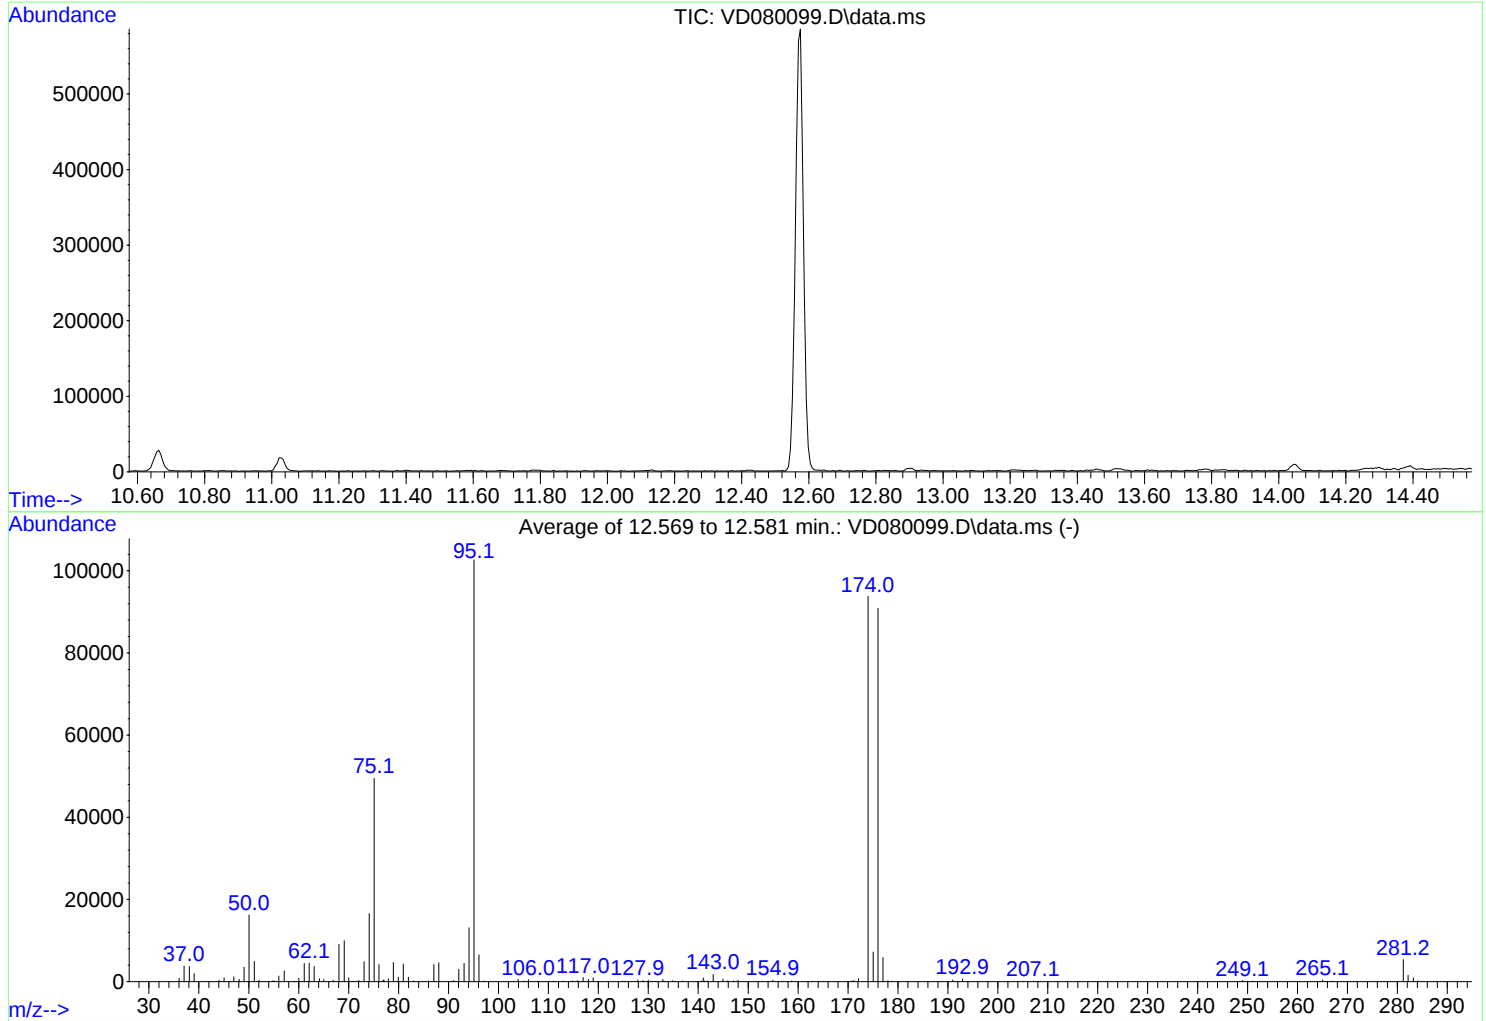

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	16219	PASS
75	95	30	80	48.2	49464	PASS
95	95	100	100	100.0	102669	PASS
96	95	5	9	6.3	6498	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.3	93765	PASS
175	174	5	9	7.7	7216	PASS
176	174	95	105	96.9	90864	PASS
177	176	5	10	6.4	5849	PASS

m/z	Abundance
40.00	999.0
44.10	433.0
50.70	164.0
60.20	161.0
207.20	176.0

Instrument :
MSVOA_D
ClientSampleId :
BFB839

m/z	Abundance
36.10	904.0
37.00	3980.0
38.10	4460.0
39.00	2296.0
40.00	974.0
44.00	740.0
45.10	1133.0
47.00	1103.0
48.10	675.0
49.00	3753.0
50.10	18960.0
51.10	5821.0
52.10	347.0
54.00	252.0
55.00	340.0
56.00	1481.0
57.10	3079.0
59.00	202.0
60.00	1047.0
61.10	4809.0
62.10	5292.0
63.10	3730.0
64.20	932.0
65.00	447.0
67.00	519.0
68.10	10431.0
69.10	11602.0
70.00	1329.0
73.10	4893.0
74.10	18024.0
75.10	53976.0
76.10	4503.0
76.90	625.0
77.90	935.0
78.90	5046.0
80.00	1052.0
80.90	4904.0
81.90	939.0
83.00	271.0
85.90	226.0
87.10	5139.0
88.00	4872.0
91.10	494.0
92.00	3337.0
93.10	4830.0
94.10	14173.0
95.10	111136.0
96.10	7147.0
97.10	189.0
103.00	229.0
104.00	584.0
105.00	185.0
106.10	471.0
112.90	176.0
114.80	165.0
115.90	406.0
117.00	1177.0
118.00	470.0
119.00	914.0
127.90	488.0
128.90	395.0
130.00	420.0
130.90	188.0
132.90	641.0
134.90	278.0
141.00	1448.0
142.00	300.0
143.00	1926.0
144.10	173.0
145.00	681.0
146.00	196.0
147.00	152.0
147.90	662.0
152.80	209.0
155.00	306.0
157.00	218.0
158.80	167.0
171.20	534.0
172.20	1059.0
174.00	98112.0
175.10	8545.0
176.00	94704.0
177.00	6184.0
178.00	235.0
190.90	304.0
191.20	337.0
192.90	430.0
207.10	249.0
249.10	356.0
250.80	157.0
265.00	281.0
266.90	164.0

Instrument :
MSVOA_D
ClientSampleId :
BFB839

281.20	4764.0
282.10	1285.0
283.20	985.0
284.20	327.0

Instrument :
MSVOA_D
ClientSampleId :
BFB839

m/z	Abundance
36.00	844.0
37.10	4890.0
38.10	3995.0
39.10	1699.0
40.10	941.0
40.80	200.0
44.00	724.0
45.00	1060.0
46.10	232.0
47.00	1599.0
48.00	656.0
49.10	4182.0
50.00	17528.0
51.10	5676.0
51.90	307.0
53.10	170.0
55.10	254.0
56.00	1566.0
57.10	2553.0
58.00	226.0
59.20	178.0
59.90	1075.0
61.10	5140.0
62.10	4724.0
63.10	4619.0
64.20	616.0
65.00	573.0
66.90	301.0
68.00	9328.0
69.10	10056.0
70.00	777.0
71.90	693.0
73.10	5777.0
74.10	18528.0
75.10	55344.0
76.00	4882.0
76.90	570.0
77.10	560.0
78.00	484.0
79.00	5498.0
79.90	1112.0
81.00	4868.0
82.00	1445.0
83.10	197.0
87.10	3965.0
88.00	4792.0
90.90	293.0
92.00	2965.0
93.10	4703.0
94.10	15263.0
95.10	116080.0
96.10	6971.0
97.10	265.0
103.90	539.0
106.00	661.0
110.90	229.0
112.00	213.0
112.90	225.0
114.90	183.0
116.10	324.0
116.90	1086.0
118.00	705.0
118.90	1080.0
124.90	260.0
125.30	207.0
127.80	305.0
129.00	316.0
130.00	312.0
130.80	189.0
132.90	309.0
133.30	298.0
134.90	370.0
136.80	250.0
141.00	1255.0
143.00	2038.0
144.80	711.0
145.90	295.0
147.10	156.0
148.00	249.0
154.90	365.0
158.60	153.0
162.90	221.0
165.10	166.0
170.70	278.0
171.00	288.0
172.10	714.0
174.00	103592.0
175.00	7783.0
176.00	99200.0
177.00	6236.0
178.10	204.0
178.80	253.0

Instrument :
MSVOA_D
ClientSampleId :
BFB839

191.00	454.0
193.00	999.0
193.90	156.0
205.10	251.0
207.00	363.0
249.10	259.0
251.20	233.0
265.10	403.0
267.00	172.0
281.20	5433.0
282.10	1745.0
283.20	1169.0
284.00	241.0

Instrument :
MSVOA_D
ClientSampleId :
BFB839

m/z	Abundance
36.00	589.0
37.10	2619.0
38.00	2566.0
39.10	1818.0
40.00	783.0
44.10	735.0
45.10	667.0
47.10	800.0
48.10	436.0
49.00	2532.0
50.00	12169.0
51.10	3285.0
52.10	299.0
54.80	442.0
56.00	1059.0
57.10	2247.0
60.10	792.0
61.10	3207.0
62.10	3467.0
63.10	2810.0
64.10	552.0
65.00	396.0
66.80	248.0
68.10	7507.0
69.10	8210.0
70.00	731.0
72.10	583.0
73.10	3853.0
74.10	13172.0
75.10	39072.0
76.10	3089.0
77.00	491.0
78.00	522.0
79.00	3429.0
80.00	1083.0
81.00	3089.0
82.00	821.0
86.00	414.0
87.00	3421.0
88.10	4122.0
90.70	398.0
92.10	2756.0
93.10	3810.0
94.10	9896.0
95.10	80792.0
96.10	5376.0
104.00	544.0
104.90	198.0
105.90	240.0
107.80	234.0
111.10	228.0
114.90	177.0
115.80	350.0
116.90	695.0
118.00	488.0
119.00	850.0
124.90	156.0
128.00	337.0
130.00	283.0
133.00	567.0
135.10	206.0
136.80	201.0
140.70	487.0
141.20	755.0
141.90	231.0
143.00	1358.0
145.00	486.0
146.00	167.0
147.00	232.0
147.90	190.0
155.00	372.0
156.70	166.0
158.70	174.0
170.90	354.0
172.00	437.0
174.00	79592.0
175.10	5320.0
176.00	78688.0
177.00	5128.0
177.90	273.0
191.00	463.0
193.00	485.0
207.10	299.0
249.00	301.0
265.10	463.0
265.90	186.0
281.20	5887.0
282.20	1621.0
283.10	660.0
284.00	189.0
284.90	160.0

Instrument :
MSVOA_D
ClientSampleId :
BFB839