
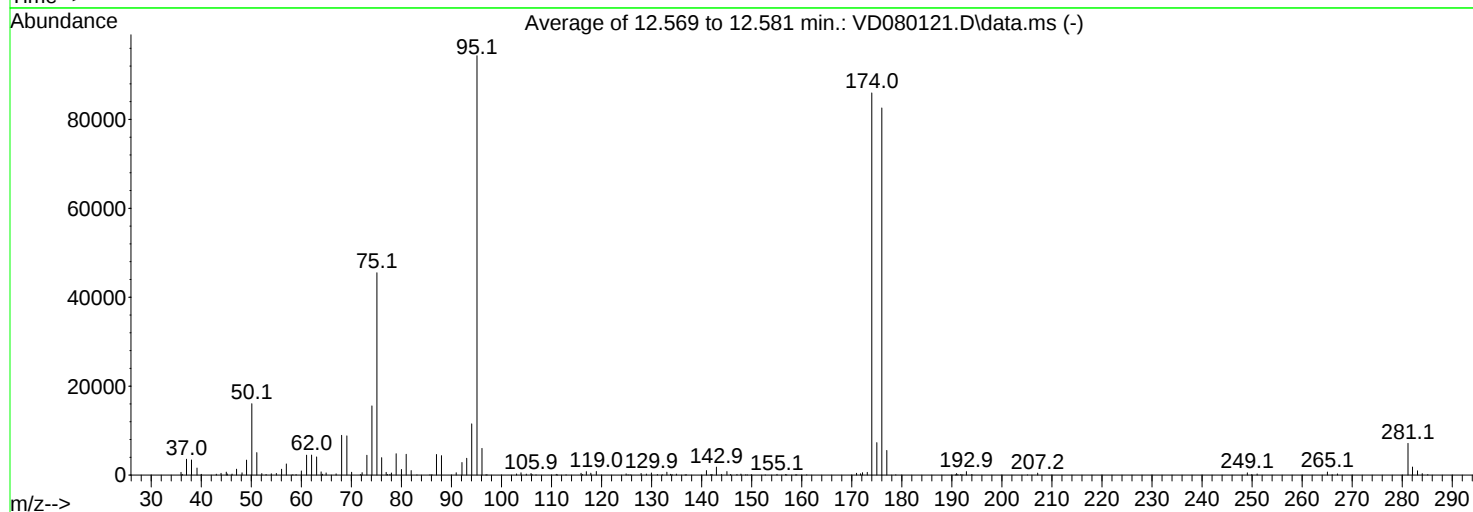


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121124\
Data File : VD080121.D
Acq On : 11 Dec 2024 08:53
Operator : RP/MD
Sample : BFB841
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB841

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM121124SMA.M
Title : SFAM01.0
Last Update : Fri Dec 13 02:01:12 2024

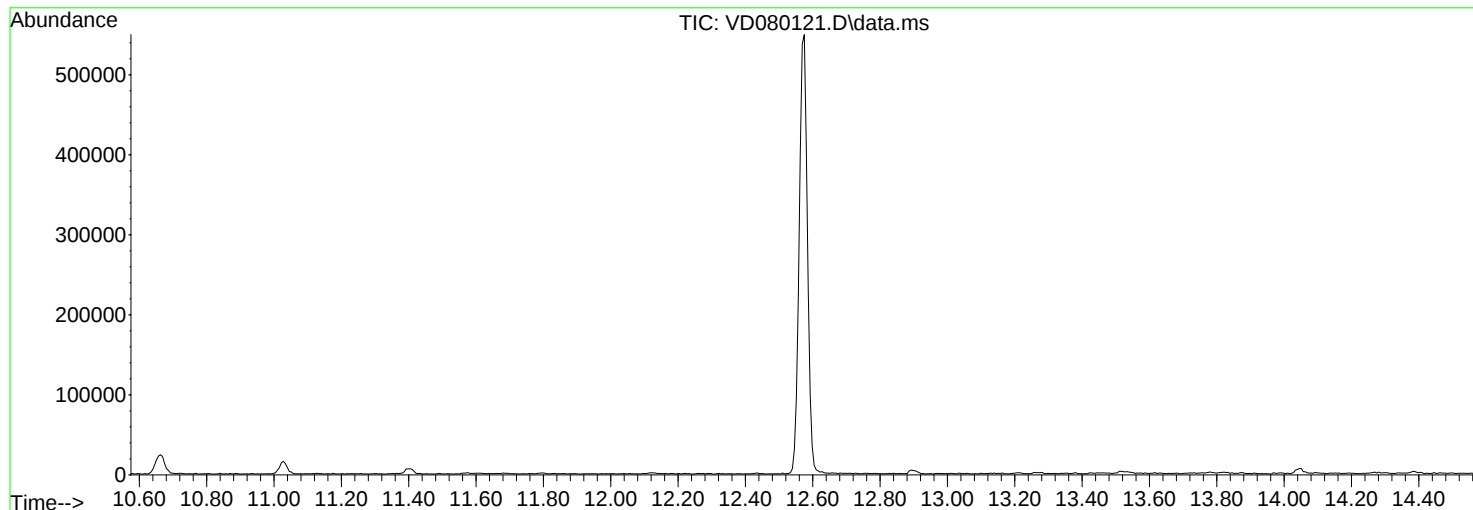

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	16056	PASS
75	95	30	80	48.2	45509	PASS
95	95	100	100	100.0	94325	PASS
96	95	5	9	6.4	6004	PASS
173	174	0.00	2	0.7	620	PASS
174	95	50	120	91.1	85957	PASS
175	174	5	9	8.5	7304	PASS
176	174	95	105	96.1	82581	PASS
177	176	5	10	6.7	5546	PASS

Scan 1858 (12.516 min): VD080121.D\data.ms
BFB841

m/z	Abundance
40.00	868.0
41.20	171.0
43.90	323.0

Instrument :
MSVOA_D
ClientSampleId :
BFB841

m/z	Abundance
36.00	933.0
37.10	4587.0
38.10	3856.0
39.10	1492.0
40.00	1120.0
43.00	268.0
44.10	757.0
45.00	961.0
46.10	260.0
47.00	1696.0
48.20	332.0
49.00	4127.0
50.10	17384.0
51.10	5927.0
52.20	347.0
52.90	216.0
54.10	307.0
54.90	450.0
56.00	1275.0
57.00	2711.0
59.00	191.0
60.00	1028.0
61.00	5113.0
62.00	5080.0
63.10	4091.0
64.10	840.0
65.00	353.0
67.00	250.0
68.10	10891.0
69.10	9460.0
70.10	771.0
72.20	968.0
73.10	4897.0
74.10	16712.0
75.10	49760.0
76.10	4517.0
77.00	569.0
78.00	425.0
79.00	5043.0
80.00	1225.0
81.00	5233.0
82.00	1177.0
85.70	240.0
87.00	5557.0
88.00	4215.0
91.00	645.0
92.10	2702.0
93.00	3969.0
94.10	13088.0
95.10	102008.0
96.10	6764.0
96.90	231.0
103.00	204.0
103.90	605.0
104.90	277.0
105.90	627.0
111.00	296.0
115.90	626.0
117.00	1049.0
117.80	317.0
119.00	1094.0
124.90	264.0
127.90	573.0
128.90	222.0
130.00	507.0
133.10	775.0
134.90	309.0
136.70	159.0
136.90	160.0
141.00	918.0
141.80	199.0
142.90	1959.0
144.00	189.0
145.00	829.0
147.10	215.0
147.90	369.0
155.10	365.0
156.80	285.0
158.80	211.0
171.00	551.0
171.80	459.0
172.20	348.0
174.00	92784.0
175.00	8172.0
176.00	87184.0
177.00	6064.0
190.70	238.0
191.20	381.0
192.20	177.0
192.90	853.0
194.00	205.0
207.20	433.0

Instrument :
MSVOA_D
ClientSampleId :
BFB841

249.10	614.0
251.00	348.0
265.10	694.0
267.00	244.0
281.10	5690.0
282.00	1454.0
283.00	814.0
284.00	240.0
285.20	153.0

Instrument :
MSVOA_D
ClientSampleId :
BFB841

m/z	Abundance
35.90	524.0
36.20	499.0
37.00	3399.0
38.00	3742.0
39.10	2036.0
40.10	1001.0
43.10	163.0
43.90	702.0
45.00	1054.0
46.20	435.0
47.10	1063.0
48.10	736.0
49.10	3145.0
50.10	17656.0
51.10	5026.0
52.00	441.0
53.00	212.0
53.90	281.0
55.00	322.0
56.10	1646.0
57.00	2797.0
58.90	176.0
60.00	1204.0
61.10	4558.0
62.10	5090.0
63.00	4982.0
63.90	770.0
65.00	632.0
66.90	420.0
68.10	9161.0
69.10	9625.0
70.10	677.0
72.10	686.0
73.10	4858.0
74.10	17000.0
75.10	50616.0
76.10	4243.0
76.90	782.0
77.70	475.0
78.10	762.0
79.00	5260.0
80.00	1537.0
81.00	5167.0
82.00	1136.0
86.10	219.0
87.00	4889.0
88.00	4856.0
90.90	558.0
92.10	3030.0
93.00	4175.0
94.00	12322.0
95.10	105360.0
96.10	6569.0
97.10	266.0
102.90	206.0
103.80	521.0
105.00	227.0
105.90	457.0
106.90	161.0
110.90	220.0
112.90	236.0
115.90	603.0
117.00	685.0
117.90	538.0
118.90	561.0
124.80	276.0
125.30	244.0
127.90	249.0
129.00	236.0
129.80	458.0
131.10	234.0
133.00	425.0
133.90	296.0
134.90	168.0
136.90	179.0
141.00	1083.0
142.10	281.0
143.00	2117.0
143.90	176.0
145.10	900.0
145.80	163.0
147.00	263.0
147.80	303.0
149.10	236.0
149.90	167.0
152.70	152.0
156.80	193.0
161.00	219.0
170.90	429.0
172.10	766.0
173.10	1859.0
174.00	94856.0

Instrument :
MSVOA_D
ClientSampleId :
BFB841

175.00	7910.0
176.00	90400.0
177.00	5942.0
190.90	494.0
191.80	243.0
193.00	706.0
194.00	182.0
207.10	417.0
249.10	447.0
249.90	181.0
251.00	263.0
265.00	557.0
266.00	170.0
267.10	297.0
281.10	8199.0
282.10	2219.0
283.10	776.0
284.00	406.0
285.00	220.0

Instrument :
MSVOA_D
ClientSampleId :
BFB841

m/z	Abundance
36.00	381.0
37.10	2739.0
38.00	2611.0
39.20	1236.0
40.00	996.0
41.30	182.0
42.90	199.0
44.00	713.0
45.20	768.0
47.10	1232.0
48.20	474.0
49.00	2843.0
50.10	13128.0
51.10	4211.0
52.20	215.0
54.00	303.0
55.10	323.0
56.10	1038.0
57.00	1995.0
58.30	266.0
60.10	560.0
61.00	3786.0
62.10	3353.0
63.00	3175.0
63.90	563.0
64.20	580.0
64.90	486.0
66.90	163.0
68.00	6786.0
69.10	7378.0
69.90	453.0
71.80	357.0
73.10	3635.0
74.10	12983.0
75.10	36152.0
76.00	2999.0
76.90	509.0
77.20	426.0
77.90	256.0
78.90	4099.0
80.00	1052.0
80.90	3622.0
81.80	744.0
83.10	154.0
87.00	3450.0
88.00	4034.0
90.90	383.0
92.10	2756.0
93.10	3190.0
94.00	9139.0
95.10	75608.0
96.10	4678.0
103.10	379.0
104.00	434.0
105.00	187.0
106.10	337.0
111.20	159.0
116.20	370.0
116.90	613.0
117.80	441.0
119.00	769.0
125.00	315.0
125.70	194.0
127.90	266.0
129.00	257.0
130.00	450.0
131.20	204.0
132.20	161.0
133.00	780.0
133.70	251.0
134.10	248.0
135.00	207.0
140.90	1051.0
142.00	169.0
143.00	1312.0
145.00	691.0
145.70	237.0
148.80	184.0
154.90	171.0
157.00	219.0
159.00	219.0
170.90	257.0
171.70	457.0
172.20	504.0
174.00	70232.0
175.00	5830.0
176.00	70160.0
177.00	4632.0
178.80	226.0
191.00	552.0
191.80	222.0
192.80	809.0

Instrument :
MSVOA_D
ClientSampleId :
BFB841

205.10	170.0
207.10	476.0
248.90	481.0
250.90	164.0
265.00	823.0
267.10	270.0
281.20	7526.0
282.10	1772.0
283.10	1305.0
284.00	342.0

Instrument :
MSVOA_D
ClientSampleId :
BFB841