
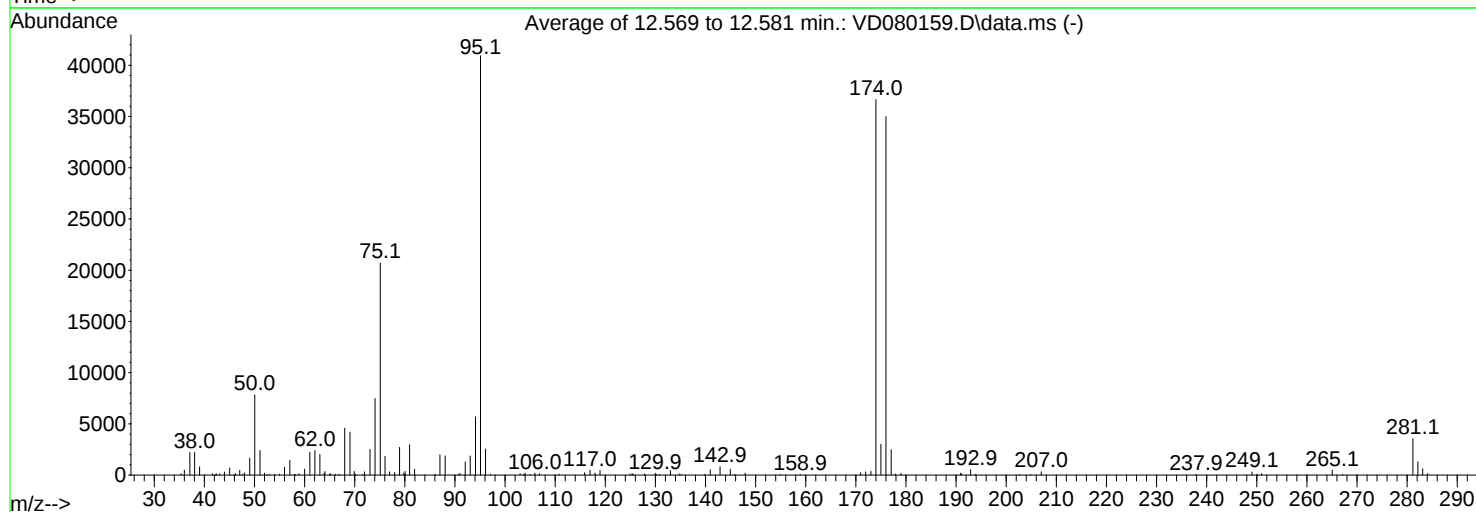


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121324\
Data File : VD080159.D
Acq On : 13 Dec 2024 08:20
Operator : RP/MD
Sample : BFB843
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB843

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM121324SMA.M
Title : SFAM01.0
Last Update : Fri Dec 13 23:13:13 2024

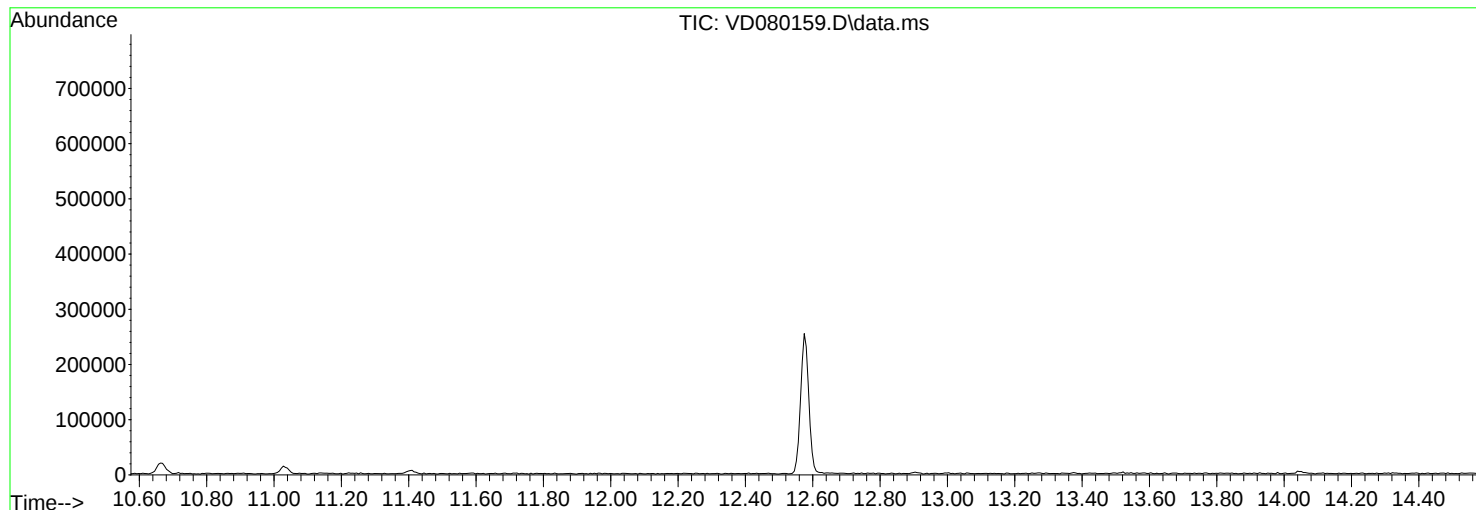

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	7841	PASS
75	95	30	80	50.6	20707	PASS
95	95	100	100	100.0	40933	PASS
96	95	5	9	6.2	2541	PASS
173	174	0.00	2	1.0	373	PASS
174	95	50	120	89.5	36653	PASS
175	174	5	9	8.2	3018	PASS
176	174	95	105	95.5	34992	PASS
177	176	5	10	7.1	2481	PASS

Scan 1860 (12.528 min): VD080159.D\data.ms
BFB843

m/z	Abundance
39.10	165.0
40.00	1083.0
40.70	203.0
44.00	272.0
65.60	164.0

Instrument :
MSVOA_D
ClientSampleId :
BFB843

m/z	Abundance
35.40	263.0
36.00	439.0
37.10	2343.0
38.10	1959.0
39.00	852.0
40.10	1012.0
41.70	179.0
42.20	206.0
43.10	157.0
44.00	532.0
45.00	767.0
46.20	194.0
47.00	433.0
48.10	245.0
49.10	1497.0
50.00	6720.0
51.10	2196.0
55.90	681.0
57.10	1366.0
58.00	185.0
58.80	169.0
60.00	577.0
61.00	2180.0
62.00	2067.0
63.10	1953.0
63.90	545.0
65.00	303.0
68.00	4075.0
69.00	3686.0
69.90	579.0
71.60	188.0
72.00	260.0
73.10	2115.0
74.10	6990.0
75.10	19424.0
76.00	1905.0
76.90	230.0
78.10	226.0
78.90	2324.0
80.10	474.0
81.00	2564.0
81.90	548.0
87.00	1636.0
88.00	1731.0
90.80	281.0
92.10	1178.0
93.00	1590.0
94.10	5357.0
95.10	37600.0
96.20	2718.0
97.10	210.0
103.00	197.0
104.00	293.0
106.90	177.0
116.00	210.0
117.00	475.0
119.00	405.0
124.90	259.0
125.60	207.0
127.80	158.0
129.90	303.0
133.00	158.0
134.70	166.0
140.90	394.0
142.90	704.0
144.90	584.0
147.90	181.0
170.90	199.0
171.90	342.0
174.00	31632.0
175.00	2879.0
176.00	30352.0
177.10	1798.0
190.90	215.0
193.00	268.0
193.90	231.0
207.00	479.0
249.00	182.0
265.20	183.0
267.10	167.0
281.10	2446.0
282.10	973.0
283.20	409.0
284.10	186.0

Instrument :
MSVOA_D
ClientSampleId :
BFB843

m/z	Abundance
35.90	661.0
37.10	2004.0
38.00	2818.0
39.10	1242.0
40.00	987.0
41.50	175.0
42.40	160.0
43.00	197.0
44.00	558.0
45.10	808.0
46.20	259.0
47.10	489.0
47.70	260.0
49.10	2022.0
50.10	9430.0
51.10	2678.0
52.10	311.0
53.00	158.0
55.00	275.0
56.00	796.0
57.10	1431.0
58.20	182.0
58.90	228.0
60.00	576.0
61.10	2275.0
62.10	2800.0
63.00	2093.0
64.10	542.0
65.20	168.0
66.10	229.0
68.00	5484.0
69.00	4736.0
69.90	507.0
71.90	320.0
73.10	2981.0
74.00	8004.0
75.10	23104.0
76.10	1978.0
77.00	262.0
77.90	511.0
79.00	2882.0
79.80	624.0
80.90	3174.0
82.00	531.0
87.00	1758.0
88.00	2233.0
91.00	310.0
92.00	1139.0
93.10	2111.0
94.10	5975.0
95.10	44760.0
96.00	2773.0
103.70	255.0
105.90	260.0
115.80	221.0
116.90	573.0
117.90	386.0
118.80	512.0
125.30	312.0
127.90	215.0
130.20	221.0
130.80	187.0
133.10	451.0
135.10	204.0
141.00	585.0
142.90	1092.0
144.90	456.0
145.80	188.0
147.80	163.0
158.90	213.0
171.00	266.0
171.90	290.0
173.00	1118.0
174.00	40864.0
175.00	3110.0
176.00	38664.0
177.00	3173.0
177.90	305.0
179.00	287.0
191.10	312.0
192.90	536.0
207.00	206.0
237.90	213.0
249.00	318.0
250.90	207.0
265.10	658.0
281.20	4008.0
282.20	1409.0
283.00	554.0

Instrument :
MSVOA_D
ClientSampleId :
BFB843

m/z	Abundance
35.30	178.0
36.10	331.0
37.10	2318.0
38.10	1892.0
39.00	841.0
40.00	945.0
40.80	223.0
42.50	167.0
44.00	644.0
45.10	548.0
45.90	155.0
47.10	499.0
47.90	397.0
49.00	1453.0
50.10	7372.0
51.10	2347.0
51.90	274.0
52.50	182.0
54.00	224.0
56.10	805.0
57.00	1577.0
60.00	619.0
61.00	2265.0
62.10	2353.0
63.10	2008.0
64.00	502.0
65.10	203.0
66.90	239.0
68.00	4182.0
69.10	4181.0
70.10	370.0
71.90	386.0
73.00	2428.0
74.10	7449.0
75.10	19592.0
76.10	1645.0
76.90	448.0
78.90	2913.0
80.00	610.0
80.90	3130.0
82.00	619.0
86.10	175.0
87.00	2539.0
88.10	1679.0
91.00	186.0
92.00	1541.0
93.00	1882.0
94.10	5723.0
95.10	40440.0
96.10	2133.0
103.00	216.0
104.00	316.0
105.00	210.0
106.00	328.0
106.80	216.0
110.80	225.0
115.70	234.0
117.00	389.0
118.00	231.0
119.00	406.0
125.40	164.0
130.00	265.0
133.00	741.0
134.80	196.0
139.80	162.0
140.90	571.0
142.90	678.0
145.00	698.0
148.00	253.0
154.90	188.0
171.00	241.0
172.00	293.0
174.00	37464.0
175.00	3064.0
176.00	35960.0
177.00	2472.0
179.00	218.0
190.90	334.0
192.90	813.0
202.70	161.0
204.90	172.0
207.00	278.0
249.10	400.0
250.10	215.0
251.00	207.0
265.00	605.0
281.10	4198.0
282.20	1497.0
283.10	870.0
284.10	237.0

Instrument :
MSVOA_D
ClientSampleId :
BFB843