


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD121418\
Data File : VD060566.D
Acq On : 14 Dec 2018 11:23
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Title : SW846 8260
Last Update : Thu Dec 06 01:49:20 2018

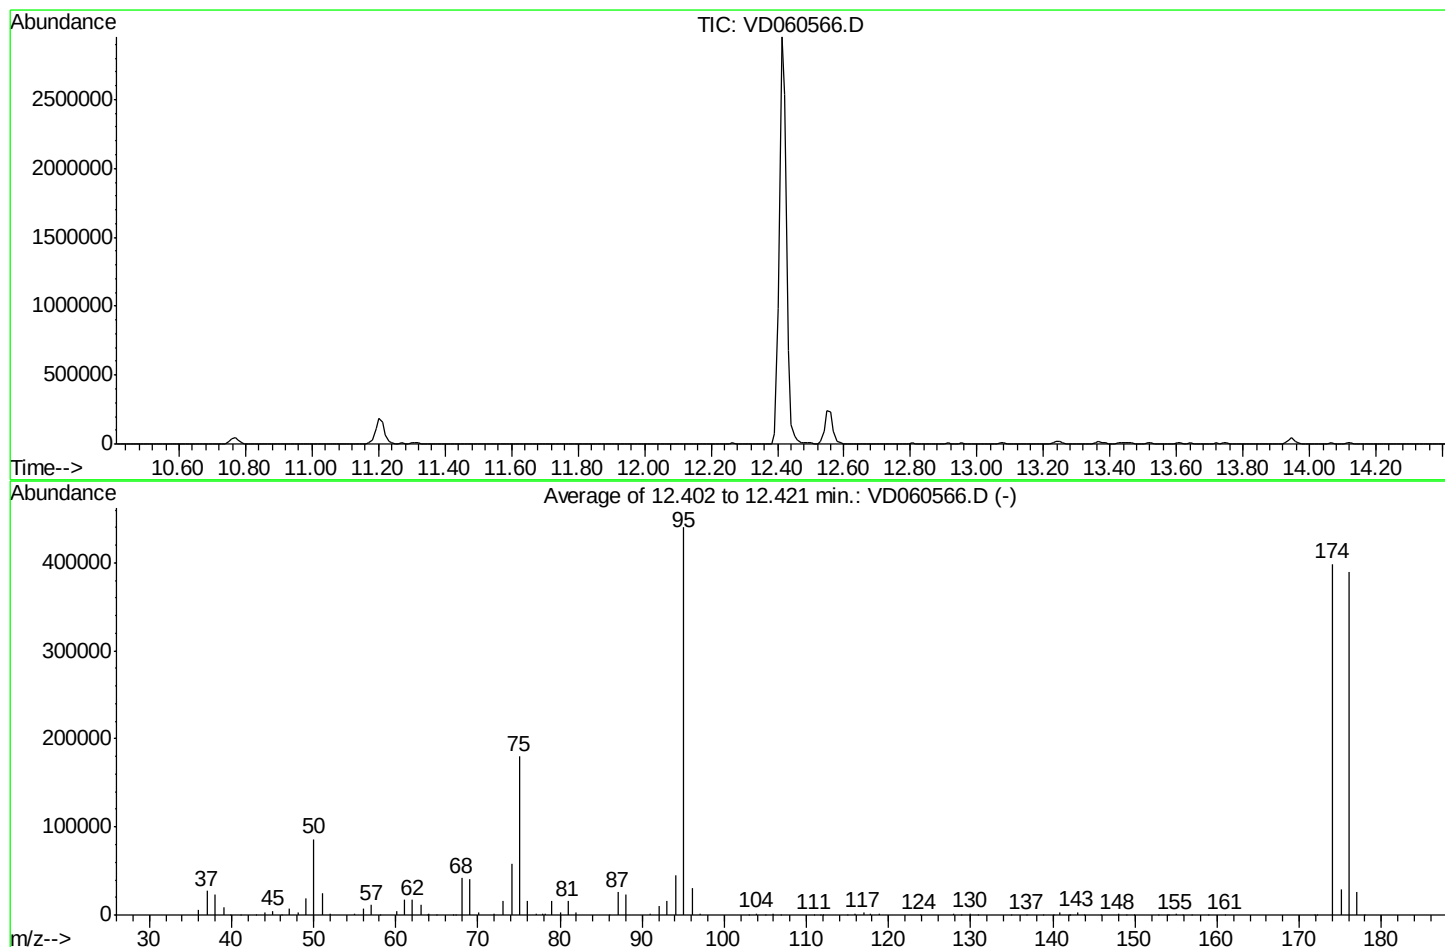

AutoFind: Scans 1105, 1106, 1107; Background Corrected with Scan 1101

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	85936	PASS
75	95	30	60	40.9	179853	PASS
95	95	100	100	100.0	440170	PASS
96	95	5	9	6.9	30252	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.6	398698	PASS
175	174	5	9	7.3	29081	PASS
176	174	95	101	97.9	390160	PASS
177	176	5	9	6.7	26329	PASS