
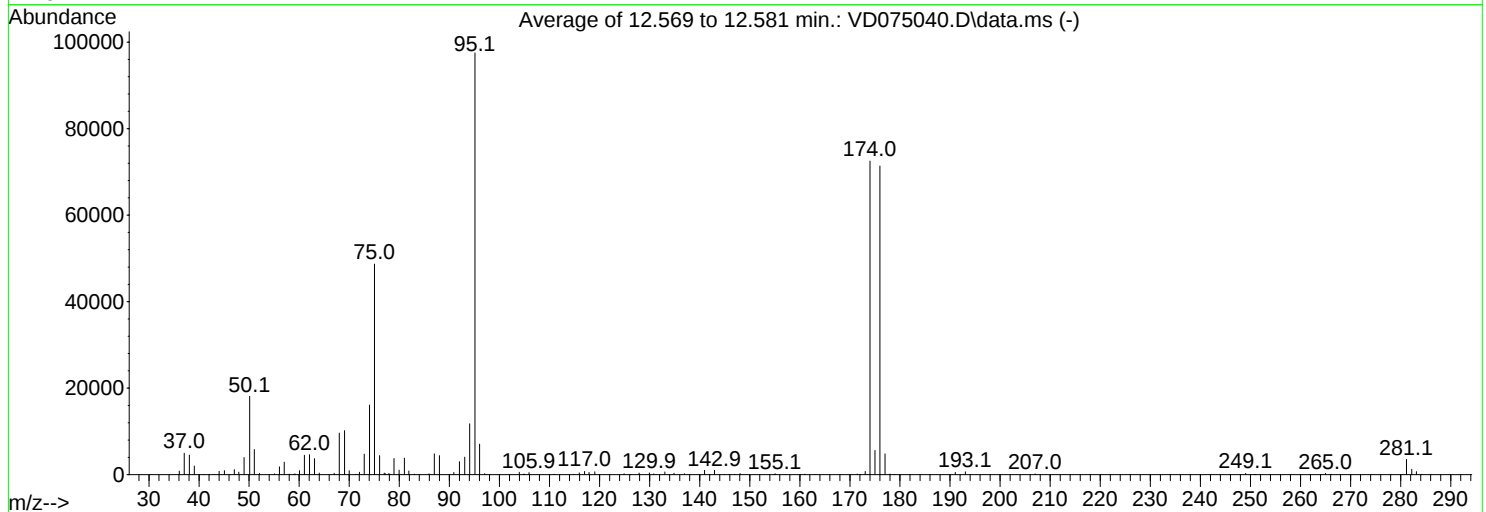


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122222\
 Data File : VD075040.D
 Acq On : 22 Dec 2022 09:35
 Operator : KP/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122222S.M
 Title : SW846 8260
 Last Update : Fri Dec 23 05:54:19 2022

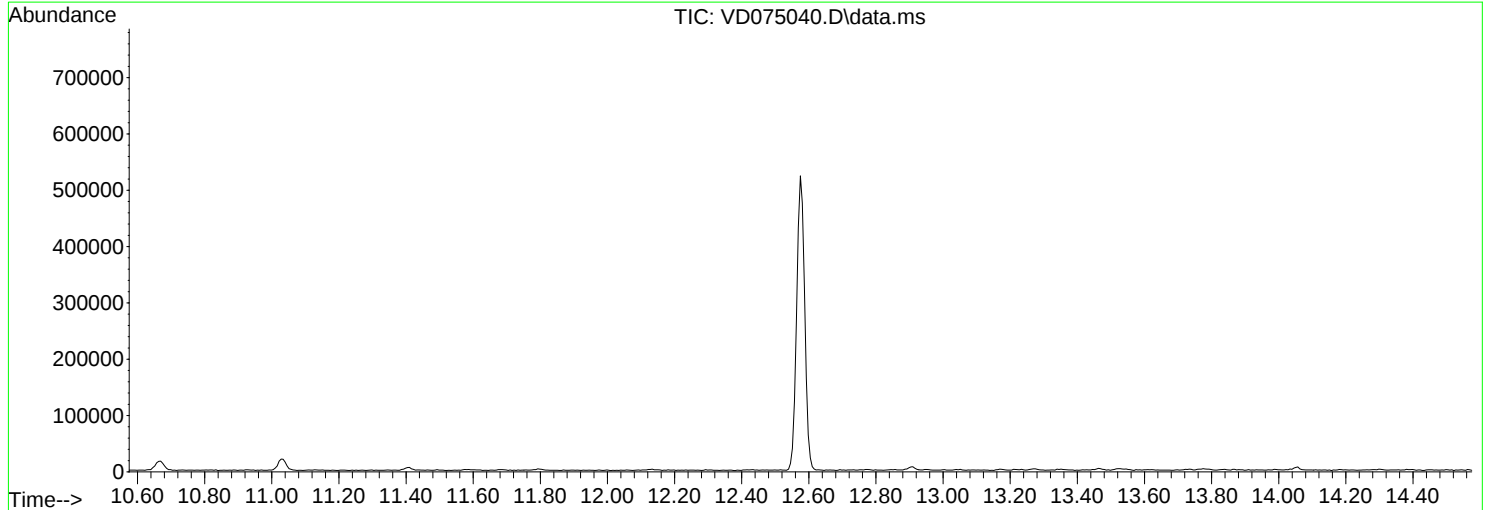

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	18080	PASS
75	95	30	60	49.9	48693	PASS
95	95	100	100	100.0	97528	PASS
96	95	5	9	7.3	7084	PASS
173	174	0.00	2	1.0	739	PASS
174	95	50	100	74.3	72499	PASS
175	174	5	9	7.7	5591	PASS
176	174	95	101	98.4	71371	PASS
177	176	5	9	6.7	4810	PASS