


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD122718\
 Data File : VD060719.D
 Acq On : 27 Dec 2018 10:37
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122018S.M
 Title : SW846 8260
 Last Update : Fri Dec 21 17:37:47 2018

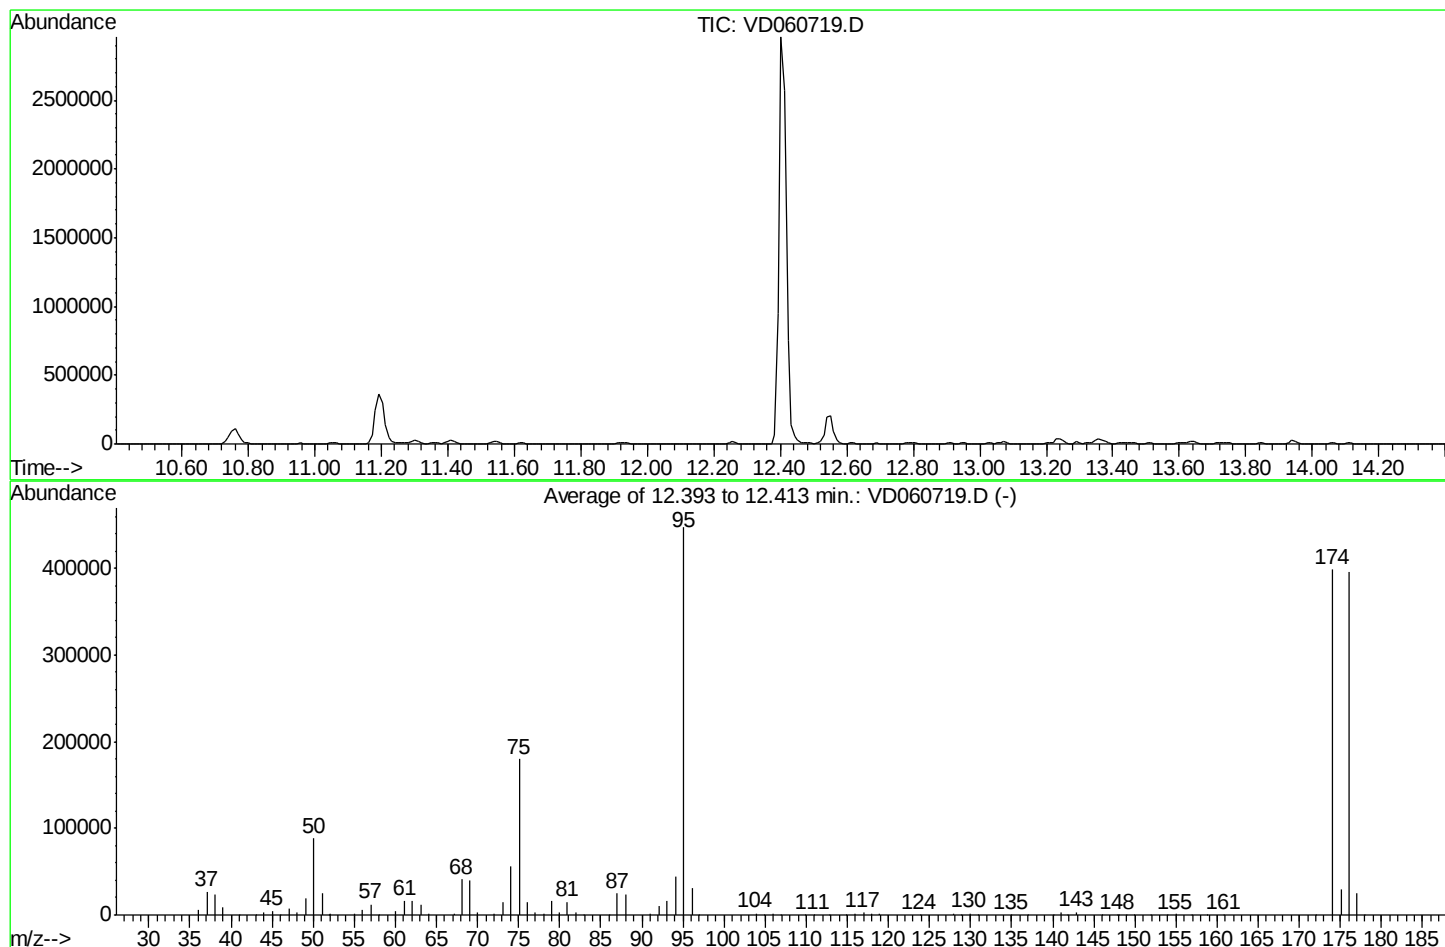

AutoFind: Scans 1135, 1136, 1137; Background Corrected with Scan 1131

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	88226	PASS
75	95	30	60	40.1	179512	PASS
95	95	100	100	100.0	447232	PASS
96	95	5	9	6.8	30431	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.0	398162	PASS
175	174	5	9	7.5	29720	PASS
176	174	95	101	99.4	395728	PASS
177	176	5	9	6.4	25321	PASS