

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN010219\
Data File : VN053244.D
Acq On : 2 Jan 2019 14:58
Operator : MD\SY
Sample : K1023-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PURGE-WATER

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	410	427	446	rBV	426622	925689	1.29%	0.902%
2	6.828	1549	1572	1604	rBV	679416	1986217	2.76%	1.936%
3	7.587	1788	1808	1819	rBV	654426	1650267	2.29%	1.608%
4	7.664	1819	1832	1865	rVB	1308089	3133442	4.36%	3.054%
5	8.024	1926	1944	1969	rBV	687470	1592211	2.21%	1.552%
6	8.583	2101	2118	2146	rVB	1910944	3969080	5.52%	3.868%
7	8.834	2169	2196	2212	rBV2	441231	979410	1.36%	0.954%
8	10.088	2568	2586	2600	rBV	3077914	5619348	7.81%	5.476%
9	10.632	2738	2755	2788	rBV	40002508	71934681	100.00%	70.100%
10	11.406	2981	2996	3018	rBV	2731516	4664687	6.48%	4.546%
11	12.400	3290	3305	3327	rBV	1988603	3295782	4.58%	3.212%
12	13.342	3586	3598	3610	rBV	1774733	2865820	3.98%	2.793%


Sum of corrected areas: 102616634

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN010219\
Data File : VN053244.D
Acq On : 2 Jan 2019 14:58
Operator : MD\SY
Sample : K1023-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PURGE-WATER

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

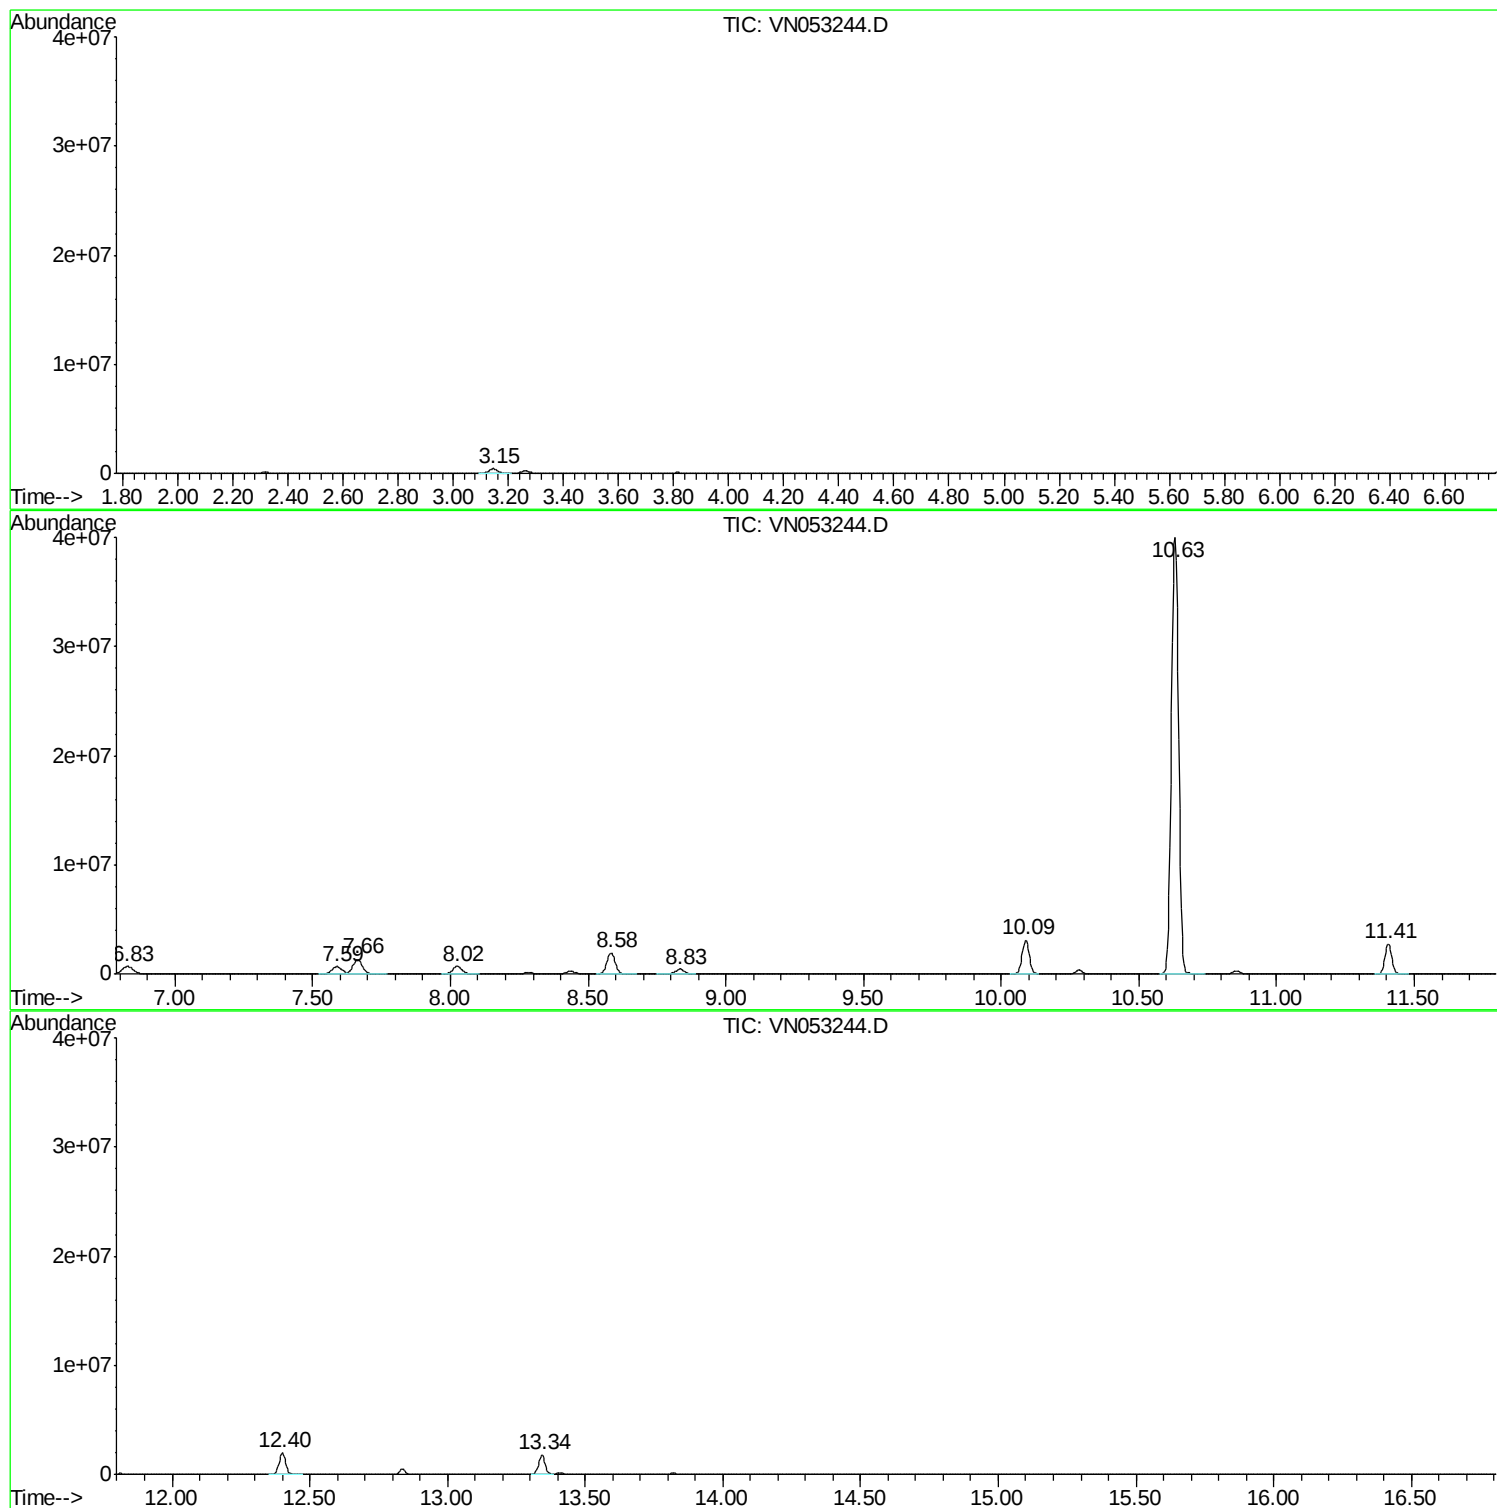

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN010219\
Data File : VN053244.D
Acq On : 2 Jan 2019 14:58
Operator : MD\SY
Sample : K1023-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampled :
PURGE-WATER










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.15	14.77 ug/l	925689	Pentafluorobenzene	7.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Pentane	72	C5H12	000109-66-0	91
2		Oxirane, ethyl-	72	C4H8O	000106-88-7	40
3		Butane, 2,3-dimethyl-	86	C6H14	000079-29-8	36
4		Diaziridine,3,3-dimethyl-	72	C3H8N2	004901-76-2	32
5		Cyclobutane, methyl-	70	C5H10	000598-61-8	9

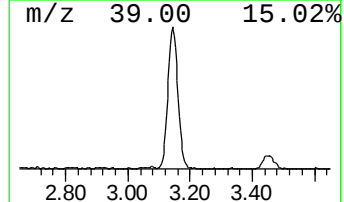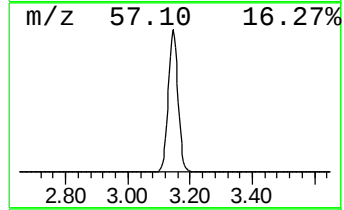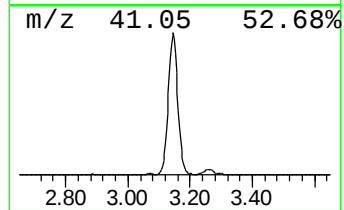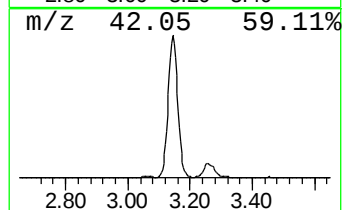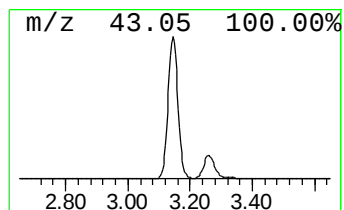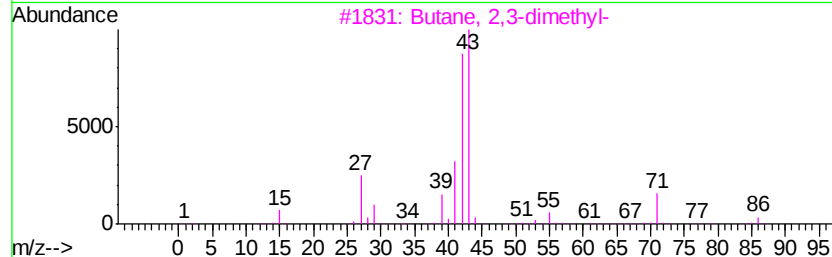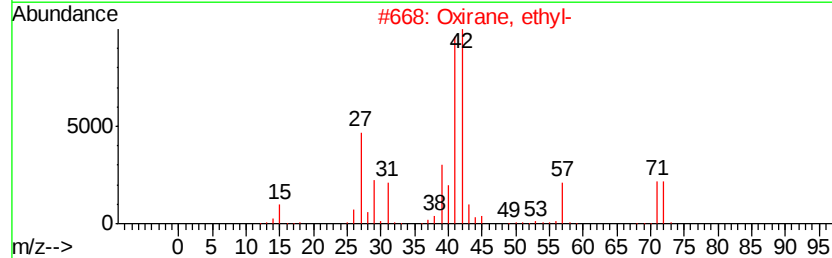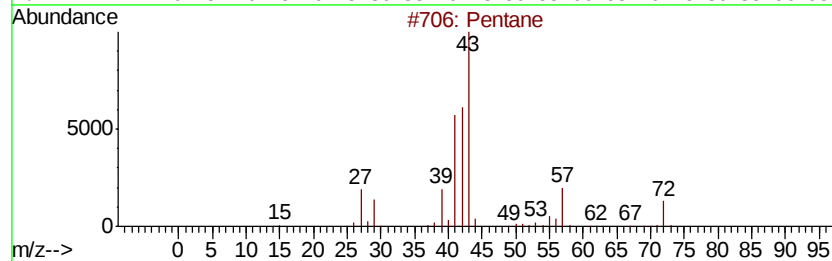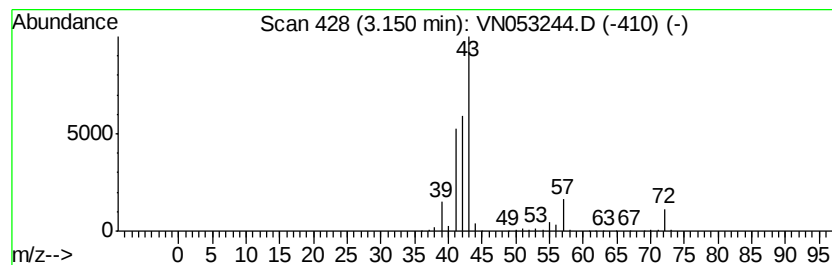

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN010219\
Data File : VN053244.D
Acq On : 2 Jan 2019 14:58
Operator : MD\SY
Sample : K1023-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PURGE-WATER

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentane	3.15	14.8	ug/l	925689	1	7.66	3133440	50.0