


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN010219\
 Data File : VN053235.D
 Acq On : 2 Jan 2019 8:31
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
 Title : SW846 8260
 Last Update : Tue Dec 18 13:03:37 2018

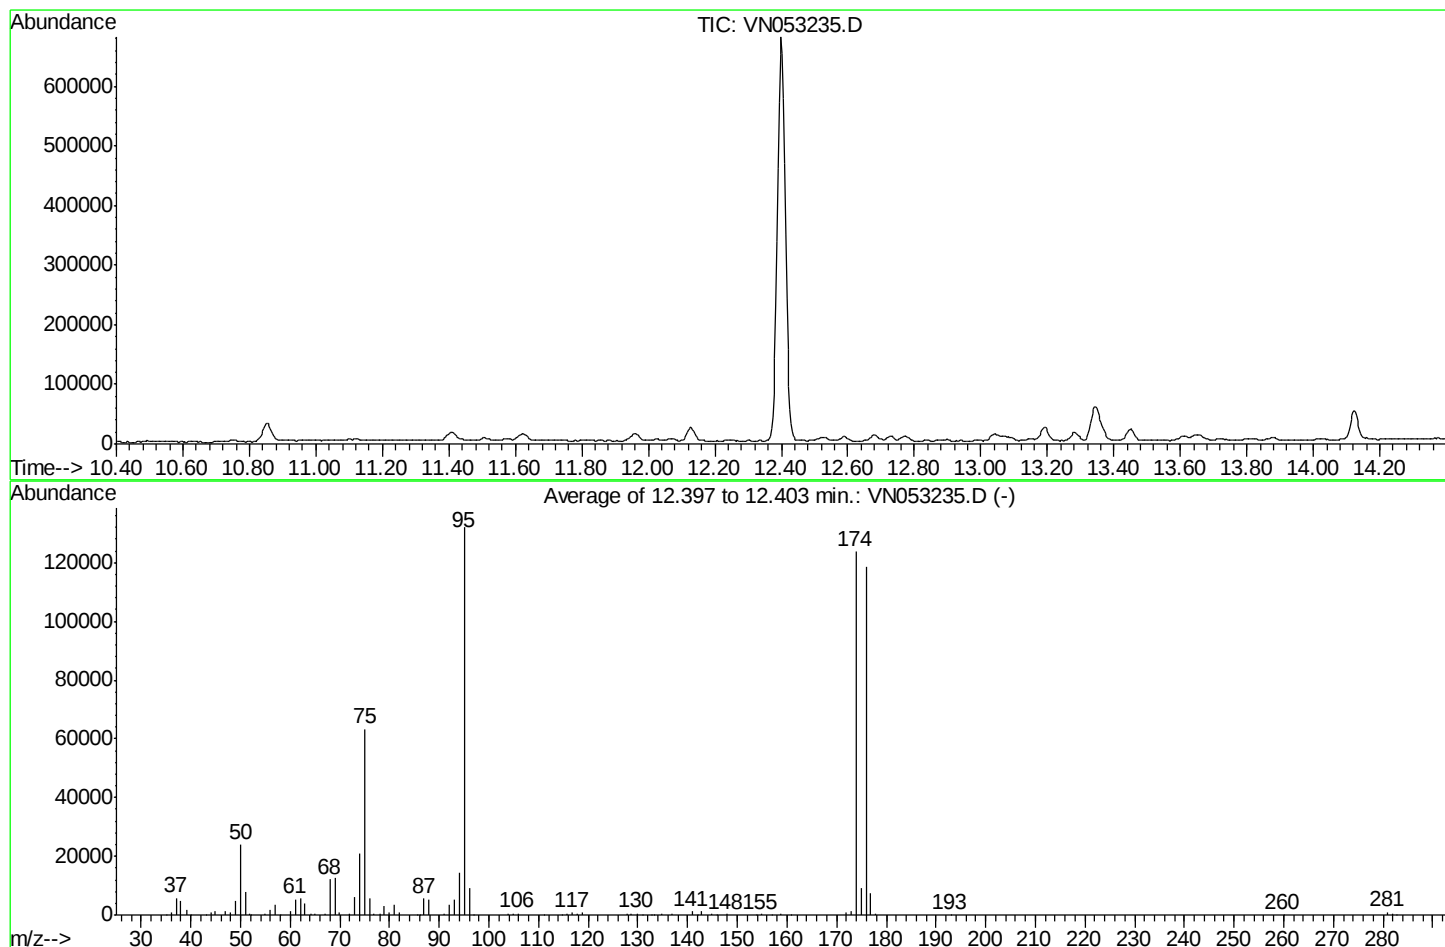

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	23938	PASS
75	95	30	60	48.0	63349	PASS
95	95	100	100	100.0	132037	PASS
96	95	5	9	6.8	9030	PASS
173	174	0.00	2	0.9	1159	PASS
174	95	50	100	93.7	123661	PASS
175	174	5	9	7.6	9367	PASS
176	174	95	101	95.9	118592	PASS
177	176	5	9	6.4	7577	PASS