
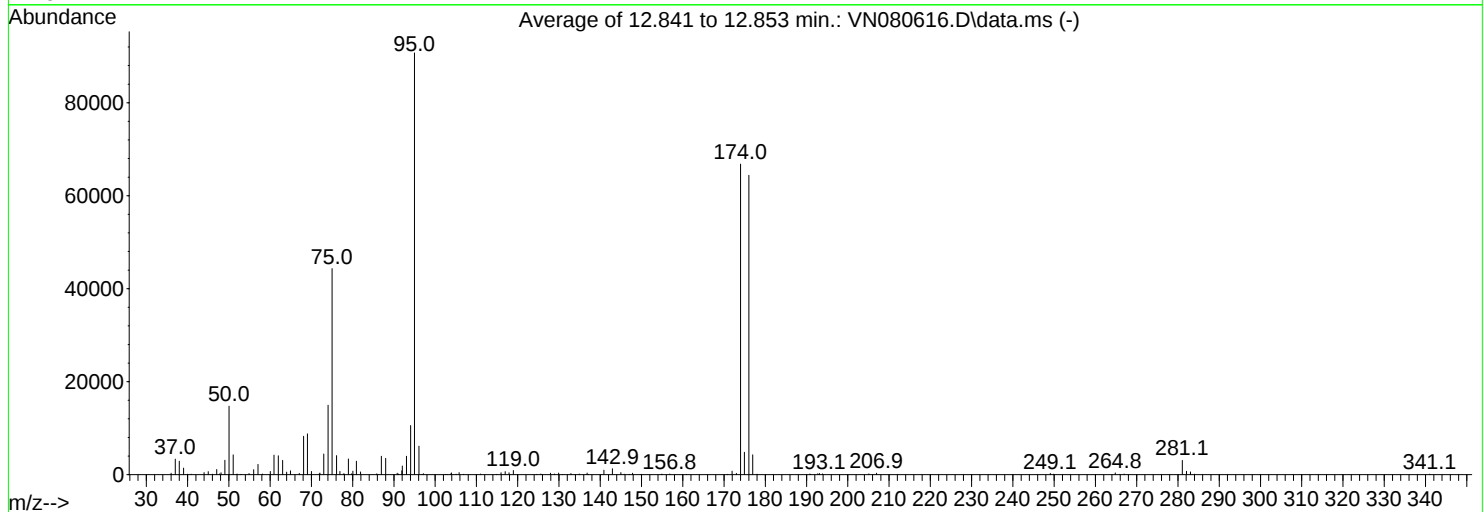


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010224\
Data File : VN080616.D
Acq On : 02 Jan 2024 09:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122723W.M
Title : SW846 8260
Last Update : Thu Dec 28 03:07:01 2023

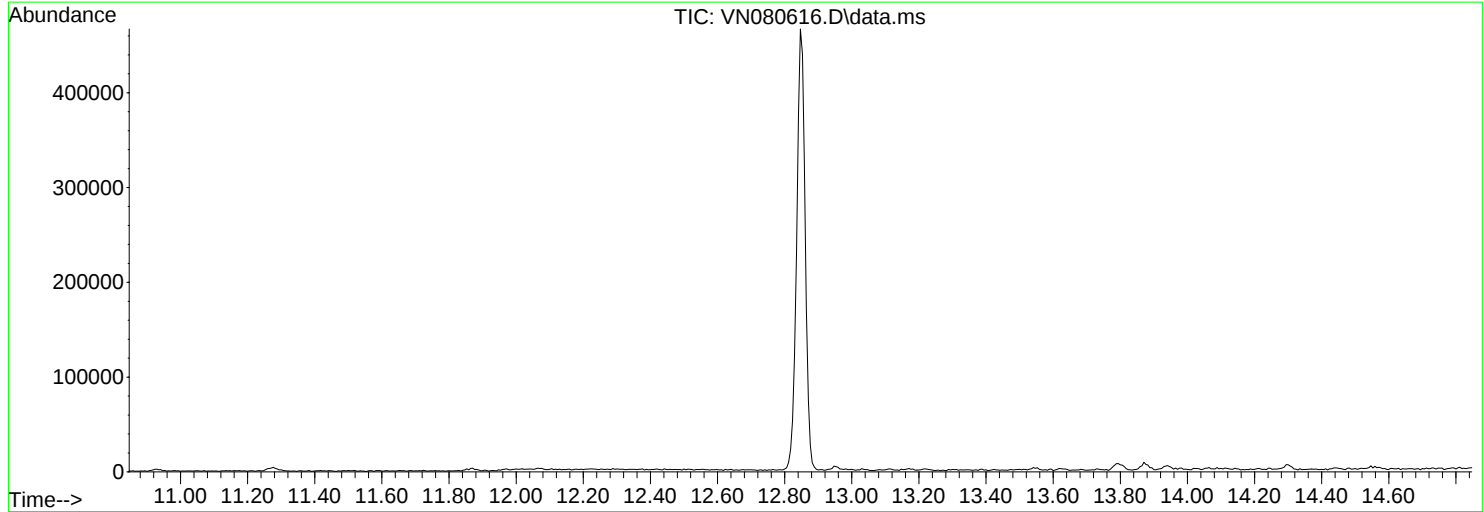

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	14726	PASS
75	95	30	60	48.9	44336	PASS
95	95	100	100	100.0	90736	PASS
96	95	5	9	6.8	6144	PASS
173	174	0.00	2	0.4	262	PASS
174	95	50	100	73.6	66803	PASS
175	174	5	9	7.2	4811	PASS
176	174	95	101	96.4	64413	PASS
177	176	5	9	6.6	4273	PASS

Average of 12.841 to 12.853 min.: VN080616.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	326	48.10	428	60.95	4211	73.00	4451
37.00	3349	49.05	3102	62.00	4064	74.05	1494
38.00	2903	50.05	14726	63.05	3072	75.00	4433
39.05	1396	51.05	4274	64.00	546	76.10	408
40.00	99	52.00	133	64.95	841	76.90	707
40.85	118	52.90	62	67.05	276	77.75	186
44.00	444	54.90	257	68.10	8258	78.00	125
45.00	672	56.00	1055	69.05	8787	78.95	3382
46.05	103	57.05	2216	70.00	700	79.70	171
47.05	1097	58.15	124	71.90	198	80.05	745
47.80	185	60.05	702	72.05	345	80.90	2881

Average of 12.841 to 12.853 min.: VN080616.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	584	95.00	90736	111.05	142	130.90	52
85.85	184	96.05	6144	114.90	58	132.90	253
86.10	72	96.80	82	115.95	422	133.90	55
86.95	3972	97.15	194	116.95	653	134.90	150
88.00	3499	102.60	65	117.90	414	136.80	334
90.80	300	102.90	51	118.95	880	137.10	73
91.10	152	103.70	128	124.60	61	140.90	948
91.90	847	103.95	372	125.60	147	142.95	1286
92.05	1846	105.05	110	127.95	321	145.00	452
93.05	3957	105.80	444	128.90	149	145.80	109
94.05	10587	106.90	75	129.90	333	147.00	69

Average of 12.841 to 12.853 min.: VN080616.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.85	306	176.00	64413	249.90	118		
149.90	62	176.95	4273	264.80	374		
154.80	90	178.00	119	265.90	56		
155.00	74	190.80	152	266.95	151		
156.85	155	191.00	65	281.05	3064		
160.90	58	192.75	221	282.05	710		
170.80	64	193.10	246	283.05	578		
171.95	751	193.85	160	284.00	92		
173.00	262	205.10	179	341.05	106		
174.00	66803	206.95	296				
174.95	4811	249.05	268				

Instrument :

MSVOA_N

ClientSampleId :

BFB