

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN010319\
 Data File : VN053250.D
 Acq On : 3 Jan 2019 9:42
 Operator : MD\SY
 Sample : VN0103WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 3 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0103WBL01

Quant Time: Jan 04 06:38:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 18 13:03:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	1158100	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	1797692	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1658352	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	646659	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	567571	48.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.58%	
35) Dibromofluoromethane	7.59	113	509234	62.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	124.02%	
50) Toluene-d8	10.09	98	2202537	49.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.92%	
62) 4-Bromofluorobenzene	12.40	95	756189	48.86	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.72%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN010319\
Data File : VN053250.D
Acq On : 3 Jan 2019 9:42
Operator : MD\SY
Sample : VN0103WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 3 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
VN0103WBL01

Quant Time: Jan 04 06:38:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 18 13:03:37 2018
Response via : Initial Calibration

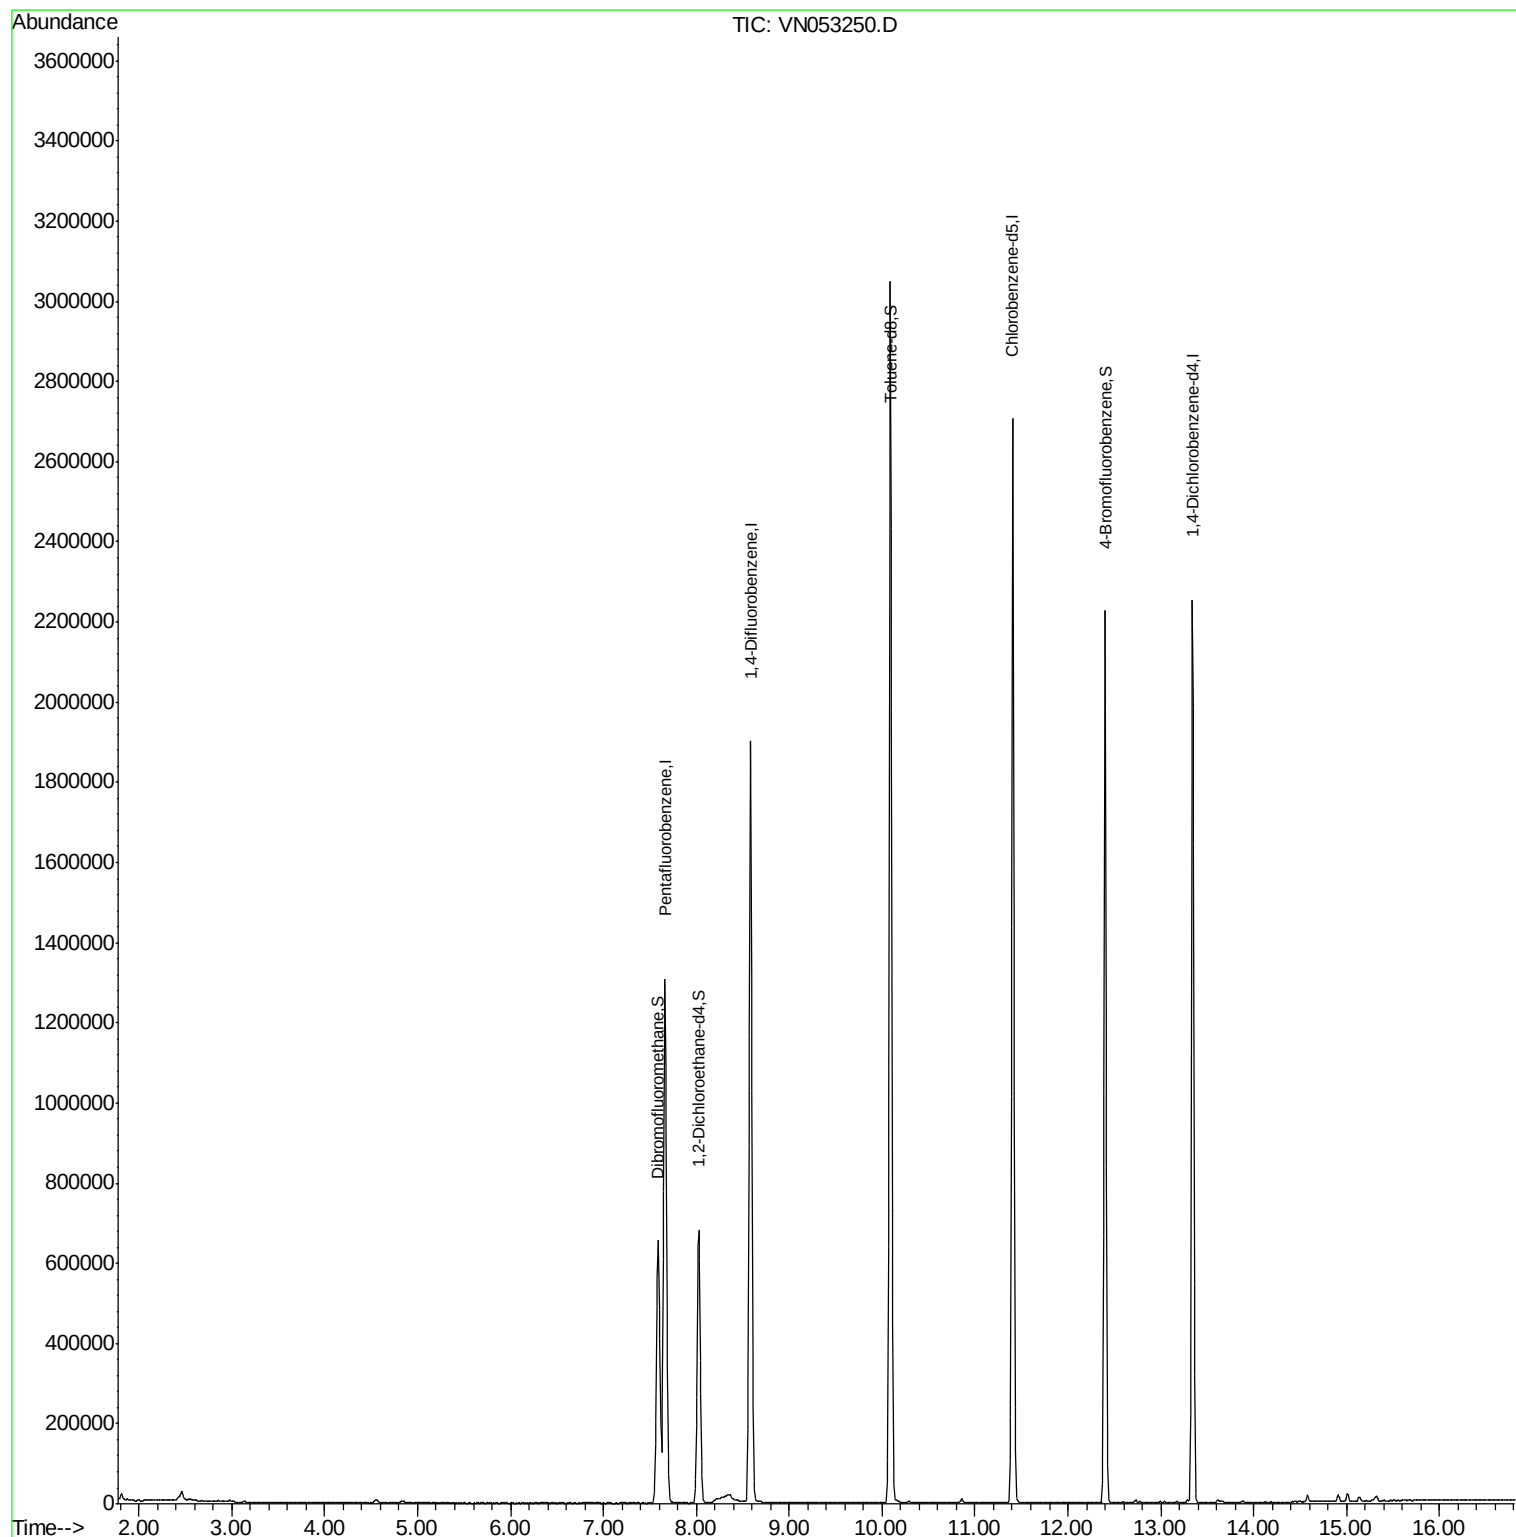

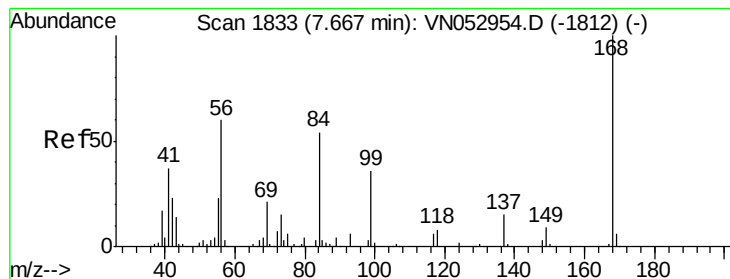

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.66 min Scan# 1832

Delta R.T. -0.00 min

Lab File: VN053250.D

Acq: 3 Jan 2019 9:42

Instrument :

MSVOA_N

ClientSampled :


VN0103WBL01

Tot Ion:168 Resp: 1158100

Ion Ratio Lower Upper

168 100

99 50.0 40.2 60.2

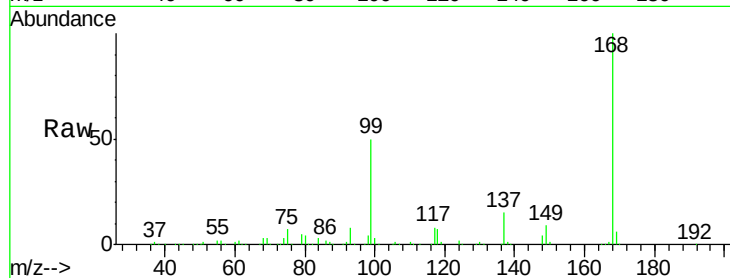

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.66

500000

400000



300000

200000

100000

0

Time-->

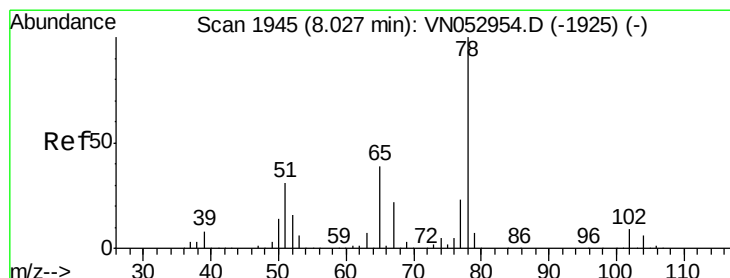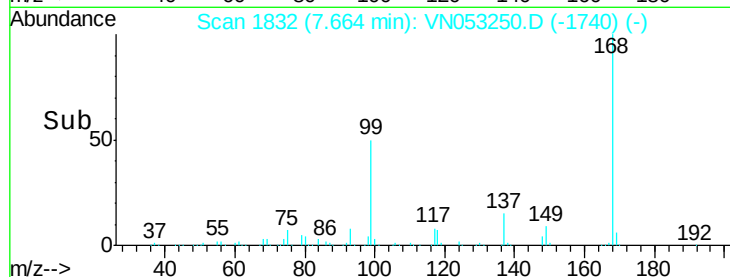

#33

1,2-Dichloroethane-d4

Concen: Below ug/l

RT: 8.03 min Scan# 1945

Delta R.T. 0.00 min

Lab File: VN053250.D


Acq: 3 Jan 2019 9:42

Tgt Ion: 65 Resp: 567571

Ion Ratio Lower Upper

65 100

67 55.0 0.0 110.4

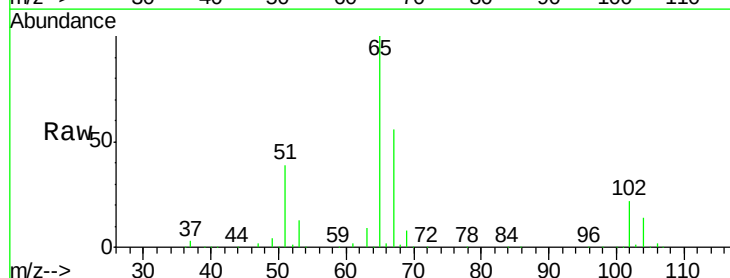

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

8.03

250000

200000


150000


100000

50000

0

Time-->

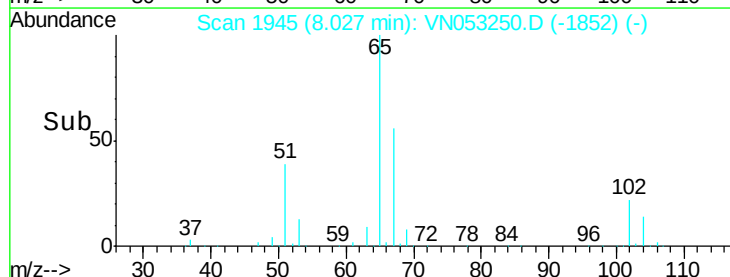

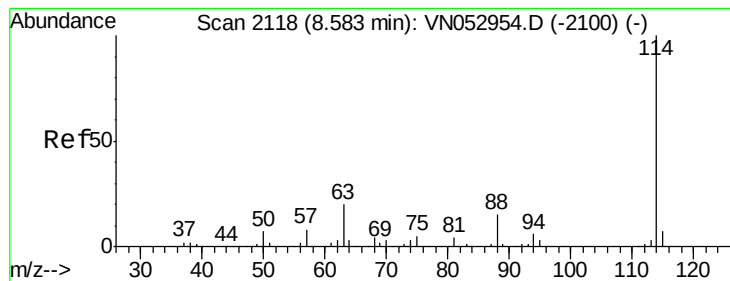

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.58 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN053250.D

Acq: 3 Jan 2019 9:42

Instrument :

MSVOA_N

ClientSampleId :

VN0103WBL01


Tot Ion:114 Resp: 1797692

Ion Ratio Lower Upper

114 100

63 19.7 0.0 39.8




88 15.6 0.0 31.0

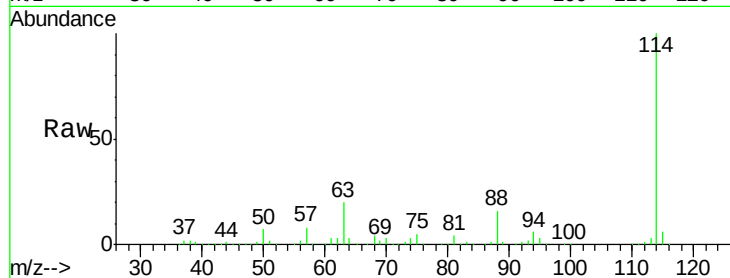

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

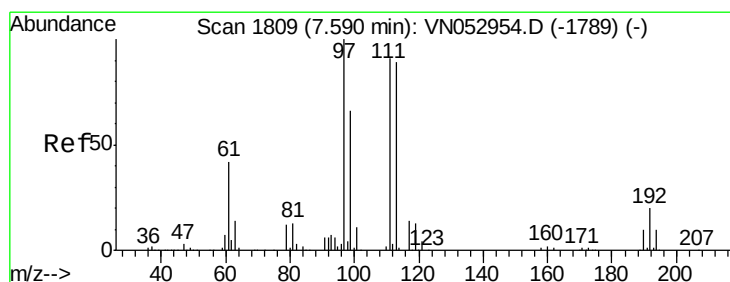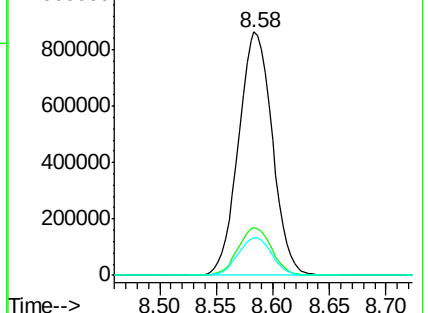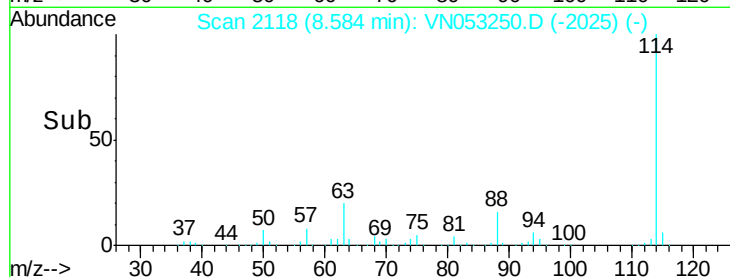

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 7.59 min Scan# 1809

Delta R.T. 0.00 min

Lab File: VN053250.D

Acq: 3 Jan 2019 9:42


Tgt Ion:113 Resp: 509234

Ion Ratio Lower Upper

113 100

111 102.8 83.0 124.4



192 22.9 17.5 26.3

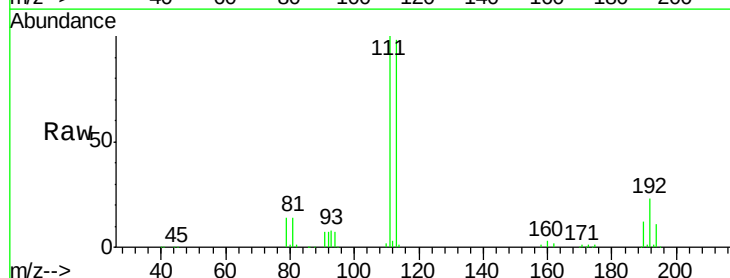


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

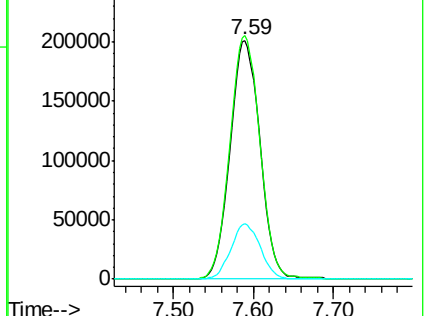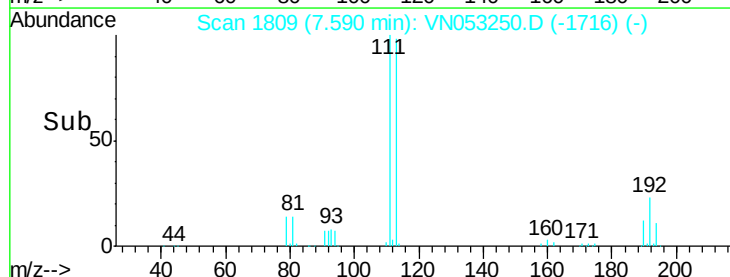

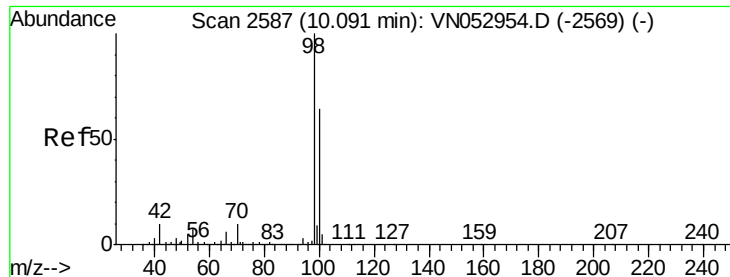

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2586

Delta R.T. -0.00 min

Lab File: VN053250.D

Acq: 3 Jan 2019 9:42

Instrument :

MSVOA_N

ClientSampled :


VN0103WBL01

Tot Ion: 98 Resp: 2202537

Ion Ratio Lower Upper




98 100

100 64.6 51.6 77.4

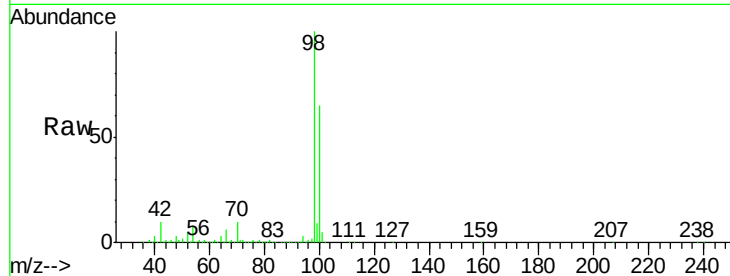

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

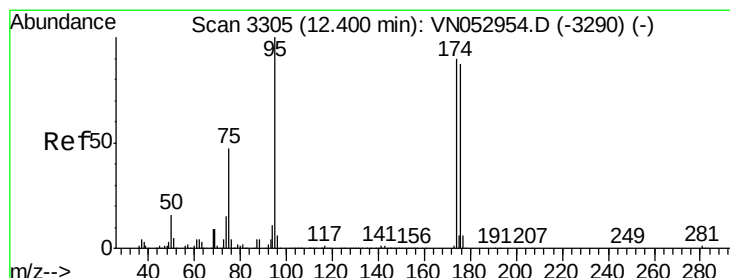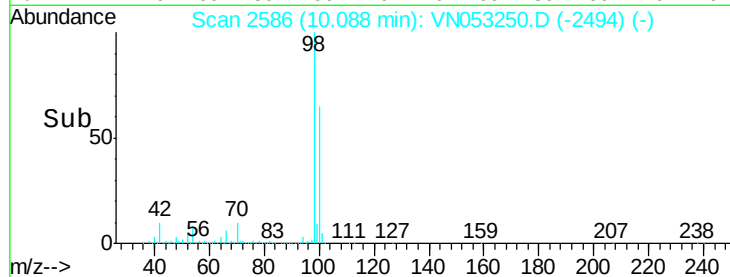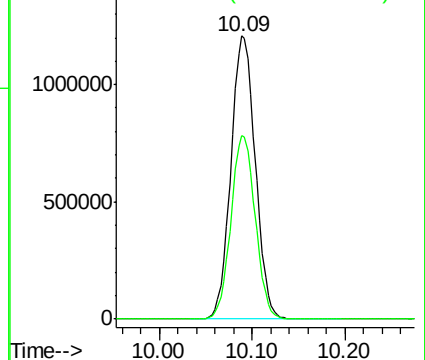

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN053250.D

Acq: 3 Jan 2019 9:42


Tgt Ion: 95 Resp: 756189

Ion Ratio Lower Upper

95 100

174 90.9 0.0 178.8



176 88.7 0.0 173.8

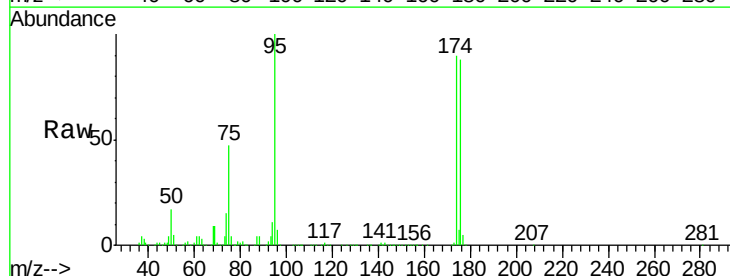


Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

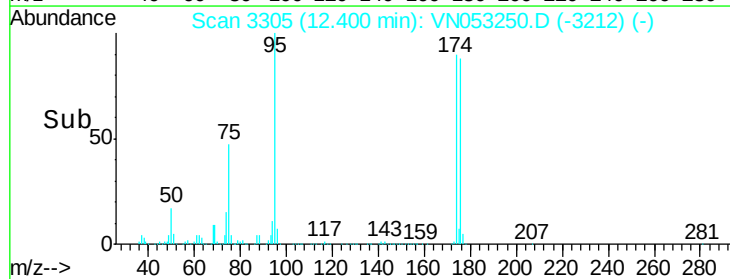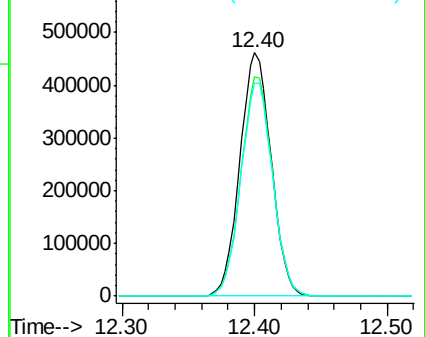


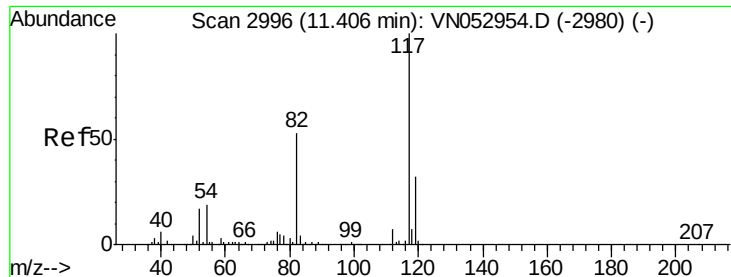




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN053250.D
Acq: 3 Jan 2019 9:42

Instrument :
MSVOA_N
ClientSampleId :
VN0103WBL01

Tot Ion:117 Resp: 1658352
Ion Ratio Lower Upper
117 100
82 53.6 42.8 64.2
119 32.3 25.5 38.3

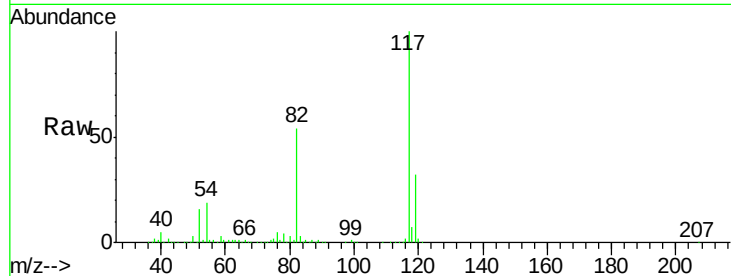


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

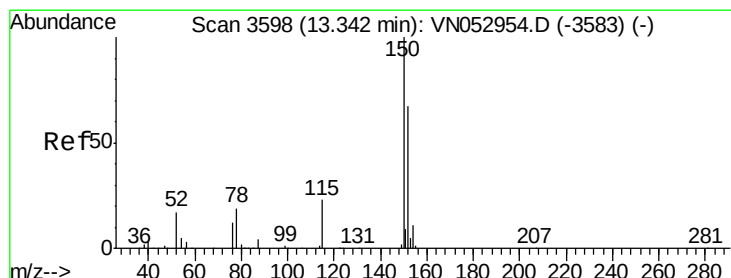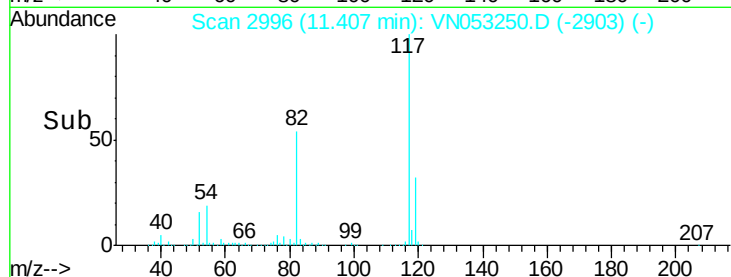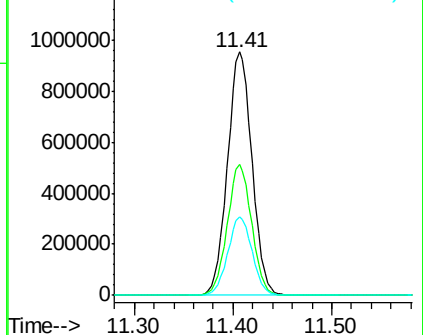

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN053250.D
Acq: 3 Jan 2019 9:42

Tgt Ion:152 Resp: 646659
Ion Ratio Lower Upper
152 100
115 55.3 28.3 85.0
150 157.4 0.0 347.8

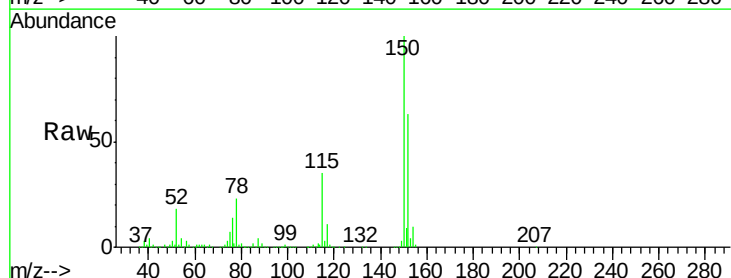

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

