

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010322\
 Data File : VN070450.D
 Acq On : 3 Jan 2022 20:40
 Operator : JC/MD
 Sample : M5236-02ME
 Misc : 6.86g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-2ME

Quant Time: Jan 04 01:38:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.078	168	1058310	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	2045150	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2295495	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.672	152	1172404	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.432	65	776813	51.051	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 102.100%			
35) Dibromofluoromethane	8.016	113	561355	45.365	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 90.740%			
50) Toluene-d8	10.438	98	2709231	53.595	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 107.200%			
62) 4-Bromofluorobenzene	12.731	95	1198786	65.660	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 131.320%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.220	50	15813	0.969	ug/l #	43
6) Chloroethane	3.022	64	3218	0.359	ug/l #	43
11) Tert butyl alcohol	5.315	59	34140	13.475	ug/l #	71
16) Acetone	4.296	43	5976	0.605	ug/l #	86
18) Methyl Acetate	4.859	43	10782	0.377	ug/l #	58
20) Methylene Chloride	5.068	84	22187	1.623	ug/l	89
25) 2-Butanone	7.354	43	67848	5.455	ug/l	92
29) Tetrahydrofuran	7.699	42	8553	1.153	ug/l #	59
31) Cyclohexane	8.075	56	24523	1.021	ug/l #	14
36) 1,1-Dichloropropene	8.078	75	87098	4.255	ug/l #	48
37) Ethyl Acetate	7.354	43	67848	2.557	ug/l #	68
38) Carbon Tetrachloride	8.078	117	103391	5.289	ug/l #	16
41) Methacrylonitrile	7.697	41	4907	0.370	ug/l #	28
43) Isopropyl Acetate	8.652	43	23144	0.553	ug/l #	55
59) 2-Hexanone	11.049	43	14020	0.731	ug/l #	26
67) Ethyl Benzene	11.843	91	22728	0.255	ug/l	95
68) m/p-Xylenes	11.948	106	17903	0.551	ug/l	95
74) N-amyl acetate	12.363	43	79806	1.743	ug/l #	66
75) 1,1,2,2-Tetrachloroethane	12.806	83	2525	0.510	ug/l #	26
76) 1,2,3-Trichloropropane	12.728	75	654618	20.563	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.058	105	106035	1.215	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.728	75	654618	68.218	ug/l #	6
83) tert-Butylbenzene	13.366	119	32154	0.419	ug/l #	66
84) 1,2,4-Trimethylbenzene	13.366	105	267928	3.189	ug/l	98
85) sec-Butylbenzene	13.498	105	190783	1.829	ug/l	97
86) p-Isopropyltoluene	13.613	119	132465	1.617	ug/l	97
89) n-Butylbenzene	13.906	91	49426	0.723	ug/l #	1
90) Hexachloroethane	14.214	117	49181	3.455	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.619	75	3745	0.594	ug/l #	10
95) Naphthalene	15.499	128	49876	2.697	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.721	180	8330	1.269	ug/l #	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010322\
 Data File : VN070450.D
 Acq On : 3 Jan 2022 20:40
 Operator : JC/MD
 Sample : M5236-02ME
 Misc : 6.86g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-2ME

Quant Time: Jan 04 01:38:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

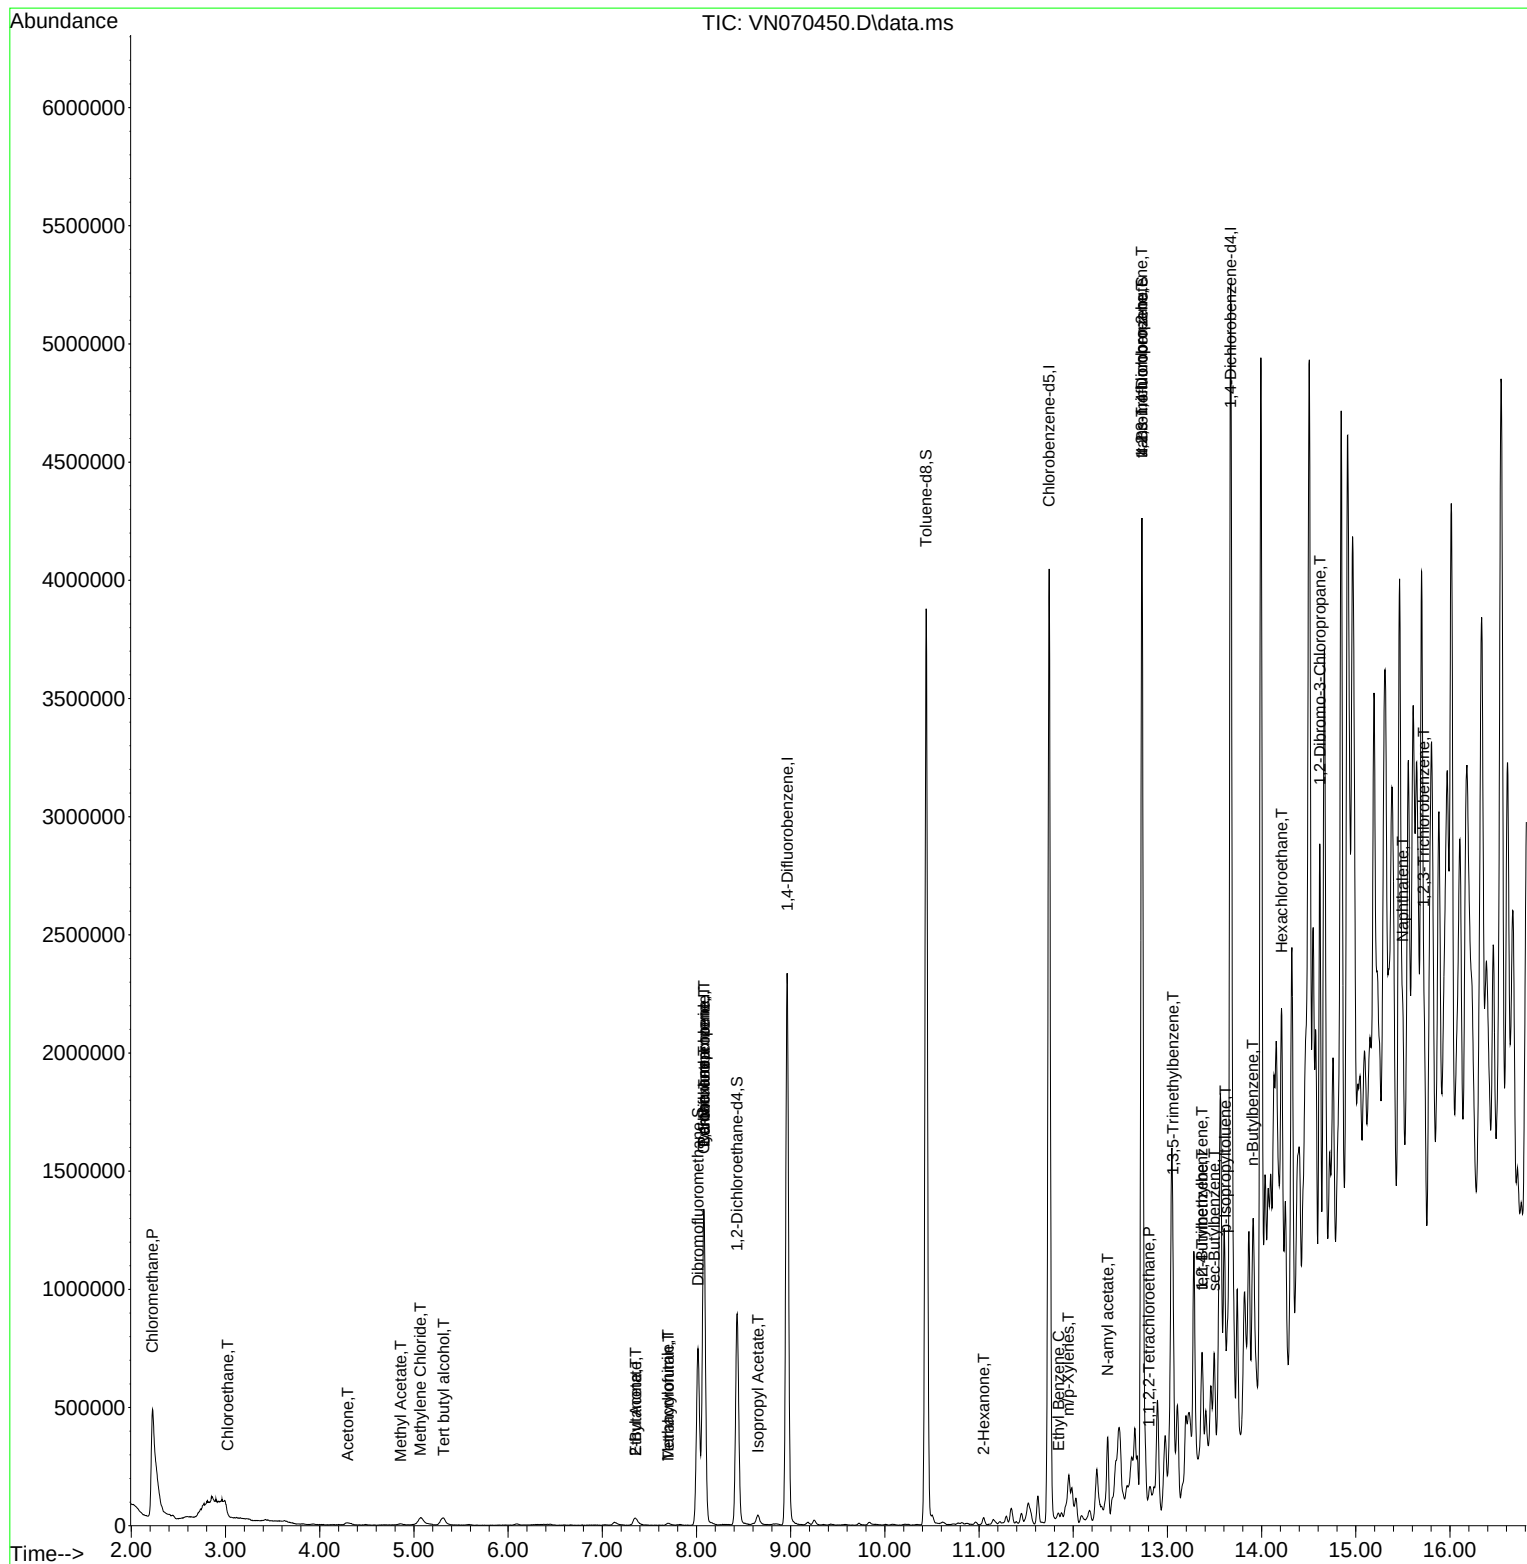

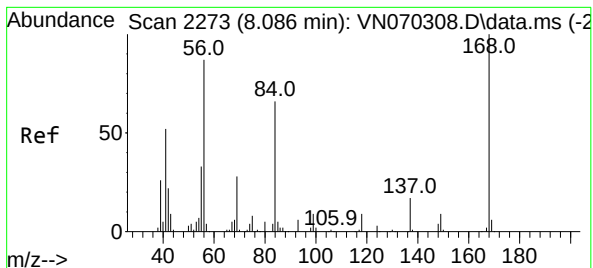

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.078 min Scan# 21

Delta R.T. -0.008 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40

Instrument :

MSVOA_N

ClientSampleId :





SB-2ME

Tgt Ion:168 Resp: 1058310

Ion Ratio Lower Upper

168 100

99 58.7 41.3 61.9

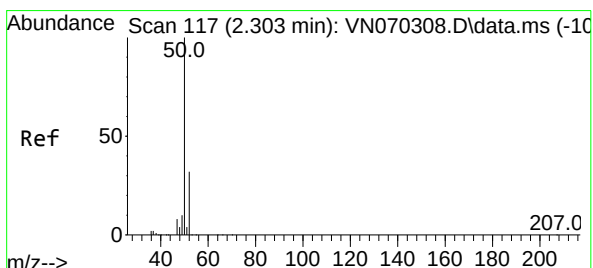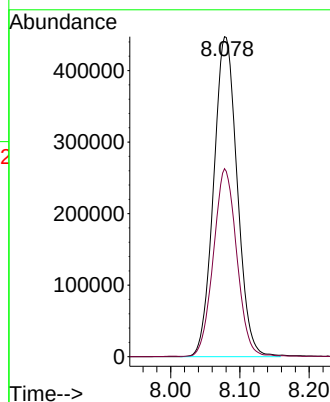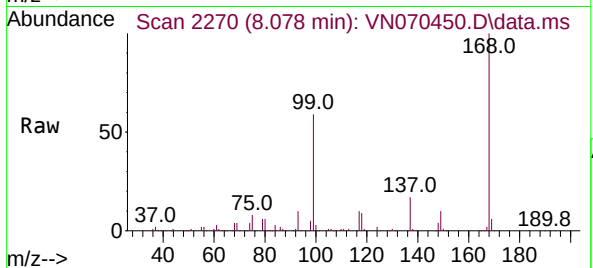

#3

Chloromethane

Concen: 0.969 ug/l

RT: 2.220 min Scan# 86

Delta R.T. -0.083 min

Lab File: VN070450.D




Acq: 3 Jan 2022 20:40


Tgt Ion: 50 Resp: 15813

Ion Ratio Lower Upper

50 100

52 0.0 25.4 38.0#


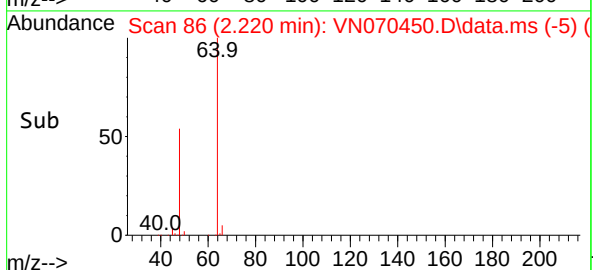

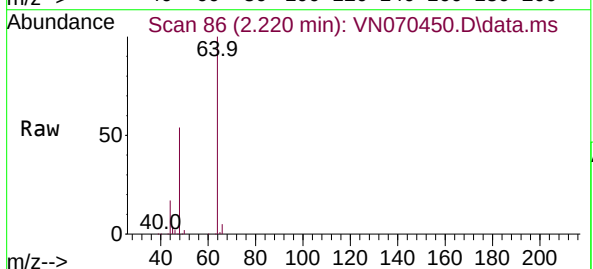




#6
Chloroethane
Concen: 0.359 ug/l
RT: 3.022 min Scan# 31
Delta R.T. 0.003 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion: 64 Resp: 3218
Ion Ratio Lower Upper
64 100
66 0.7 26.3 39.5#

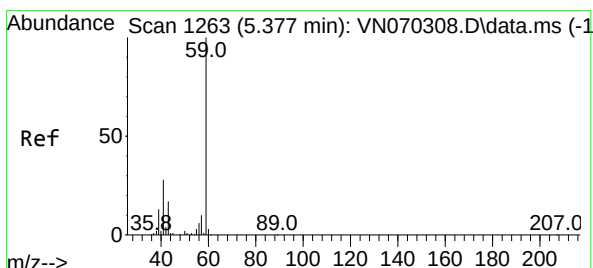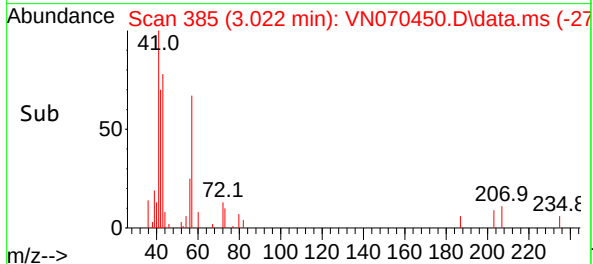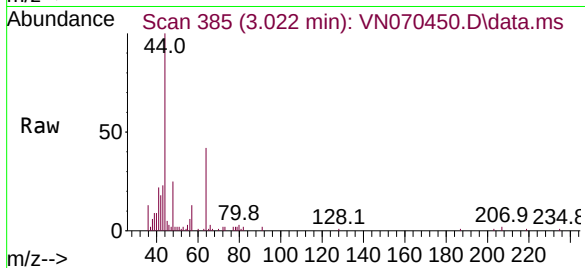

#11
Tert butyl alcohol
Concen: 13.475 ug/l
RT: 5.315 min Scan# 1240
Delta R.T. -0.062 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion: 59 Resp: 34140
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


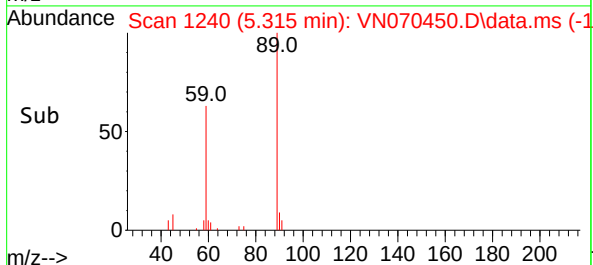

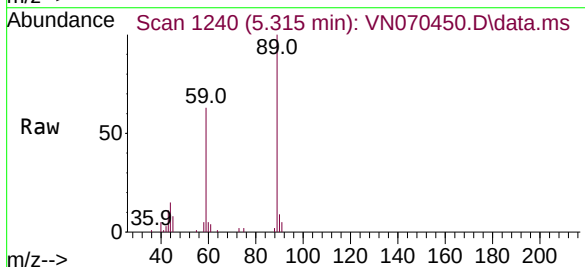


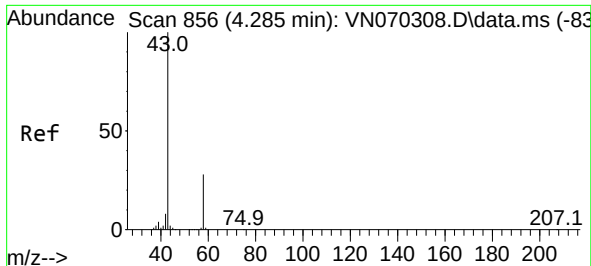

#16
Acetone
Concen: 0.605 ug/l
RT: 4.296 min Scan# 80
Delta R.T. 0.011 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion: 43 Resp: 5976
Ion Ratio Lower Upper
43 100
58 36.4 23.1 34.7#

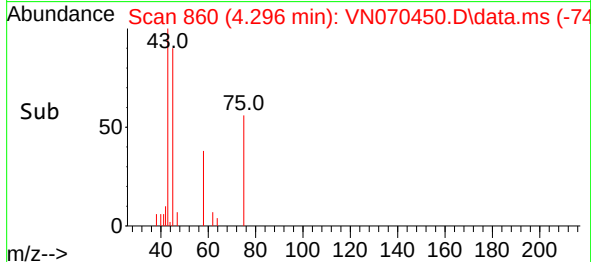

#18
Methyl Acetate
Concen: 0.377 ug/l
RT: 4.859 min Scan# 1070
Delta R.T. 0.005 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion: 43 Resp: 10782
Ion Ratio Lower Upper
43 100
74 3.5 19.4 29.2#

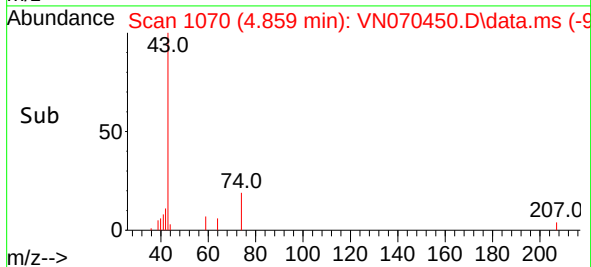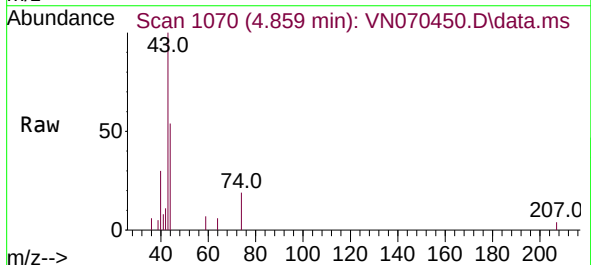



#20

Methylene Chloride

Concen: 1.623 ug/l

RT: 5.068 min Scan# 1158

Delta R.T. -0.027 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40

Instrument :

MSVOA_N

ClientSampleId :

SB-2ME

Tgt Ion: 84 Resp: 22187





Ion Ratio Lower Upper

84 100

49 136.6 93.5 140.3

51 39.4 29.4 44.2

86 67.5 53.0 79.4

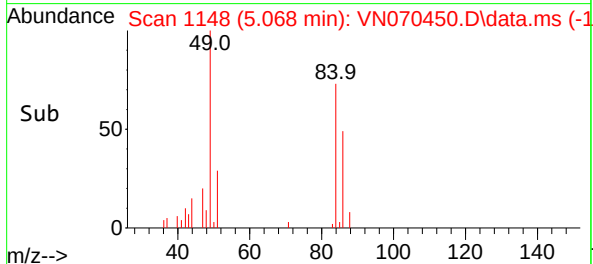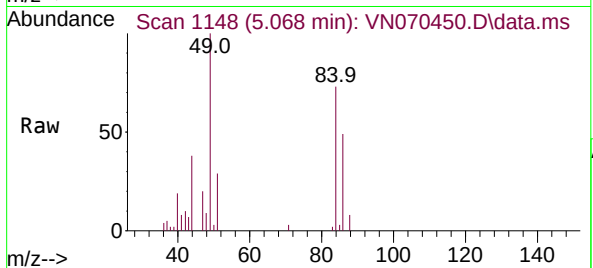

#25

2-Butanone

Concen: 5.455 ug/l

RT: 7.354 min Scan# 2000

Delta R.T. 0.019 min

Lab File: VN070450.D




Acq: 3 Jan 2022 20:40


Tgt Ion: 43 Resp: 67848

Ion Ratio Lower Upper

43 100

72 23.2 21.7 32.5

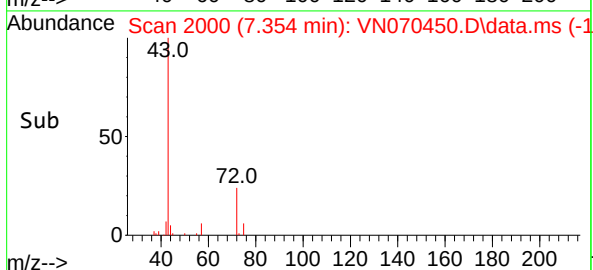

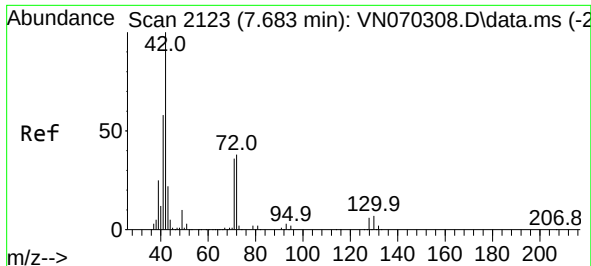

#29

Tetrahydrofuran

Concen: 1.153 ug/l

RT: 7.699 min Scan# 2123

Delta R.T. 0.016 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40

Instrument :

MSVOA_N

ClientSampleId :

SB-2ME





Tgt Ion: 42 Resp: 8553

Ion Ratio Lower Upper

42 100

72 21.5 36.3 54.5#

71 14.2 34.7 52.1#

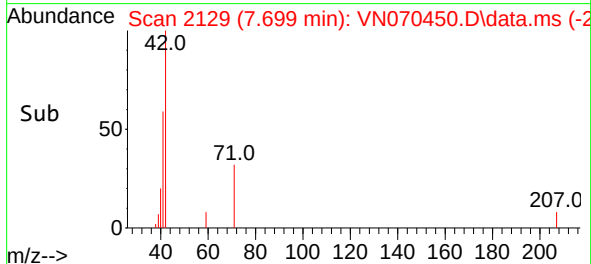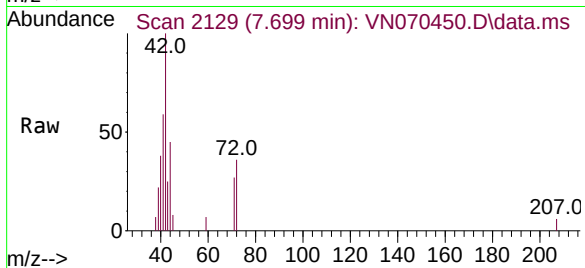

#31

Cyclohexane

Concen: 1.021 ug/l

RT: 8.075 min Scan# 2269

Delta R.T. -0.019 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40




Tgt Ion: 56 Resp: 24523


Ion Ratio Lower Upper

56 100

69 162.0 27.1 40.7#

84 125.5 73.4 110.0#

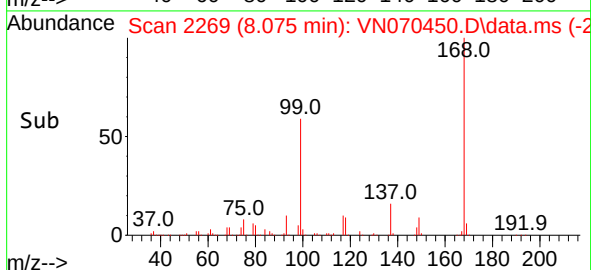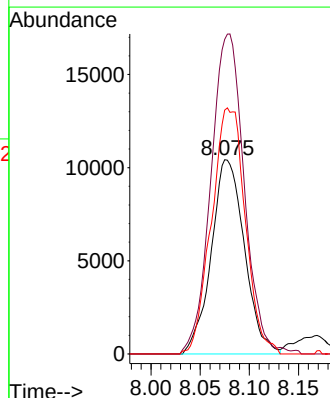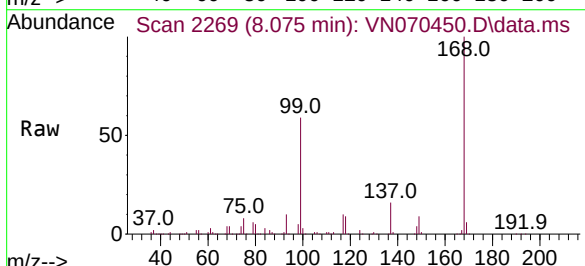

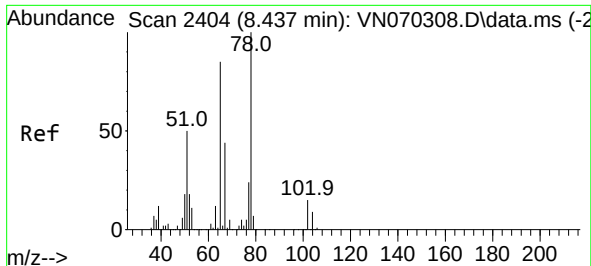

#33

1,2-Dichloroethane-d4

Concen: 51.051 ug/l

RT: 8.432 min Scan# 24

Delta R.T. -0.005 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40

Instrument :

MSVOA_N

ClientSampleId :





SB-2ME

Tgt Ion: 65 Resp: 776813

Ion Ratio Lower Upper

65 100

67 52.5 0.0 103.0

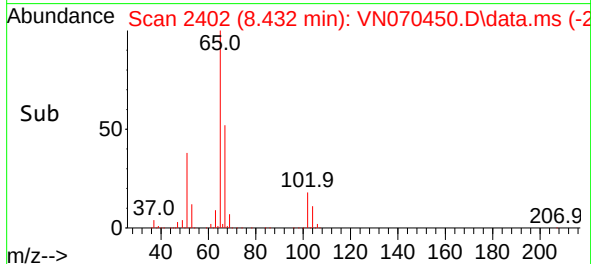

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 2600

Delta R.T. -0.005 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40




Tgt Ion: 114 Resp: 2045150


Ion Ratio Lower Upper

114 100

63 23.0 0.0 37.8

88 16.4 0.0 27.4


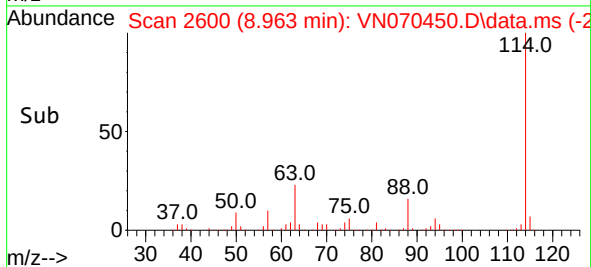

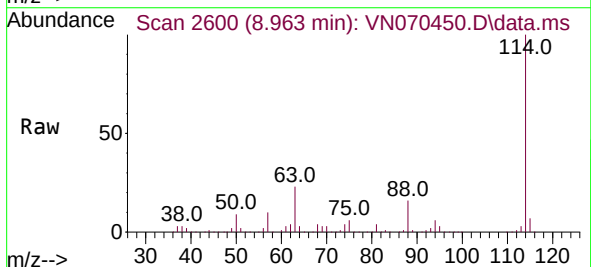


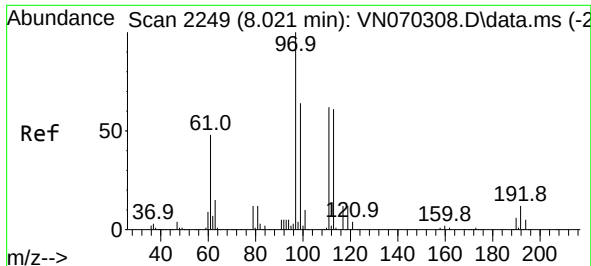

#35
Dibromofluoromethane
Concen: 45.365 ug/l
RT: 8.016 min Scan# 21
Delta R.T. -0.005 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion:113 Resp: 561355
Ion Ratio Lower Upper
113 100
111 103.6 82.2 123.2
192 19.5 16.9 25.3

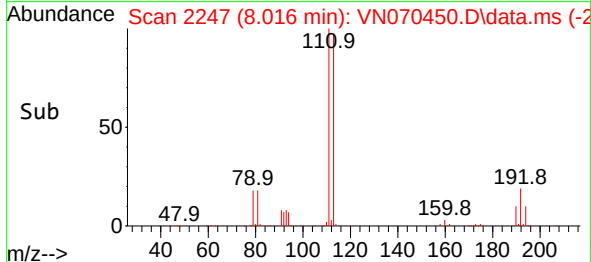

#36
1,1-Dichloropropene
Concen: 4.255 ug/l
RT: 8.078 min Scan# 2270
Delta R.T. -0.142 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion: 75 Resp: 87098
Ion Ratio Lower Upper
75 100
110 8.0 18.4 55.2#
77 0.0 24.4 36.6#

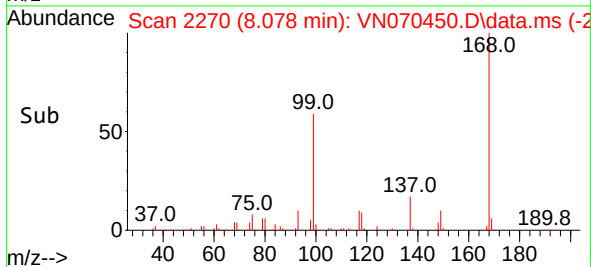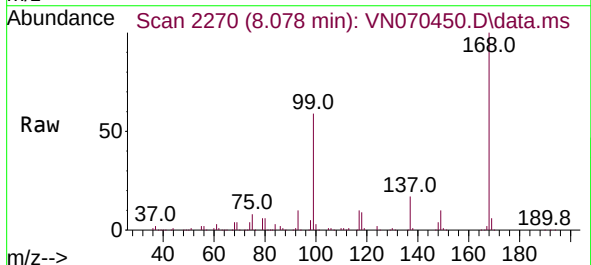



#37

Ethyl Acetate

Concen: 2.557 ug/l

RT: 7.354 min Scan# 20

Delta R.T. -0.058 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40

Instrument :

MSVOA_N

ClientSampleId :

SB-2ME





Tgt Ion: 43 Resp: 67848

Ion Ratio Lower Upper

43 100

61 0.0 11.5 17.3#

70 0.0 7.9 11.9#

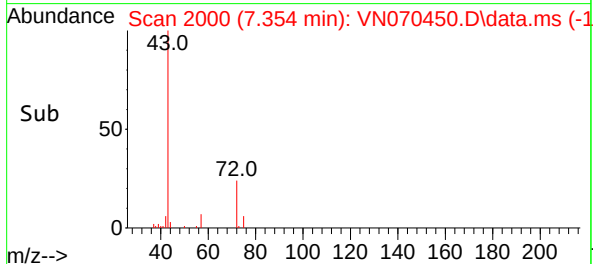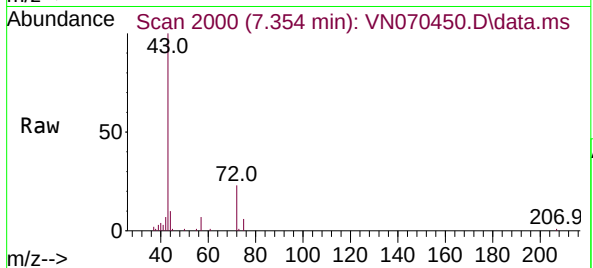

#38

Carbon Tetrachloride

Concen: 5.289 ug/l

RT: 8.078 min Scan# 2270

Delta R.T. -0.128 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40




Tgt Ion: 117 Resp: 103391


Ion Ratio Lower Upper

117 100

119 5.2 76.1 114.1#

121 0.0 24.2 36.2#


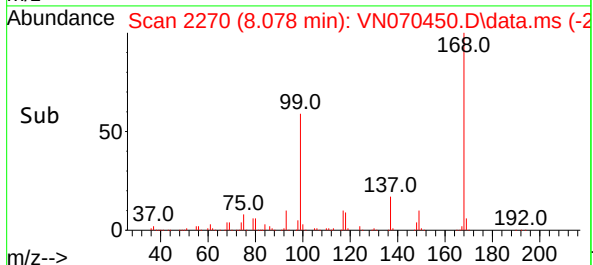
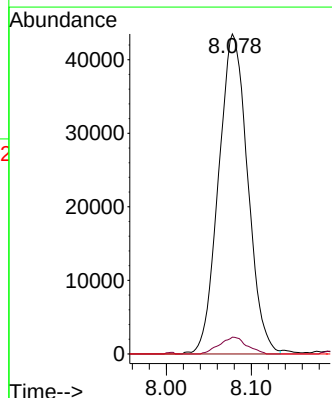
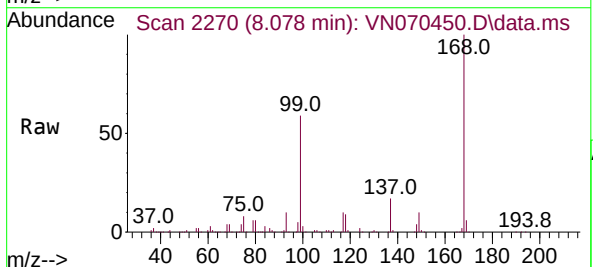




#41
Methacrylonitrile
Concen: 0.370 ug/l
RT: 7.697 min Scan# 2106
Delta R.T. 0.059 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion:	41	Resp:	4907
Ion	Ratio	Lower	Upper
41	100		
39	23.9	48.1	72.1#
67	0.0	68.3	102.5#
52	0.0	29.6	44.4#

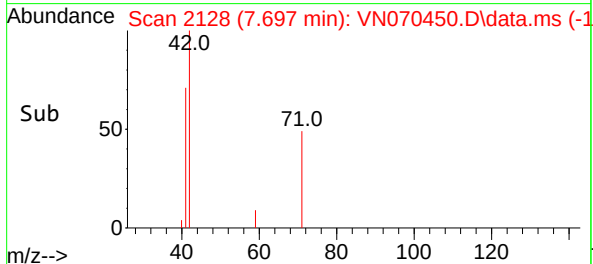

#43
Isopropyl Acetate
Concen: 0.553 ug/l
RT: 8.652 min Scan# 2484
Delta R.T. 0.092 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion:	43	Resp:	23144
Ion	Ratio	Lower	Upper
43	100		
61	0.0	20.4	30.6#
87	0.0	11.2	16.8#


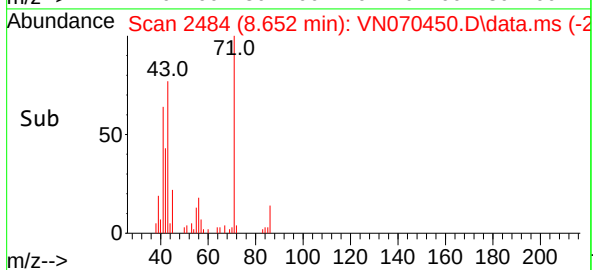

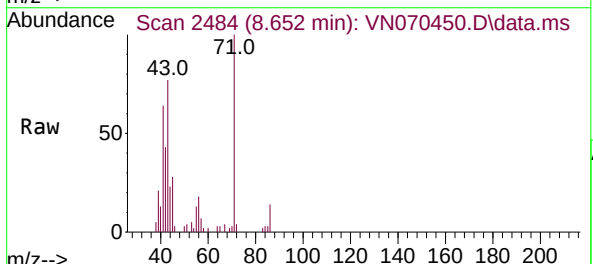




#50
Toluene-d8
Concen: 53.595 ug/l
RT: 10.438 min Scan# 3150
Delta R.T. -0.002 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion: 98 Resp: 2709231
Ion Ratio Lower Upper
98 100
100 64.4 50.4 75.6

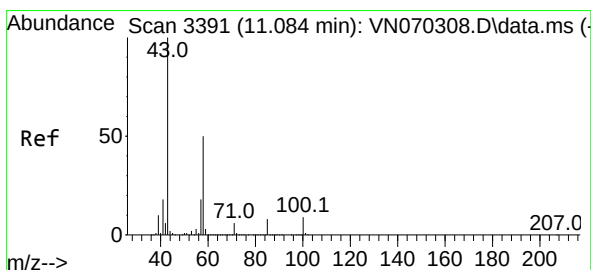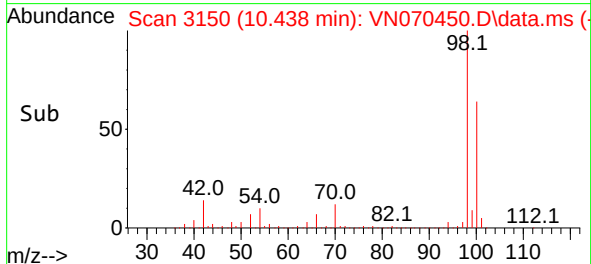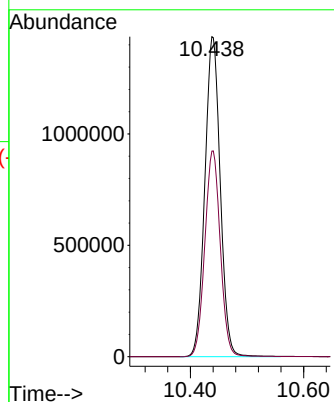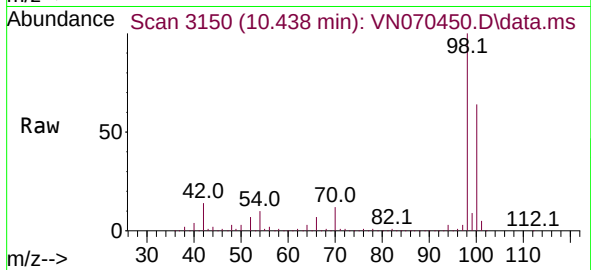

#59
2-Hexanone
Concen: 0.731 ug/l
RT: 11.049 min Scan# 3378
Delta R.T. -0.035 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion: 43 Resp: 14020
Ion Ratio Lower Upper
43 100
58 1.2 26.9 80.7#


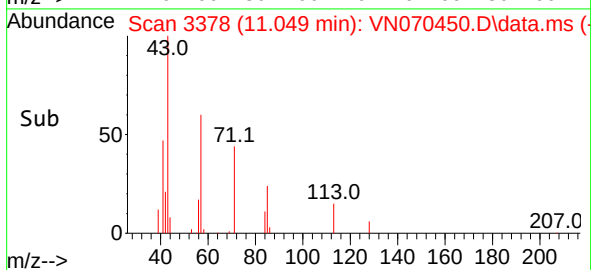
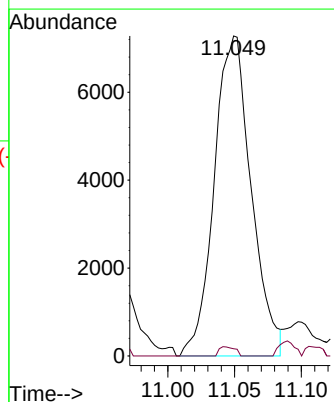
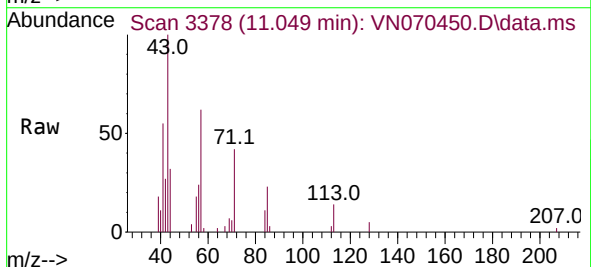


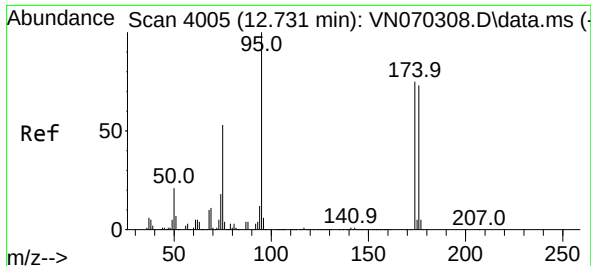

#62
4-Bromofluorobenzene
Concen: 65.660 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion: 95 Resp: 1198786
Ion Ratio Lower Upper
95 100
174 76.0 0.0 187.2
176 73.8 0.0 181.4

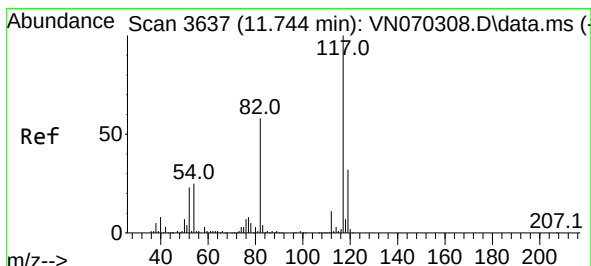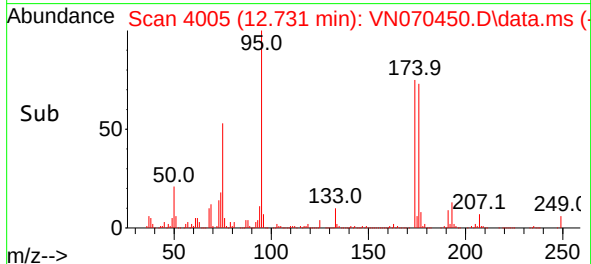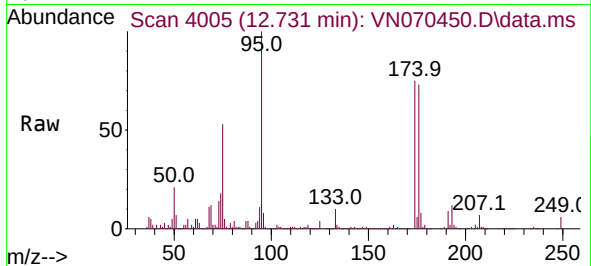

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.000 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion: 117 Resp: 2295495
Ion Ratio Lower Upper
117 100
82 58.8 42.4 63.6
119 32.0 25.4 38.2



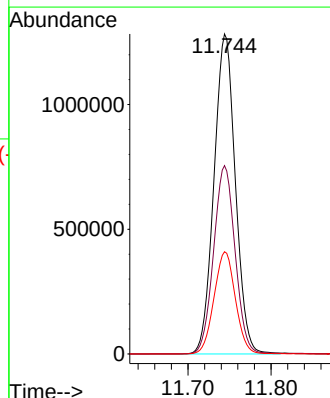
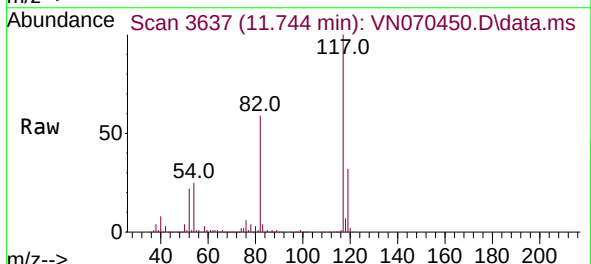




#67
Ethyl Benzene
Concen: 0.255 ug/l
RT: 11.843 min Scan# 3713
Delta R.T. 0.000 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion: 91 Resp: 22728
Ion Ratio Lower Upper
91 100
106 29.5 25.7 38.5

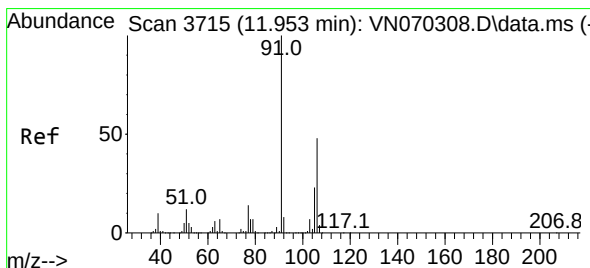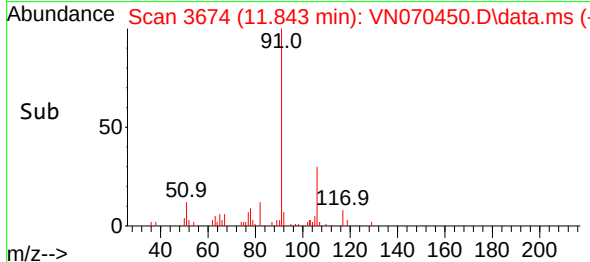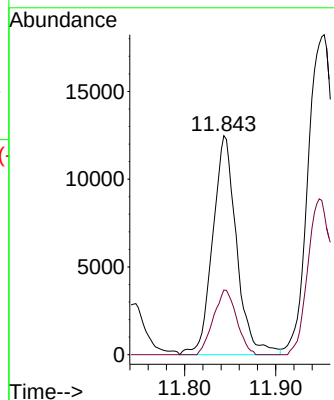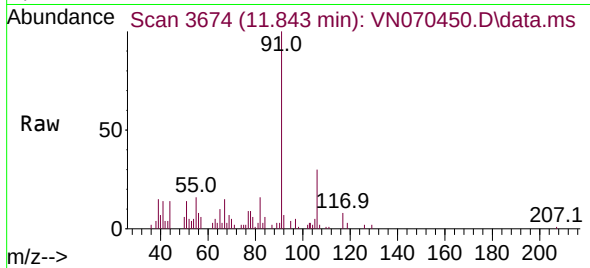

#68
m/p-Xylenes
Concen: 0.551 ug/l
RT: 11.948 min Scan# 3713
Delta R.T. -0.005 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion:106 Resp: 17903
Ion Ratio Lower Upper
106 100
91 208.0 160.6 240.8


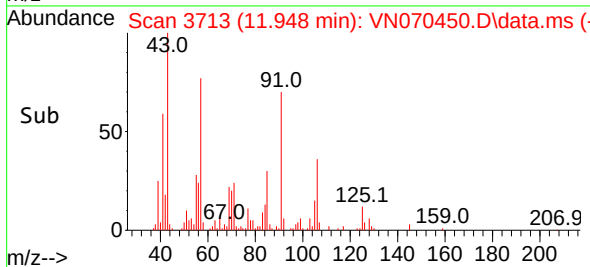
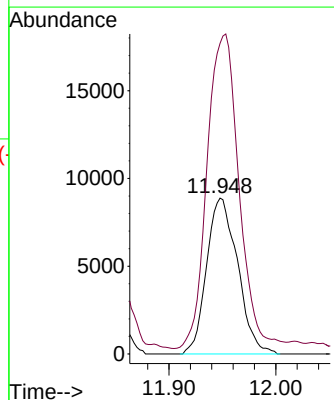
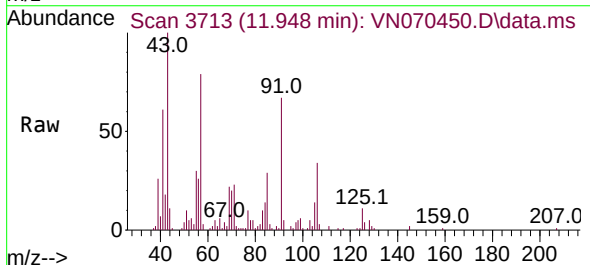




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.672 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VN070450.D
 Acq: 3 Jan 2022 20:40




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-2ME


Tgt Ion:152 Resp: 1172404
 Ion Ratio Lower Upper
 152 100
 115 60.7 27.5 82.5
 150 157.1 0.0 344.4

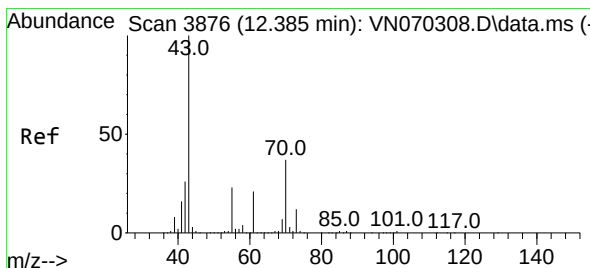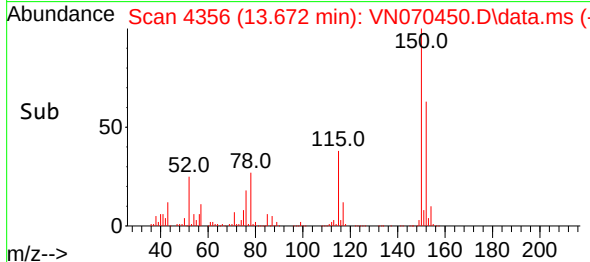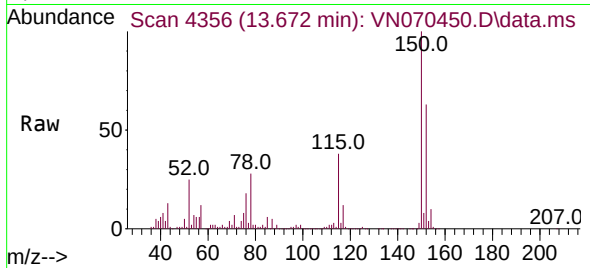

#74
 N-ethyl acetate
 Concen: 1.743 ug/l
 RT: 12.363 min Scan# 3868
 Delta R.T. -0.022 min
 Lab File: VN070450.D
 Acq: 3 Jan 2022 20:40

Tgt Ion: 43 Resp: 79806
 Ion Ratio Lower Upper
 43 100
 70 17.9 33.4 50.0#
 55 16.9 19.3 28.9#
 61 0.6 18.5 27.7#


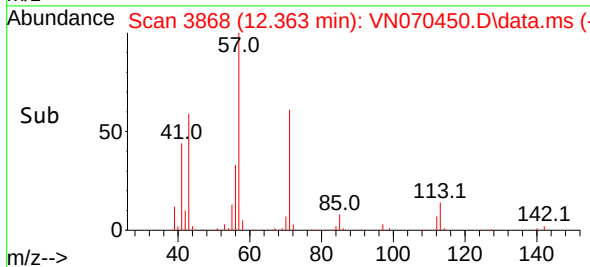

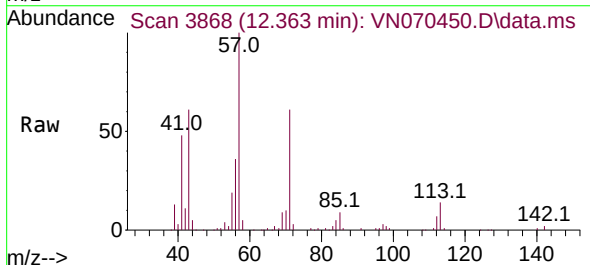




#75
1,1,2,2-Tetrachloroethane
Concen: 0.510 ug/l
RT: 12.806 min Scan# 4003
Delta R.T. -0.019 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion: 83 Resp: 2525
Ion Ratio Lower Upper
83 100
131 0.0 5.5 16.5#
85 128.8 32.4 97.2#

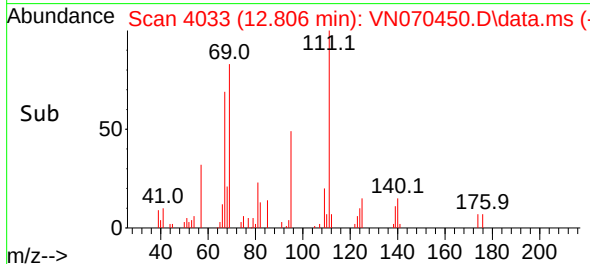

#76
1,2,3-Trichloropropane
Concen: 20.563 ug/l
RT: 12.728 min Scan# 4004
Delta R.T. -0.150 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion: 75 Resp: 654618
Ion Ratio Lower Upper
75 100
77 1.3 82.6 247.8#

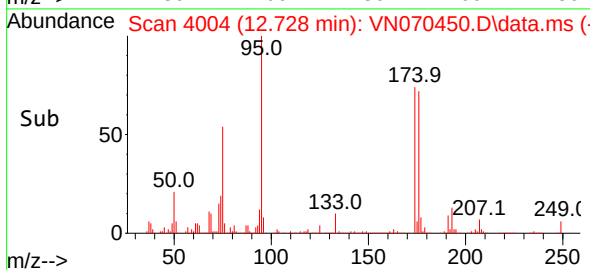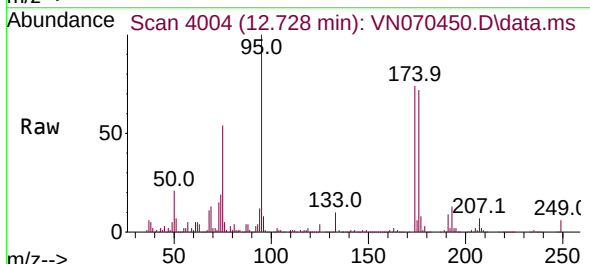



#80

1,3,5-Trimethylbenzene

Concen: 1.215 ug/l

RT: 13.058 min Scan# 41

Delta R.T. 0.000 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40

Instrument :

MSVOA_N

ClientSampleId :





SB-2ME

Tgt Ion:105 Resp: 106035

Ion Ratio Lower Upper

105 100

120 48.3 24.6 73.6

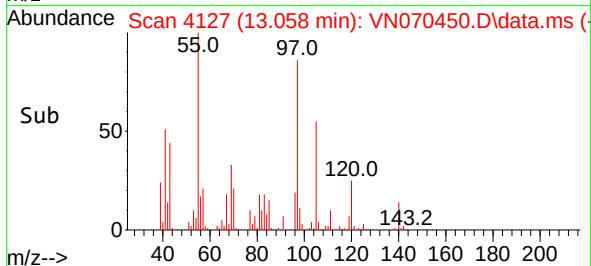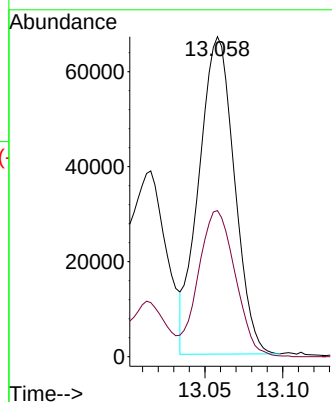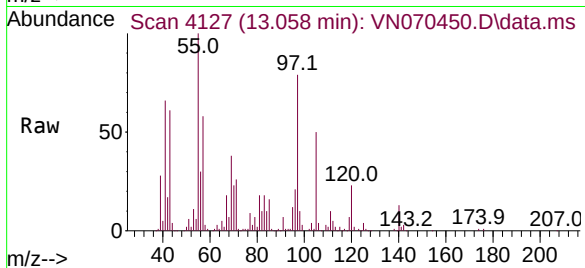

#81

trans-1,4-Dichloro-2-butene

Concen: 68.218 ug/l

RT: 12.728 min Scan# 4004

Delta R.T. 0.104 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40




Tgt Ion: 75 Resp: 654618


Ion Ratio Lower Upper

75 100

53 0.3 90.5 135.7#

89 1.1 38.2 57.4#


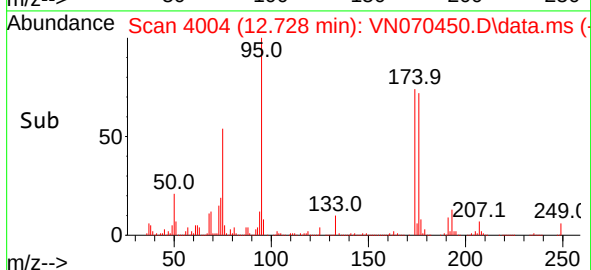

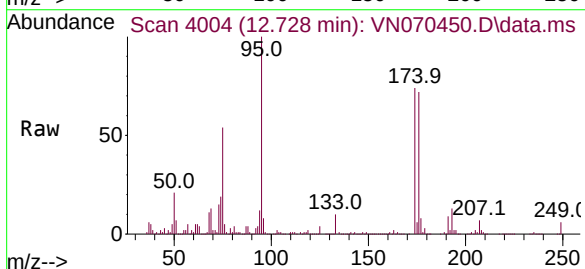




#83
 tert-Butylbenzene
 Concen: 0.419 ug/l
 RT: 13.366 min Scan# 41
 Delta R.T. 0.045 min
 Lab File: VN070450.D
 Acq: 3 Jan 2022 20:40




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-2ME


Tgt Ion:119 Resp: 32154
 Ion Ratio Lower Upper
 119 100
 91 85.0 31.5 94.5
 134 0.0 12.4 37.4#

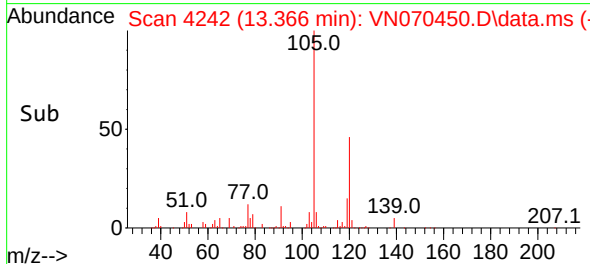

#84
 1,2,4-Trimethylbenzene
 Concen: 3.189 ug/l
 RT: 13.366 min Scan# 4242
 Delta R.T. 0.000 min
 Lab File: VN070450.D
 Acq: 3 Jan 2022 20:40

Tgt Ion:105 Resp: 267928
 Ion Ratio Lower Upper
 105 100
 120 44.4 22.8 68.4

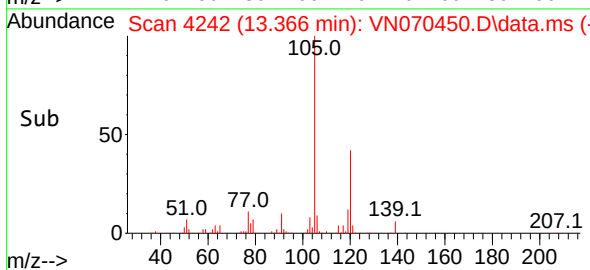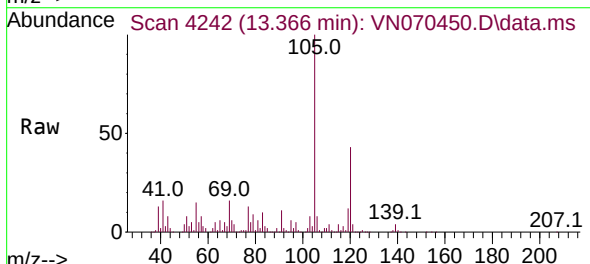



#85

sec-Butylbenzene

Concen: 1.829 ug/l

RT: 13.498 min Scan# 4291

Delta R.T. -0.003 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40

Instrument :

MSVOA_N

ClientSampleId :





SB-2ME

Tgt Ion:105 Resp: 190783

Ion Ratio Lower Upper

105 100

134 21.9 10.4 31.1

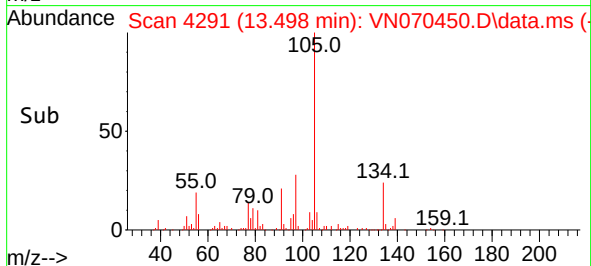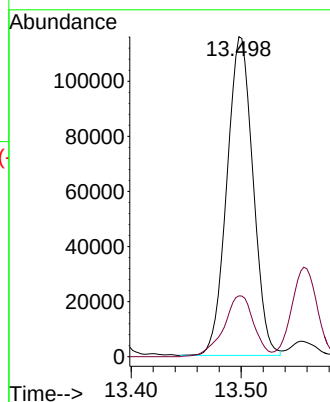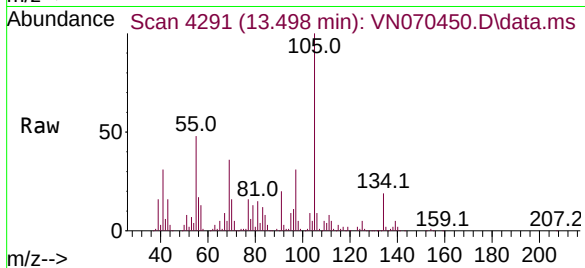

#86

p-Isopropyltoluene

Concen: 1.617 ug/l

RT: 13.613 min Scan# 4334

Delta R.T. 0.000 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40




Tgt Ion:119 Resp: 132465


Ion Ratio Lower Upper

119 100

134 24.7 13.6 40.7

91 23.7 11.4 34.1

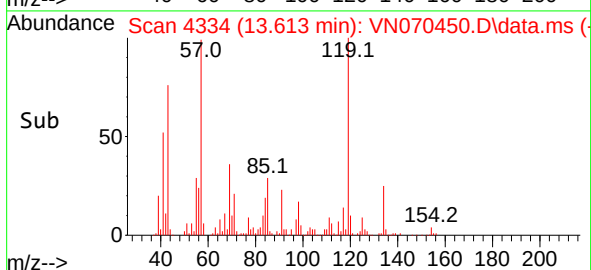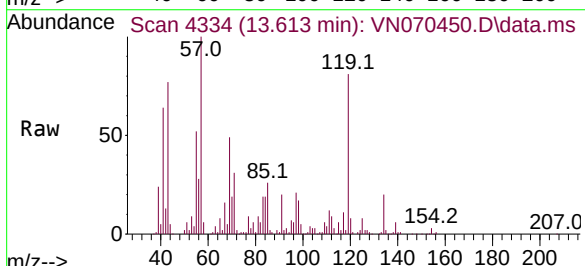



#89

n-Butylbenzene

Concen: 0.723 ug/l

RT: 13.906 min Scan# 4456

Delta R.T. -0.034 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40





Instrument :

MSVOA_N

ClientSampleId :

SB-2ME

Tgt Ion:	91	Resp:	49426
Ion	Ratio	Lower	Upper
91	100		
92	0.0	25.4	76.0#
134	386.0	13.6	40.8#

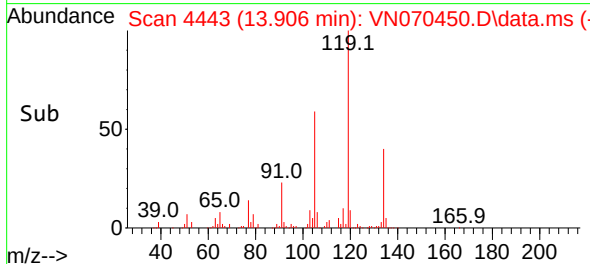

#90

Hexachloroethane

Concen: 3.455 ug/l




RT: 14.214 min Scan# 4558


Delta R.T. 0.005 min

Lab File: VN070450.D

Acq: 3 Jan 2022 20:40

Tgt Ion:	117	Resp:	49181
Ion	Ratio	Lower	Upper
117	100		
201	0.0	43.9	131.6#


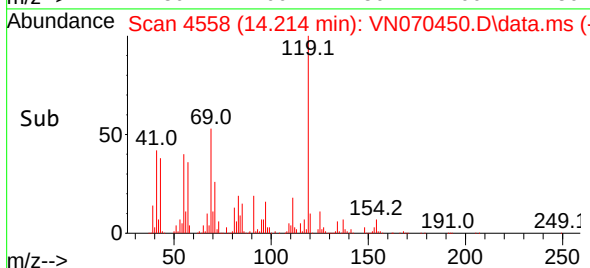
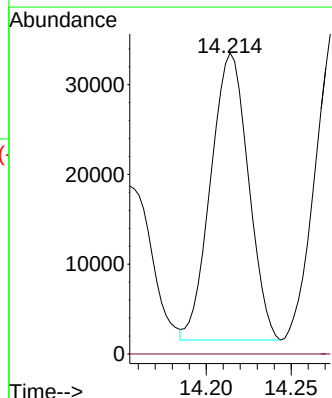
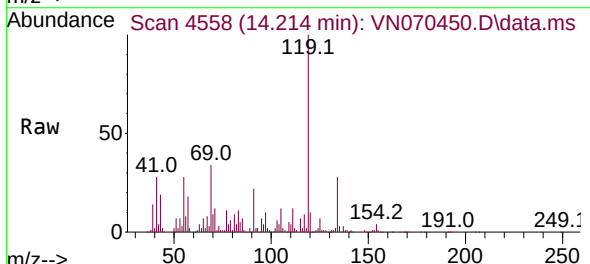




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.594 ug/l
RT: 14.619 min Scan# 41
Delta R.T. 0.019 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40




Instrument :
MSVOA_N
ClientSampleId :
SB-2ME


Tgt Ion: 75 Resp: 3745
Ion Ratio Lower Upper
75 100
155 29.6 46.9 140.7#
157 0.0 60.6 181.7#

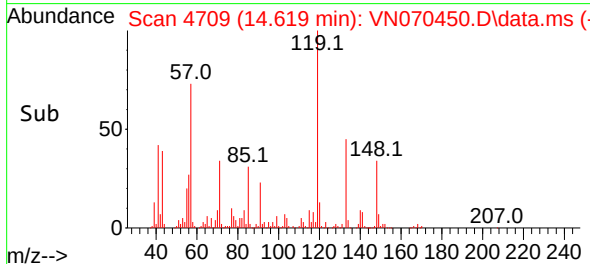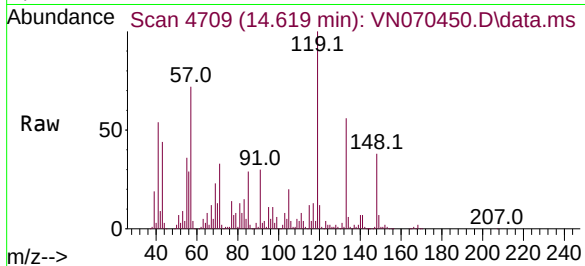

#95
Naphthalene
Concen: 2.697 ug/l
RT: 15.499 min Scan# 5037
Delta R.T. -0.005 min
Lab File: VN070450.D
Acq: 3 Jan 2022 20:40

Tgt Ion: 128 Resp: 49876
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 0.0 8.7 13.1#

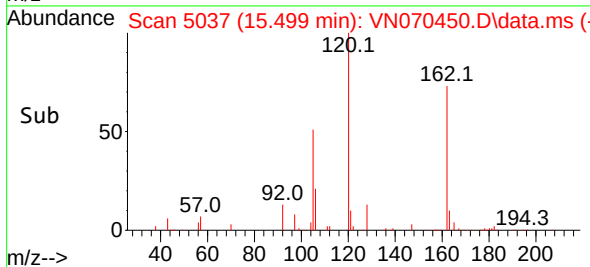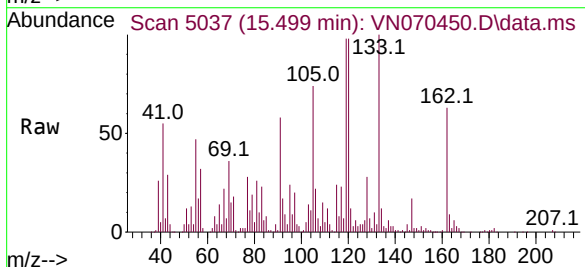

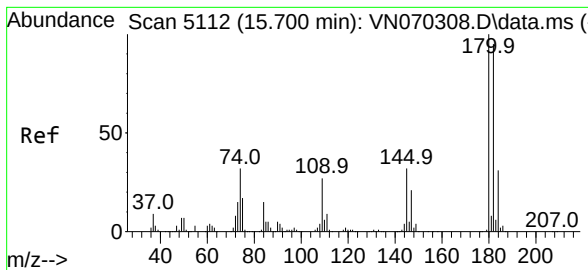

#96
 1,2,3-Trichlorobenzene
 Concen: 1.269 ug/l
 RT: 15.721 min Scan# 51
 Delta R.T. 0.021 min
 Lab File: VN070450.D
 Acq: 3 Jan 2022 20:40

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-2ME

Tgt Ion:180 Resp: 8330
 Ion Ratio Lower Upper
 180 100
 182 50.2 47.4 142.2
 145 0.0 15.0 45.1#

