

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010322\
 Data File : VN070435.D
 Acq On : 3 Jan 2022 14:20
 Operator : JC/MD
 Sample : M5234-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TB-12-23-21

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M

Title : SW846 8260

Signal : TIC: VN070435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.236	81	92	103	rBV2	110570	235923	4.70%	0.903%
2	4.291	841	858	878	rBV	24123	65941	1.31%	0.252%
3	4.583	941	967	994	rBV	94223	317053	6.32%	1.214%
4	5.095	1139	1158	1180	rBV4	35117	108335	2.16%	0.415%
5	8.021	2226	2249	2260	rBV3	621134	1498994	29.87%	5.739%
6	8.086	2260	2273	2298	rVB	1211894	2782221	55.44%	10.651%
7	8.437	2383	2404	2445	rBV	780393	1834742	36.56%	7.024%
8	8.965	2581	2601	2639	rBV	1850955	3858107	76.88%	14.770%
9	10.440	3131	3151	3188	rBV	2653721	5018286	100.00%	19.212%
10	11.744	3618	3637	3666	rBV	2373957	4356759	86.82%	16.679%
11	12.731	3986	4005	4033	rBV	1757829	3153378	62.84%	12.072%
12	13.672	4340	4356	4386	rBV	1663337	2890897	57.61%	11.067%




Sum of corrected areas: 26120636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010322\
Data File : VN070435.D
Acq On : 3 Jan 2022 14:20
Operator : JC/MD
Sample : M5234-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-12-23-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

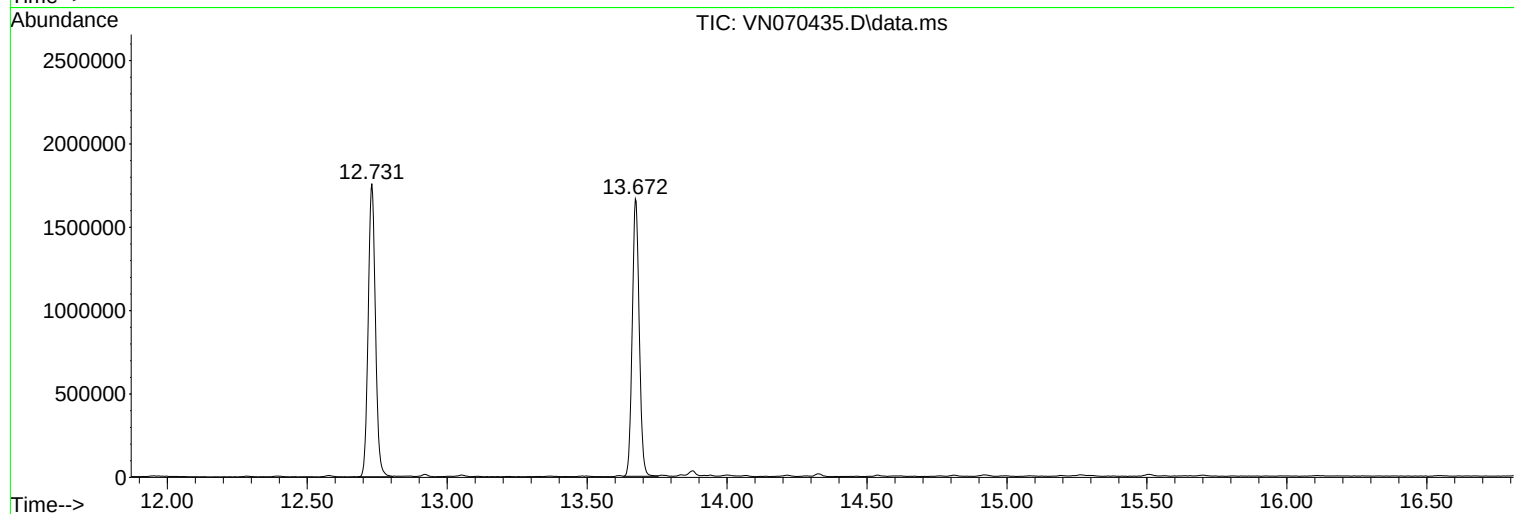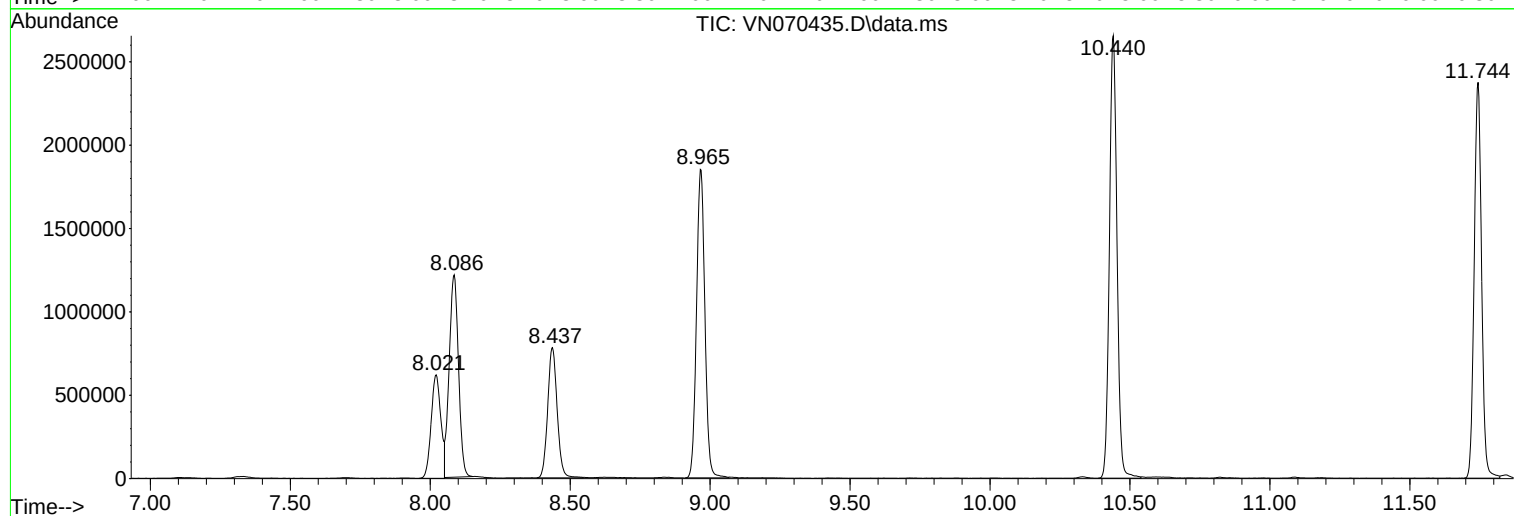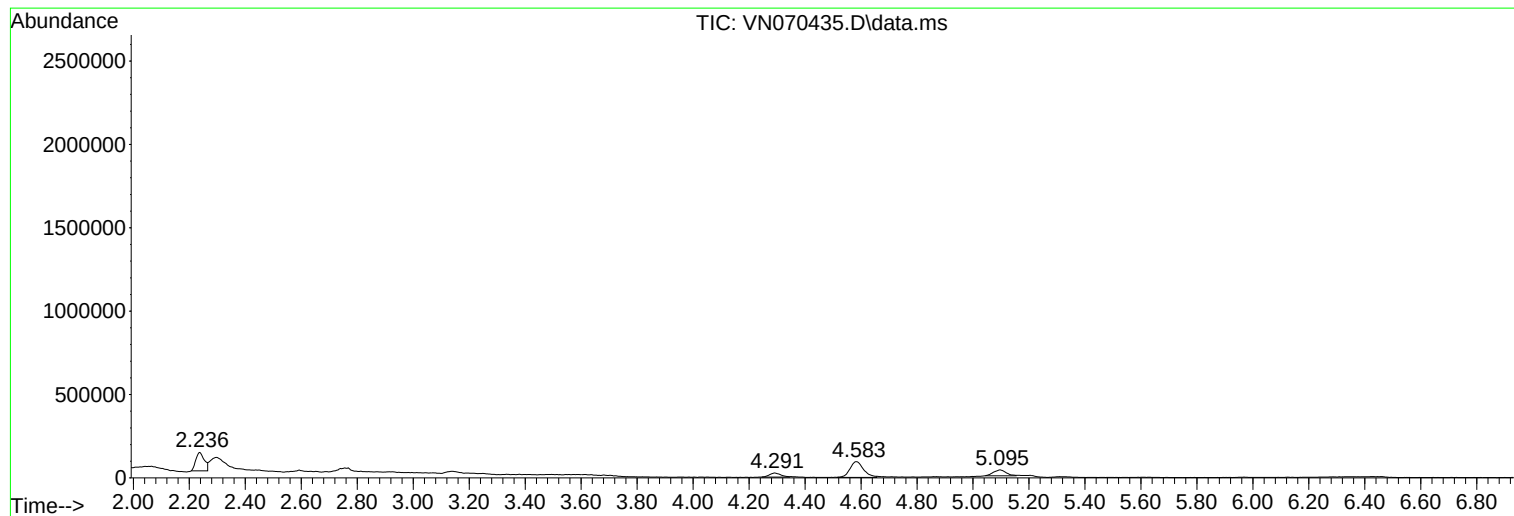

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010322\
Data File : VN070435.D
Acq On : 3 Jan 2022 14:20
Operator : JC/MD
Sample : M5234-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-12-23-21










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.583	5.70 ug/l	317053	Pentafluorobenzene	8.086

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			4-Penten-2-ol	86	C5H10O	000625-31-0	9
3			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	9
4			2-Pentanol	88	C5H12O	006032-29-7	9
5			(S)-(+)-2-Pentanol	88	C5H12O	026184-62-3	9

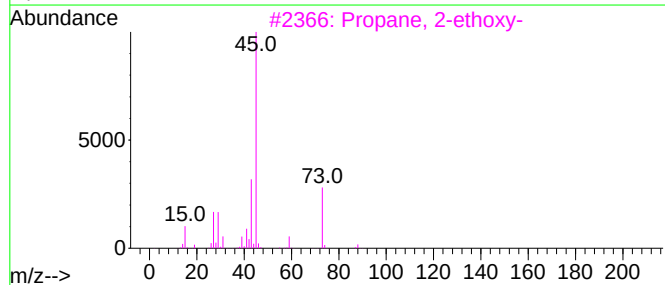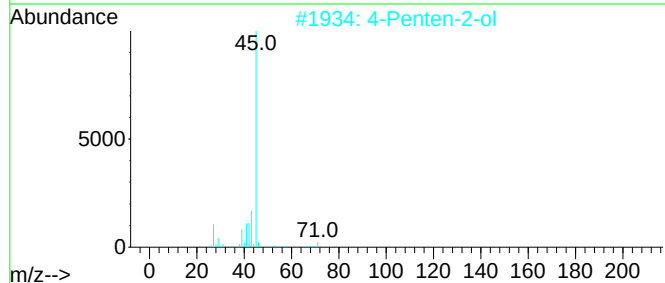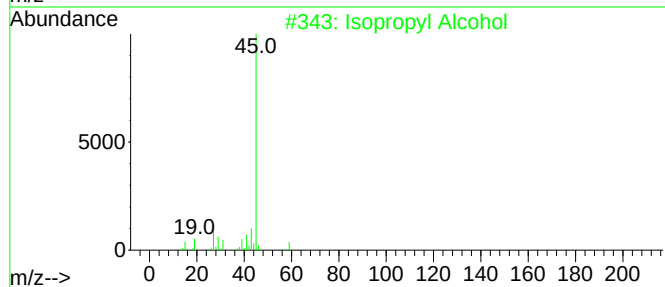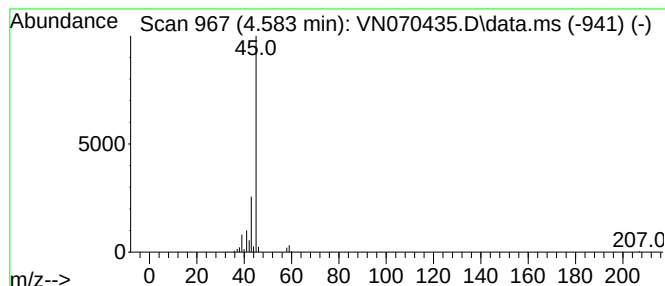

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010322\
Data File : VN070435.D
Acq On : 3 Jan 2022 14:20
Operator : JC/MD
Sample : M5234-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-12-23-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	4.583	5.7	ug/l	317053	1	8.086	2782220	50.0