



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010323\
Data File : VN076056.D
Acq On : 03 Jan 2023 11:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

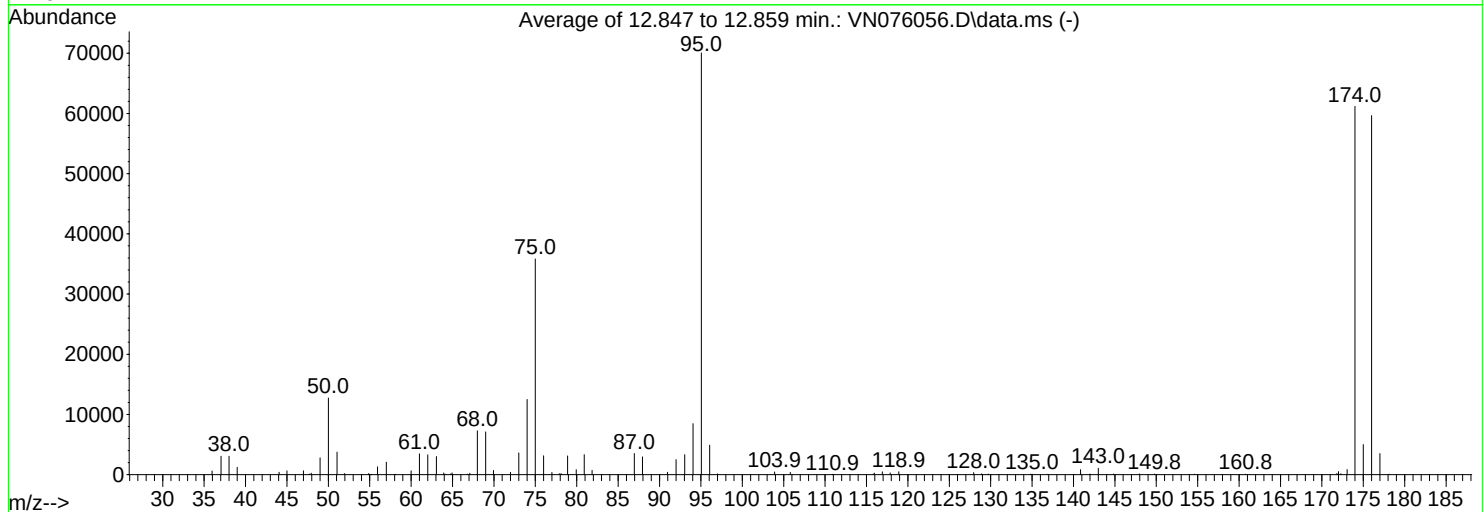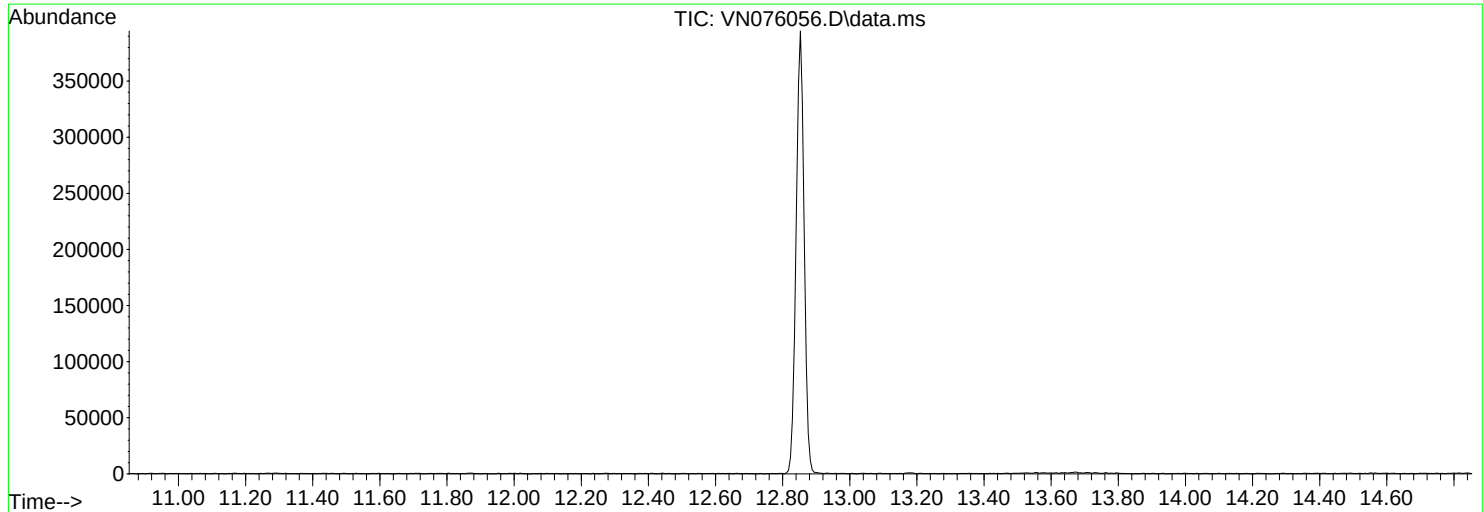

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	12736	PASS
75	95	30	60	51.2	35840	PASS
95	95	100	100	100.0	70067	PASS
96	95	5	9	7.0	4905	PASS
173	174	0.00	2	1.4	855	PASS
174	95	50	100	87.3	61173	PASS
175	174	5	9	8.2	4999	PASS
176	174	95	101	97.5	59645	PASS
177	176	5	9	5.9	3503	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	618	51.05	3752	63.05	3003	73.00	3621
37.05	3063	51.95	189	63.95	300	74.00	1249
38.00	3063	54.85	157	64.20	75	75.00	3584
39.00	1231	55.00	85	64.80	146	76.00	313
44.05	400	55.20	61	64.95	286	77.00	377
45.00	651	55.95	1315	66.80	92	77.90	175
47.00	631	57.00	2070	67.10	236	78.10	178
47.70	105	58.10	52	68.00	7280	78.90	3106
47.95	234	60.00	651	69.00	7104	79.95	836
49.00	2798	61.00	3468	69.95	682	80.90	3313
50.00	12736	62.00	3293	72.00	370	81.85	725

Average of 12.847 to 12.859 min.: VN076056.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	3509	105.80	366	130.90	55	160.80	76
87.95	2966	110.90	51	134.80	85	171.80	178
90.95	398	115.80	109	135.00	88	172.00	515
92.00	2492	115.95	276	136.90	71	172.30	171
93.05	3338	116.90	490	140.85	830	173.05	855
94.05	8486	117.85	296	142.00	115	174.00	61173
95.05	70067	118.90	495	143.00	1073	175.00	4999
96.05	4905	127.95	336	144.85	122	176.00	59645
97.00	146	128.90	133	147.95	136	177.00	3503
103.90	459	129.70	116	149.80	122	178.10	74
105.00	66	130.00	55	154.60	82		

Instrument :

MSVOA_N

ClientSampleId :

BFB