
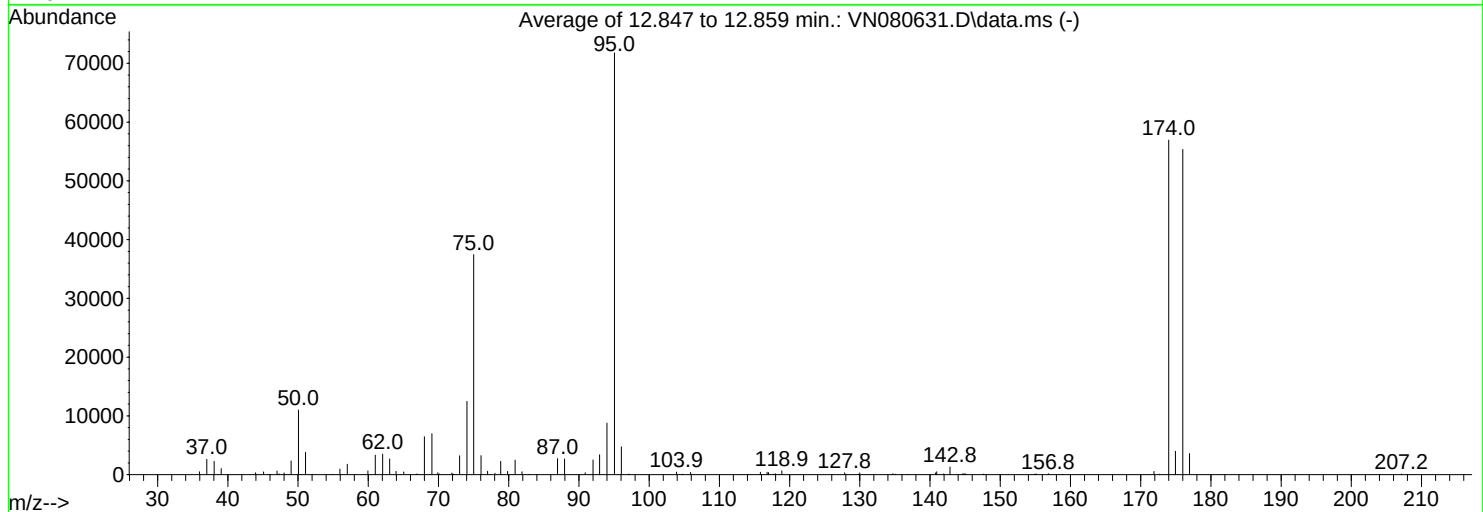


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010324\
Data File : VN080631.D
Acq On : 03 Jan 2024 10:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122723W.M
Title : SW846 8260
Last Update : Thu Dec 28 03:07:01 2023

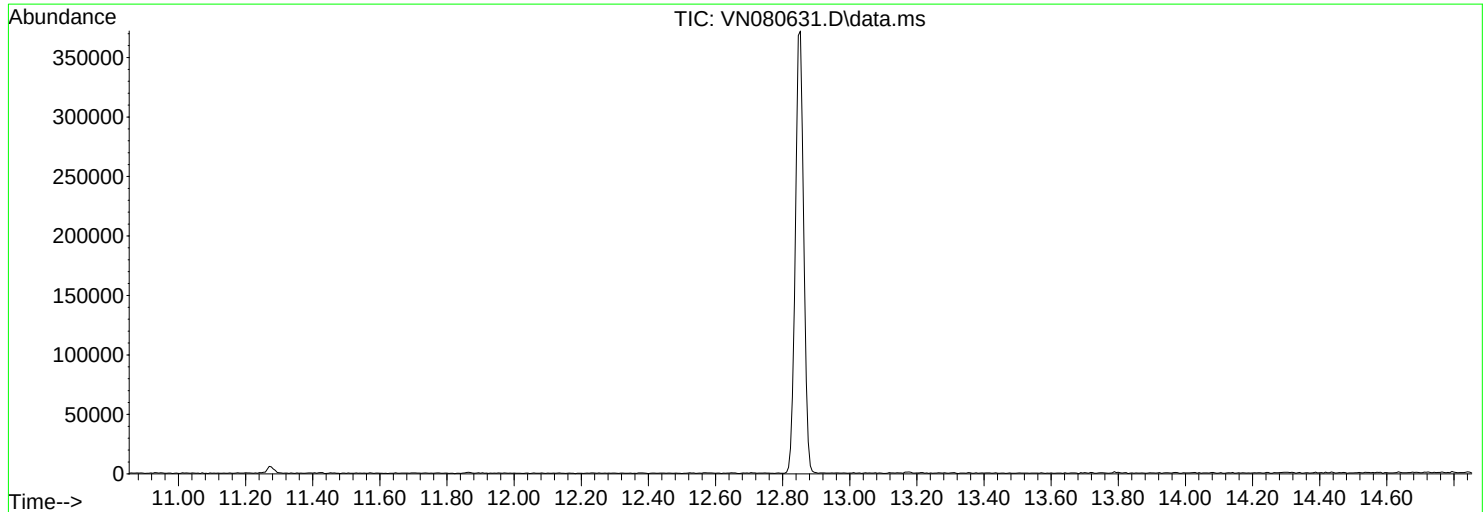

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	10998	PASS
75	95	30	60	52.2	37440	PASS
95	95	100	100	100.0	71787	PASS
96	95	5	9	6.6	4754	PASS
173	174	0.00	2	0.2	98	PASS
174	95	50	100	79.3	56941	PASS
175	174	5	9	7.0	3976	PASS
176	174	95	101	97.2	55363	PASS
177	176	5	9	6.5	3610	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	504	48.00	289	63.05	2671	74.05	1247
37.00	2605	49.00	2357	63.95	567	75.00	3744
38.05	2264	50.05	10998	65.05	457	76.05	324
39.05	1051	51.05	3803	66.95	147	77.00	58
39.90	34	52.10	98	68.00	6450	78.05	248
43.95	322	54.90	60	69.05	6969	78.85	2272
45.10	471	55.95	959	69.90	332	79.85	549
45.80	54	57.00	1761	70.10	141	80.90	2480
46.10	53	59.95	628	71.90	279	81.90	507
47.00	622	61.00	3318	72.10	100	82.90	69
47.30	151	62.05	3493	73.00	3215	86.95	2737

Average of 12.847 to 12.859 min.: VN080631.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	2680	115.85	405	136.80	58	156.85	161
90.90	319	116.80	412	140.80	311	158.90	53
92.00	2512	117.00	351	140.95	491	171.90	549
92.95	3385	117.70	81	141.95	145	172.70	98
94.00	8756	117.95	173	142.85	1318	174.00	56941
95.05	71787	118.90	658	144.70	196	174.95	3976
96.05	4754	127.85	335	144.90	129	176.00	55363
97.10	101	129.80	81	145.10	128	176.95	3610
103.90	448	130.00	288	147.65	123	207.15	117
104.80	80	134.70	171	154.90	76		
105.90	378	135.10	72	155.10	141		

Instrument :

MSVOA_N

ClientSampleId :

BFB