

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010422\
 Data File : VN070454.D
 Acq On : 4 Jan 2022 11:00
 Operator : JC/MD
 Sample : VN0104MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0104MBL01

Quant Time: Jan 05 03:12:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.083	168	1108291	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.965	114	2122604	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.741	117	2498963	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.672	152	1052685	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	816855	51.261	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	102.520%
35) Dibromofluoromethane	8.021	113	618303	48.144	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.280%
50) Toluene-d8	10.440	98	2803708	53.440	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	106.880%
62) 4-Bromofluorobenzene	12.728	95	1265138	66.766	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	133.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010422\
Data File : VN070454.D
Acq On : 4 Jan 2022 11:00
Operator : JC/MD
Sample : VN0104MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0104MBL01

Quant Time: Jan 05 03:12:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration




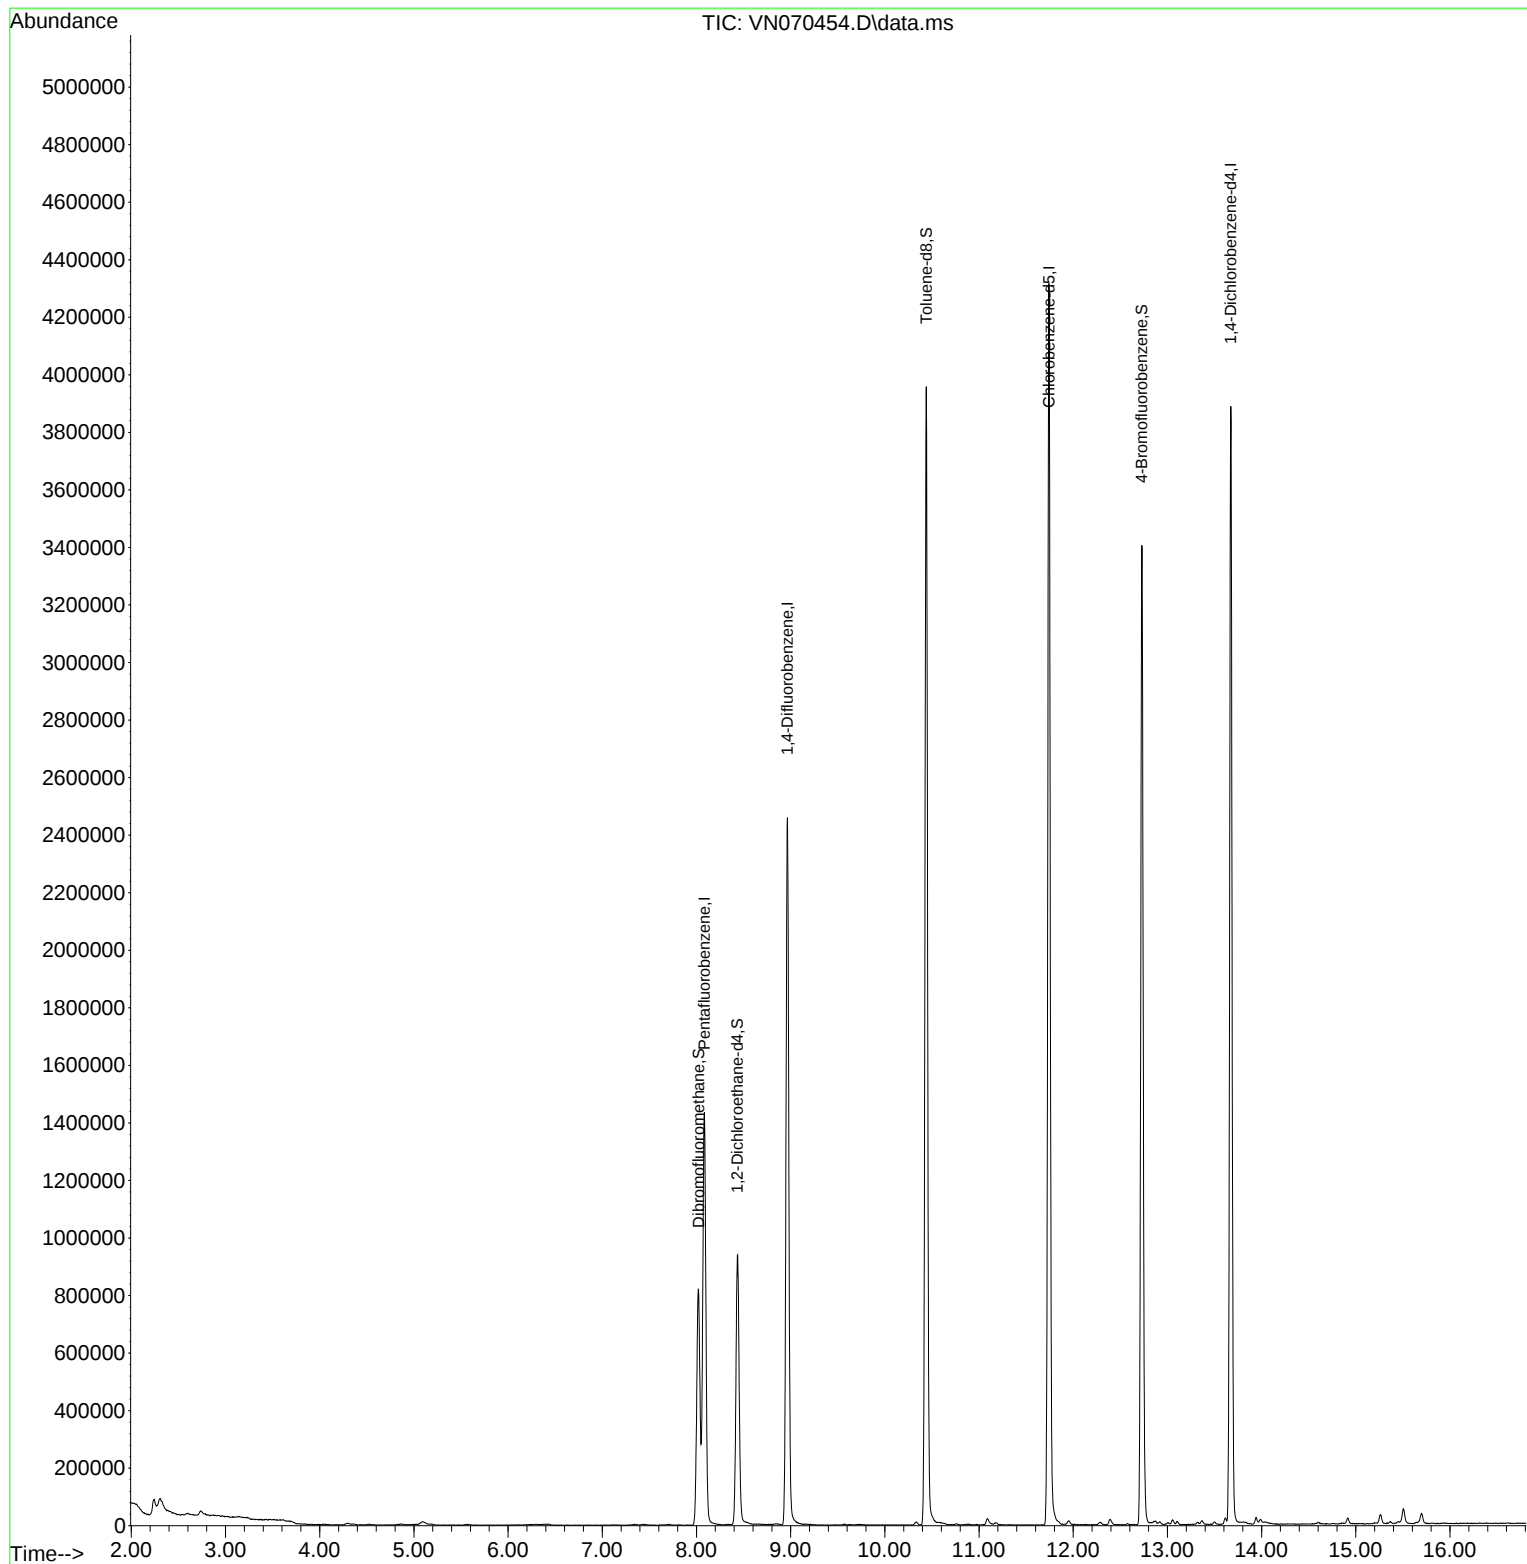


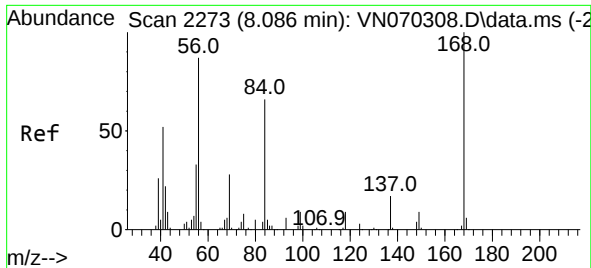

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.003 min
Lab File: VN070454.D
Acq: 4 Jan 2022 11:00




Instrument :
MSVOA_N
ClientSampleId :
VN0104MBL01


Tgt Ion:168 Resp: 1108291
Ion Ratio Lower Upper
168 100
99 58.7 41.3 61.9

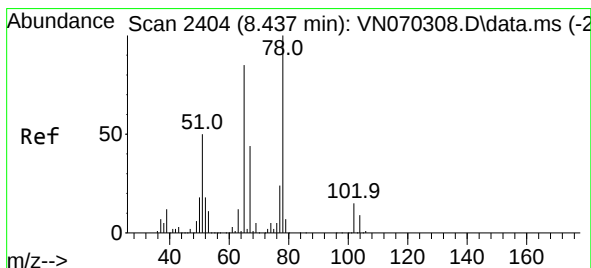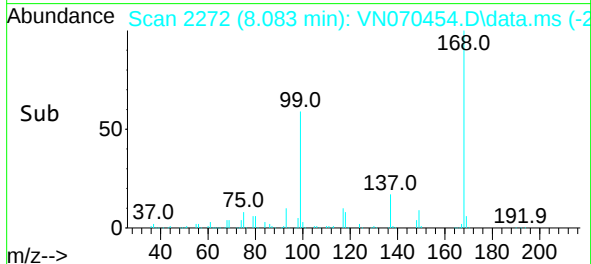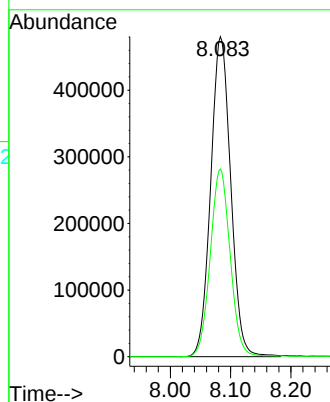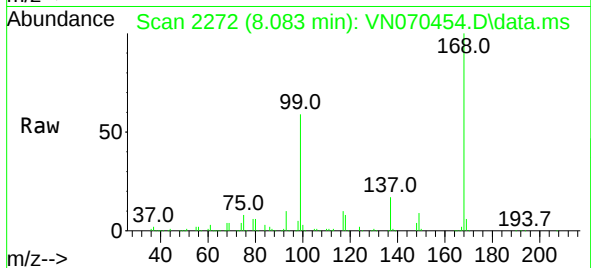

#33
1,2-Dichloroethane-d4
Concen: 51.261 ug/l
RT: 8.434 min Scan# 2403
Delta R.T. -0.003 min
Lab File: VN070454.D
Acq: 4 Jan 2022 11:00

Tgt Ion: 65 Resp: 816855
Ion Ratio Lower Upper
65 100
67 52.5 0.0 103.0

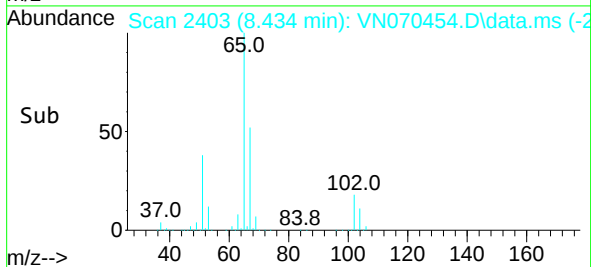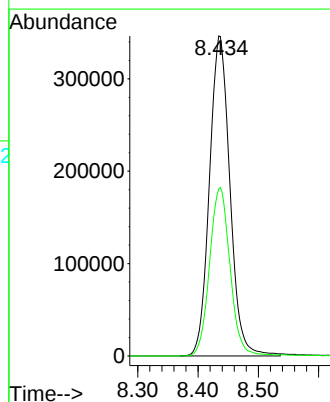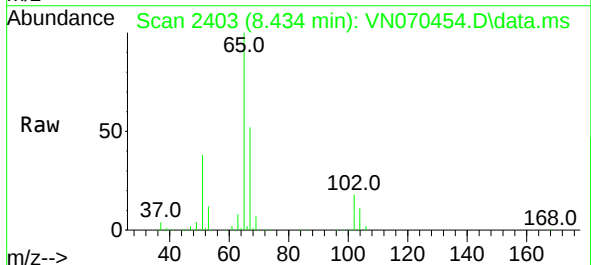

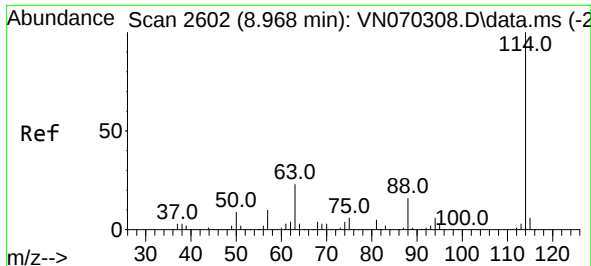

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.965 min Scan# 2

Delta R.T. -0.003 min

Lab File: VN070454.D

Acq: 4 Jan 2022 11:00

Instrument :

MSVOA_N

ClientSampleId :

VN0104MBL01





Tgt Ion:114 Resp: 2122604

Ion Ratio Lower Upper

114 100

63 23.4 0.0 37.8

88 16.3 0.0 27.4

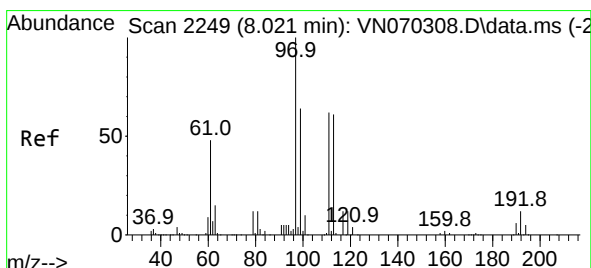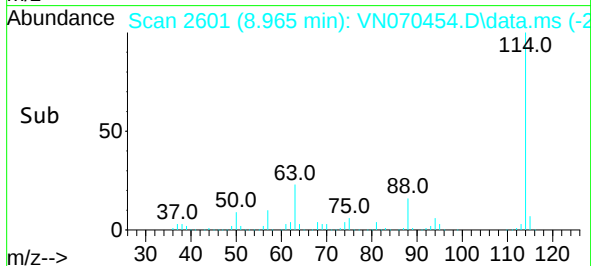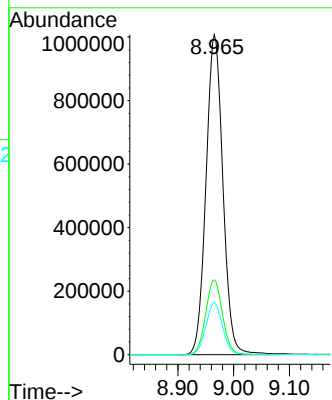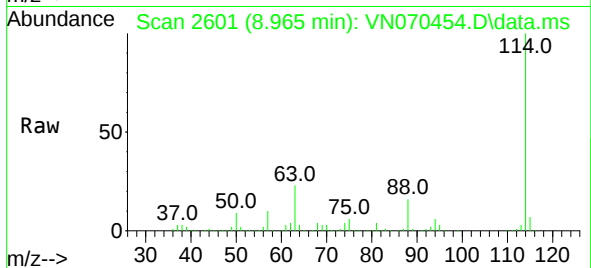

#35

Dibromofluoromethane

Concen: 48.144 ug/l

RT: 8.021 min Scan# 2249

Delta R.T. 0.000 min

Lab File: VN070454.D

Acq: 4 Jan 2022 11:00




Tgt Ion:113 Resp: 618303


Ion Ratio Lower Upper

113 100

111 102.5 82.2 123.2

192 19.2 16.9 25.3


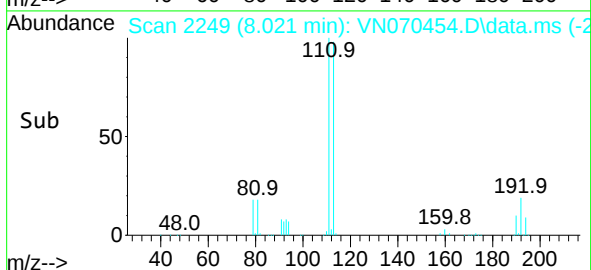
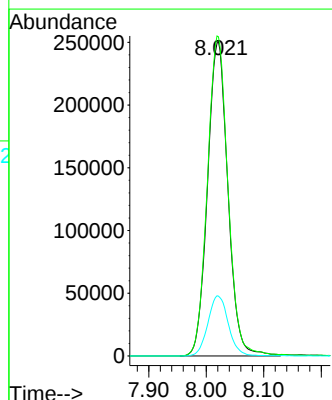
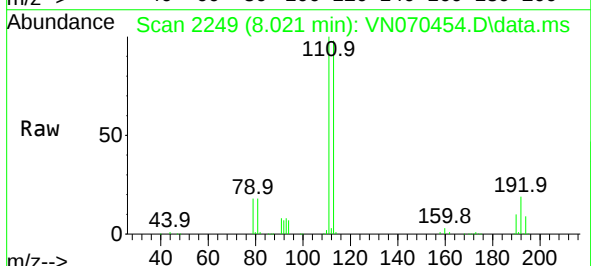


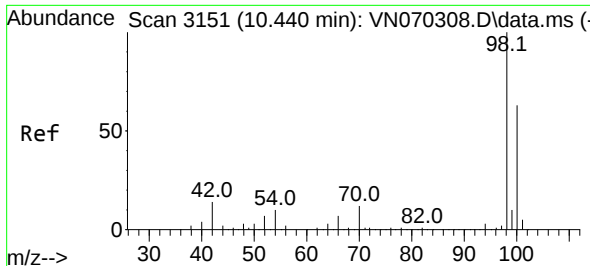

#50
Toluene-d8
Concen: 53.440 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. 0.000 min
Lab File: VN070454.D
Acq: 4 Jan 2022 11:00




Instrument :
MSVOA_N
ClientSampleId :
VN0104MBL01


Tgt Ion: 98 Resp: 2803708
Ion Ratio Lower Upper
98 100
100 64.0 50.4 75.6

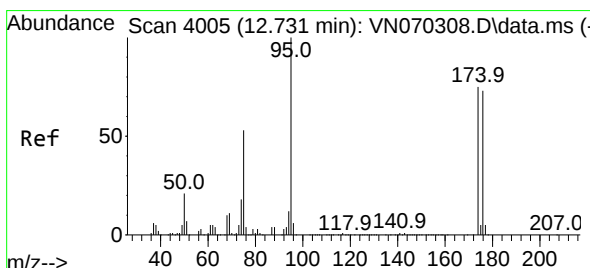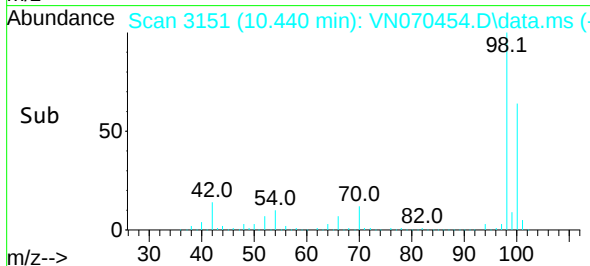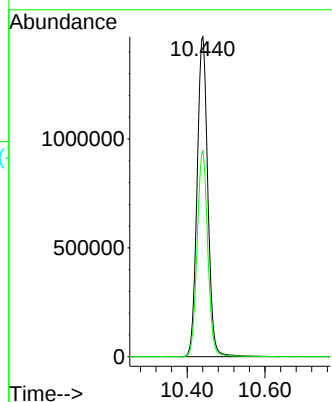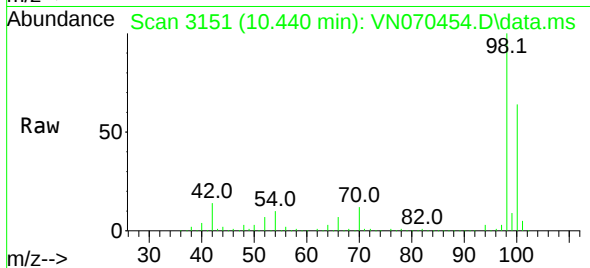

#62
4-Bromofluorobenzene
Concen: 66.766 ug/l
RT: 12.728 min Scan# 4004
Delta R.T. -0.003 min
Lab File: VN070454.D
Acq: 4 Jan 2022 11:00

Tgt Ion: 95 Resp: 1265138
Ion Ratio Lower Upper
95 100
174 75.3 0.0 187.2
176 72.8 0.0 181.4

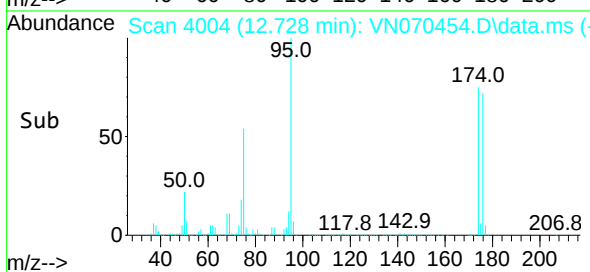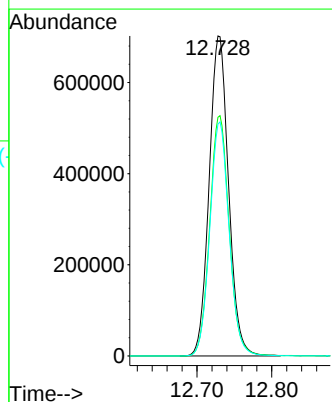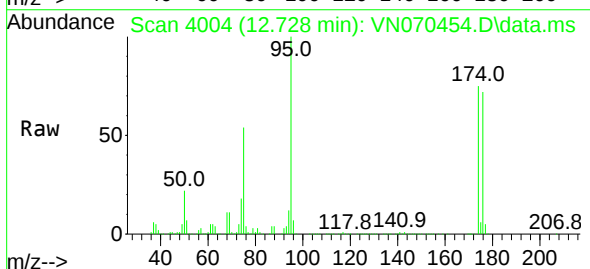

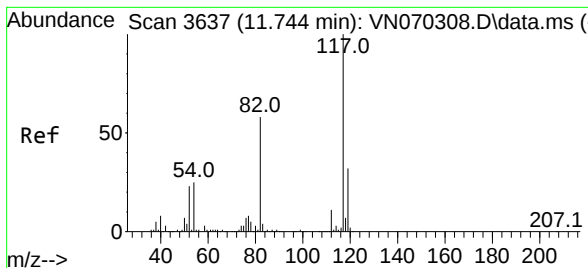

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.741 min Scan# 3636

Delta R.T. -0.003 min

Lab File: VN070454.D

Acq: 4 Jan 2022 11:00

Instrument :

MSVOA_N

ClientSampleId :

VN0104MBL01





Tgt Ion:117 Resp: 2498963

Ion Ratio Lower Upper

117 100

82 59.5 42.4 63.6

119 31.8 25.4 38.2

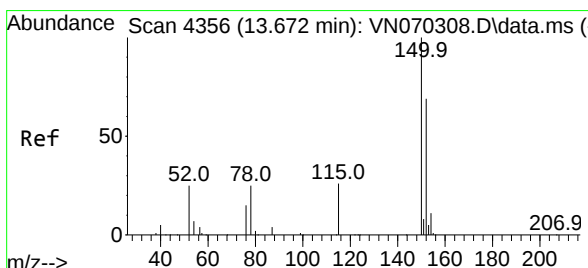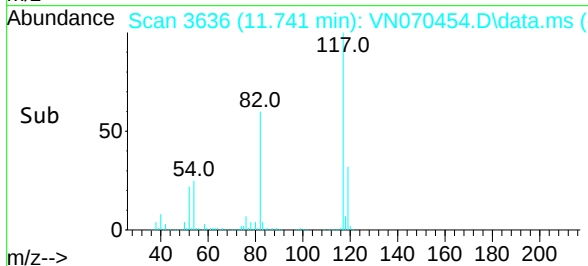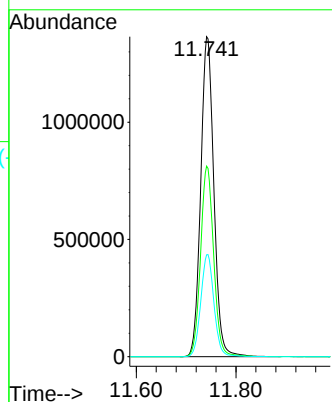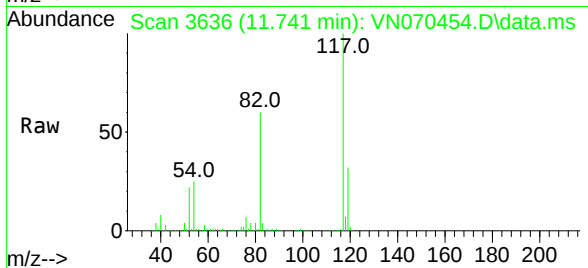

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.672 min Scan# 4356

Delta R.T. 0.000 min

Lab File: VN070454.D

Acq: 4 Jan 2022 11:00

Tgt Ion:152 Resp: 1052685

Ion Ratio Lower Upper

152 100

115 61.0 27.5 82.5

150 157.9 0.0 344.4

