

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010422\
 Data File : VN070469.D
 Acq On : 4 Jan 2022 17:33
 Operator : JC/MD
 Sample : M5251-05
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-6D

Manual Integrations
 APPROVED

Reviewed By : John Carlone 01/05/2022
 Supervised By : Mahesh Dadoda 01/05/2022

Quant Time: Jan 05 03:19:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.083	168	947656	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.965	114	1626098	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1403673	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.672	152	472625	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	677295	49.708	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.420%		
35) Dibromofluoromethane	8.019	113	471009	47.873	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	95.740%		
50) Toluene-d8	10.441	98	1888763	46.993	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	93.980%		
62) 4-Bromofluorobenzene	12.731	95	653151	44.994	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	89.980%		
Target Compounds					Qvalue	
9) 1,1,2-Trichlorotrifluo...	4.213	101	5155m	0.526	ug/l	
11) Tert butyl alcohol	5.377	59	24185	10.660	ug/l #	71
12) 1,1-Dichloroethene	4.178	96	4223	0.438	ug/l	94
16) Acetone	4.288	43	42671	4.824	ug/l	91
19) Methyl tert-butyl Ether	5.618	73	247635	6.909	ug/l #	59
22) Diisopropyl ether	6.503	45	18628	0.437	ug/l #	86
25) 2-Butanone	7.346	43	11874	1.066	ug/l #	81
27) cis-1,2-Dichloroethene	7.324	96	3528	0.289	ug/l	50
29) Tetrahydrofuran	7.692	42	7363m	1.108	ug/l	
30) Chloroform	7.820	83	10422	0.489	ug/l	100
40) Benzene	8.459	78	89155	1.787	ug/l	96
44) Trichloroethene	9.215	130	20541	1.733	ug/l	97
59) 2-Hexanone	11.087	43	17693	1.161	ug/l	83
64) Tetrachloroethene	10.972	164	3087	0.304	ug/l	96
67) Ethyl Benzene	11.846	91	12919	0.237	ug/l	92
68) m/p-Xylenes	11.951	106	13946	0.702	ug/l	81
74) N-amyl acetate	12.390	43	10455	0.567	ug/l #	87
84) 1,2,4-Trimethylbenzene	13.367	105	25042	0.739	ug/l	96
85) sec-Butylbenzene	13.501	105	11451	0.272	ug/l	98
86) p-Isopropyltoluene	13.619	119	6888	0.209	ug/l	93
87) 1,3-Dichlorobenzene	13.619	146	5332	0.316	ug/l	97
88) 1,4-Dichlorobenzene	13.694	146	7088m	0.426	ug/l	
89) n-Butylbenzene	13.943	91	11456	0.416	ug/l	95
91) 1,2-Dichlorobenzene	13.986	146	5561	0.336	ug/l	97
93) 1,2,4-Trichlorobenzene	15.263	180	7844	1.007	ug/l	94
96) 1,2,3-Trichlorobenzene	15.700	180	9491	2.078	ug/l	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010422\
Data File : VN070469.D
Acq On : 4 Jan 2022 17:33
Operator : JC/MD
Sample : M5251-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
MW-6D

Manual Integrations
APPROVED

Reviewed By : John Carlone 01/05/2022
Supervised By : Mahesh Dadoda 01/05/2022


Quant Time: Jan 05 03:19:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration

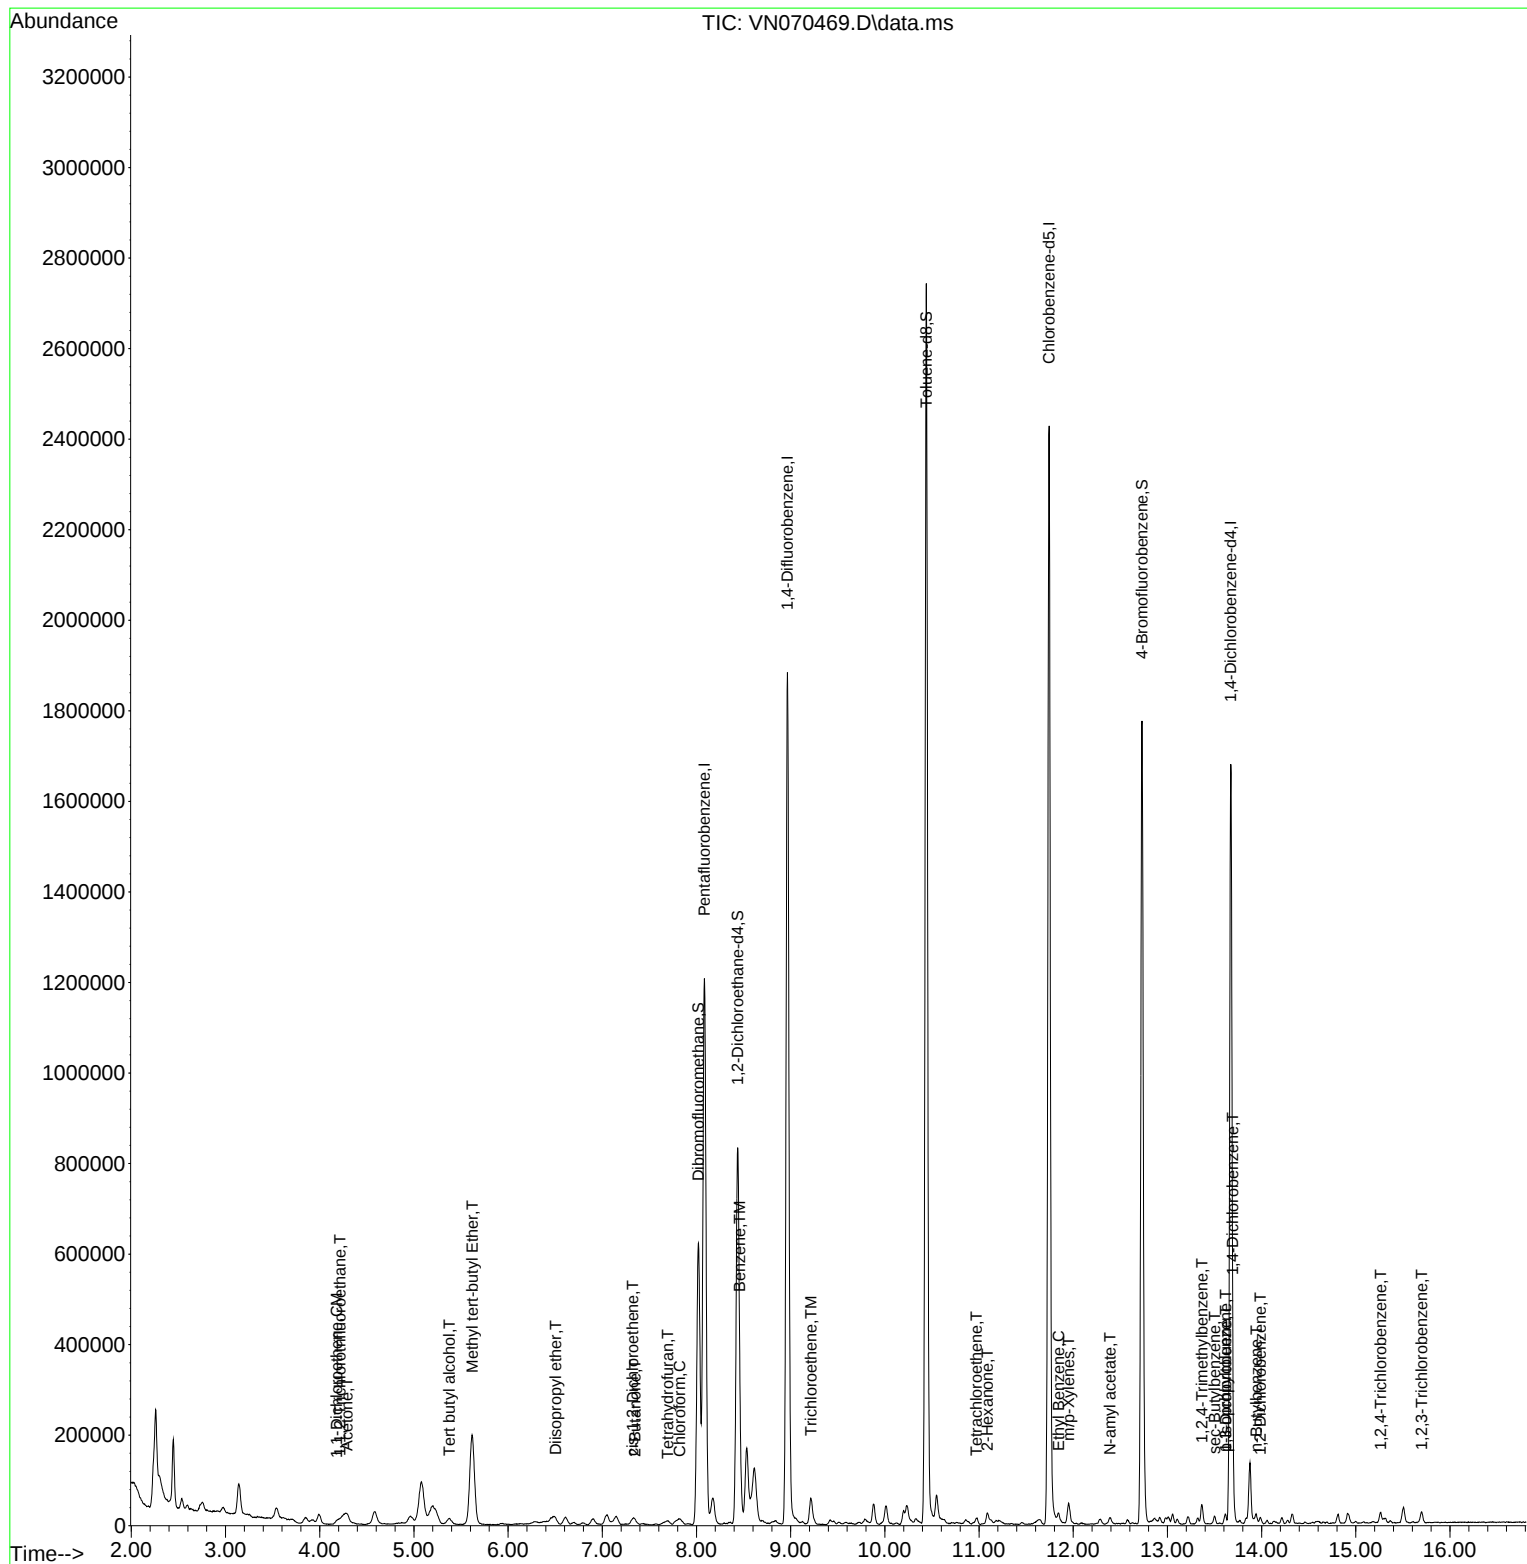



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.003 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D




Tgt Ion:168 Resp: 947650
Ion Ratio Lower Upper
168 100
99 58.3 41.3 61.9

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

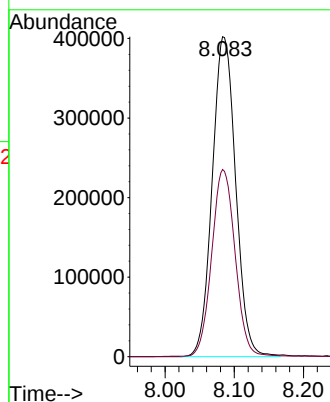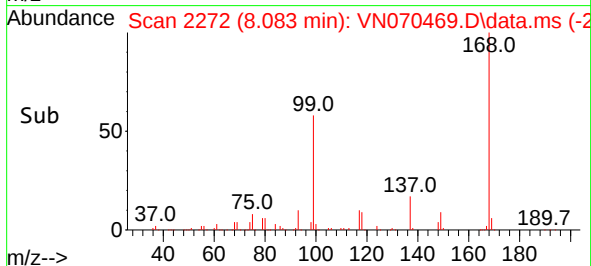


#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.526 ug/l m
RT: 4.213 min Scan# 829
Delta R.T. 0.003 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

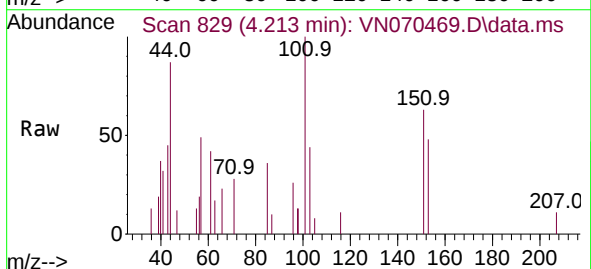


Tgt Ion:101 Resp: 5155
Ion Ratio Lower Upper
101 100
85 24.1 37.2 55.8#
151 69.3 65.9 98.9

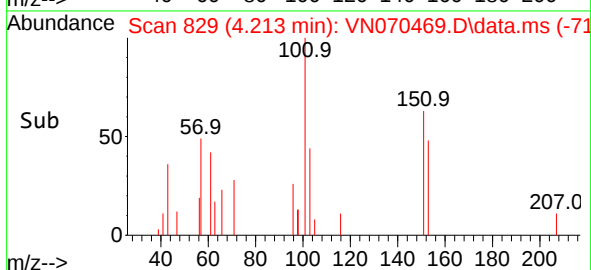

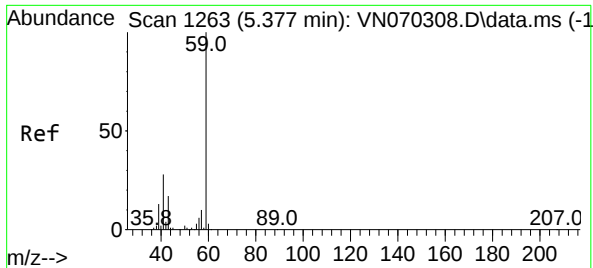

#11
Tert butyl alcohol
Concen: 10.660 ug/l
RT: 5.377 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D

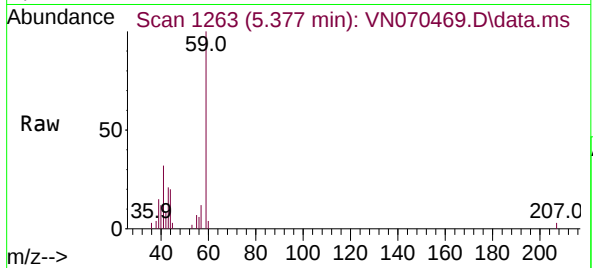


Tgt Ion: 59 Resp: 2418
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

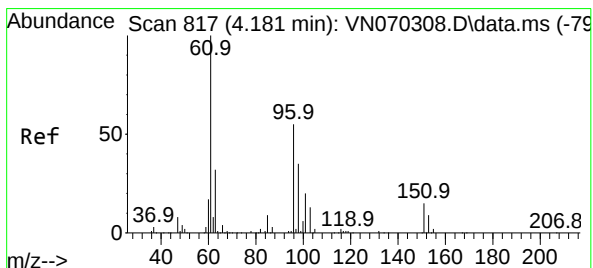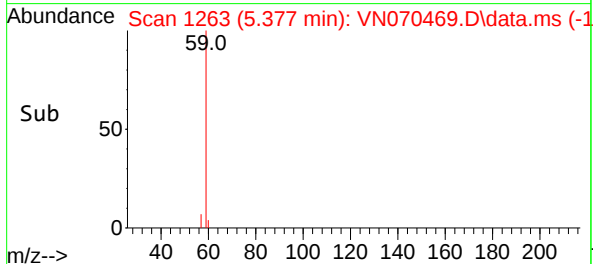


#12
1,1-Dichloroethene
Concen: 0.438 ug/l
RT: 4.178 min Scan# 816
Delta R.T. -0.003 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

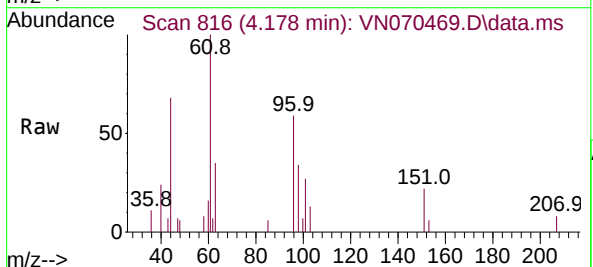


Tgt Ion: 96 Resp: 4223
Ion Ratio Lower Upper
96 100
61 170.0 131.0 196.6
98 58.2 52.4 78.6

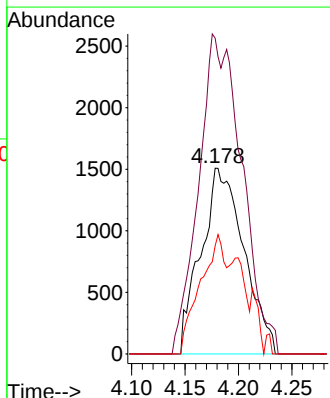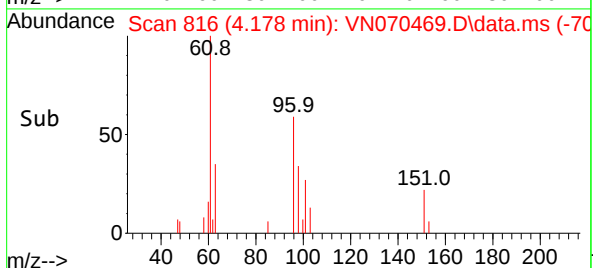

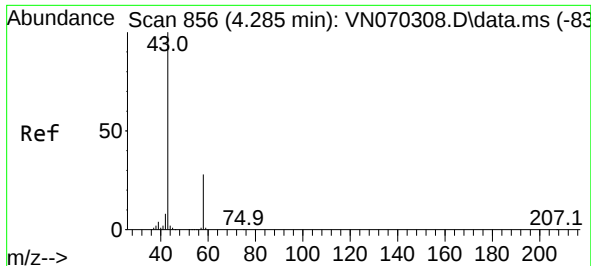

#16
Acetone
Concen: 4.824 ug/l
RT: 4.288 min Scan# 857
Delta R.T. 0.003 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D

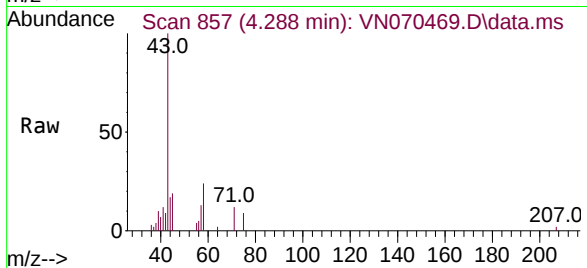


Tgt Ion: 43 Resp: 4267
Ion Ratio Lower Upper
43 100
58 24.2 23.1 34.7

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

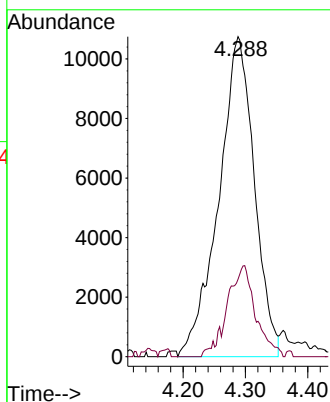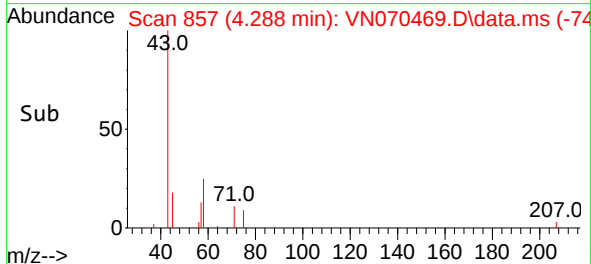


#19
Methyl tert-butyl Ether
Concen: 6.909 ug/l
RT: 5.618 min Scan# 1353
Delta R.T. 0.002 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

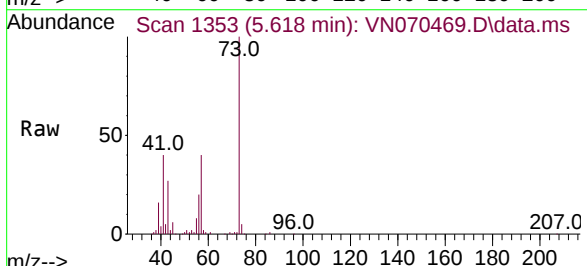

Tgt Ion: 73 Resp: 247635
Ion Ratio Lower Upper
73 100
57 40.1 16.8 25.2#

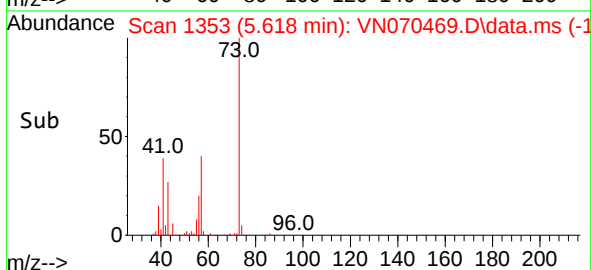

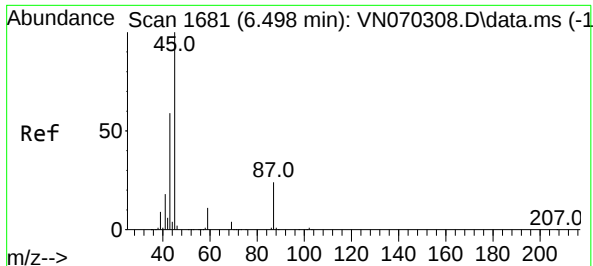

#22

Diisopropyl ether

Concen: 0.437 ug/l

RT: 6.503 min Scan# 1

Delta R.T. 0.005 min

Lab File: VN070469.D


Acq: 4 Jan 2022 17:33

Instrument :

MSVOA_N

ClientSampleId :

MW-6D

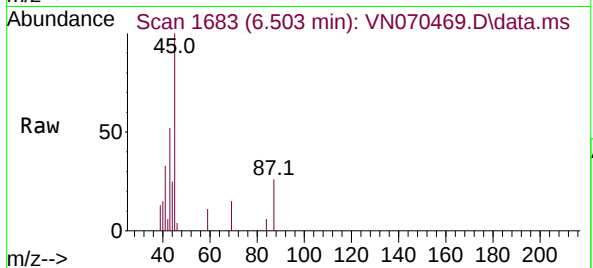

Tgt Ion: 45 Resp: 18628

Ion Ratio Lower Upper

45 100

43 48.9 51.7 77.5

87 25.7 23.2 34.8




59 11.4 9.4 14.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/05/2022

Supervised By :Mahesh Dadoda 01/05/2022

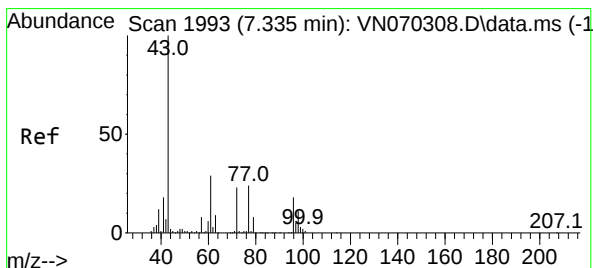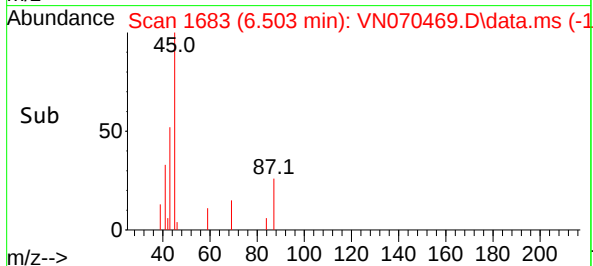

#25

2-Butanone

Concen: 1.066 ug/l

RT: 7.346 min Scan# 1997

Delta R.T. 0.011 min

Lab File: VN070469.D




Acq: 4 Jan 2022 17:33


Tgt Ion: 43 Resp: 11874

Ion Ratio Lower Upper

43 100


72 17.1 21.7 32.5

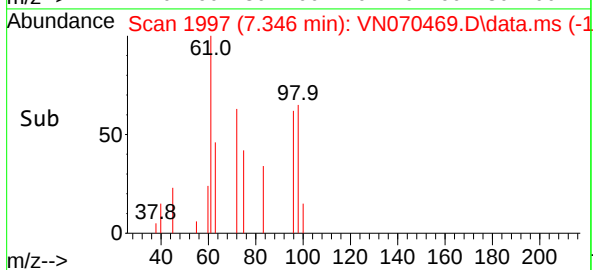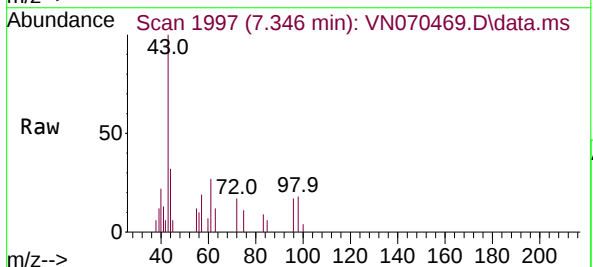

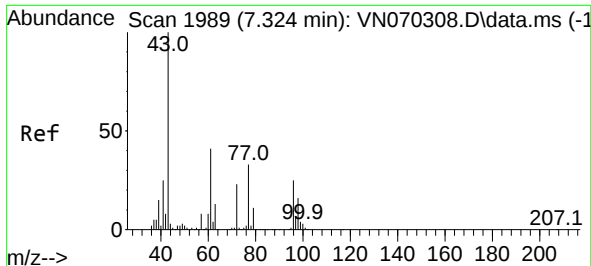

#27
 cis-1,2-Dichloroethene
 Concen: 0.289 ug/l
 RT: 7.324 min Scan# 1989
 Delta R.T. 0.000 min
 Lab File: VN070469.D
 Acq: 4 Jan 2022 17:33




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-6D

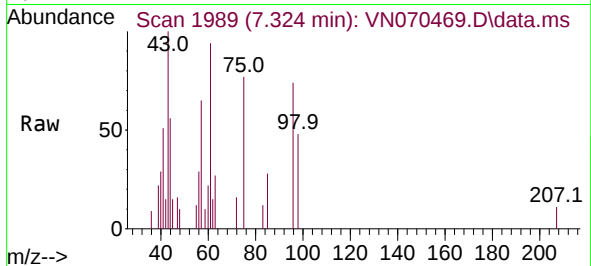


Tgt Ion: 96 Resp: 3528
 Ion Ratio Lower Upper
 96 100
 61 85.7 0.0 275.0
 98 14.4 0.0 129.6

Manual Integrations
 APPROVED



Reviewed By :John Carlone 01/05/2022
 Supervised By :Mahesh Dadoda 01/05/2022

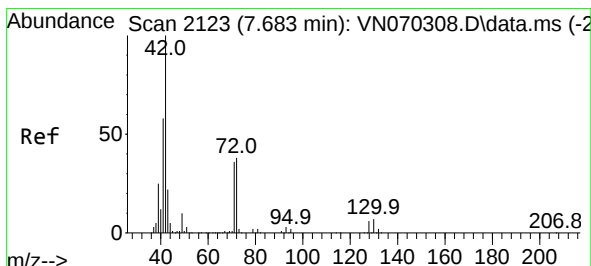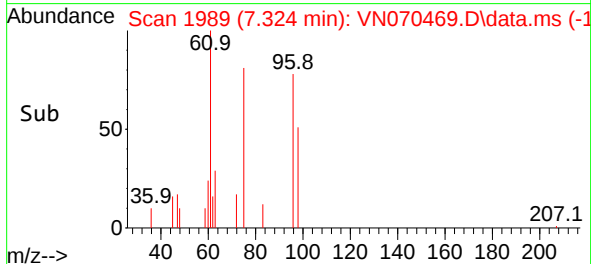


#29
 Tetrahydrofuran
 Concen: 1.108 ug/l m
 RT: 7.692 min Scan# 2126
 Delta R.T. 0.009 min
 Lab File: VN070469.D
 Acq: 4 Jan 2022 17:33

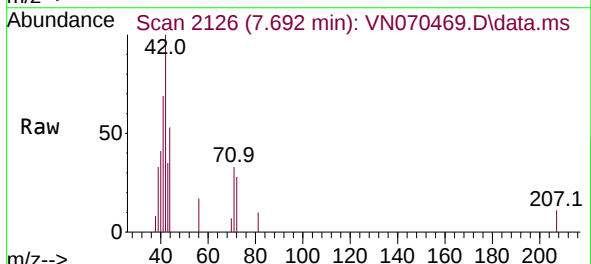


Tgt Ion: 42 Resp: 7363
 Ion Ratio Lower Upper
 42 100
 72 13.3 36.3 54.5#
 71 16.8 34.7 52.1#

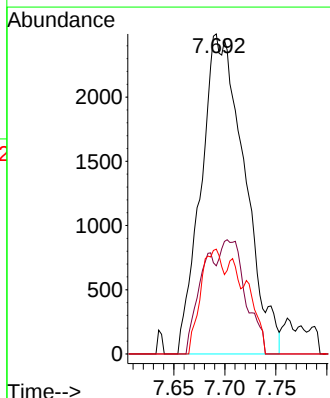

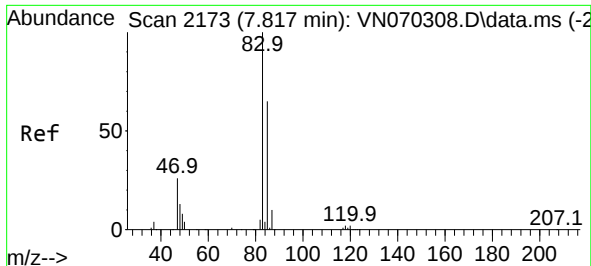

#30
Chloroform
Concen: 0.489 ug/l
RT: 7.820 min Scan# 2173
Delta R.T. 0.003 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D



Tgt Ion: 83 Resp: 1042
Ion Ratio Lower Upper
83 100
85 64.8 51.9 77.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

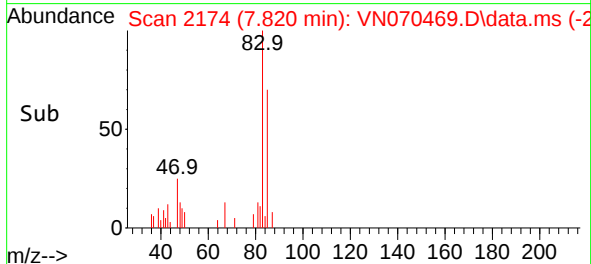

#33
1,2-Dichloroethane-d4
Concen: 49.708 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

Tgt Ion: 65 Resp: 677295
Ion Ratio Lower Upper
65 100
67 53.1 0.0 103.0

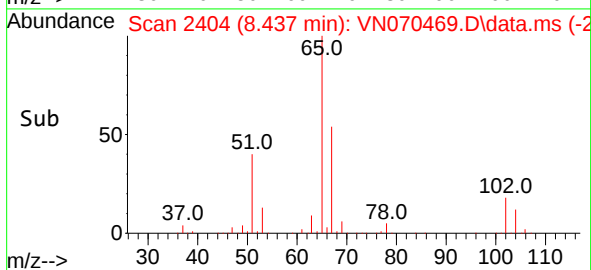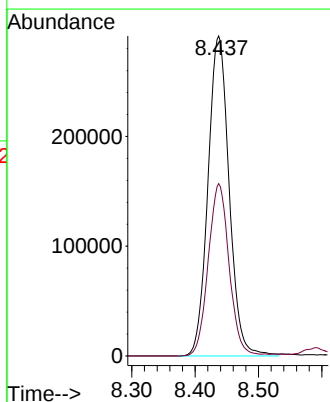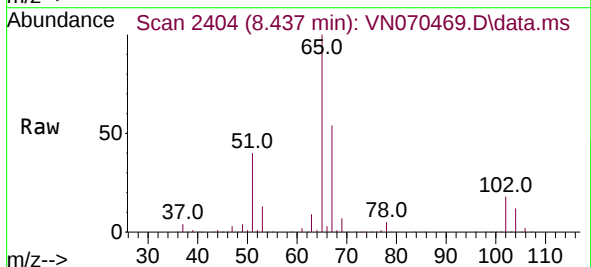



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.965 min Scan# 2601

Delta R.T. -0.003 min

Lab File: VN070469.D

Acq: 4 Jan 2022 17:33

Instrument :

MSVOA_N

ClientSampleId :

MW-6D

Tgt Ion:114 Resp: 1626098

Ion Ratio Lower Upper

114 100

63 23.0 0.0 37.8





88 16.8 0.0 27.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/05/2022

Supervised By :Mahesh Dadoda 01/05/2022

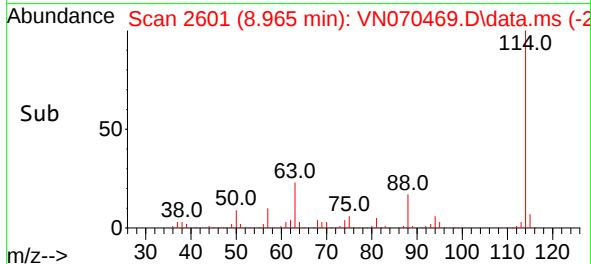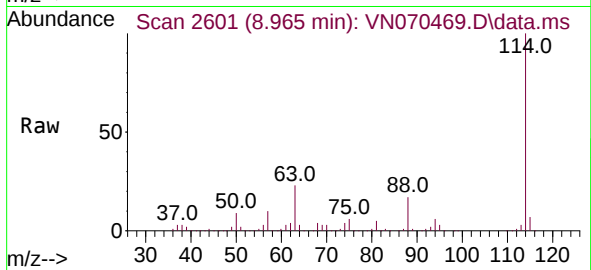

#35

Dibromofluoromethane

Concen: 47.873 ug/l

RT: 8.019 min Scan# 2248

Delta R.T. -0.002 min

Lab File: VN070469.D

Acq: 4 Jan 2022 17:33




Tgt Ion:113 Resp: 471009


Ion Ratio Lower Upper

113 100

111 103.1 82.2 123.2


192 19.5 16.9 25.3

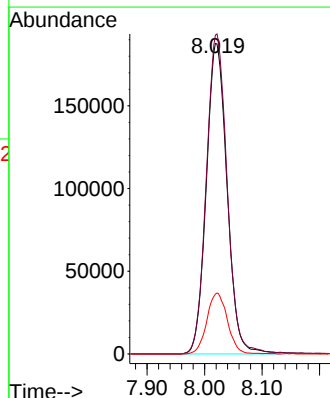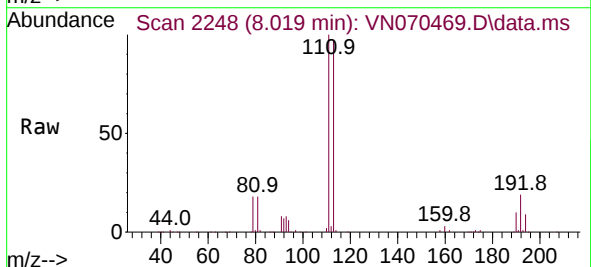



#40
Benzene
Concen: 1.787 ug/l
RT: 8.459 min Scan# 2412
Delta R.T. 0.001 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D



Tgt Ion: 78 Resp: 8915
Ion Ratio Lower Upper
78 100
77 21.1 18.6 27.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

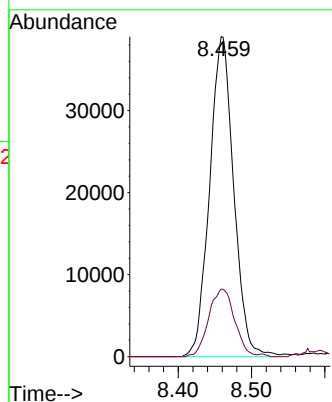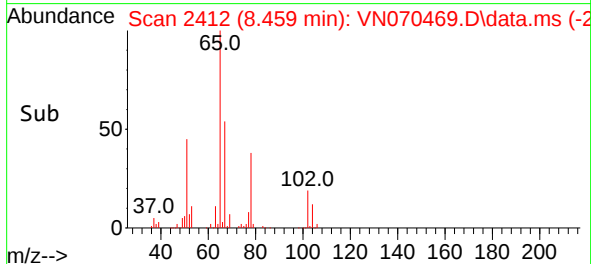

#44
Trichloroethene
Concen: 1.733 ug/l
RT: 9.215 min Scan# 2694
Delta R.T. -0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33


Tgt Ion:130 Resp: 20541
Ion Ratio Lower Upper
130 100
95 98.4 0.0 191.2

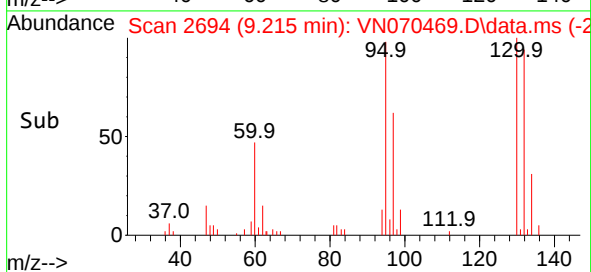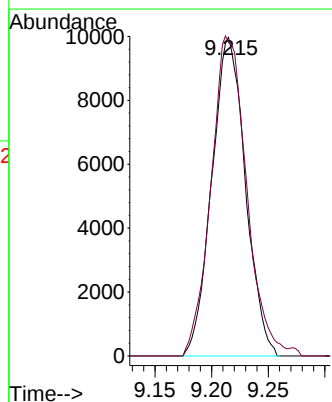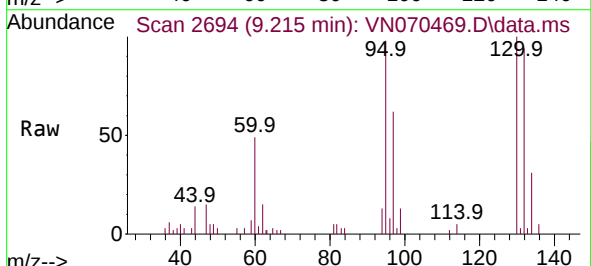



#50
Toluene-d8
Concen: 46.993 ug/l
RT: 10.441 min Scan# 3151
Delta R.T. 0.001 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D




Tgt Ion: 98 Resp: 188876
Ion Ratio Lower Upper
98 100
100 64.5 50.4 75.6

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

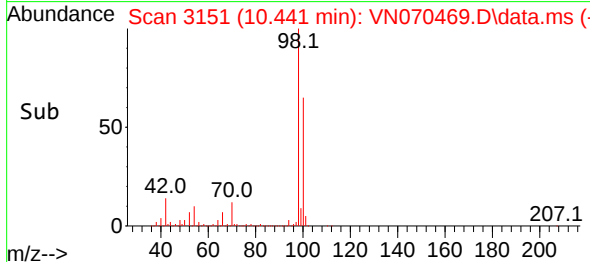


#59
2-Hexanone
Concen: 1.161 ug/l
RT: 11.087 min Scan# 3392
Delta R.T. 0.003 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

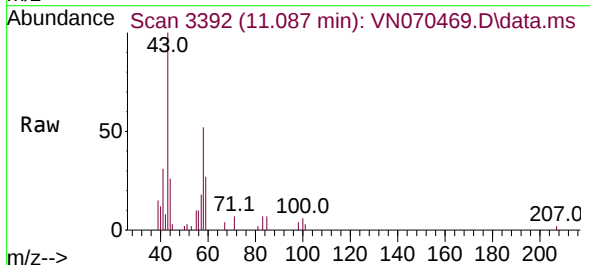


Tgt Ion: 43 Resp: 17693
Ion Ratio Lower Upper
43 100
58 41.6 26.9 80.7

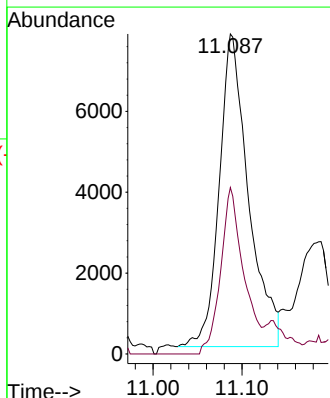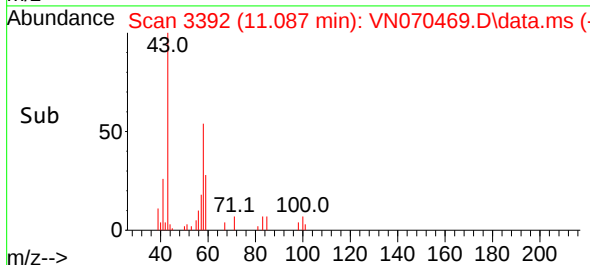



#62
4-Bromofluorobenzene
Concen: 44.994 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D




Tgt Ion: 95 Resp: 65315
Ion Ratio Lower Upper
95 100
174 76.4 0.0 187.2
176 73.6 0.0 181.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

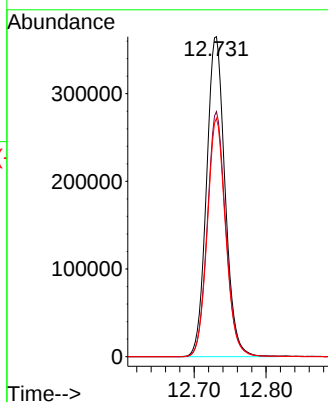


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Tgt Ion:117 Resp: 1403673
Ion Ratio Lower Upper
117 100
82 58.8 42.4 63.6
119 32.3 25.4 38.2

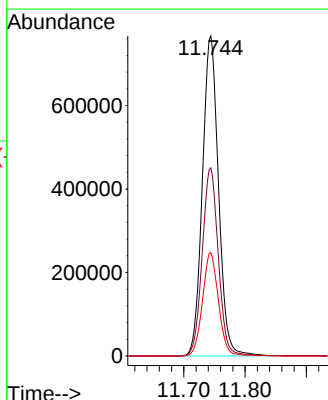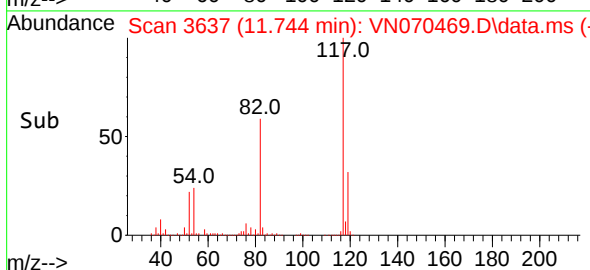



#64
Tetrachloroethene
Concen: 0.304 ug/l
RT: 10.972 min Scan# 31
Delta R.T. -0.005 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D




Tgt Ion:164 Resp: 308
Ion Ratio Lower Upper
164 100
166 123.0 101.9 152.9
129 89.6 72.0 108.0
131 96.2 70.9 106.3

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

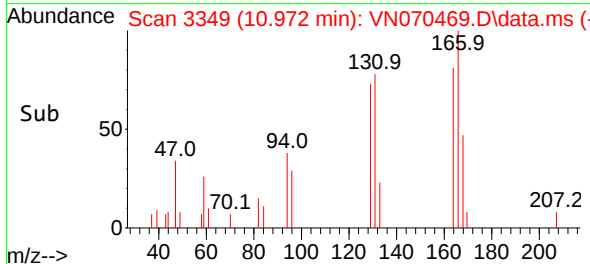


#67
Ethyl Benzene
Concen: 0.237 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. 0.003 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

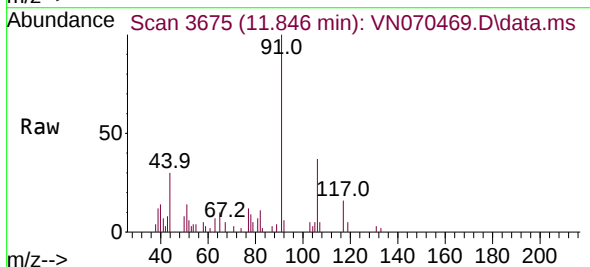


Tgt Ion: 91 Resp: 12919
Ion Ratio Lower Upper
91 100
106 36.7 25.7 38.5

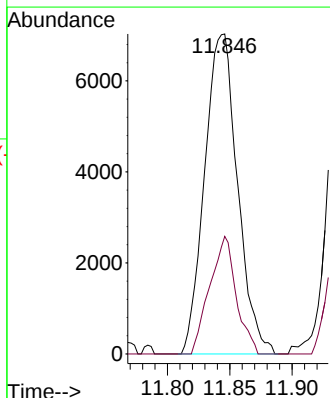



#68
m/p-Xylenes
Concen: 0.702 ug/l
RT: 11.951 min Scan# 3714
Delta R.T. -0.002 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D



Tgt Ion:106 Resp: 13940
Ion Ratio Lower Upper
106 100
91 229.6 160.6 240.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

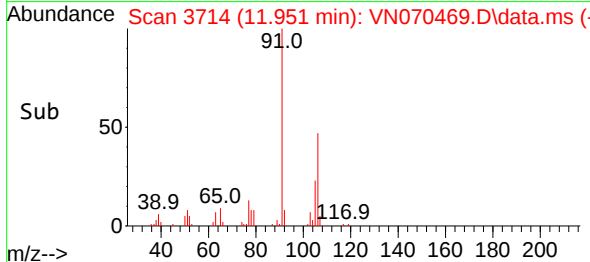

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.672 min Scan# 4356
Delta R.T. 0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33


Tgt Ion:152 Resp: 472625
Ion Ratio Lower Upper
152 100
115 60.3 27.5 82.5
150 155.6 0.0 344.4

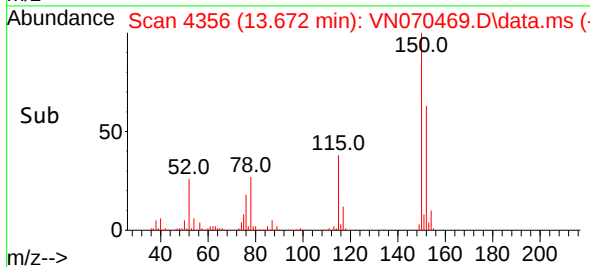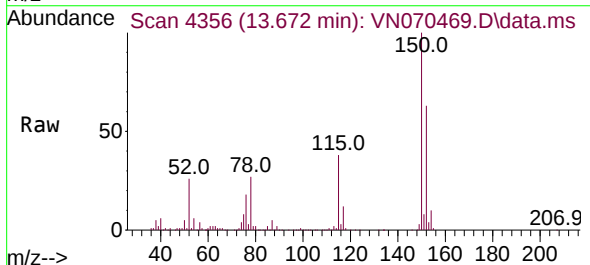



#74
N-amy1 acetate
Concen: 0.567 ug/l
RT: 12.390 min Scan# 3876
Delta R.T. 0.005 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D



Tgt Ion: 43 Resp: 1045
Ion Ratio Lower Upper
43 100
70 37.4 33.4 50.0
55 30.5 19.3 28.9
61 10.8 18.5 27.7#




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

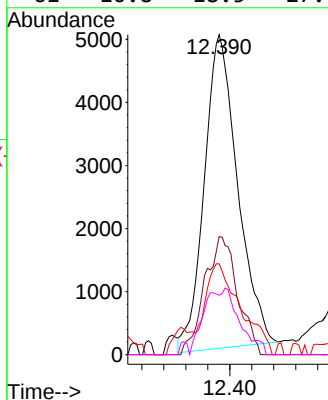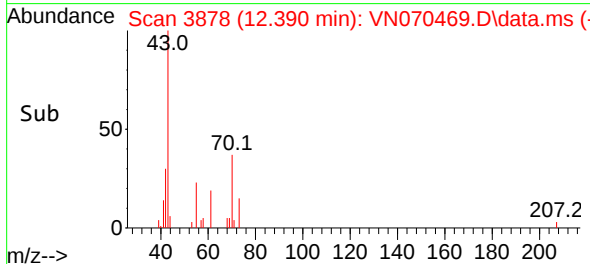

#84
1,2,4-Trimethylbenzene
Concen: 0.739 ug/l
RT: 13.367 min Scan# 4242
Delta R.T. 0.001 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

Tgt Ion:105 Resp: 25042
Ion Ratio Lower Upper
105 100
120 43.2 22.8 68.4

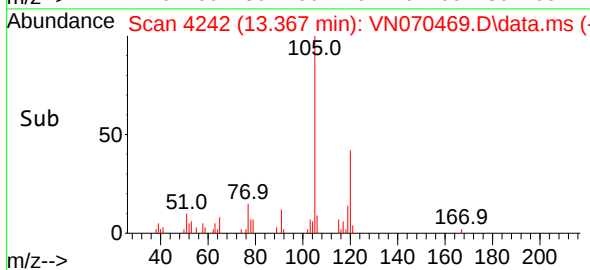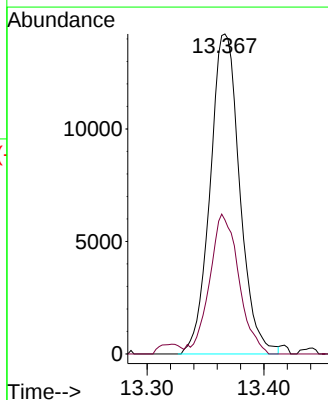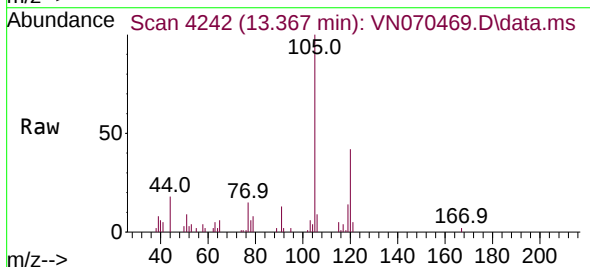







#85
 sec-Butylbenzene
 Concen: 0.272 ug/l
 RT: 13.501 min Scan# 4292
 Delta R.T. -0.000 min
 Lab File: VN070469.D
 Acq: 4 Jan 2022 17:33

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-6D

Tgt Ion:105 Resp: 1145
 Ion Ratio Lower Upper
 105 100
 134 19.9 10.4 31.1




Manual Integrations
 APPROVED


Reviewed By :John Carlone 01/05/2022
 Supervised By :Mahesh Dadoda 01/05/2022

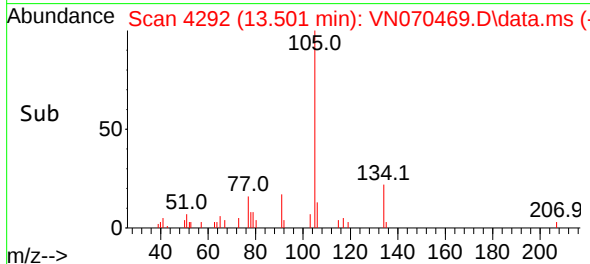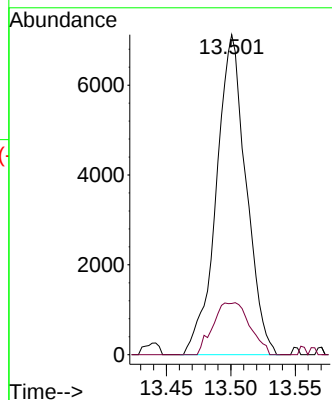

#86
 p-Isopropyltoluene
 Concen: 0.209 ug/l
 RT: 13.619 min Scan# 4336
 Delta R.T. 0.006 min
 Lab File: VN070469.D
 Acq: 4 Jan 2022 17:33

Tgt Ion:119 Resp: 6888
 Ion Ratio Lower Upper
 119 100
 134 21.1 13.6 40.7
 91 23.6 11.4 34.1

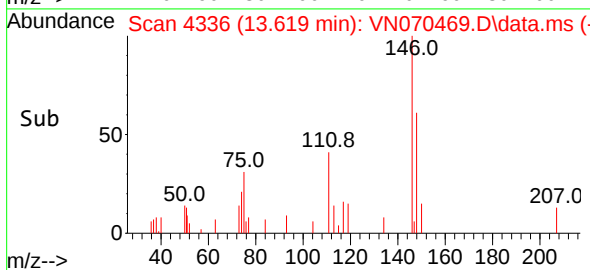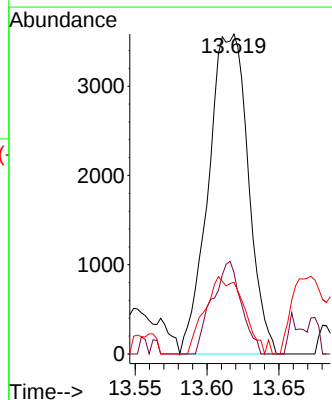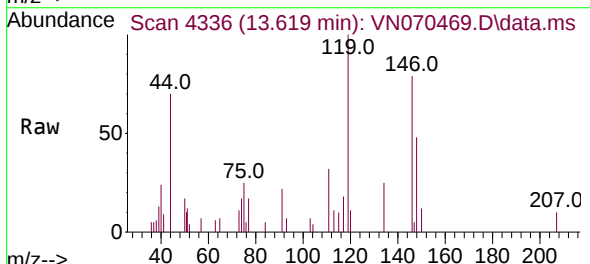



#87

1,3-Dichlorobenzene

Concen: 0.316 ug/l

RT: 13.619 min Scan# 4334

Delta R.T. 0.006 min

Lab File: VN070469.D

Acq: 4 Jan 2022 17:33

Instrument :

MSVOA_N

ClientSampleId :

MW-6D





Tgt Ion:146	Resp:	533
Ion Ratio	Lower	Upper
146	100	
111	39.6	18.6 55.6
148	61.4	31.6 95.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/05/2022

Supervised By :Mahesh Dadoda 01/05/2022

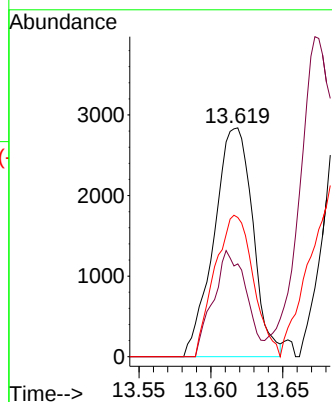

#88

1,4-Dichlorobenzene

Concen: 0.426 ug/l m




RT: 13.694 min Scan# 4364


Delta R.T. -0.000 min

Lab File: VN070469.D

Acq: 4 Jan 2022 17:33

Tgt Ion:146	Resp:	7088
Ion Ratio	Lower	Upper
146	100	
111	29.8	18.3 54.8
148	46.2	31.8 95.4

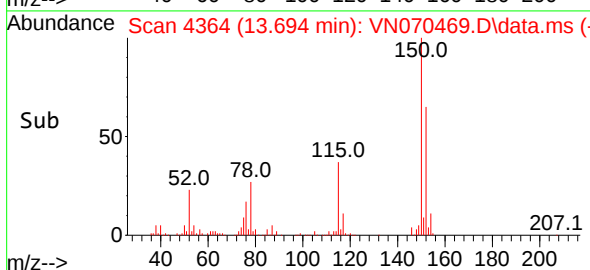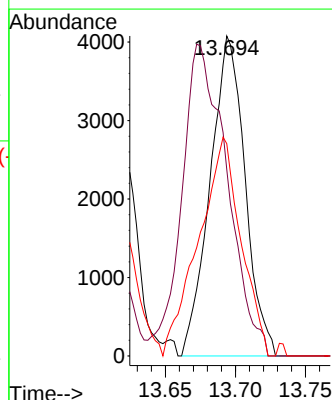







#89
n-Butylbenzene
Concen: 0.416 ug/l
RT: 13.943 min Scan# 4456
Delta R.T. 0.003 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

Instrument :
MSVOA_N
ClientSampleId :
MW-6D

Tgt Ion: 91 Resp: 11456
Ion Ratio Lower Upper
91 100
92 55.4 25.4 76.0
134 27.7 13.6 40.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

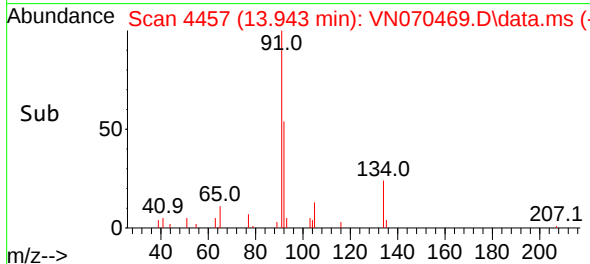

#91
1,2-Dichlorobenzene
Concen: 0.336 ug/l
RT: 13.986 min Scan# 4473
Delta R.T. 0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33


Tgt Ion:146 Resp: 5561
Ion Ratio Lower Upper
146 100
111 41.9 19.1 57.3
148 64.9 32.1 96.3

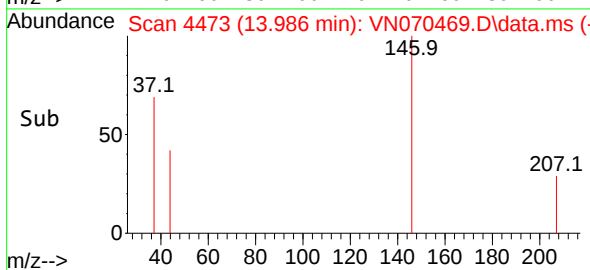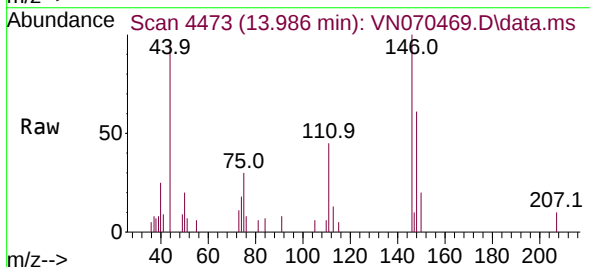

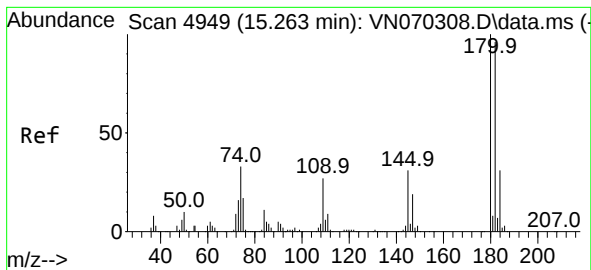

#93
1,2,4-Trichlorobenzene
Concen: 1.007 ug/l
RT: 15.263 min Scan# 4949
Delta R.T. -0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33




Instrument :
MSVOA_N
ClientSampleId :
MW-6D

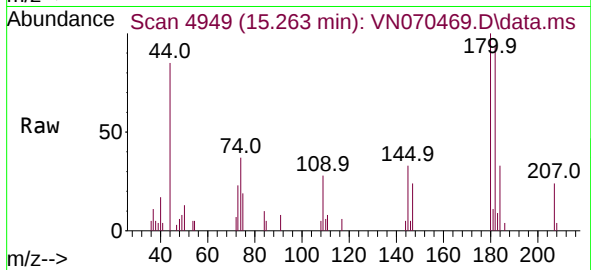


Tgt Ion:180 Resp: 7844
Ion Ratio Lower Upper
180 100
182 97.1 48.3 144.9
145 41.4 14.5 43.5

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

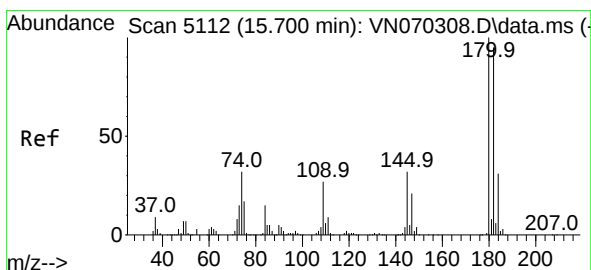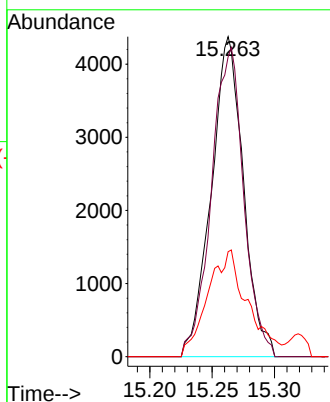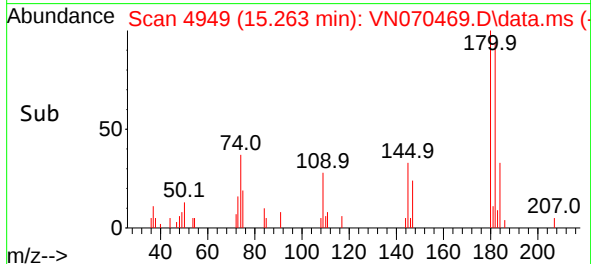

#96
1,2,3-Trichlorobenzene
Concen: 2.078 ug/l
RT: 15.700 min Scan# 5112
Delta R.T. -0.000 min
Lab File: VN070469.D
Acq: 4 Jan 2022 17:33

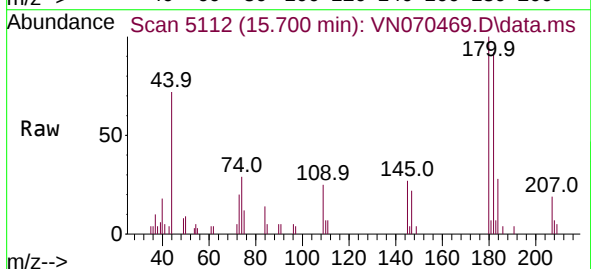

Tgt Ion:180 Resp: 9491
Ion Ratio Lower Upper
180 100
182 95.7 47.4 142.2
145 37.9 15.0 45.1

