

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010422\
 Data File : VN070465.D
 Acq On : 4 Jan 2022 15:52
 Operator : JC/MD
 Sample : N1003-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M

Title : SW846 8260

Signal : TIC: VN070465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.231	78	90	102	rBV3	296337	559159	9.83%	1.949%
2	4.578	942	965	998	rBV2	59388	205609	3.61%	0.717%
3	8.021	2225	2249	2260	rBV2	701689	1715838	30.17%	5.981%
4	8.083	2260	2272	2300	rVB	1294437	2986548	52.51%	10.411%
5	8.437	2379	2404	2433	rBV	905212	2084583	36.65%	7.267%
6	8.965	2580	2601	2632	rBV	1986498	4155747	73.06%	14.487%
7	10.440	3131	3151	3186	rBV	3037314	5688025	100.00%	19.828%
8	11.744	3618	3637	3671	rBV	2520291	4640910	81.59%	16.178%
9	12.731	3986	4005	4031	rBV	1988062	3536518	62.17%	12.328%
10	13.672	4339	4356	4380	rBV	1766193	3113746	54.74%	10.854%




Sum of corrected areas: 28686683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010422\
Data File : VN070465.D
Acq On : 4 Jan 2022 15:52
Operator : JC/MD
Sample : N1003-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

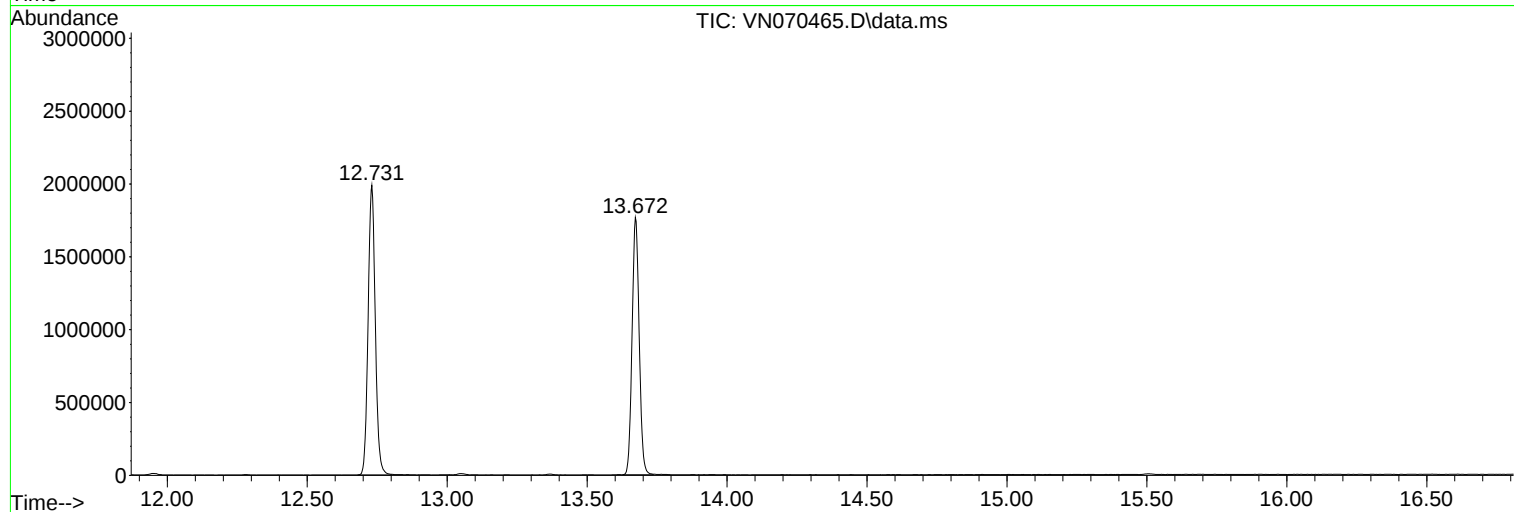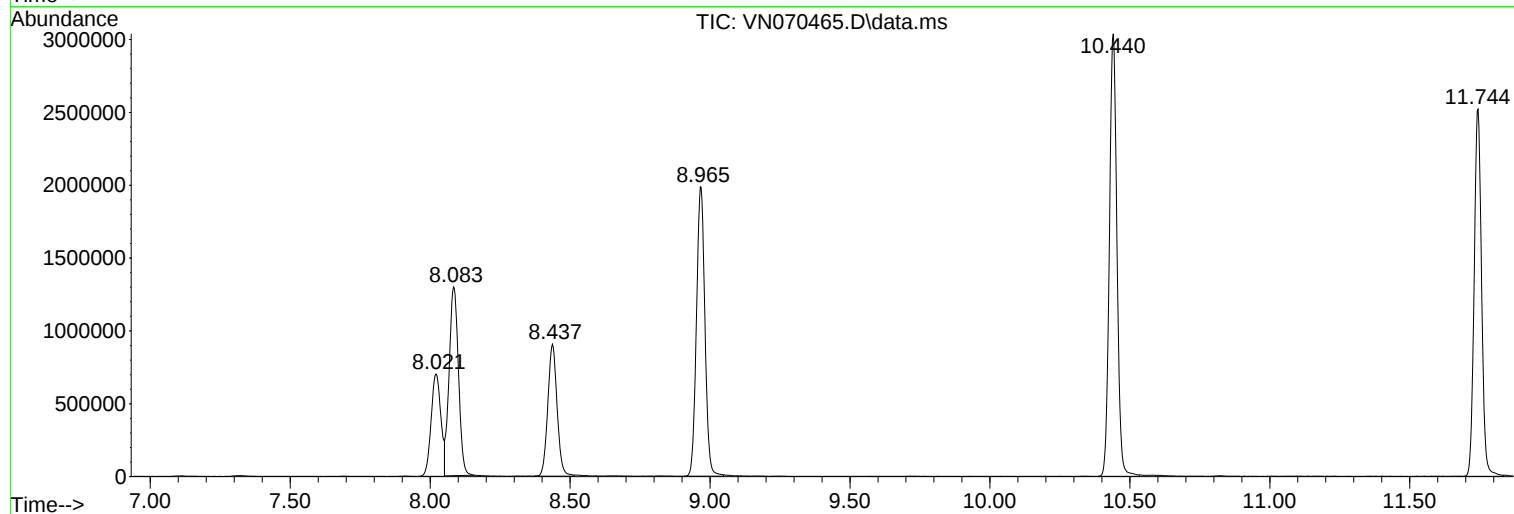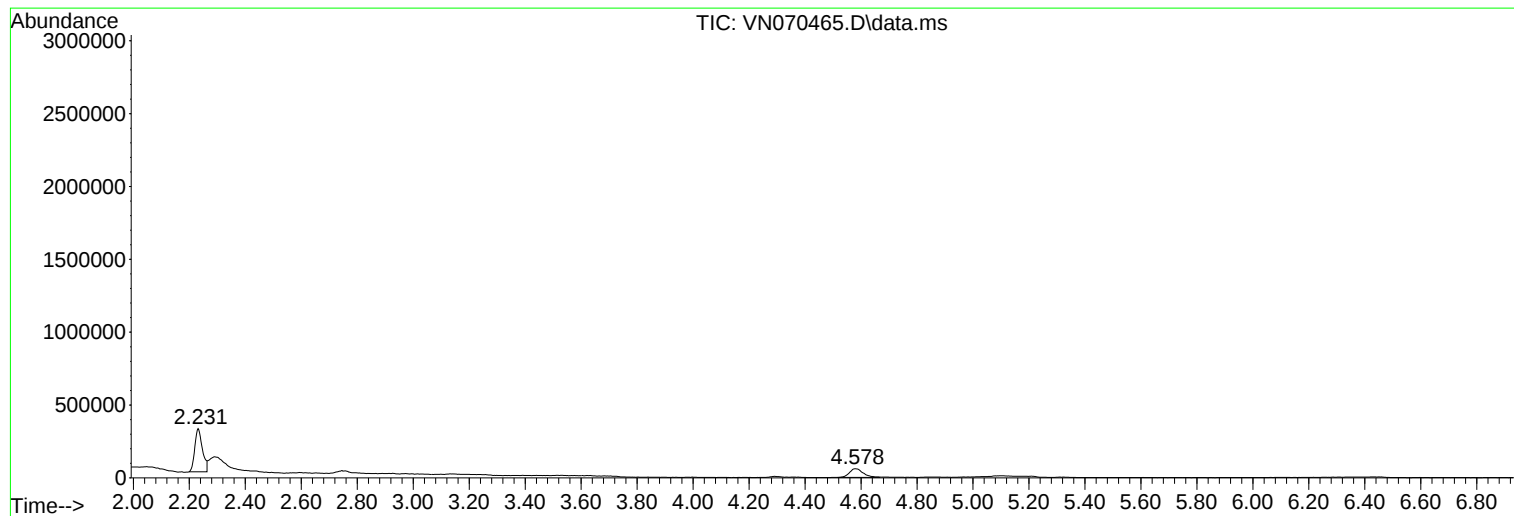

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010422\
Data File : VN070465.D
Acq On : 4 Jan 2022 15:52
Operator : JC/MD
Sample : N1003-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	2.231	9.4	ug/l	559159	1	8.086	2986550	50.0