


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010422\
Data File : VN070452.D
Acq On : 4 Jan 2022 9:55
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Title : SW846 8260
Last Update : Mon Dec 27 18:47:12 2021

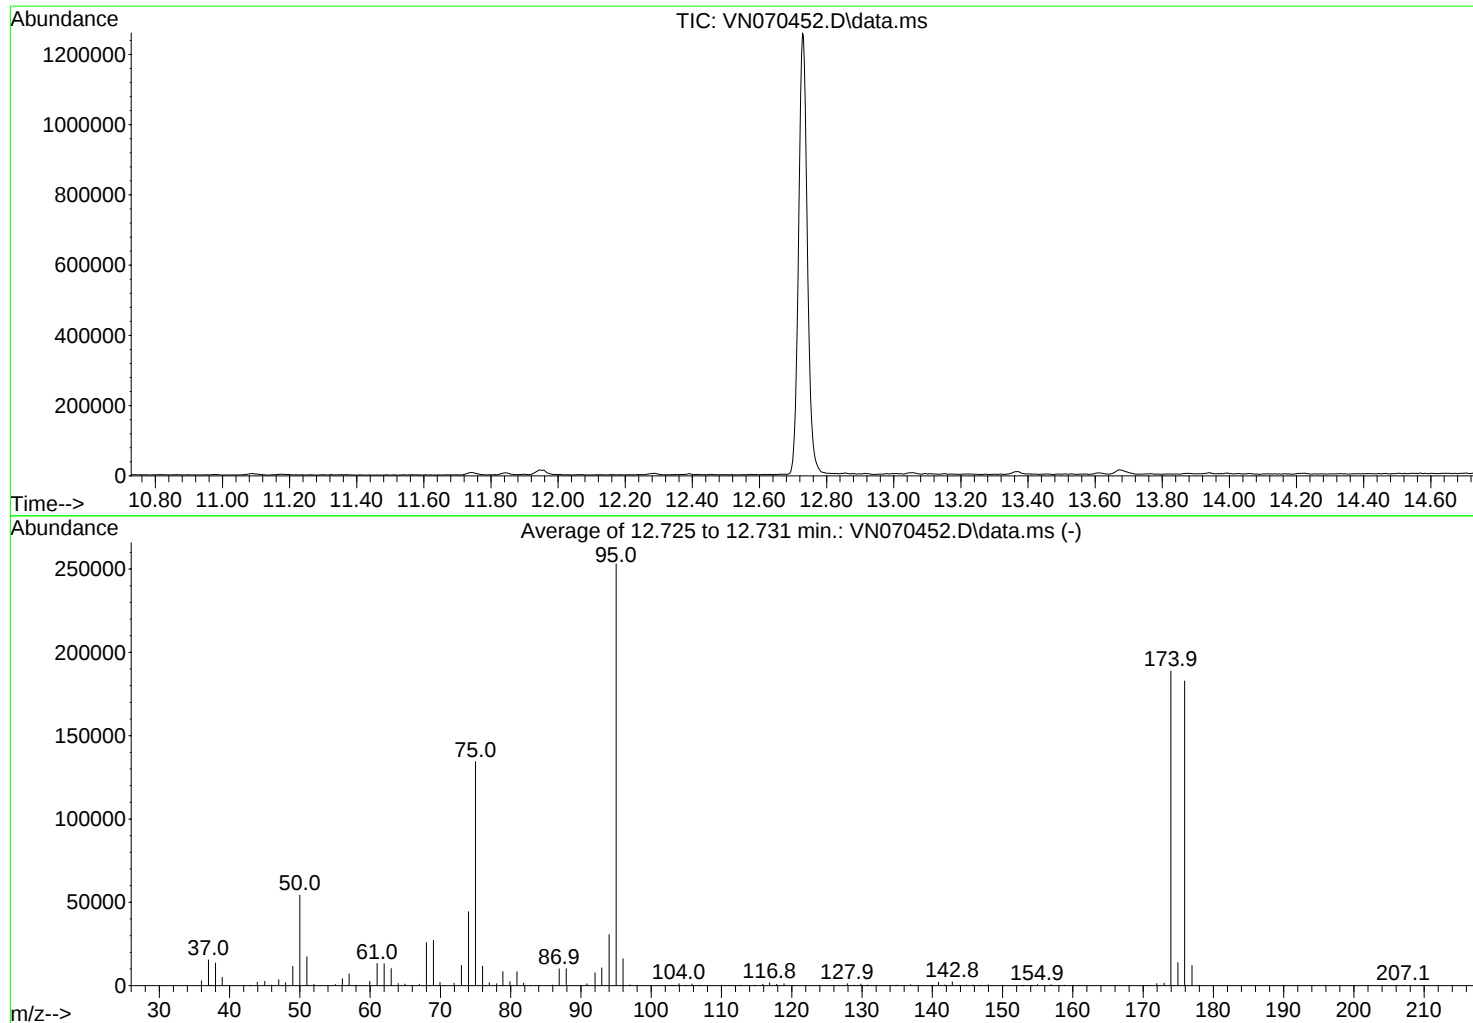

AutoFind: Scans 4003, 4004, 4005; Background Corrected with Scan 3984

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.5	54328	PASS
75	95	30	60	53.1	134464	PASS
95	95	100	100	100.0	253141	PASS
96	95	5	9	6.4	16145	PASS
173	174	0.00	2	0.8	1551	PASS
174	95	50	100	74.6	188757	PASS
175	174	5	9	7.4	13874	PASS
176	174	95	101	96.8	182784	PASS
177	176	5	9	6.6	12075	PASS