
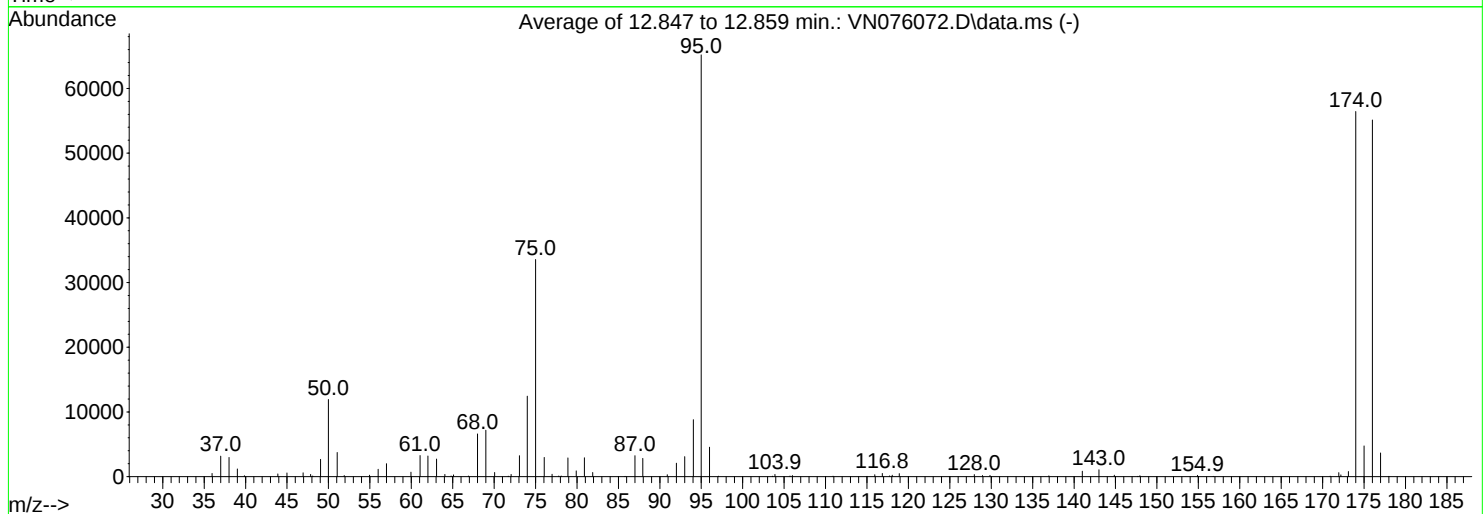


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010423\
Data File : VN076072.D
Acq On : 04 Jan 2023 11:00
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

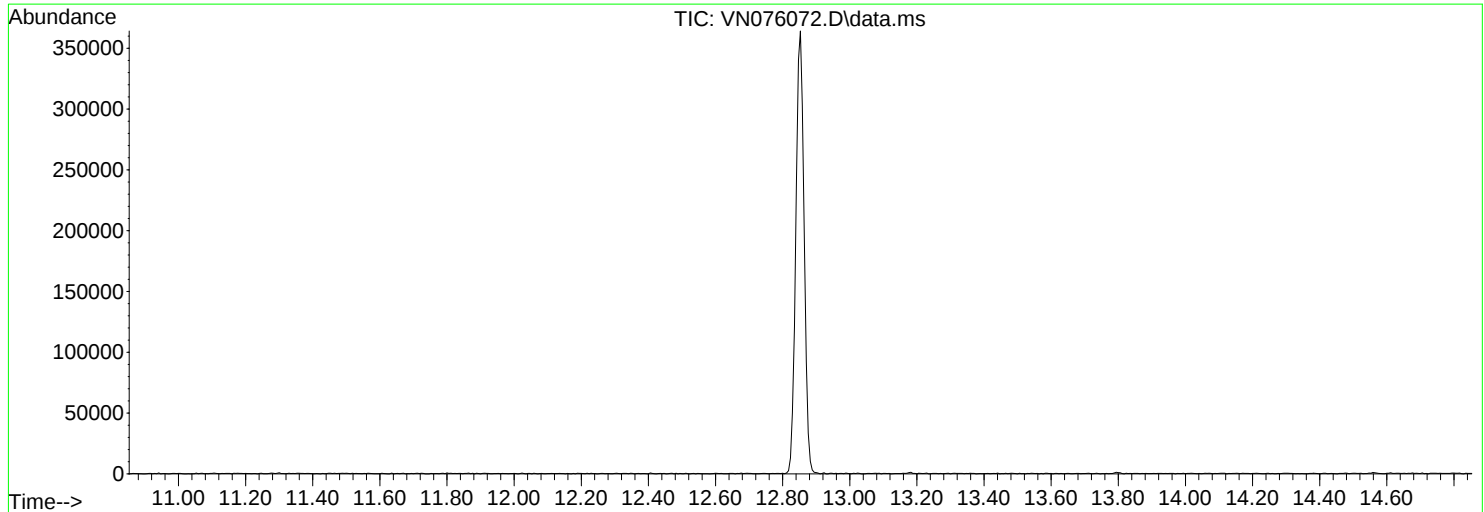

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	11921	PASS
75	95	30	60	51.5	33555	PASS
95	95	100	100	100.0	65195	PASS
96	95	5	9	7.0	4561	PASS
173	174	0.00	2	1.4	792	PASS
174	95	50	100	86.6	56440	PASS
175	174	5	9	8.4	4753	PASS
176	174	95	101	97.6	55112	PASS
177	176	5	9	6.6	3654	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	506	50.00	11921	64.80	102	76.05	2951
37.00	3174	51.05	3726	65.10	269	77.00	361
38.00	2981	51.90	173	66.90	93	77.80	101
39.00	1201	54.95	214	68.00	6611	78.10	91
39.85	153	56.00	1149	69.00	7179	78.90	2885
43.90	420	57.00	2015	70.05	640	79.90	882
45.00	568	59.95	699	71.70	72	80.90	2927
46.95	603	61.05	3272	72.05	345	81.90	658
47.85	353	62.00	3199	73.05	3250	85.80	53
48.10	93	63.05	2731	74.00	12452	87.00	3248
49.05	2674	64.05	343	75.00	33555	87.95	2832

Average of 12.847 to 12.859 min.: VN076072.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	311	110.90	69	141.00	840	174.00	56440
92.00	2091	115.00	53	143.00	1073	175.00	4753
93.00	3093	115.95	303	144.85	225	176.00	55112
94.05	8797	116.85	499	147.70	50	177.00	3654
95.00	65195	117.75	135	147.95	144	178.00	54
96.00	4561	118.05	226	154.90	199		
97.10	68	118.90	460	156.80	54		
103.60	80	127.95	323	170.90	79		
103.90	350	128.95	174	171.95	631		
105.70	110	129.85	191	172.20	283		
106.00	174	136.95	120	173.10	792		

Instrument :

MSVOA_N

ClientSampleId :

BFB