


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN010519\
Data File : VN053284.D
Acq On : 4 Jan 2019 16:14
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N010519W.M
Title : SW846 8260
Last Update : Mon Jan 07 09:34:27 2019

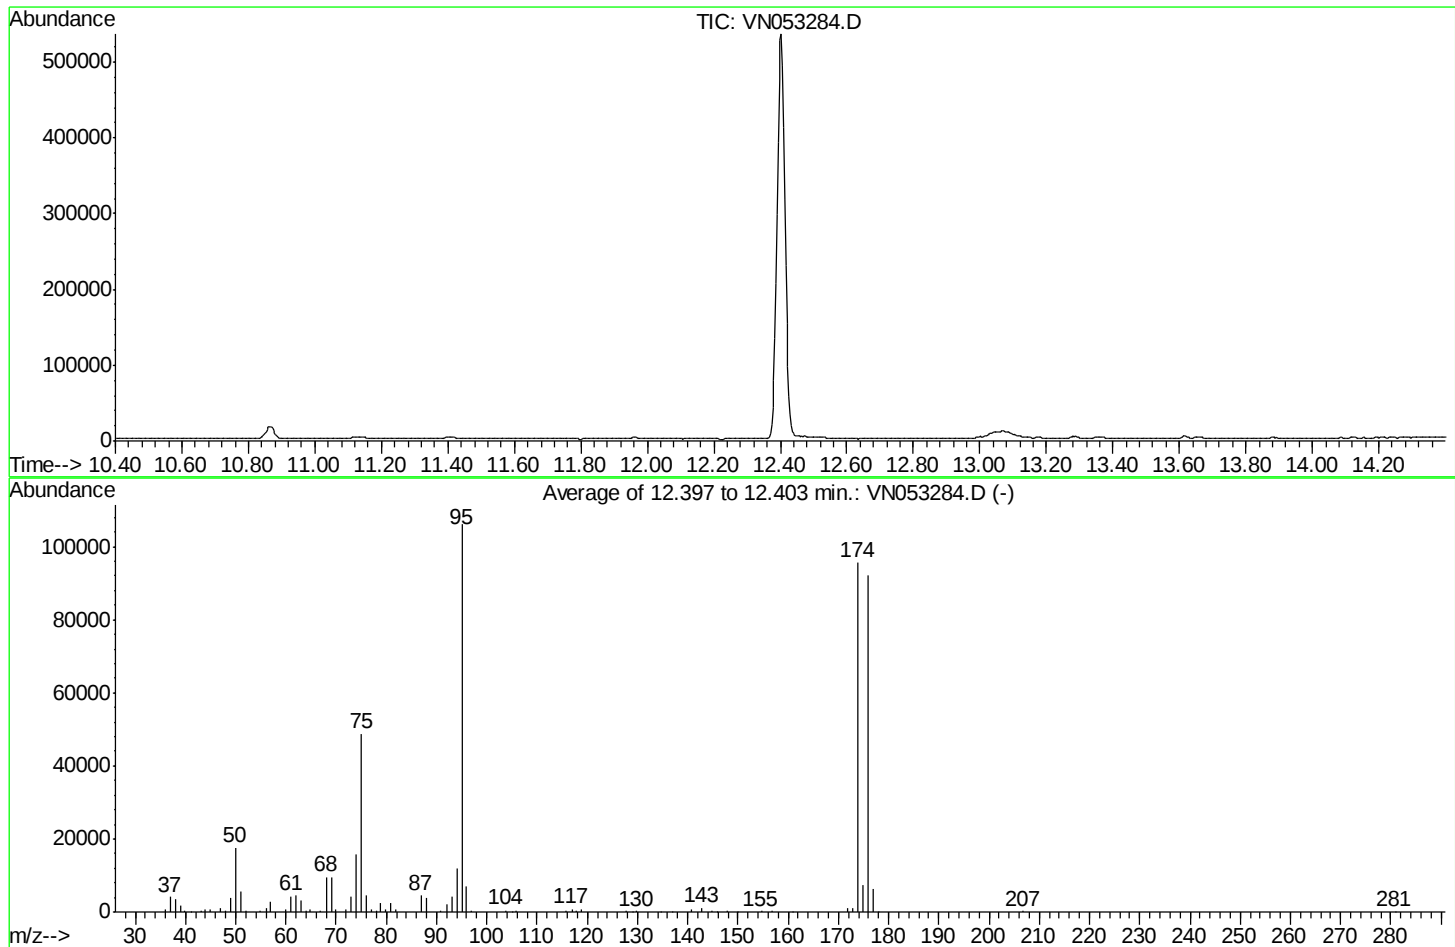

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	17634	PASS
75	95	30	60	46.0	48794	PASS
95	95	100	100	100.0	106112	PASS
96	95	5	9	6.5	6891	PASS
173	174	0.00	2	1.0	933	PASS
174	95	50	100	90.1	95584	PASS
175	174	5	9	7.8	7425	PASS
176	174	95	101	96.5	92221	PASS
177	176	5	9	6.9	6350	PASS