

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010522\
 Data File : VN070490.D
 Acq On : 5 Jan 2022 15:31
 Operator : JC/MD
 Sample : N1012-07
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jan 06 12:35:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	952880	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.965	114	1601741	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1442641	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	494220	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	663415	48.422	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	96.840%
35) Dibromofluoromethane	8.021	113	464337	47.913	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	95.820%
50) Toluene-d8	10.440	98	1894749	47.859	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	95.720%
62) 4-Bromofluorobenzene	12.731	95	696120	48.683	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	97.360%


Target Compounds				Qvalue		
3) Chloromethane	2.303	50	4120	0.280	ug/l	93
11) Tert butyl alcohol	5.366	59	27925	12.241	ug/l #	86
13) Acrolein	4.028	56	439	0.237	ug/l #	14
14) Allyl chloride	4.586	41	95568	4.343	ug/l #	69
16) Acetone	4.283	43	20073058	2256.967	ug/l	97
18) Methyl Acetate	4.578	43	276570	10.750	ug/l #	51
22) Diisopropyl ether	6.584	45	15561	0.363	ug/l #	1
23) Vinyl Acetate	6.581	43	37126	1.117	ug/l #	72
25) 2-Butanone	7.340	43	83775	7.481	ug/l #	89
29) Tetrahydrofuran	7.702	42	6568	0.983	ug/l #	52
31) Cyclohexane	8.083	56	23218	1.074	ug/l #	8
36) 1,1-Dichloropropene	8.083	75	77019	4.804	ug/l #	48
37) Ethyl Acetate	7.340	43	83775	4.031	ug/l #	69
38) Carbon Tetrachloride	8.083	117	90981	5.943	ug/l #	16
40) Benzene	8.461	78	24452	0.497	ug/l	96
48) Methyl methacrylate	9.534	41	6859	0.439	ug/l #	13
49) 1,4-Dioxane	9.574	88	50	0.219	ug/l #	27
51) 4-Methyl-2-Pentanone	10.330	43	97905	4.756	ug/l	96
52) Toluene	10.505	92	44374	1.492	ug/l	97
58) 2-Chloroethyl Vinyl ether	9.856	63	52	18.523	ug/l #	45
59) 2-Hexanone	11.084	43	7996	0.533	ug/l	92
67) Ethyl Benzene	11.846	91	20467	0.365	ug/l	99
68) m/p-Xylenes	11.950	106	30762	1.507	ug/l	96
69) o-Xylene	12.280	106	15368	0.757	ug/l	92
71) Bromoform	12.731	173	3328	0.410	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.685	83	43209	3.027	ug/l #	32
76) 1,2,3-Trichloropropane	12.731	75	361683	26.102	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.058	105	7521	0.204	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.731	75	361683	89.412	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.366	105	16207	0.458	ug/l	92
95) Naphthalene	15.504	128	12971	2.352	ug/l	96
96) 1,2,3-Trichlorobenzene	15.705	180	1671	1.037	ug/l	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010522\
Data File : VN070490.D
Acq On : 5 Jan 2022 15:31
Operator : JC/MD
Sample : N1012-07
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Jan 06 12:35:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration

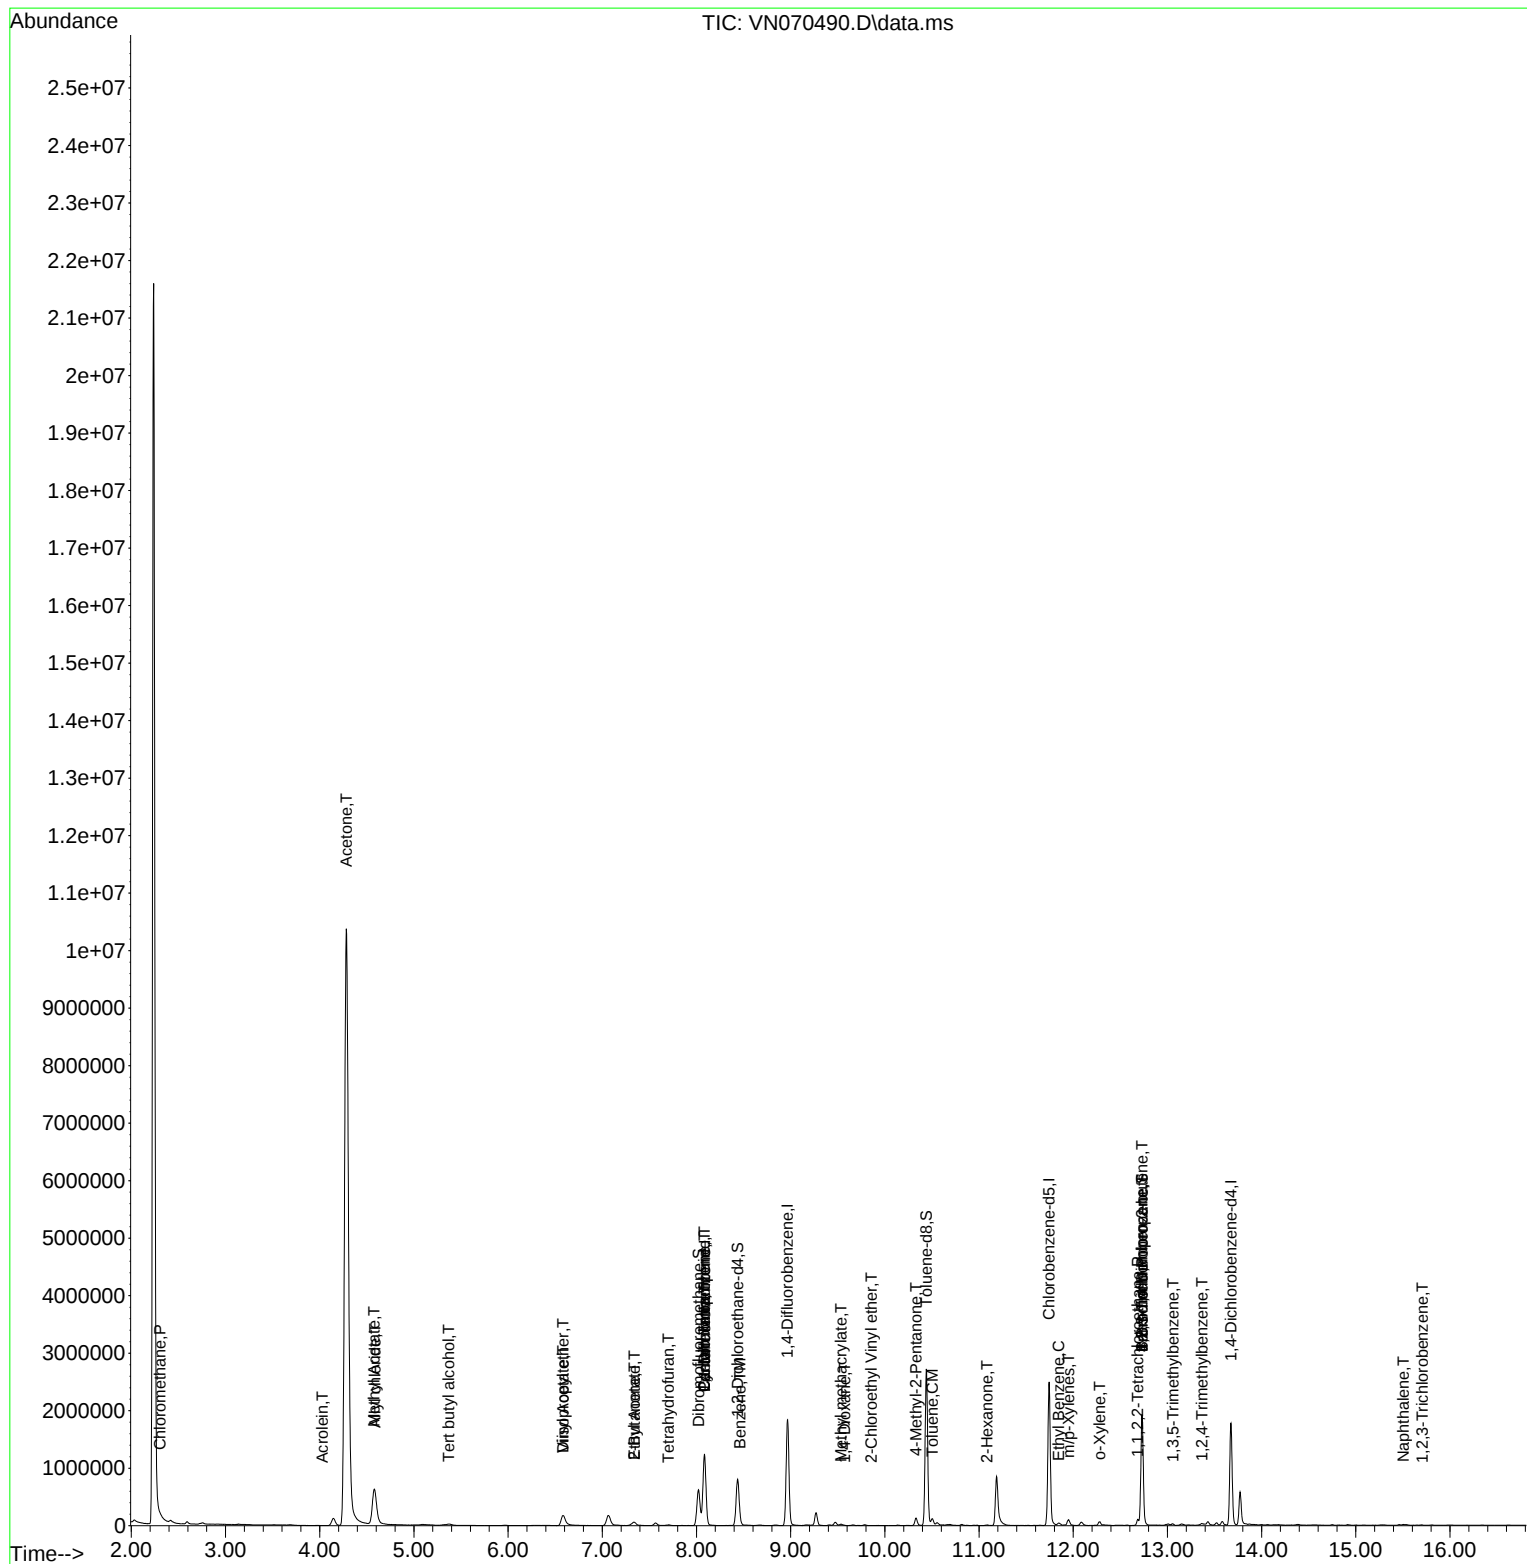






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 952880
Ion Ratio Lower Upper
168 100
99 57.2 41.3 61.9

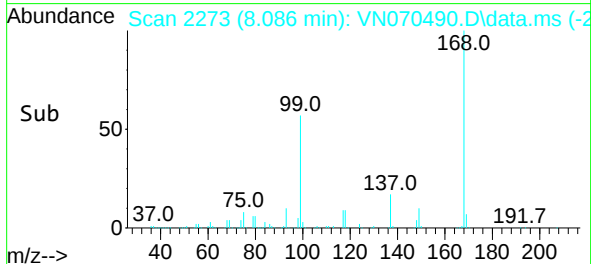

#3
Chloromethane
Concen: 0.280 ug/l
RT: 2.303 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Tgt Ion: 50 Resp: 4120
Ion Ratio Lower Upper
50 100
52 28.1 25.4 38.0

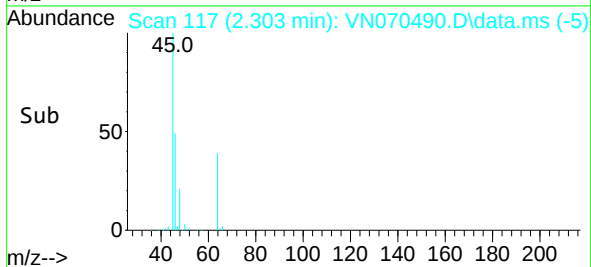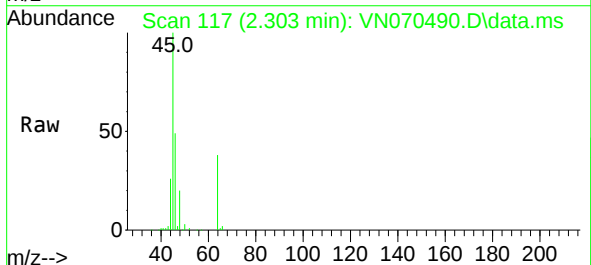

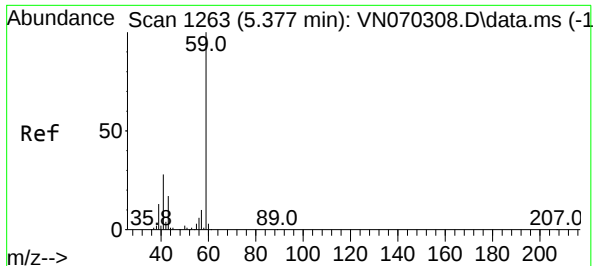

#11

Tert butyl alcohol

Concen: 12.241 ug/l

RT: 5.366 min Scan# 11

Delta R.T. -0.011 min


Lab File: VN070490.D

Acq: 5 Jan 2022 15:31

Instrument :

MSVOA_N

ClientSampleId :



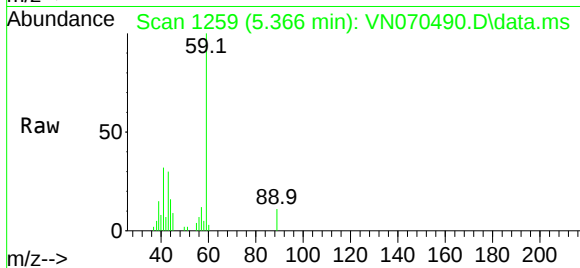


Tgt Ion: 59 Resp: 27925

Ion Ratio Lower Upper

59 100

57 16.4 8.7 13.1#

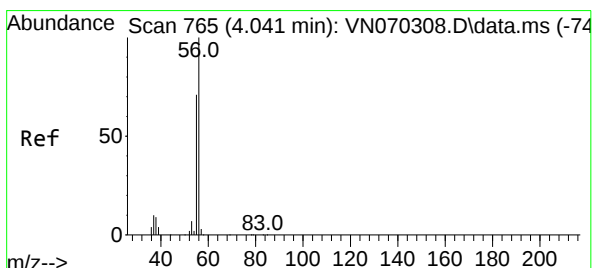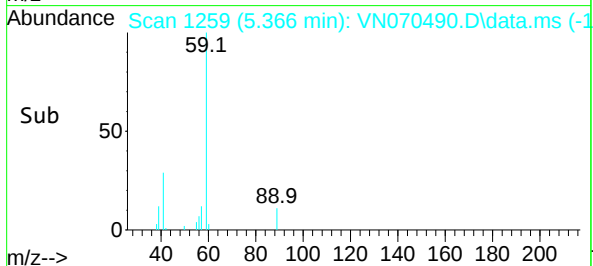

#13

Acrolein

Concen: 0.237 ug/l

RT: 4.028 min Scan# 760

Delta R.T. -0.013 min

Lab File: VN070490.D




Acq: 5 Jan 2022 15:31


Tgt Ion: 56 Resp: 439

Ion Ratio Lower Upper

56 100


55 0.0 56.6 85.0#

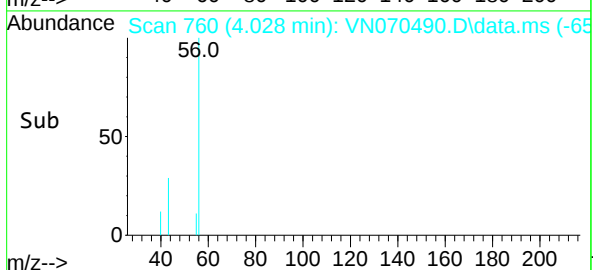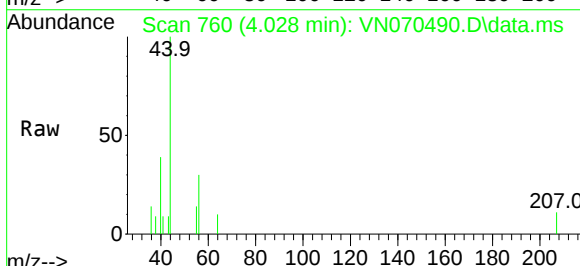






#14
 Allyl chloride
 Concen: 4.343 ug/l
 RT: 4.586 min Scan# 91
 Delta R.T. -0.254 min
 Lab File: VN070490.D
 Acq: 5 Jan 2022 15:31

Instrument :
 MSVOA_N
 ClientSampleId :



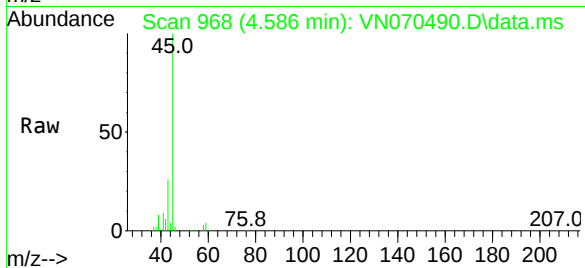



Tgt Ion: 41 Resp: 95568
 Ion Ratio Lower Upper
 41 100
 39 92.9 61.2 91.8#
 76 0.0 26.0 39.0#

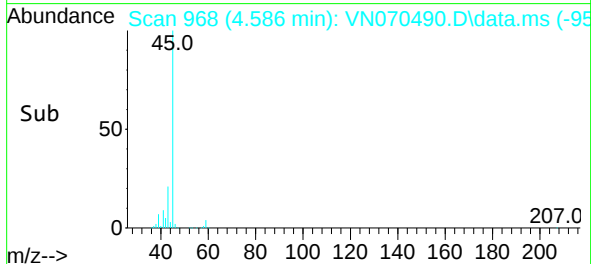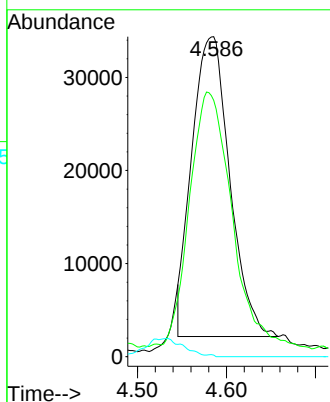

#16
 Acetone
 Concen: 2256.967 ug/l
 RT: 4.283 min Scan# 855
 Delta R.T. -0.002 min
 Lab File: VN070490.D
 Acq: 5 Jan 2022 15:31

Tgt Ion: 43 Resp: 20073058
 Ion Ratio Lower Upper
 43 100
 58 30.3 23.1 34.7


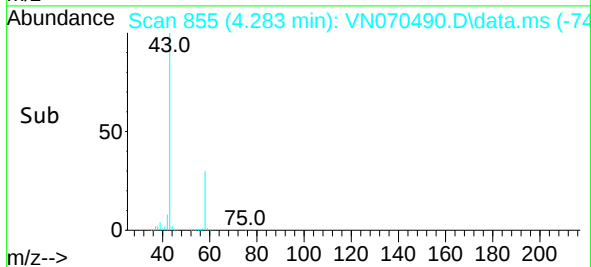
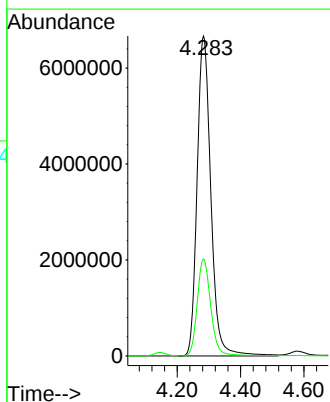
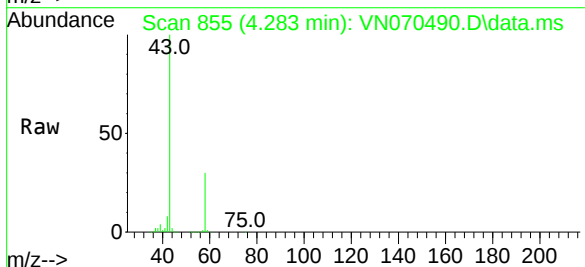




#18
Methyl Acetate
Concen: 10.750 ug/l
RT: 4.578 min Scan# 91
Delta R.T. -0.276 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 276570
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.2#

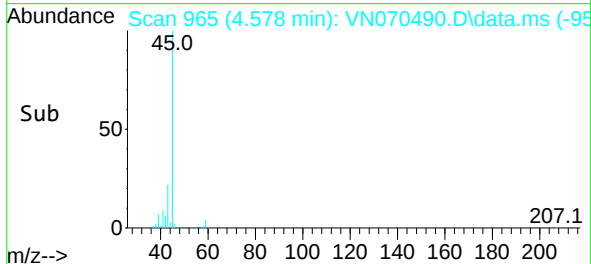

#22
Diisopropyl ether
Concen: 0.363 ug/l
RT: 6.584 min Scan# 1713
Delta R.T. 0.086 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Tgt Ion: 45 Resp: 15561
Ion Ratio Lower Upper
45 100
43 218.9 51.7 77.5#
87 0.0 23.2 34.8#
59 790.5 9.4 14.0#


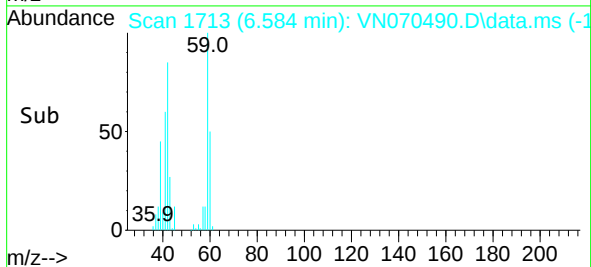

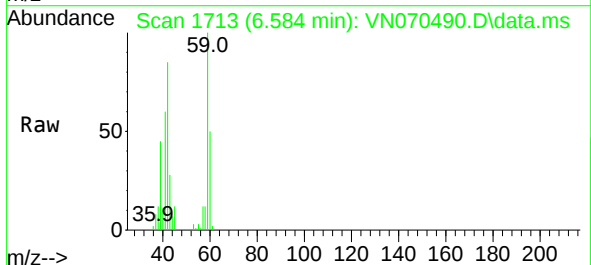


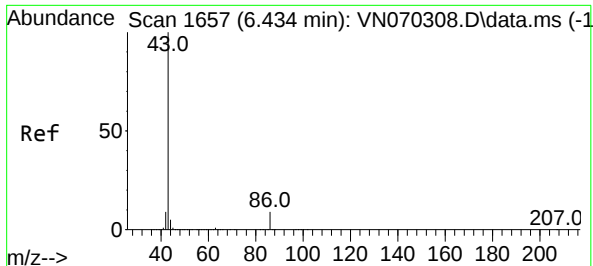

#23
 Vinyl Acetate
 Concen: 1.117 ug/l
 RT: 6.581 min Scan# 11
 Delta R.T. 0.147 min
 Lab File: VN070490.D
 Acq: 5 Jan 2022 15:31




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 43 Resp: 37126
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.5 12.7#

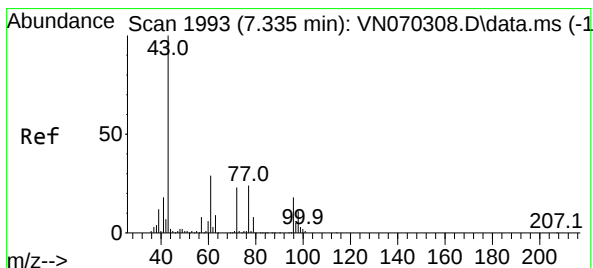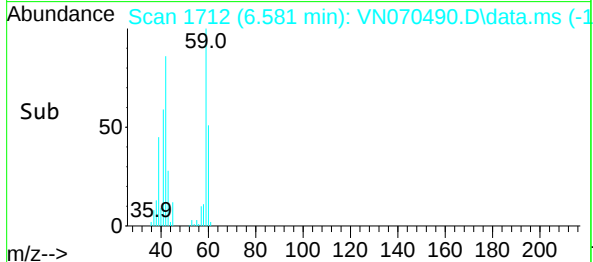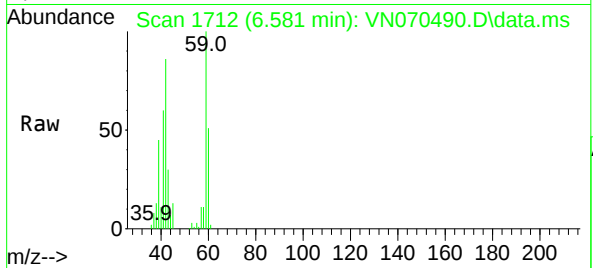

#25
 2-Butanone
 Concen: 7.481 ug/l
 RT: 7.340 min Scan# 1995
 Delta R.T. 0.005 min
 Lab File: VN070490.D
 Acq: 5 Jan 2022 15:31

Tgt Ion: 43 Resp: 83775
 Ion Ratio Lower Upper
 43 100
 72 21.6 21.7 32.5#

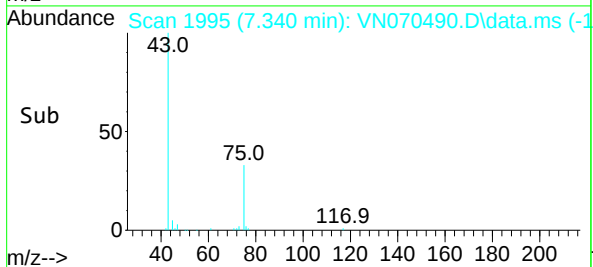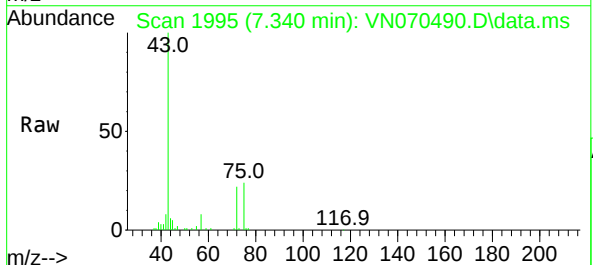



#29

Tetrahydrofuran

Concen: 0.983 ug/l

RT: 7.702 min Scan# 2123

Delta R.T. 0.019 min


Lab File: VN070490.D

Acq: 5 Jan 2022 15:31




Instrument :

MSVOA_N

ClientSampleId :

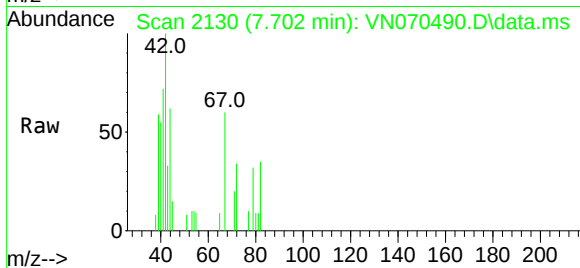

Tgt Ion:	42	Resp:	6568
Ion Ratio	Lower	Upper	
42	100		
72	24.2	36.3	54.5#
71	2.0	34.7	52.1#

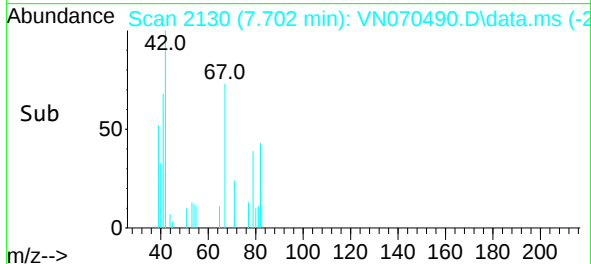

#31

Cyclohexane

Concen: 1.074 ug/l




RT: 8.083 min Scan# 2272


Delta R.T. -0.011 min

Lab File: VN070490.D

Acq: 5 Jan 2022 15:31

Tgt Ion:	56	Resp:	23218
Ion Ratio	Lower	Upper	
56	100		
69	164.4	27.1	40.7#
84	132.0	73.4	110.0#

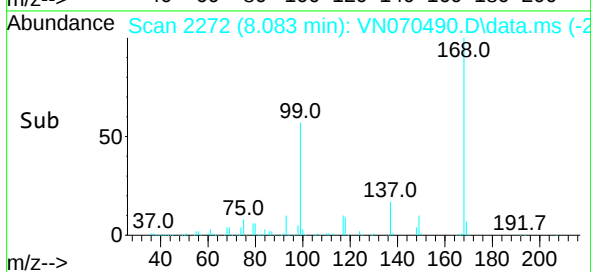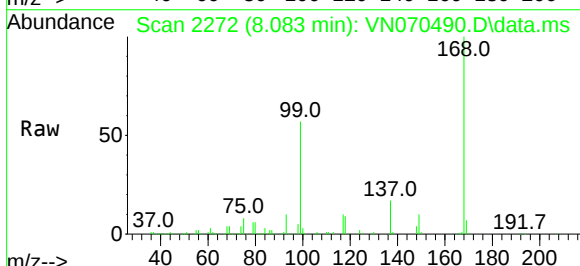



#33

1,2-Dichloroethane-d4

Concen: 48.422 ug/l

RT: 8.437 min Scan# 2404

Delta R.T. -0.000 min

Lab File: VN070490.D

Acq: 5 Jan 2022 15:31

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 663415

Ion Ratio Lower Upper

65 100

67 53.6 0.0 103.0

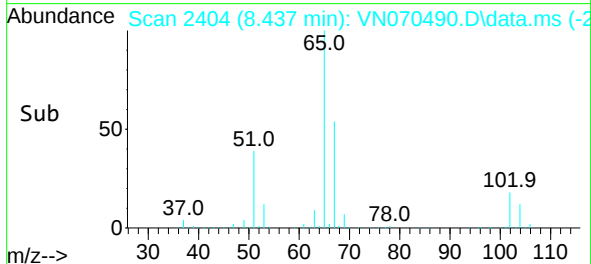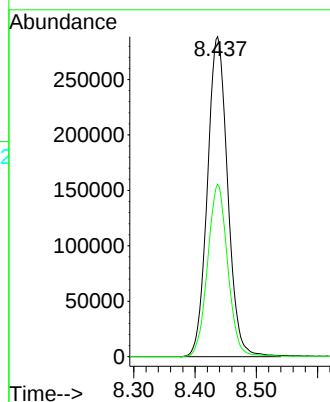

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.965 min Scan# 2601

Delta R.T. -0.003 min

Lab File: VN070490.D

Acq: 5 Jan 2022 15:31




Tgt Ion: 114 Resp: 1601741


Ion Ratio Lower Upper

114 100

63 23.6 0.0 37.8

88 16.4 0.0 27.4


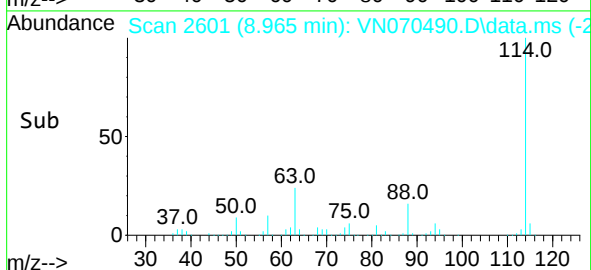
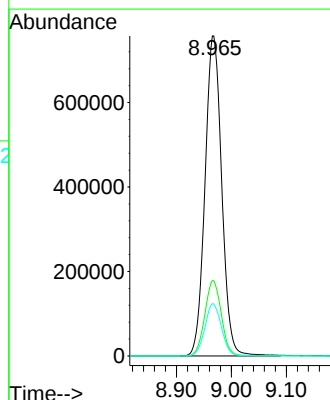





#35
Dibromofluoromethane
Concen: 47.913 ug/l
RT: 8.021 min Scan# 211
Delta R.T. 0.000 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 464337
Ion Ratio Lower Upper
113 100
111 103.5 82.2 123.2
192 19.7 16.9 25.3

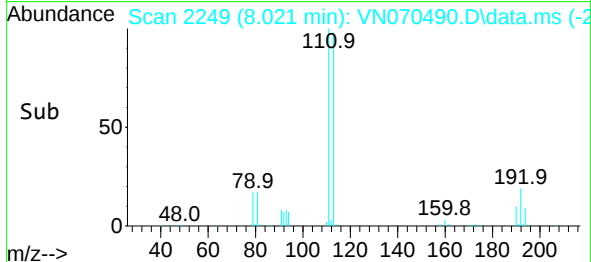

#36
1,1-Dichloropropene
Concen: 4.804 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.137 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31


Tgt Ion: 75 Resp: 77019
Ion Ratio Lower Upper
75 100
110 7.7 18.4 55.2#
77 0.0 24.4 36.6#

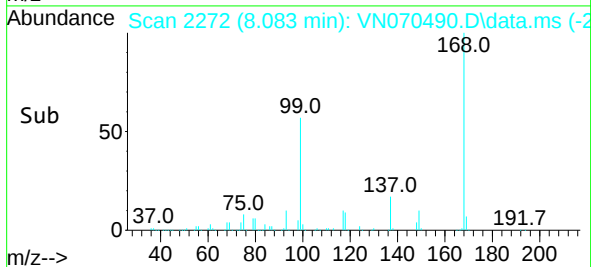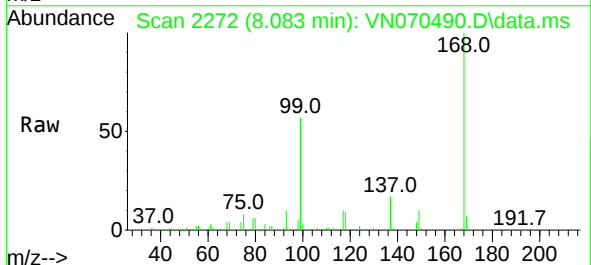






#37
Ethyl Acetate
Concen: 4.031 ug/l
RT: 7.340 min Scan# 1995
Delta R.T. -0.072 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 83775
Ion Ratio Lower Upper
43 100
61 0.3 11.5 17.3#
70 0.0 7.9 11.9#

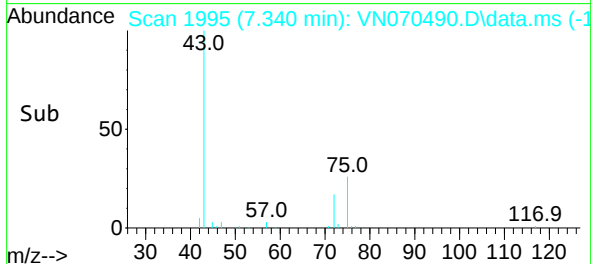

#38
Carbon Tetrachloride
Concen: 5.943 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.123 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31


Tgt Ion: 117 Resp: 90981
Ion Ratio Lower Upper
117 100
119 5.0 76.1 114.1#
121 0.0 24.2 36.2#

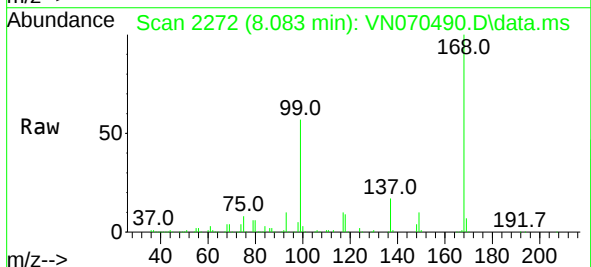






#40
Benzene
Concen: 0.497 ug/l
RT: 8.461 min Scan# 2412
Delta R.T. 0.003 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 78 Resp: 24452
Ion Ratio Lower Upper
78 100
77 25.0 18.6 27.8

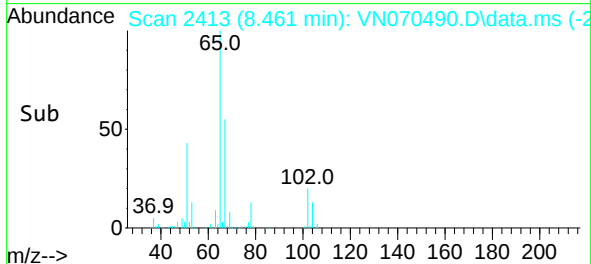

#48
Methyl methacrylate
Concen: 0.439 ug/l
RT: 9.534 min Scan# 2813
Delta R.T. -0.024 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Tgt Ion: 41 Resp: 6859
Ion Ratio Lower Upper
41 100
69 0.0 72.4 108.6#
39 9.0 58.4 87.6#

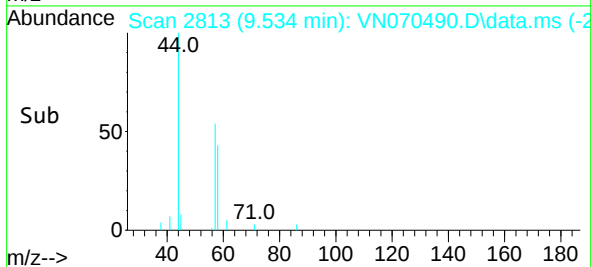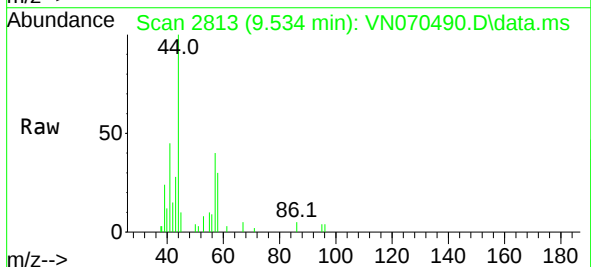



#49

1,4-Dioxane

Concen: 0.219 ug/l

RT: 9.574 min Scan# 21

Delta R.T. 0.005 min


Lab File: VN070490.D

Acq: 5 Jan 2022 15:31

Instrument :

MSVOA_N

ClientSampleId :

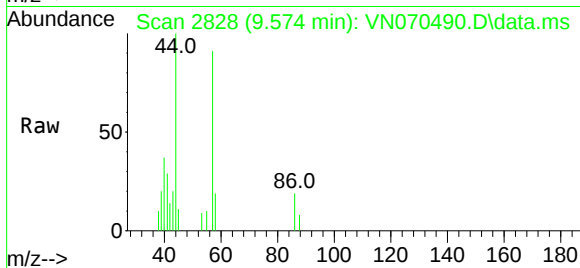




Tgt Ion: 88 Resp: 50

Ion Ratio Lower Upper

88 100

43 0.0 23.4 35.2#

58 0.0 50.6 75.8#



#50

Toluene-d8

Concen: 47.859 ug/l

RT: 10.440 min Scan# 3151

Delta R.T. 0.000 min

Lab File: VN070490.D




Acq: 5 Jan 2022 15:31


Tgt Ion: 98 Resp: 1894749

Ion Ratio Lower Upper

98 100

100 64.0 50.4 75.6


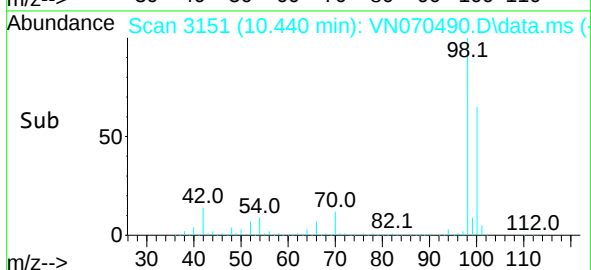

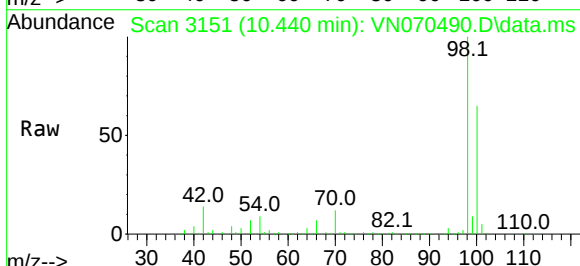




#51
4-Methyl-2-Pentanone
Concen: 4.756 ug/l
RT: 10.330 min Scan# 3110
Delta R.T. 0.000 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 97905
Ion Ratio Lower Upper
43 100
58 35.4 30.4 45.6

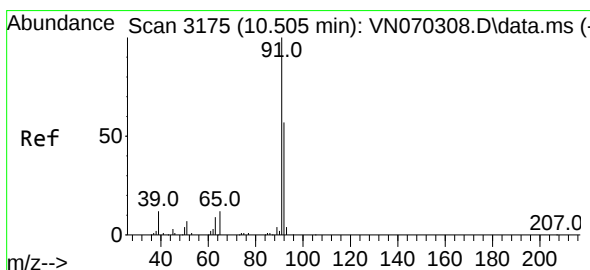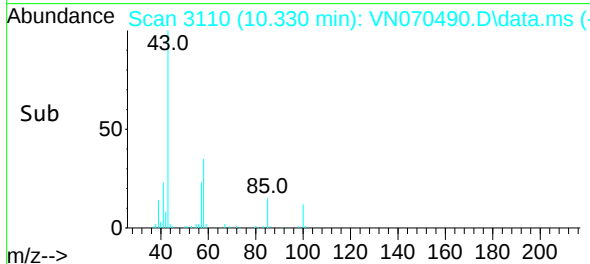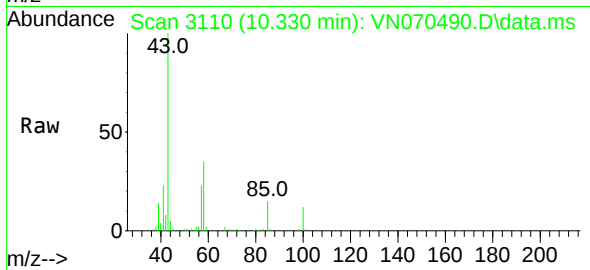

#52
Toluene
Concen: 1.492 ug/l
RT: 10.505 min Scan# 3175
Delta R.T. -0.000 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Tgt Ion: 92 Resp: 44374
Ion Ratio Lower Upper
92 100
91 173.9 142.0 213.0




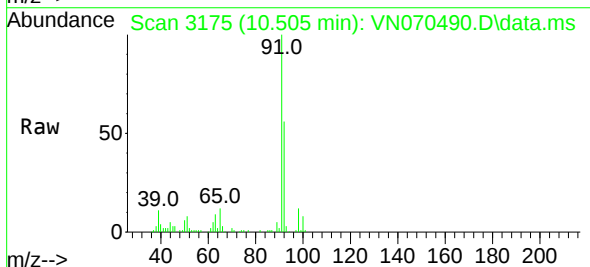




#58
2-Chloroethyl Vinyl ether
Concen: 18.523 ug/l
RT: 9.856 min Scan# 2933
Delta R.T. -0.185 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 52
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

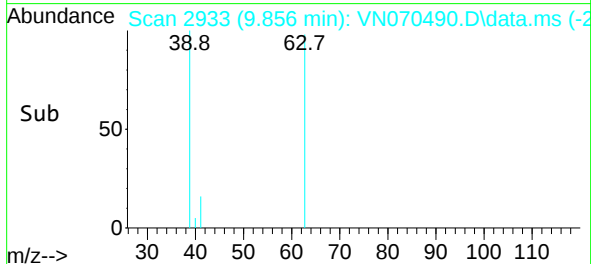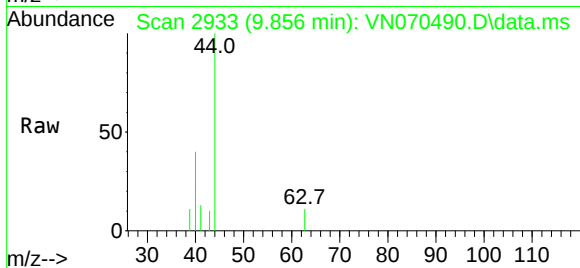

#59
2-Hexanone
Concen: 0.533 ug/l
RT: 11.084 min Scan# 3391
Delta R.T. 0.000 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Tgt Ion: 43 Resp: 7996
Ion Ratio Lower Upper
43 100
58 47.7 26.9 80.7


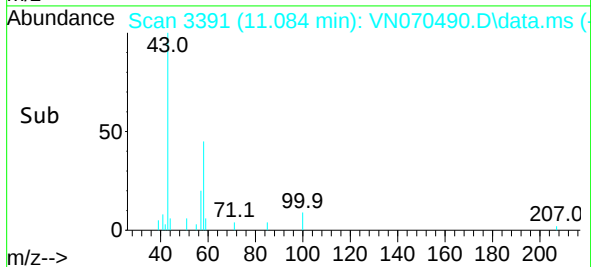

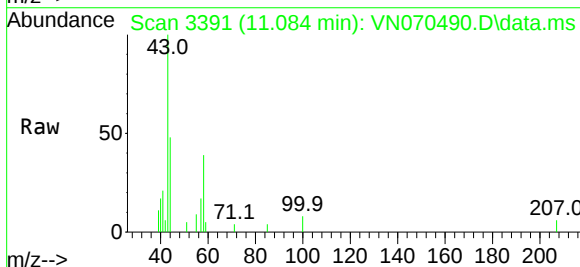




#62
4-Bromofluorobenzene
Concen: 48.683 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 696120
Ion Ratio Lower Upper
95 100
174 76.6 0.0 187.2
176 73.9 0.0 181.4

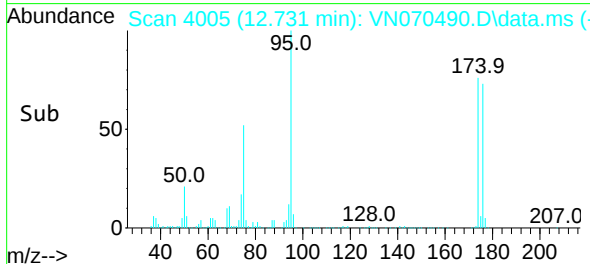

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.000 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Tgt Ion: 117 Resp: 1442641
Ion Ratio Lower Upper
117 100
82 58.8 42.4 63.6
119 31.8 25.4 38.2


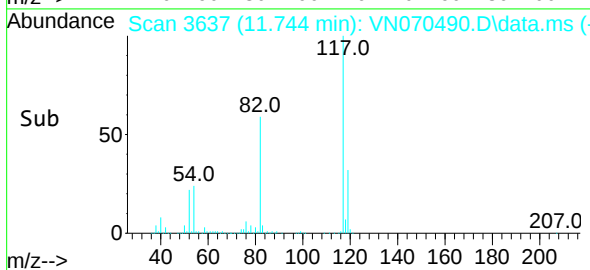

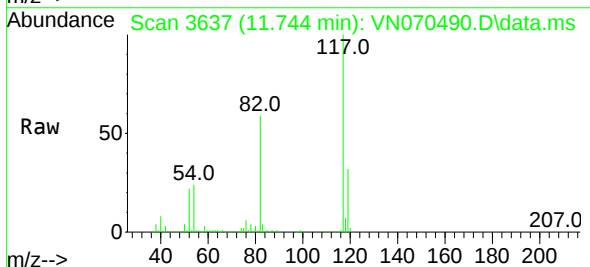




#67
Ethyl Benzene
Concen: 0.365 ug/l
RT: 11.846 min Scan# 3074
Delta R.T. 0.003 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 20467
Ion Ratio Lower Upper
91 100
106 31.7 25.7 38.5

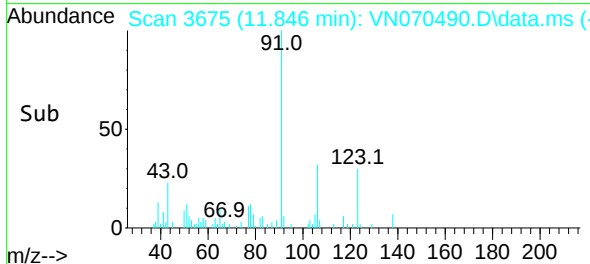

#68
m/p-Xylenes
Concen: 1.507 ug/l
RT: 11.950 min Scan# 3714
Delta R.T. -0.003 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31

Tgt Ion:106 Resp: 30762
Ion Ratio Lower Upper
106 100
91 207.0 160.6 240.8


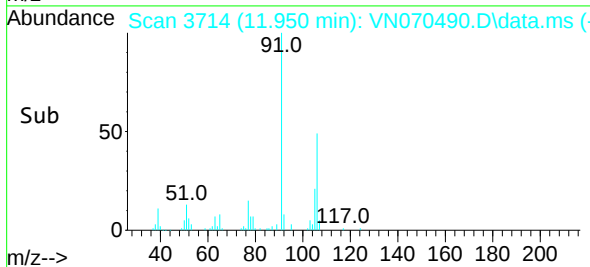

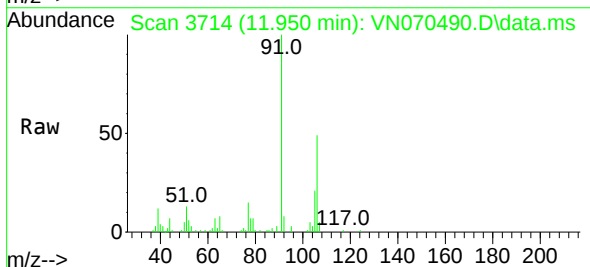




#69
o-Xylene
Concen: 0.757 ug/l
RT: 12.280 min Scan# 31
Delta R.T. 0.002 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 15368
Ion Ratio Lower Upper
106 100
91 223.5 105.8 317.3

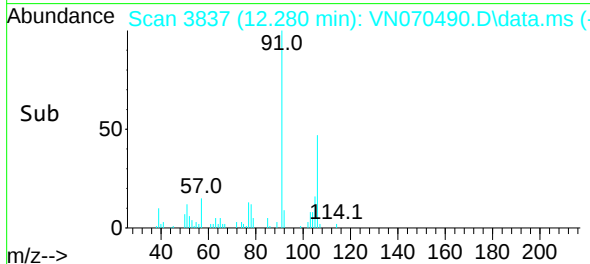

#71
Bromoform
Concen: 0.410 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.274 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31


Tgt Ion:173 Resp: 3328
Ion Ratio Lower Upper
173 100
175 1107.0 24.2 72.6#
254 0.0 0.0 0.0

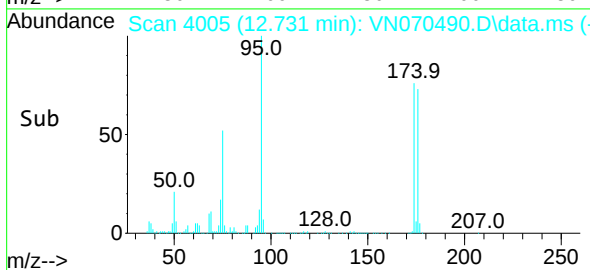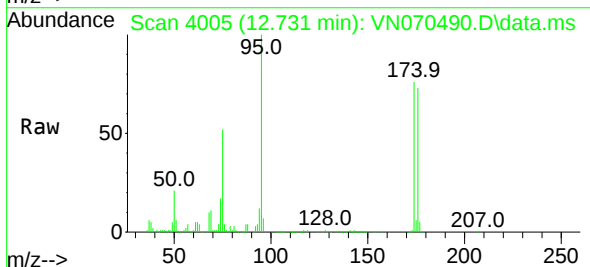






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 41
Delta R.T. 0.003 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:152 Resp: 494220
Ion Ratio Lower Upper
152 100
115 60.1 27.5 82.5
150 157.3 0.0 344.4




#75
1,1,2,2-Tetrachloroethane
Concen: 3.027 ug/l
RT: 12.685 min Scan# 3988
Delta R.T. -0.140 min
Lab File: VN070490.D
Acq: 5 Jan 2022 15:31




Tgt Ion: 83 Resp: 43209
Ion Ratio Lower Upper
83 100
131 0.0 5.5 16.5#
85 5.9 32.4 97.2#

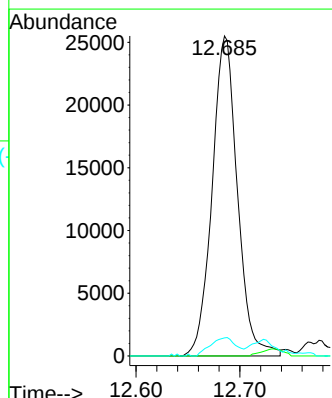






#76
 1,2,3-Trichloropropane
 Concen: 26.102 ug/l
 RT: 12.731 min Scan# 4060
 Delta R.T. -0.147 min
 Lab File: VN070490.D
 Acq: 5 Jan 2022 15:31

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion: 75 Resp: 361683
 Ion Ratio Lower Upper
 75 100
 77 1.3 82.6 247.8#



#80
 1,3,5-Trimethylbenzene
 Concen: 0.204 ug/l
 RT: 13.058 min Scan# 4127
 Delta R.T. -0.000 min
 Lab File: VN070490.D
 Acq: 5 Jan 2022 15:31


Tgt Ion: 105 Resp: 7521
 Ion Ratio Lower Upper
 105 100
 120 49.0 24.6 73.6

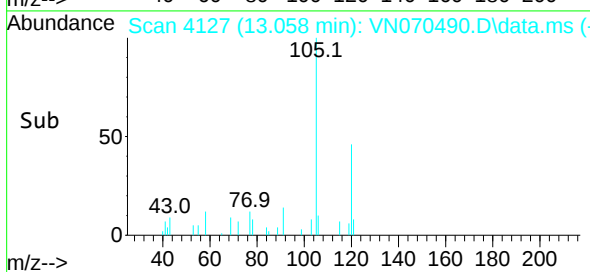






#81
 trans-1,4-Dichloro-2-butene
 Concen: 89.412 ug/l
 RT: 12.731 min Scan# 4005
 Delta R.T. 0.107 min
 Lab File: VN070490.D
 Acq: 5 Jan 2022 15:31


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion: 75 Resp: 361683
 Ion Ratio Lower Upper
 75 100
 53 0.0 90.5 135.7#
 89 0.0 38.2 57.4#




#84
 1,2,4-Trimethylbenzene
 Concen: 0.458 ug/l
 RT: 13.366 min Scan# 4242
 Delta R.T. 0.000 min
 Lab File: VN070490.D
 Acq: 5 Jan 2022 15:31



Tgt Ion: 105 Resp: 16207
 Ion Ratio Lower Upper
 105 100
 120 40.1 22.8 68.4

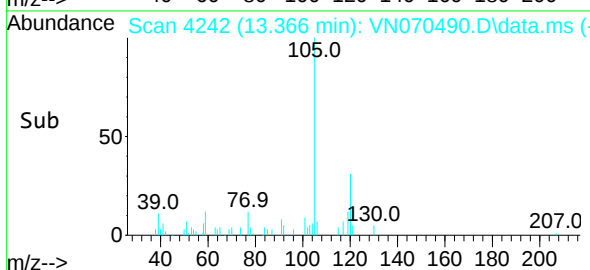



#95

Naphthalene

Concen: 2.352 ug/l

RT: 15.504 min Scan# 5039

Delta R.T. -0.000 min

Lab File: VN070490.D





Acq: 5 Jan 2022 15:31

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:	128	Resp:	12971
Ion Ratio	Lower	Upper	
128	100		
127	14.3	10.5	15.7
129	9.0	8.7	13.1

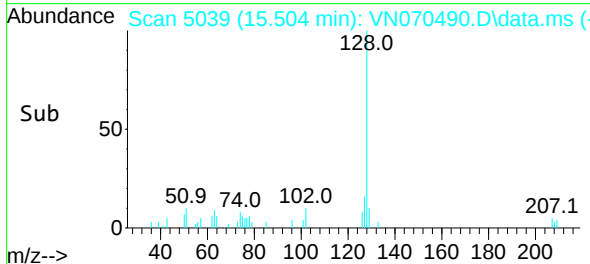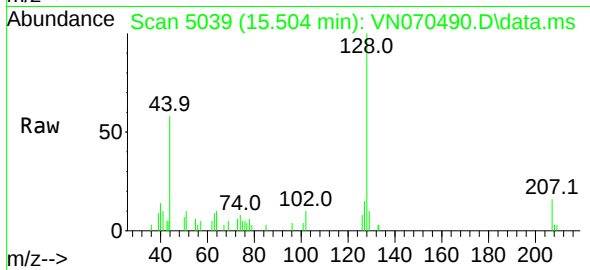

#96

1,2,3-Trichlorobenzene

Concen: 1.037 ug/l

RT: 15.705 min Scan# 5114

Delta R.T. 0.005 min

Lab File: VN070490.D

Acq: 5 Jan 2022 15:31

Tgt Ion:	180	Resp:	1671
Ion Ratio	Lower	Upper	
180	100		
182	90.7	47.4	142.2
145	28.1	15.0	45.1

