

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010522\
 Data File : VN070494.D
 Acq On : 5 Jan 2022 17:12
 Operator : JC/MD
 Sample : N1012-11
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jan 06 12:35:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	619168	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1181444	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	807228	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	199606	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	686374	77.099	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 154.200%#	
35) Dibromofluoromethane	8.021	113	457402	63.987	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 127.980%	
50) Toluene-d8	10.440	98	1208435	41.382	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 82.760%	
62) 4-Bromofluorobenzene	12.731	95	356108	33.764	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 67.520%	
Target Compounds						Qvalue
3) Chloromethane	2.301	50	6121	0.641	ug/l #	77
5) Bromomethane	2.858	94	996	0.222	ug/l	88
11) Tert butyl alcohol	5.374	59	9495	6.406	ug/l #	87
13) Acrolein	4.041	56	944	0.785	ug/l #	23
16) Acetone	4.288	43	145797	25.228	ug/l	100
17) Carbon Disulfide	4.527	76	3981	0.231	ug/l #	74
20) Methylene Chloride	5.095	84	7749	0.969	ug/l	93
25) 2-Butanone	7.064	43	685731	94.238	ug/l #	23
29) Tetrahydrofuran	7.689	42	2091	0.482	ug/l #	61
31) Cyclohexane	8.086	56	18833	1.341	ug/l #	22
36) 1,1-Dichloropropene	8.083	75	51132	4.324	ug/l #	48
37) Ethyl Acetate	7.340	43	15441	1.007	ug/l #	69
38) Carbon Tetrachloride	8.083	117	59969	5.311	ug/l #	16
39) Methylcyclohexane	9.459	83	6176	0.431	ug/l	92
40) Benzene	8.461	78	38526	1.063	ug/l	100
48) Methyl methacrylate	9.528	41	46789	4.059	ug/l #	34
49) 1,4-Dioxane	9.574	88	85	0.504	ug/l #	27
51) 4-Methyl-2-Pentanone	10.330	43	22310	1.469	ug/l	99
52) Toluene	10.502	92	264447	12.051	ug/l	99
59) 2-Hexanone	11.092	43	4671	0.422	ug/l	68
67) Ethyl Benzene	11.843	91	14177	0.452	ug/l	98
68) m/p-Xylenes	11.950	106	23412	2.050	ug/l	90
69) o-Xylene	12.275	106	8620	0.759	ug/l	90
75) 1,1,2,2-Tetrachloroethane	12.833	83	203	0.477	ug/l #	25
76) 1,2,3-Trichloropropane	12.731	75	182329	31.901	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.058	105	3715	0.250	ug/l	92
81) trans-1,4-Dichloro-2-b...	12.731	75	182329	111.602	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.369	105	8685	0.607	ug/l	90
95) Naphthalene	15.504	128	6193	2.453	ug/l #	94
96) 1,2,3-Trichlorobenzene	15.697	180	524	0.990	ug/l #	57

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010522\
Data File : VN070494.D
Acq On : 5 Jan 2022 17:12
Operator : JC/MD
Sample : N1012-11
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Jan 06 12:35:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration

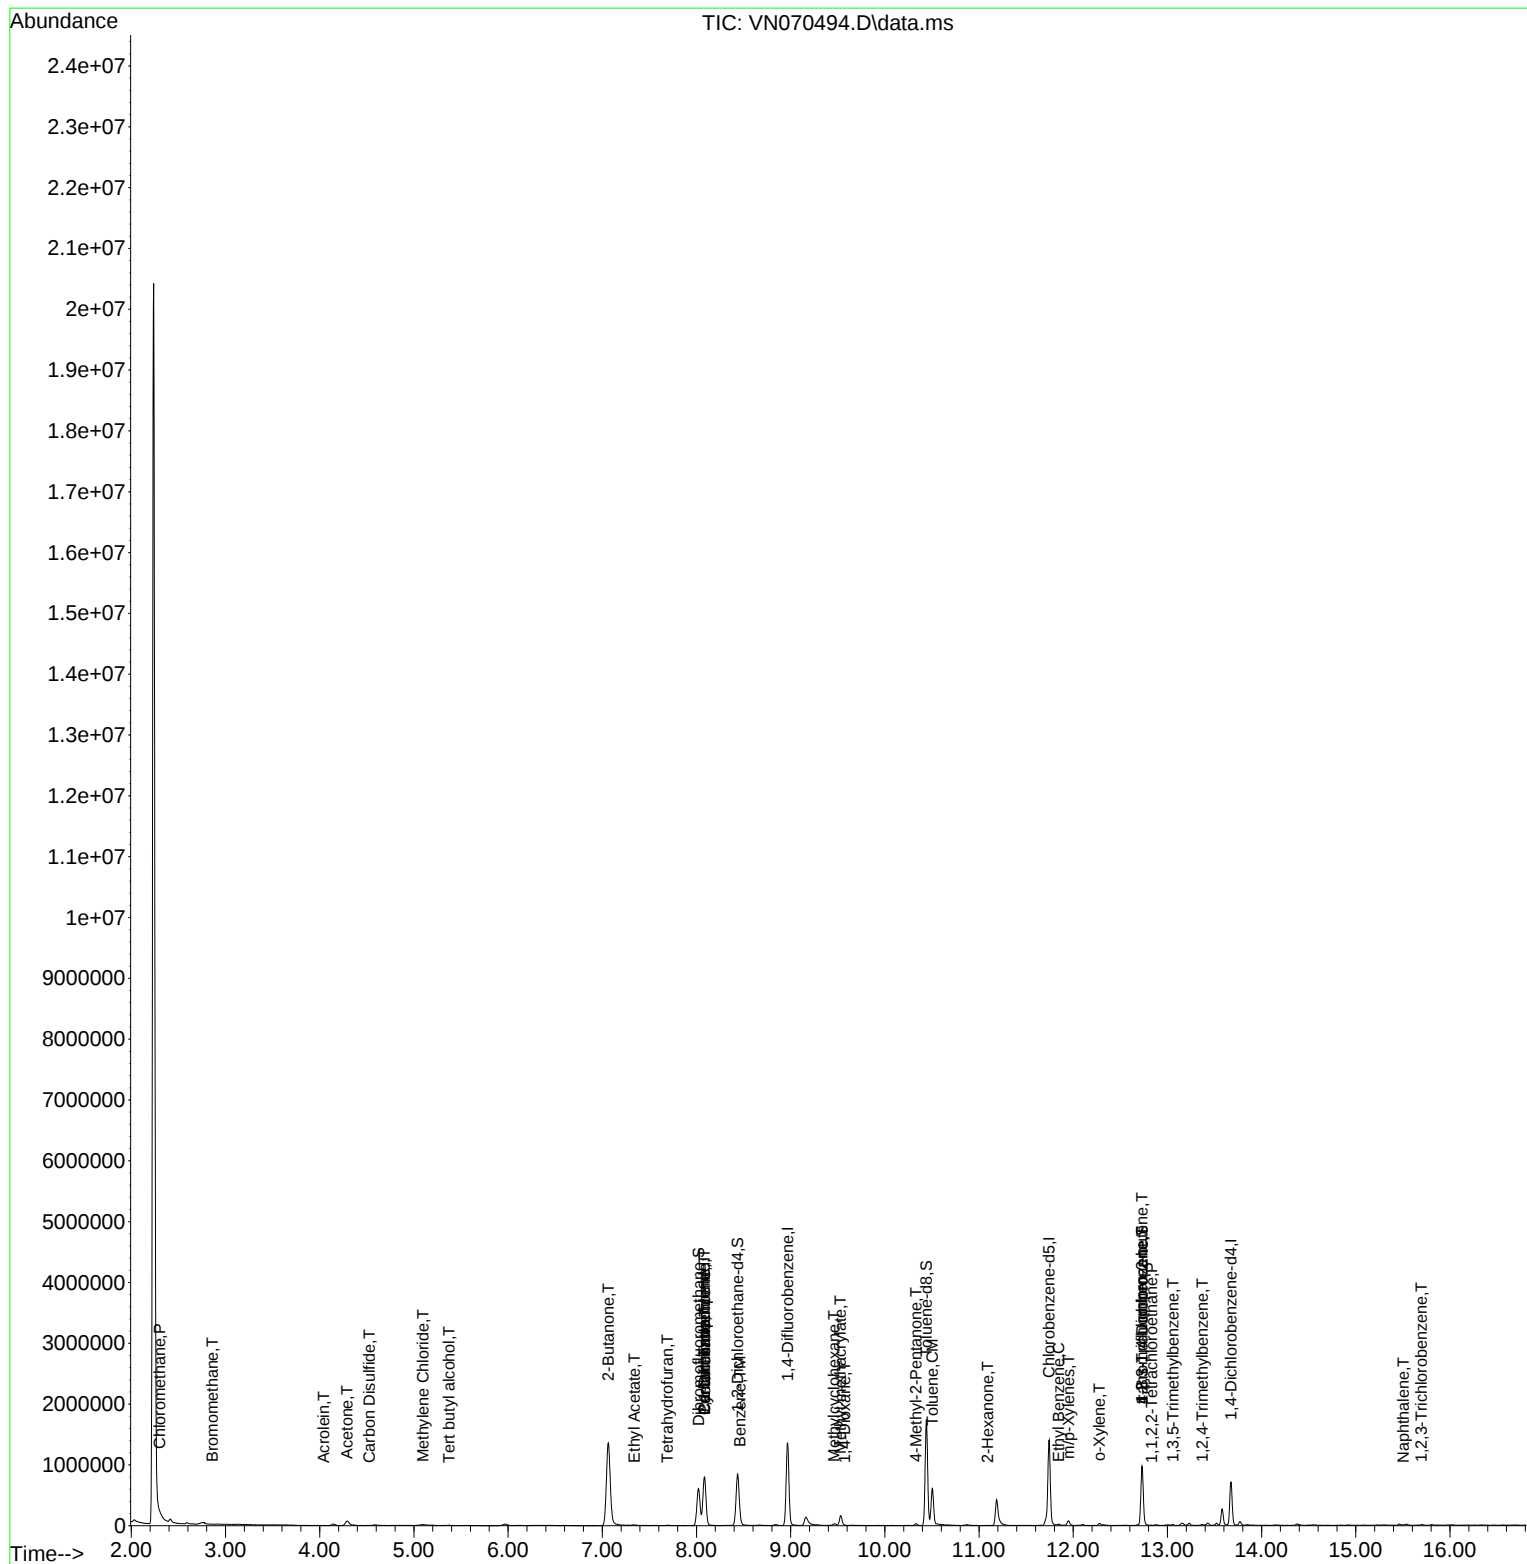






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Instrument :
MSVOA_N
ClientSampleId :



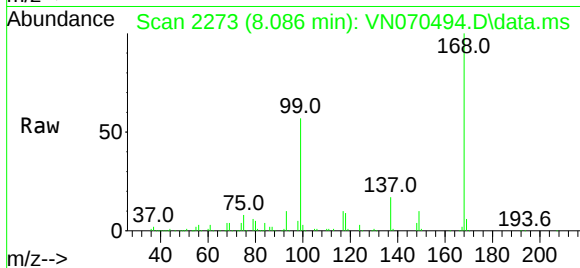



Tgt Ion:168 Resp: 619168
Ion Ratio Lower Upper
168 100
99 57.3 41.3 61.9

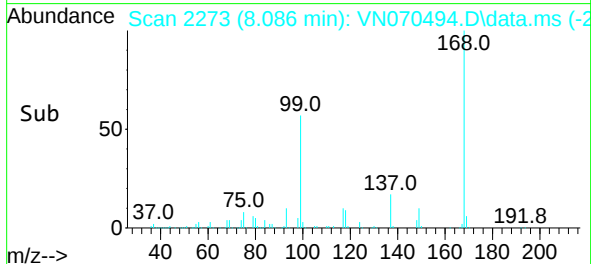

#3
Chloromethane
Concen: 0.641 ug/l
RT: 2.301 min Scan# 116
Delta R.T. -0.002 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Tgt Ion: 50 Resp: 6121
Ion Ratio Lower Upper
50 100
52 18.7 25.4 38.0#


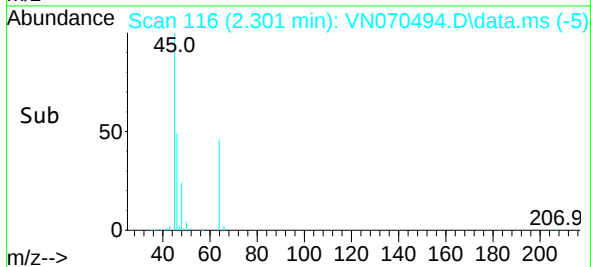

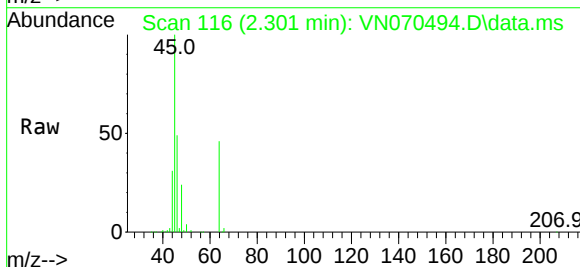




#5
Bromomethane
Concen: 0.222 ug/l
RT: 2.858 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 996
Ion Ratio Lower Upper
94 100
96 80.7 73.8 110.8

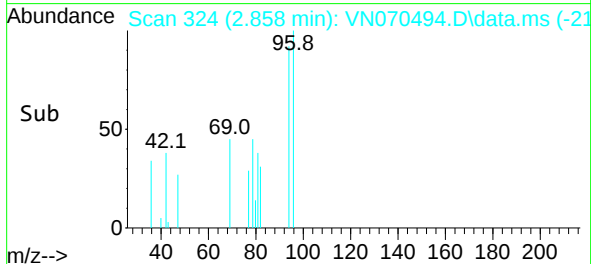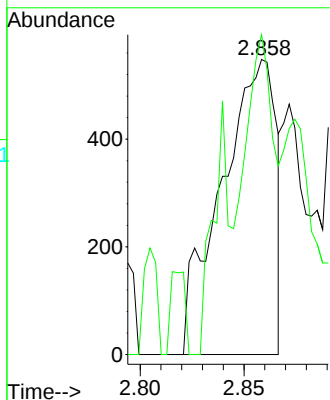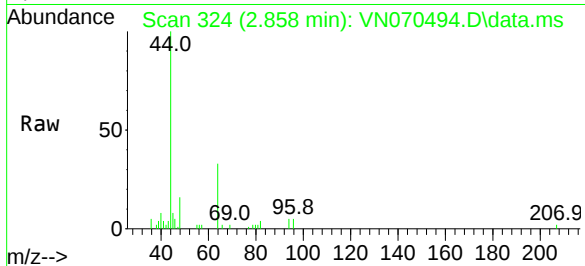

#11
Tert butyl alcohol
Concen: 6.406 ug/l
RT: 5.374 min Scan# 1262
Delta R.T. -0.003 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12


Tgt Ion: 59 Resp: 9495
Ion Ratio Lower Upper
59 100
57 6.0 8.7 13.1#

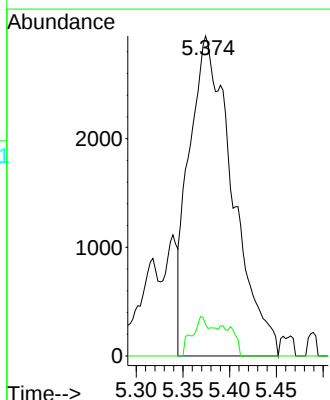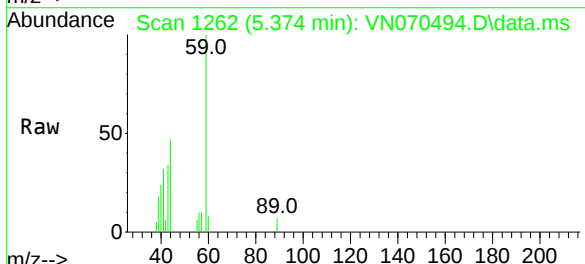






#13
Acrolein
Concen: 0.785 ug/l
RT: 4.041 min Scan# 765
Delta R.T. 0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 944
Ion Ratio Lower Upper
56 100
55 7.5 56.6 85.0#

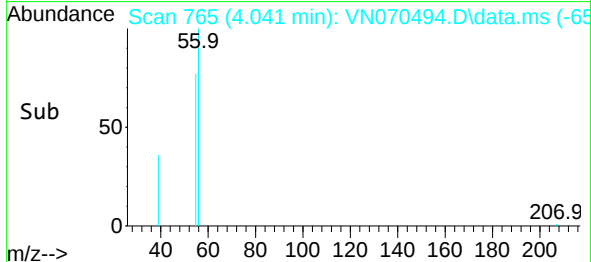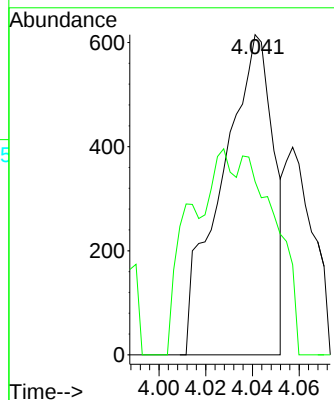

#16
Acetone
Concen: 25.228 ug/l
RT: 4.288 min Scan# 857
Delta R.T. 0.003 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12


Tgt Ion: 43 Resp: 145797
Ion Ratio Lower Upper
43 100
58 28.9 23.1 34.7

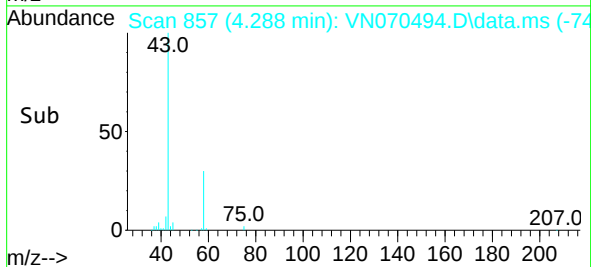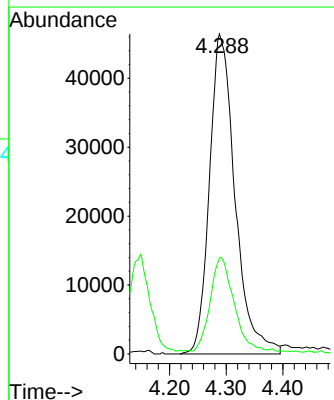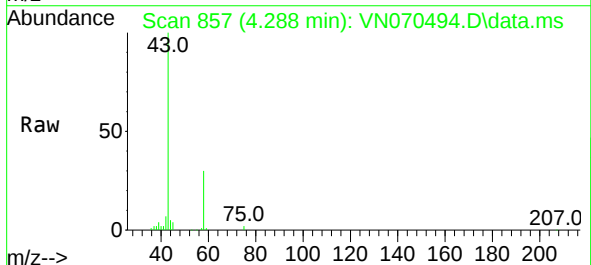



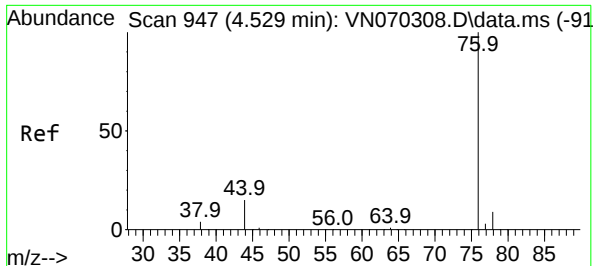


#17
Carbon Disulfide
Concen: 0.231 ug/l
RT: 4.527 min Scan# 947
Delta R.T. -0.002 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Instrument :
MSVOA_N
ClientSampleId :



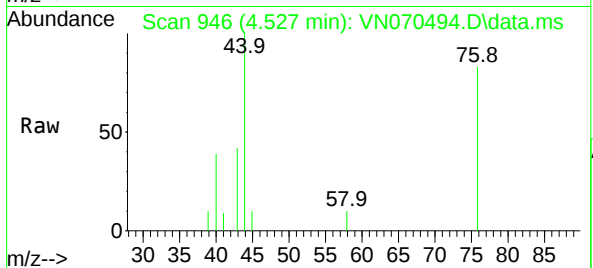



Tgt Ion: 76 Resp: 3981
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#

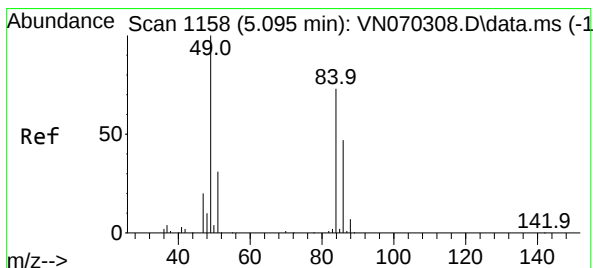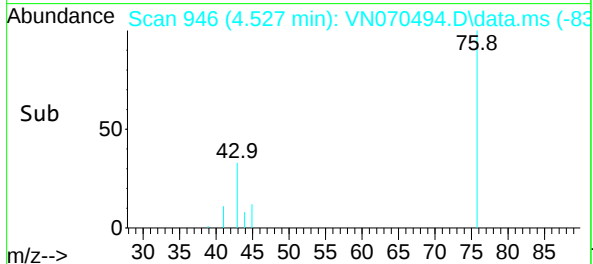

#20
Methylene Chloride
Concen: 0.969 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Tgt Ion: 84 Resp: 7749
Ion Ratio Lower Upper
84 100
49 125.3 93.5 140.3
51 34.0 29.4 44.2
86 59.6 53.0 79.4

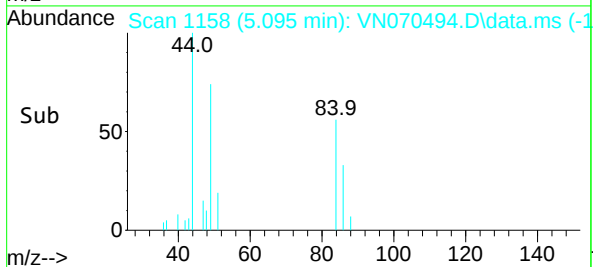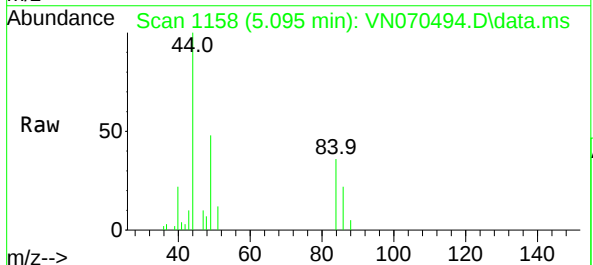

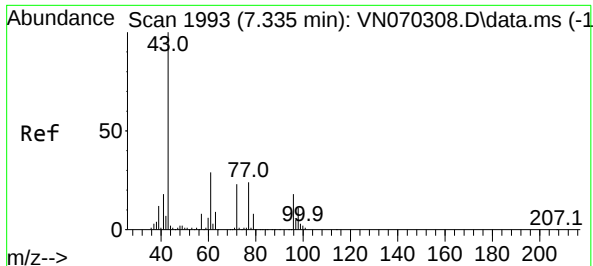

#25

2-Butanone

Concen: 94.238 ug/l

RT: 7.064 min Scan# 11

Delta R.T. -0.271 min


Lab File: VN070494.D

Acq: 5 Jan 2022 17:12

Instrument :

MSVOA_N

ClientSampleId :



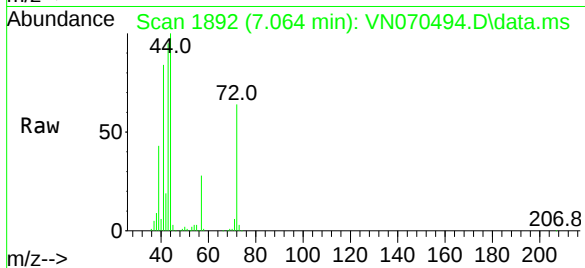


Tgt Ion: 43 Resp: 685731

Ion Ratio Lower Upper

43 100

72 67.0 21.7 32.5#

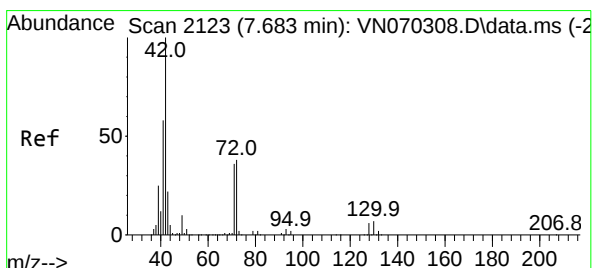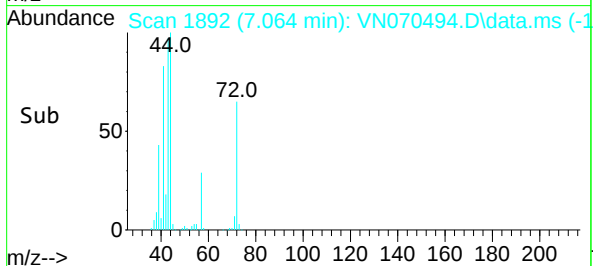

#29

Tetrahydrofuran

Concen: 0.482 ug/l

RT: 7.689 min Scan# 2125

Delta R.T. 0.006 min

Lab File: VN070494.D

Acq: 5 Jan 2022 17:12




Tgt Ion: 42 Resp: 2091


Ion Ratio Lower Upper

42 100

72 24.0 36.3 54.5#


71 14.6 34.7 52.1#

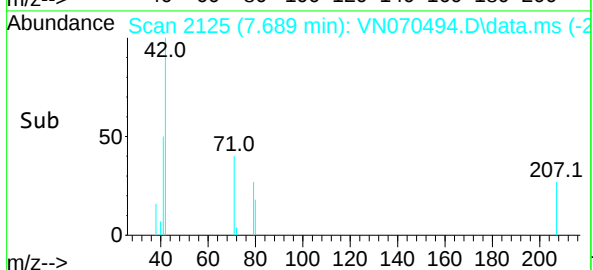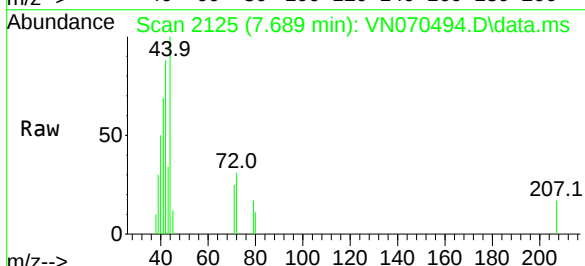






#31
Cyclohexane
Concen: 1.341 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.008 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 18833
Ion Ratio Lower Upper
56 100
69 149.2 27.1 40.7#
84 122.0 73.4 110.0#

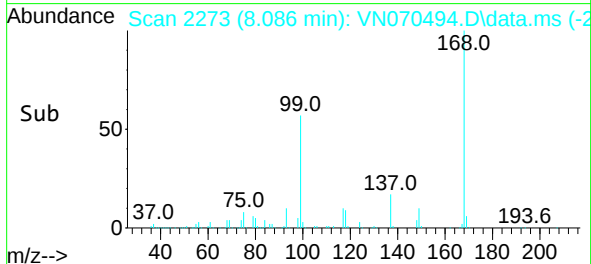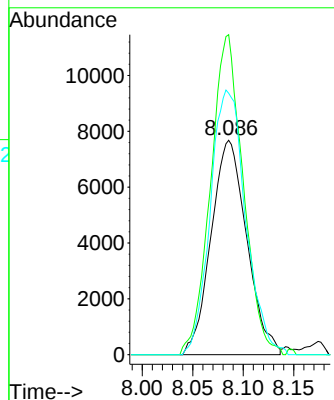

#33
1,2-Dichloroethane-d4
Concen: 77.099 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Tgt Ion: 65 Resp: 686374
Ion Ratio Lower Upper
65 100
67 53.2 0.0 103.0


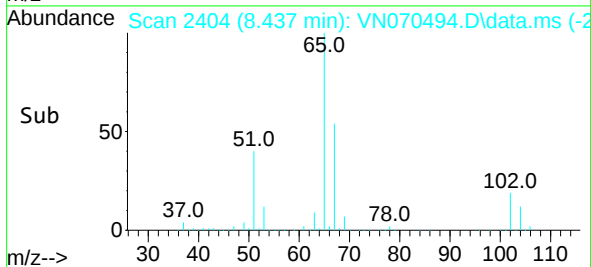
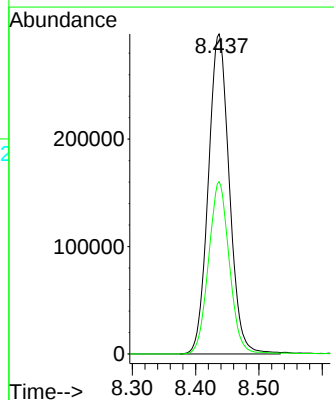
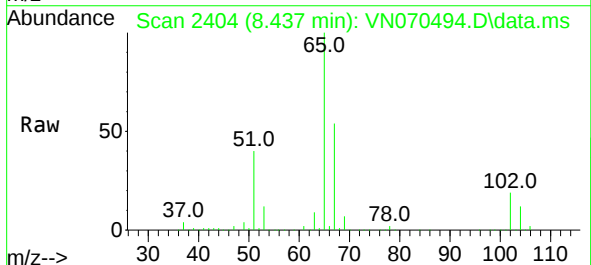




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:114 Resp: 1181444
Ion Ratio Lower Upper
114 100
63 23.4 0.0 37.8
88 16.2 0.0 27.4

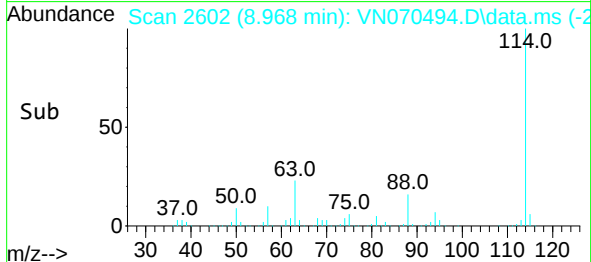

#35
Dibromofluoromethane
Concen: 63.987 ug/l
RT: 8.021 min Scan# 2249
Delta R.T. 0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12


Tgt Ion:113 Resp: 457402
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.2
192 19.7 16.9 25.3

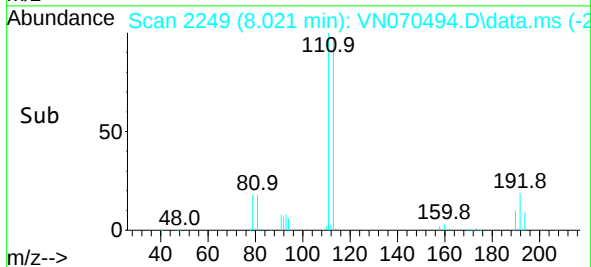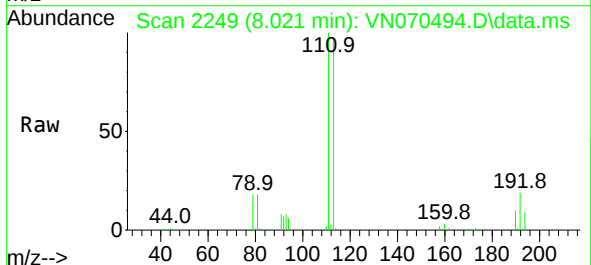






#36
 1,1-Dichloropropene
 Concen: 4.324 ug/l
 RT: 8.083 min Scan# 21
 Delta R.T. -0.137 min
 Lab File: VN070494.D
 Acq: 5 Jan 2022 17:12

Instrument :
 MSVOA_N
 ClientSampleId :



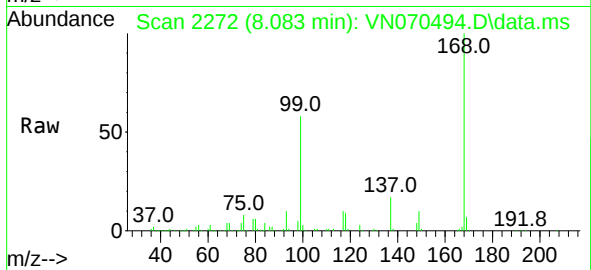



Tgt Ion: 75 Resp: 51132
 Ion Ratio Lower Upper
 75 100
 110 7.8 18.4 55.2#
 77 0.0 24.4 36.6#

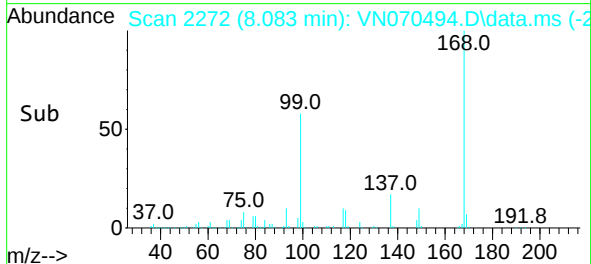

#37
 Ethyl Acetate
 Concen: 1.007 ug/l
 RT: 7.340 min Scan# 1995
 Delta R.T. -0.072 min
 Lab File: VN070494.D
 Acq: 5 Jan 2022 17:12


Tgt Ion: 43 Resp: 15441
 Ion Ratio Lower Upper
 43 100
 61 0.0 11.5 17.3#
 70 0.4 7.9 11.9#

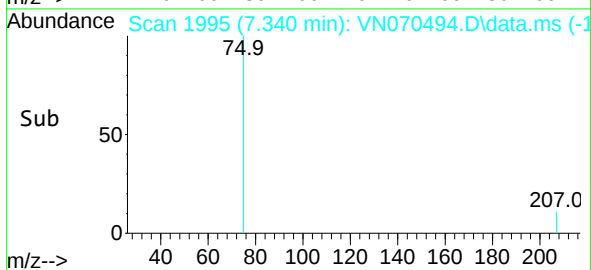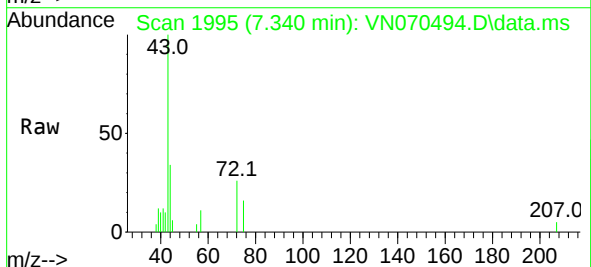






#38
Carbon Tetrachloride
Concen: 5.311 ug/l
RT: 8.083 min Scan# 211
Delta R.T. -0.123 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 59969
Ion Ratio Lower Upper
117 100
119 5.2 76.1 114.1#
121 0.0 24.2 36.2#

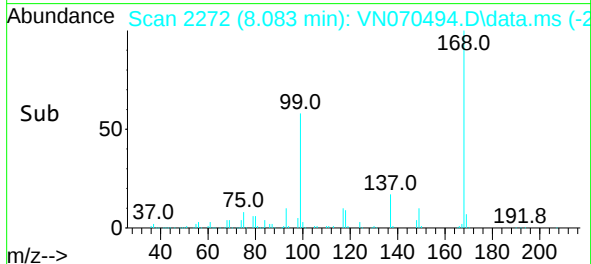

#39
Methylcyclohexane
Concen: 0.431 ug/l
RT: 9.459 min Scan# 2785
Delta R.T. -0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Tgt Ion: 83 Resp: 6176
Ion Ratio Lower Upper
83 100
55 64.1 58.1 87.1
98 51.2 38.4 57.6




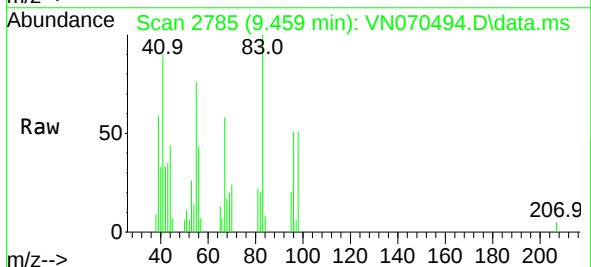




#40
Benzene
Concen: 1.063 ug/l
RT: 8.461 min Scan# 2412
Delta R.T. 0.003 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 78 Resp: 38526
Ion Ratio Lower Upper
78 100
77 23.1 18.6 27.8

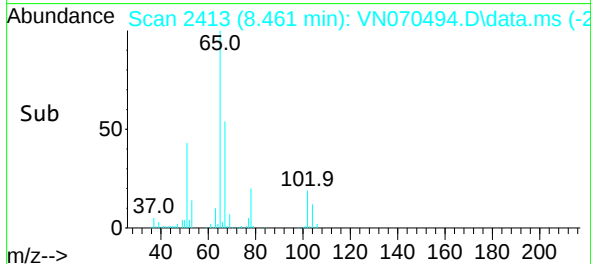

#48
Methyl methacrylate
Concen: 4.059 ug/l
RT: 9.528 min Scan# 2811
Delta R.T. -0.030 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Tgt Ion: 41 Resp: 46789
Ion Ratio Lower Upper
41 100
69 0.9 72.4 108.6#
39 47.4 58.4 87.6#

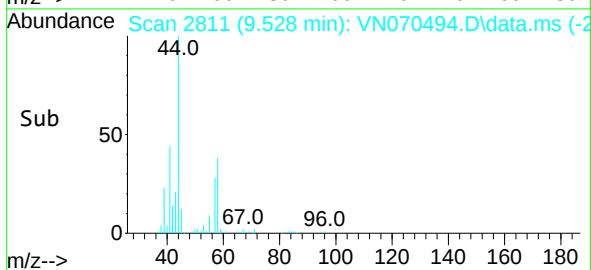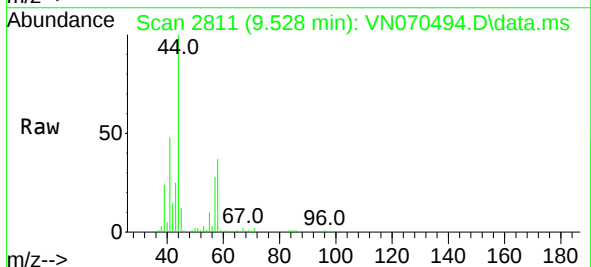



#49

1,4-Dioxane

Concen: 0.504 ug/l

RT: 9.574 min Scan# 21

Delta R.T. 0.005 min


Lab File: VN070494.D

Acq: 5 Jan 2022 17:12

Instrument :

MSVOA_N

ClientSampleId :

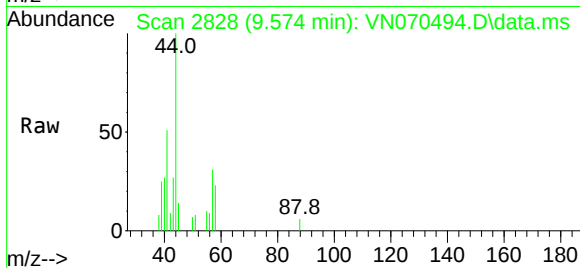




Tgt Ion: 88 Resp: 85

Ion Ratio Lower Upper

88 100

43 0.0 23.4 35.2#

58 0.0 50.6 75.8#



#50

Toluene-d8

Concen: 41.382 ug/l

RT: 10.440 min Scan# 3151

Delta R.T. 0.000 min

Lab File: VN070494.D




Acq: 5 Jan 2022 17:12


Tgt Ion: 98 Resp: 1208435

Ion Ratio Lower Upper

98 100


100 64.5 50.4 75.6

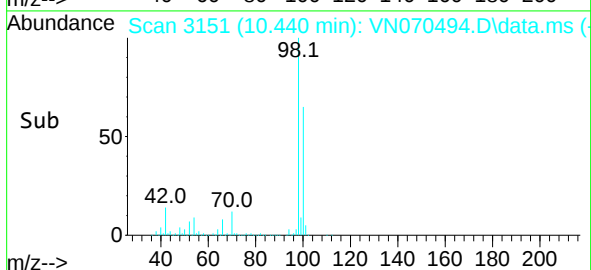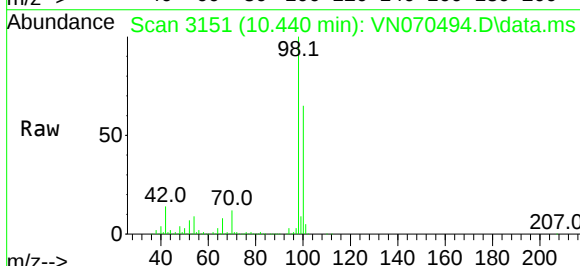






#51
4-Methyl-2-Pentanone
Concen: 1.469 ug/l
RT: 10.330 min Scan# 3110
Delta R.T. 0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 43 Resp: 22310
Ion Ratio Lower Upper
43 100
58 37.2 30.4 45.6

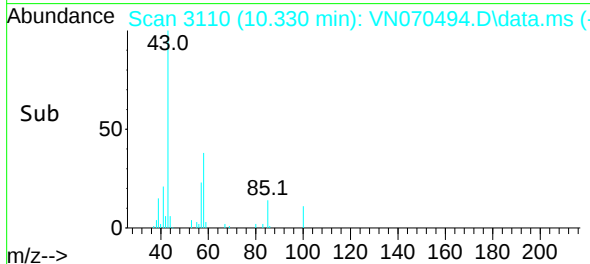


#52
Toluene
Concen: 12.051 ug/l
RT: 10.502 min Scan# 3174
Delta R.T. -0.003 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12




Tgt Ion: 92 Resp: 264447
Ion Ratio Lower Upper
92 100
91 175.5 142.0 213.0

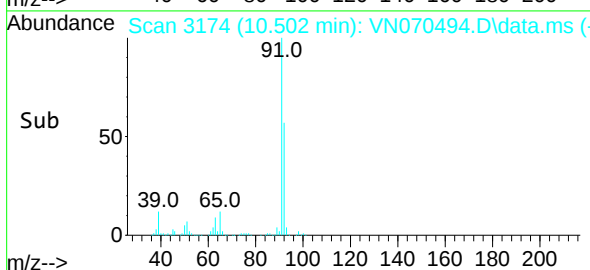






#59
2-Hexanone
Concen: 0.422 ug/l
RT: 11.092 min Scan# 31
Delta R.T. 0.008 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Instrument :
MSVOA_N
ClientSampleId :



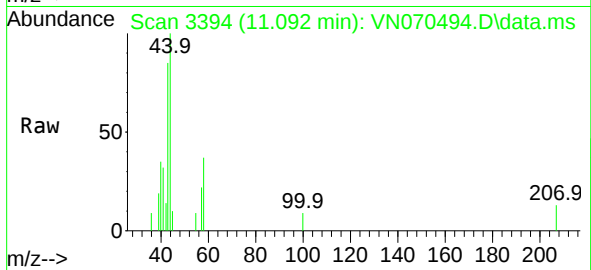



Tgt Ion: 43 Resp: 4671
Ion Ratio Lower Upper
43 100
58 31.1 26.9 80.7

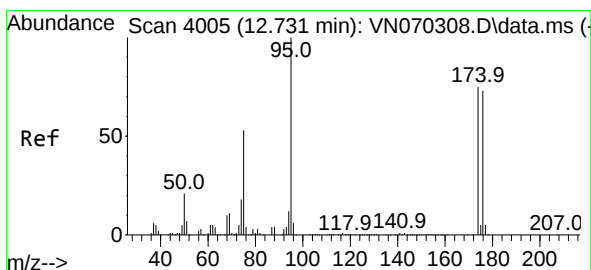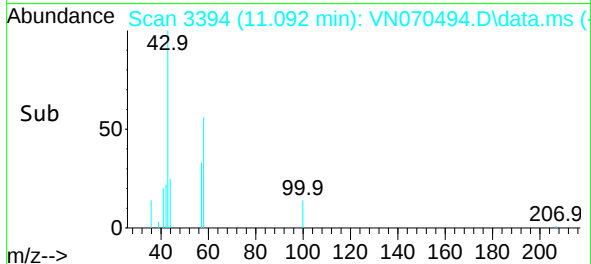

#62
4-Bromofluorobenzene
Concen: 33.764 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12


Tgt Ion: 95 Resp: 356108
Ion Ratio Lower Upper
95 100
174 76.9 0.0 187.2
176 73.0 0.0 181.4

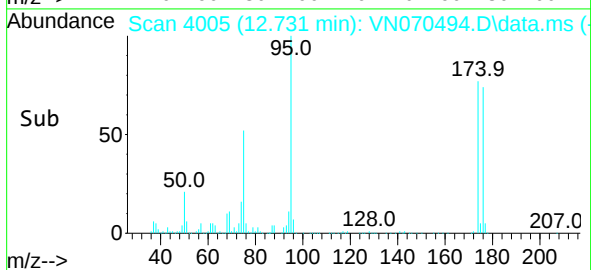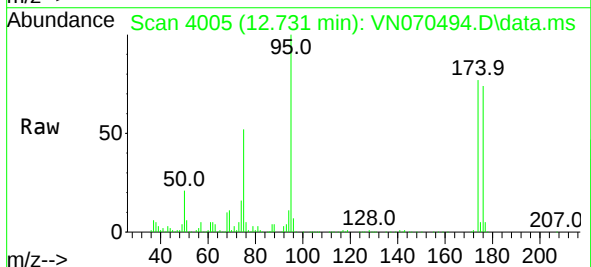






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:117 Resp: 807228




Ion	Ratio	Lower	Upper
117	100		
82	59.3	42.4	63.6
119	32.3	25.4	38.2




#67
Ethyl Benzene
Concen: 0.452 ug/l
RT: 11.843 min Scan# 3674
Delta R.T. -0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

Tgt Ion: 91 Resp: 14177

Ion	Ratio	Lower	Upper
91	100		
106	33.2	25.7	38.5

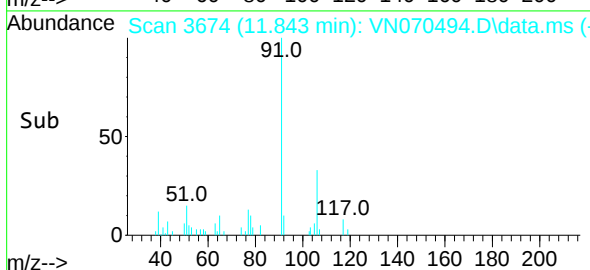



#68

m/p-Xylenes

Concen: 2.050 ug/l

RT: 11.950 min Scan# 31

Delta R.T. -0.003 min

Lab File: VN070494.D

Acq: 5 Jan 2022 17:12

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:106 Resp: 23412

Ion Ratio Lower Upper

106 100

91 216.3 160.6 240.8



#69

o-Xylene

Concen: 0.759 ug/l

RT: 12.275 min Scan# 3835

Delta R.T. -0.003 min

Lab File: VN070494.D




Acq: 5 Jan 2022 17:12


Tgt Ion:106 Resp: 8620

Ion Ratio Lower Upper

106 100


91 227.9 105.8 317.3

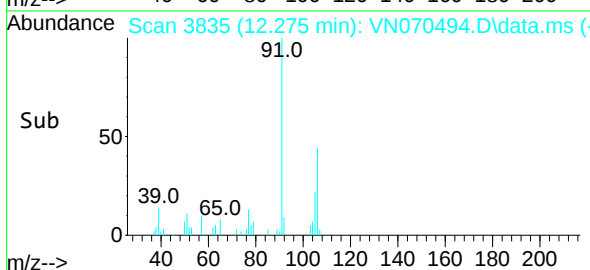






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.675 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VN070494.D
 Acq: 5 Jan 2022 17:12

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion:152 Resp: 199606
 Ion Ratio Lower Upper
 152 100
 115 58.8 27.5 82.5
 150 157.8 0.0 344.4



#75
 1,1,2,2-Tetrachloroethane
 Concen: 0.477 ug/l
 RT: 12.833 min Scan# 4043
 Delta R.T. 0.008 min
 Lab File: VN070494.D
 Acq: 5 Jan 2022 17:12

Tgt Ion: 83 Resp: 203
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.5 16.5#
 85 0.0 32.4 97.2#

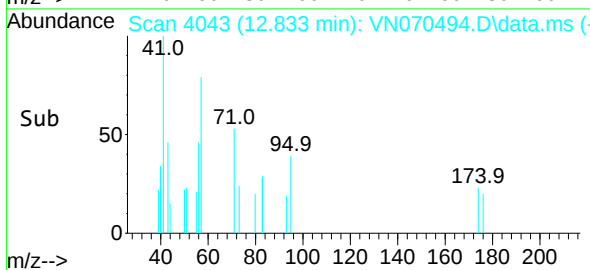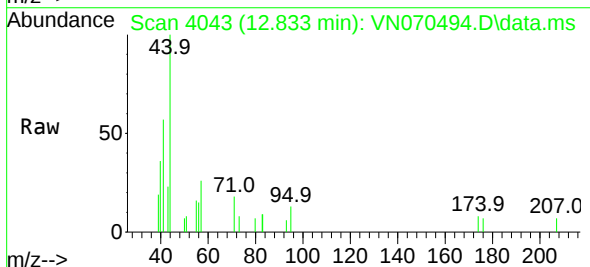



#76

1,2,3-Trichloropropane

Concen: 31.901 ug/l

RT: 12.731 min Scan# 4060

Delta R.T. -0.147 min

Lab File: VN070494.D

Acq: 5 Jan 2022 17:12

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 75 Resp: 182329

Ion Ratio Lower Upper

75 100

77 1.4 82.6 247.8#

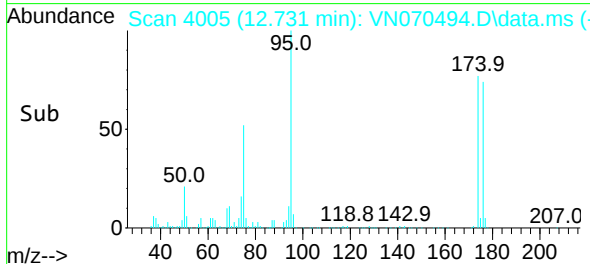

#80

1,3,5-Trimethylbenzene

Concen: 0.250 ug/l

RT: 13.058 min Scan# 4127

Delta R.T. -0.000 min

Lab File: VN070494.D




Acq: 5 Jan 2022 17:12


Tgt Ion: 105 Resp: 3715

Ion Ratio Lower Upper

105 100


120 43.8 24.6 73.6

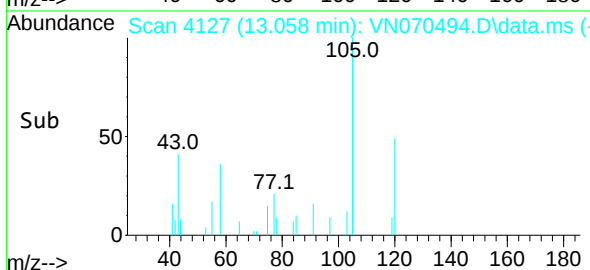






#81
 trans-1,4-Dichloro-2-butene
 Concen: 111.602 ug/l
 RT: 12.731 min Scan# 4005
 Delta R.T. 0.107 min
 Lab File: VN070494.D
 Acq: 5 Jan 2022 17:12

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion: 75 Resp: 182329
 Ion Ratio Lower Upper
 75 100
 53 0.1 90.5 135.7#
 89 0.0 38.2 57.4#



#84
 1,2,4-Trimethylbenzene
 Concen: 0.607 ug/l
 RT: 13.369 min Scan# 4243
 Delta R.T. 0.003 min
 Lab File: VN070494.D
 Acq: 5 Jan 2022 17:12


Tgt Ion: 105 Resp: 8685
 Ion Ratio Lower Upper
 105 100
 120 39.3 22.8 68.4

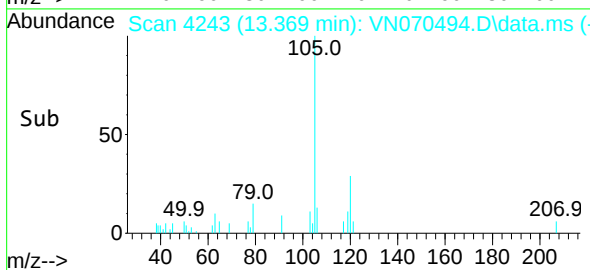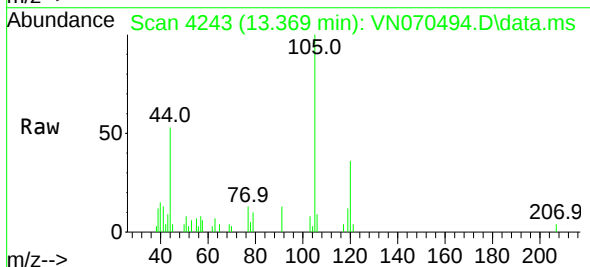






#95
Naphthalene
Concen: 2.453 ug/l
RT: 15.504 min Scan# 5039
Delta R.T. -0.000 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12


Instrument :
MSVOA_N
ClientSampleId :

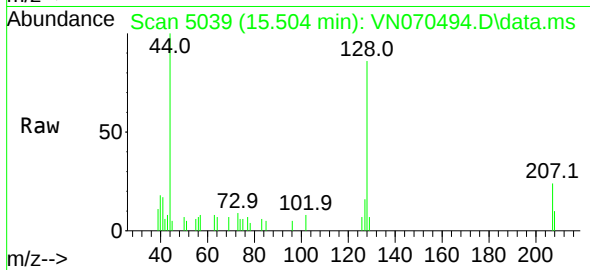

Tgt Ion:128 Resp: 6193
Ion Ratio Lower Upper
128 100
127 16.9 10.5 15.7#
129 11.3 8.7 13.1

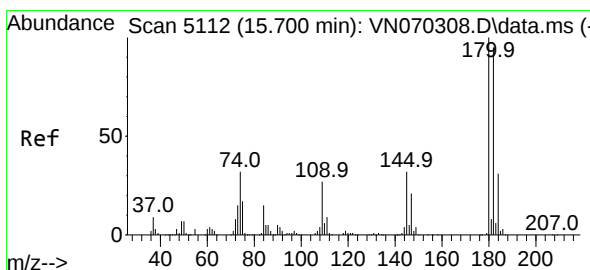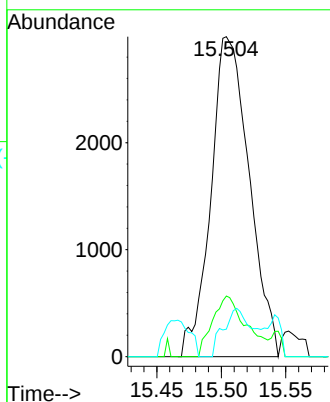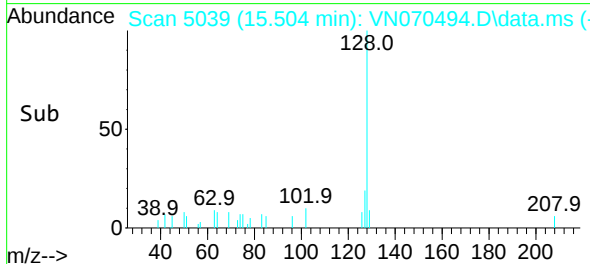

#96
1,2,3-Trichlorobenzene
Concen: 0.990 ug/l
RT: 15.697 min Scan# 5111
Delta R.T. -0.003 min
Lab File: VN070494.D
Acq: 5 Jan 2022 17:12

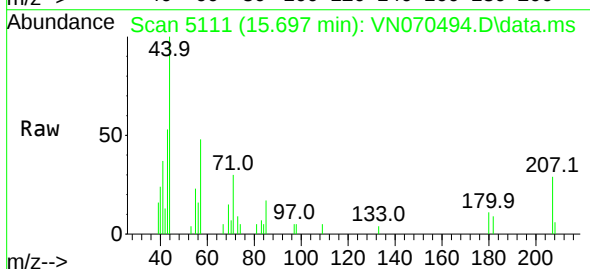

Tgt Ion:180 Resp: 524
Ion Ratio Lower Upper
180 100
182 50.6 47.4 142.2
145 10.1 15.0 45.1#

