


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010523\
Data File : VN076101.D
Acq On : 05 Jan 2023 10:05
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

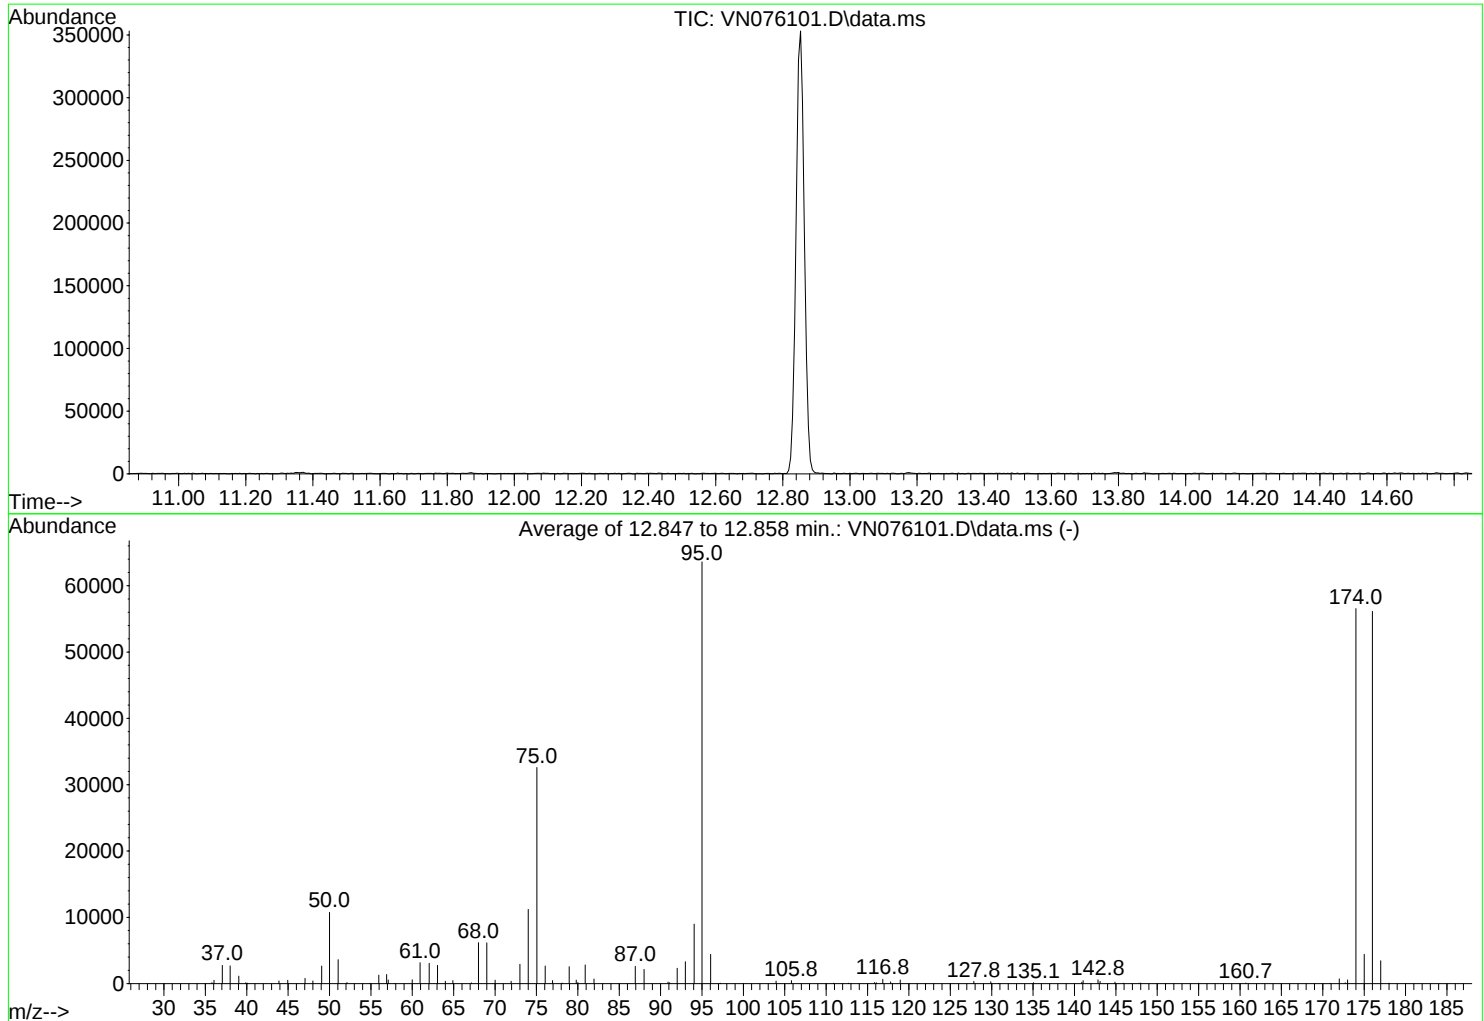

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	10746	PASS
75	95	30	60	51.3	32605	PASS
95	95	100	100	100.0	63600	PASS
96	95	5	9	6.9	4410	PASS
173	174	0.00	2	1.0	566	PASS
174	95	50	100	88.9	56544	PASS
175	174	5	9	7.8	4421	PASS
176	174	95	101	99.3	56147	PASS
177	176	5	9	6.1	3442	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	142	49.05	2649	62.05	3072	75.05	3260
36.05	498	50.00	10746	63.05	2758	76.05	2641
37.05	2753	51.05	3613	64.00	371	76.95	45
38.00	2670	52.10	182	64.90	451	78.10	10
39.05	1147	54.90	56	67.15	124	78.95	2548
39.90	157	55.95	1276	68.00	6186	79.80	540
40.10	72	56.90	1372	69.00	6153	80.00	161
43.90	413	57.10	551	70.00	542	80.90	2834
44.95	517	57.90	52	71.95	352	81.95	695
47.05	796	60.00	586	73.00	2927	86.95	2618
48.00	411	60.95	3168	74.00	11188	88.00	2150

Average of 12.847 to 12.858 min.: VN076101.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	250	112.70	80	140.90	221	170.90	51
91.10	146	113.00	50	141.05	448	172.00	731
92.00	2326	115.85	181	142.00	57	172.70	130
93.00	3314	116.10	119	142.85	590	173.00	566
94.05	8966	116.85	655	143.10	328	174.00	56544
95.00	63600	117.80	269	144.90	246	175.00	4421
96.05	4410	118.95	563	145.90	65	176.00	56147
97.20	69	127.85	329	147.80	55	177.00	3442
103.95	399	129.90	300	148.00	90	178.00	70
105.80	461	130.80	52	155.00	85		
110.90	77	135.05	151	160.70	103		

Instrument :

MSVOA_N

ClientSampleId :

BFB