

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010621\
 Data File : VN065391.D
 Acq On : 6 Jan 2021 11:02
 Operator : JC/MD
 Sample : VN0106WBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0106WBL01

Quant Time: Jan 07 01:16:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122120W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Mon Dec 21 13:17:58 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.158	128	52416	30.00	ug/l	0.01
28) 1,4-Difluorobenzene	8.553	114	280601	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.380	117	246438	30.00	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	7.991	65	109072	28.68	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	95.60%
60) 4-Bromofluorobenzene	12.376	95	95126	24.27	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	80.90%
63) Toluene-d8	10.058	98	330193	30.21	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.70%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010621\
Data File : VN065391.D
Acq On : 6 Jan 2021 11:02
Operator : JC/MD
Sample : VN0106WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0106WBL01

Quant Time: Jan 07 01:16:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122120W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Mon Dec 21 13:17:58 2020
Response via : Initial Calibration




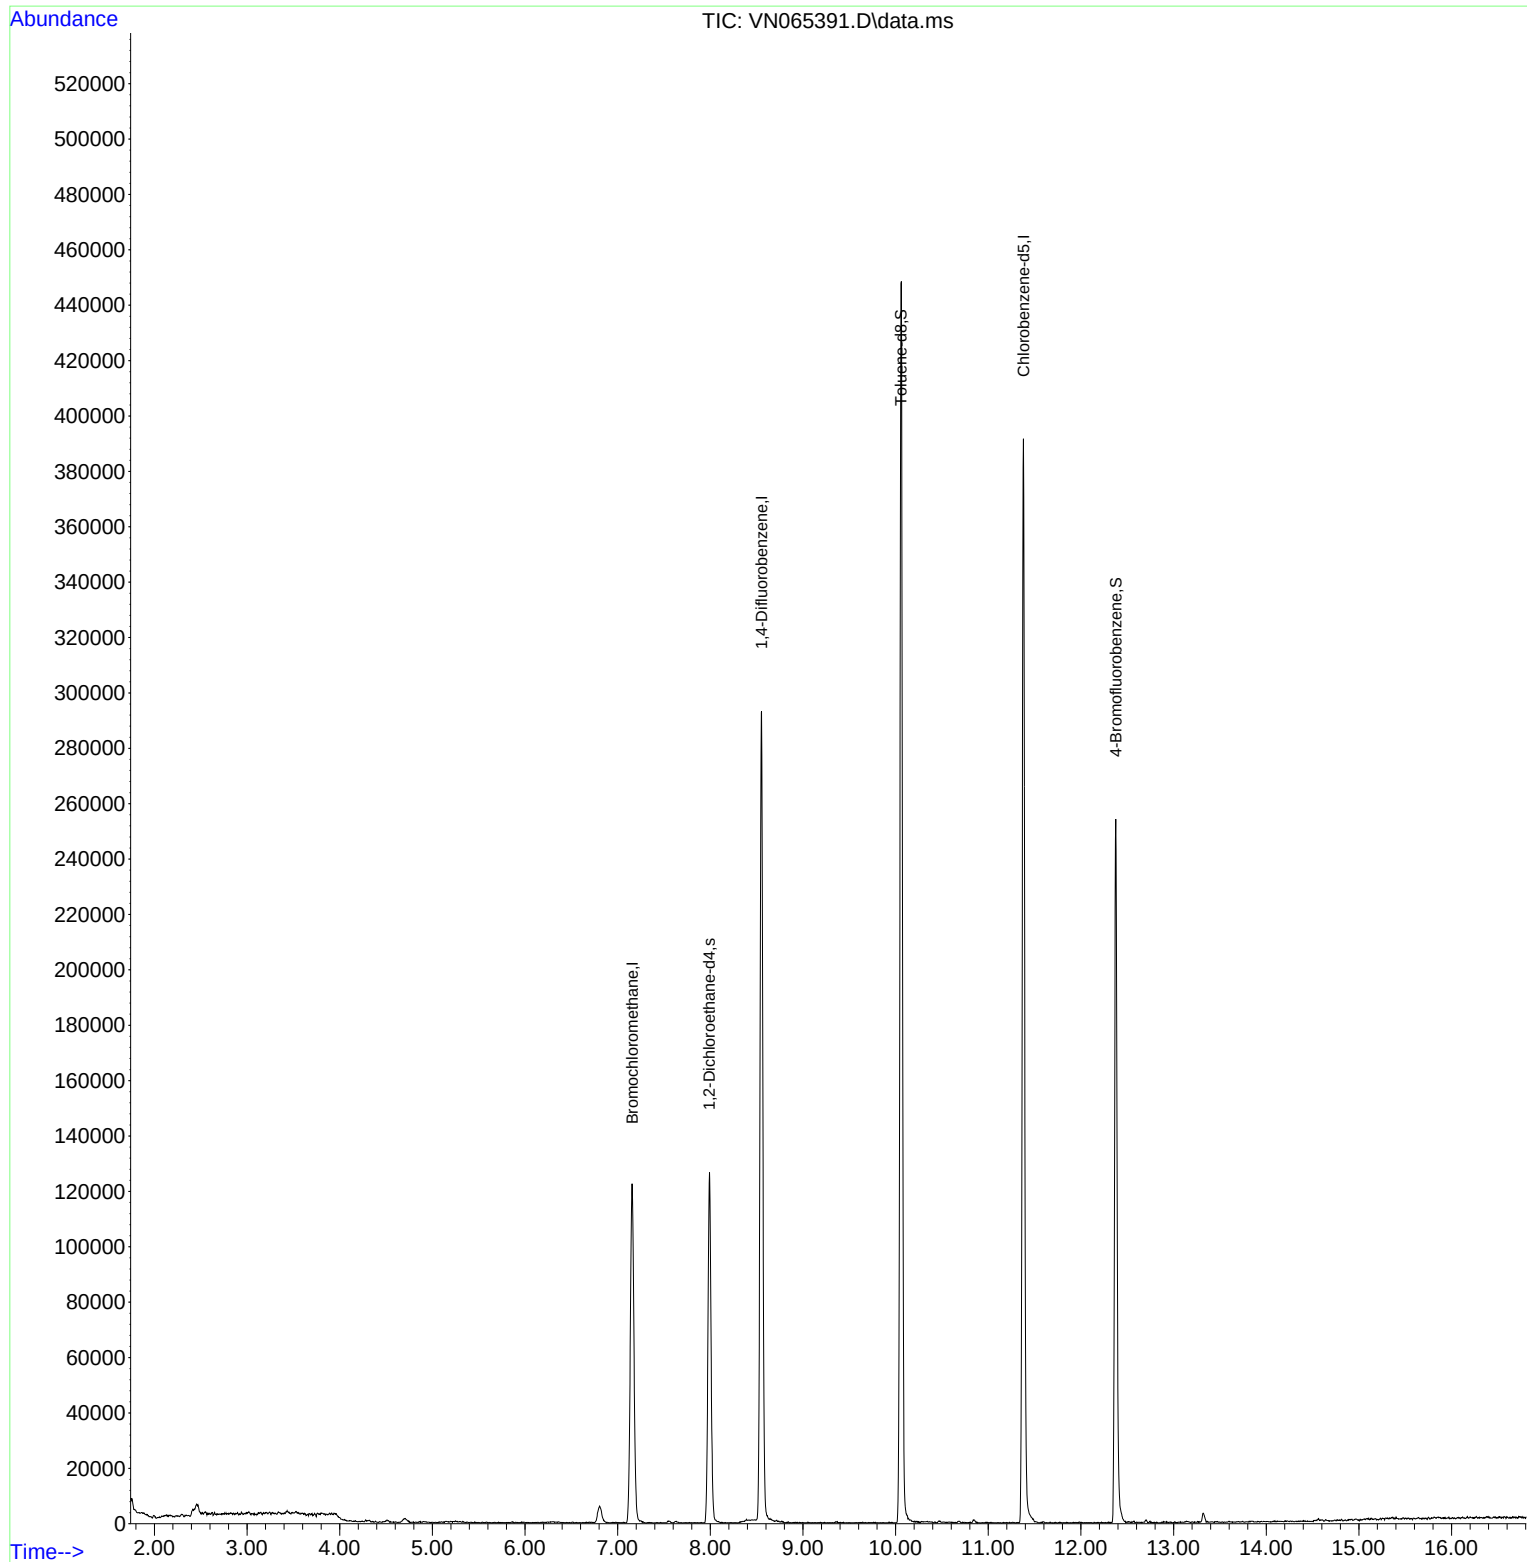


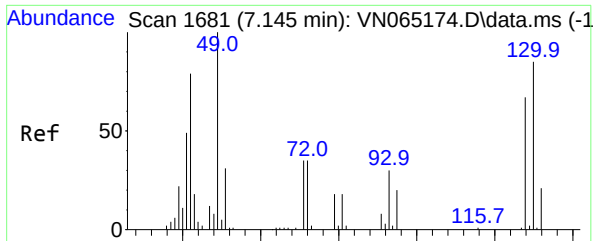

Bromochloromethane
Concen: 30.00 ug/l
RT: 7.158 min Scan# 1685
Delta R.T. 0.013 min
Lab File: VN065391.D
Acq: 6 Jan 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0106WBL01


Tgt Ion:128 Resp: 52416
Ion Ratio Lower Upper
128 100
49 147.8 0.0 475.5
130 128.2 0.0 315.3

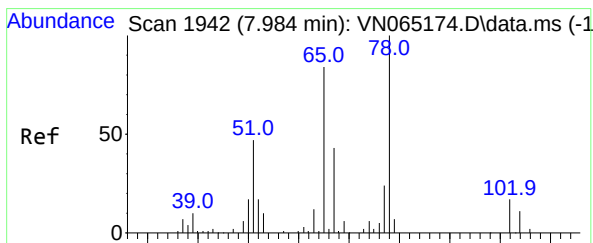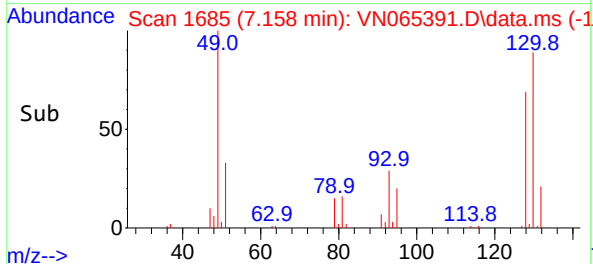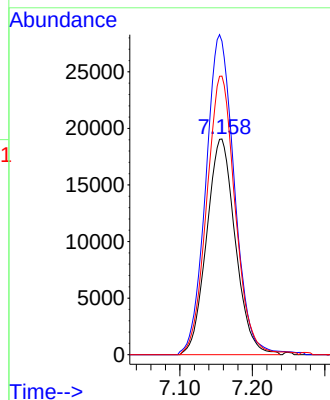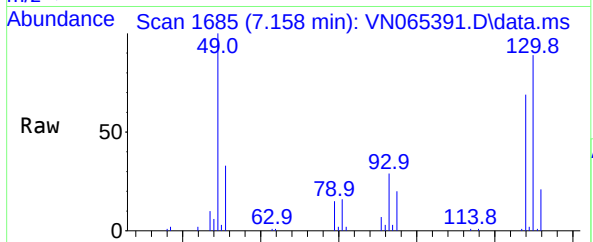

1,2-Dichloroethane-d4
Concen: 28.68 ug/l
RT: 7.991 min Scan# 1944
Delta R.T. 0.006 min
Lab File: VN065391.D
Acq: 6 Jan 2021 11:02

Tgt Ion: 65 Resp: 109072
Ion Ratio Lower Upper
65 100
67 52.9 41.1 61.7


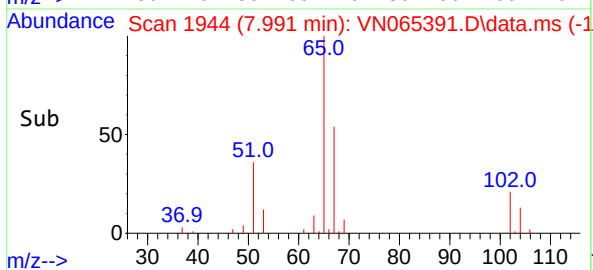
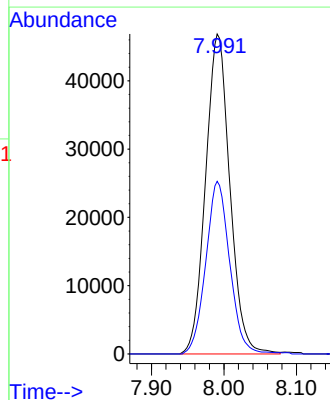
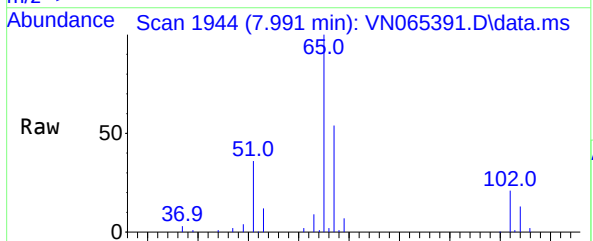


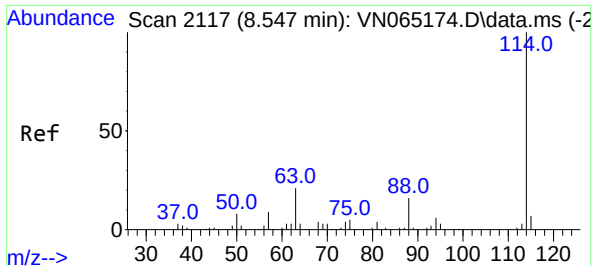

#28
1,4-Difluorobenzene
Concen: 30.00 ug/l
RT: 8.553 min Scan# 2119
Delta R.T. 0.006 min
Lab File: VN065391.D
Acq: 6 Jan 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0106WBL01


Tgt Ion:114 Resp: 280601
Ion Ratio Lower Upper
114 100
63 19.1 18.5 27.7
88 15.2 13.0 19.6

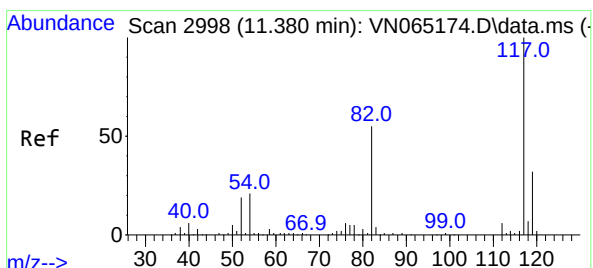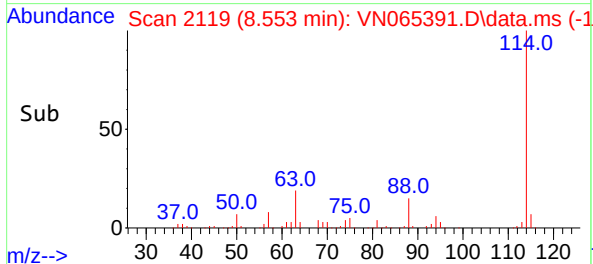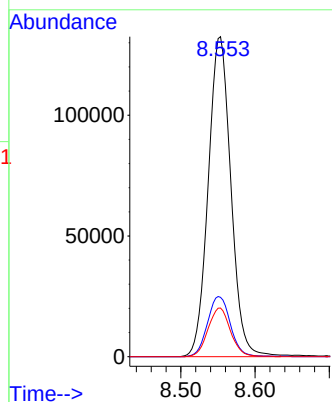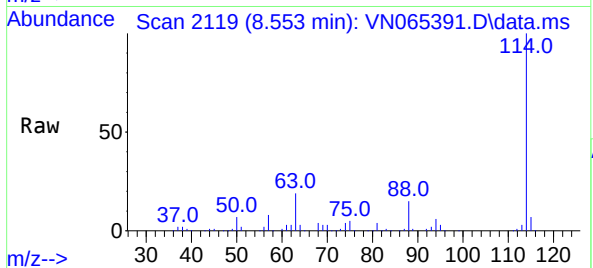

#57
Chlorobenzene-d5
Concen: 30.00 ug/l
RT: 11.380 min Scan# 2998
Delta R.T. 0.000 min
Lab File: VN065391.D
Acq: 6 Jan 2021 11:02

Tgt Ion:117 Resp: 246438
Ion Ratio Lower Upper
117 100
82 52.8 47.8 71.8
119 32.2 25.7 38.5


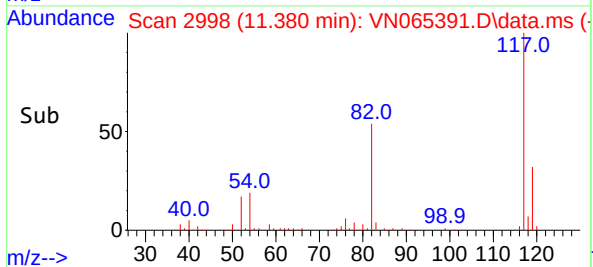
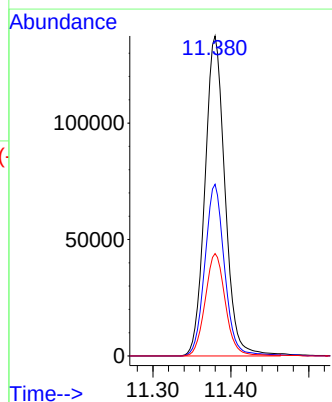
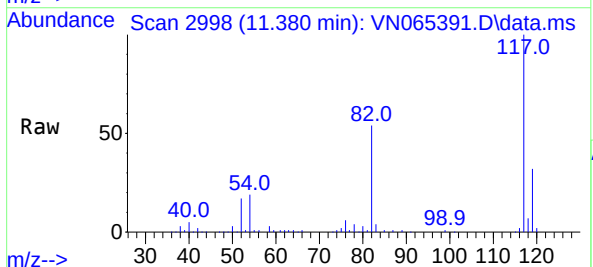


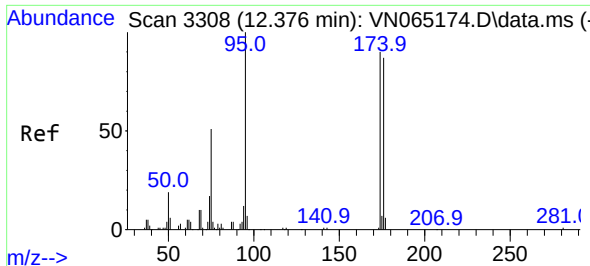

#60
4-Bromofluorobenzene
Concen: 24.27 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.000 min
Lab File: VN065391.D
Acq: 6 Jan 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0106WBL01

Tgt Ion: 95 Resp: 95126
Ion Ratio Lower Upper
95 100
174 93.2 56.4 84.6#
176 90.7 53.3 79.9#

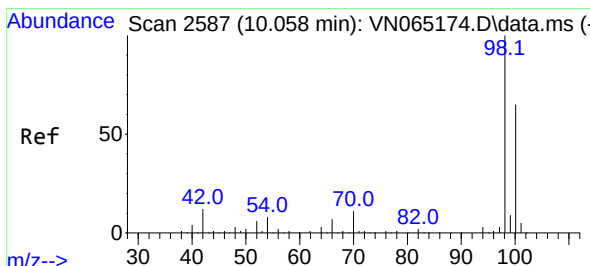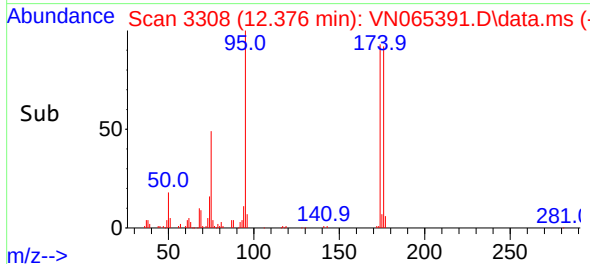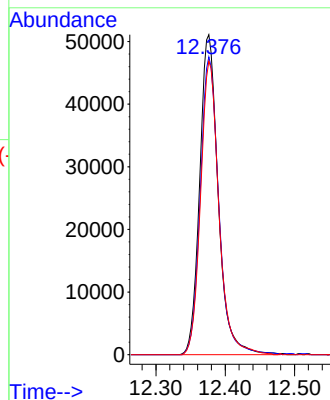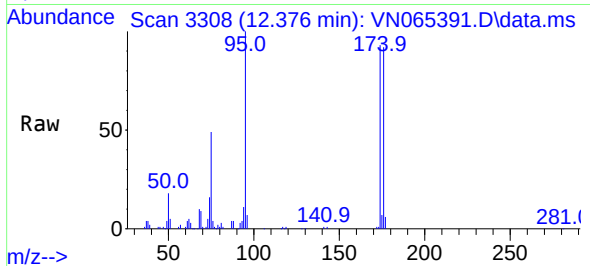

#63
Toluene-d8
Concen: 30.21 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. 0.000 min
Lab File: VN065391.D
Acq: 6 Jan 2021 11:02

Tgt Ion: 98 Resp: 330193
Ion Ratio Lower Upper
98 100
100 64.3 49.4 74.2

