
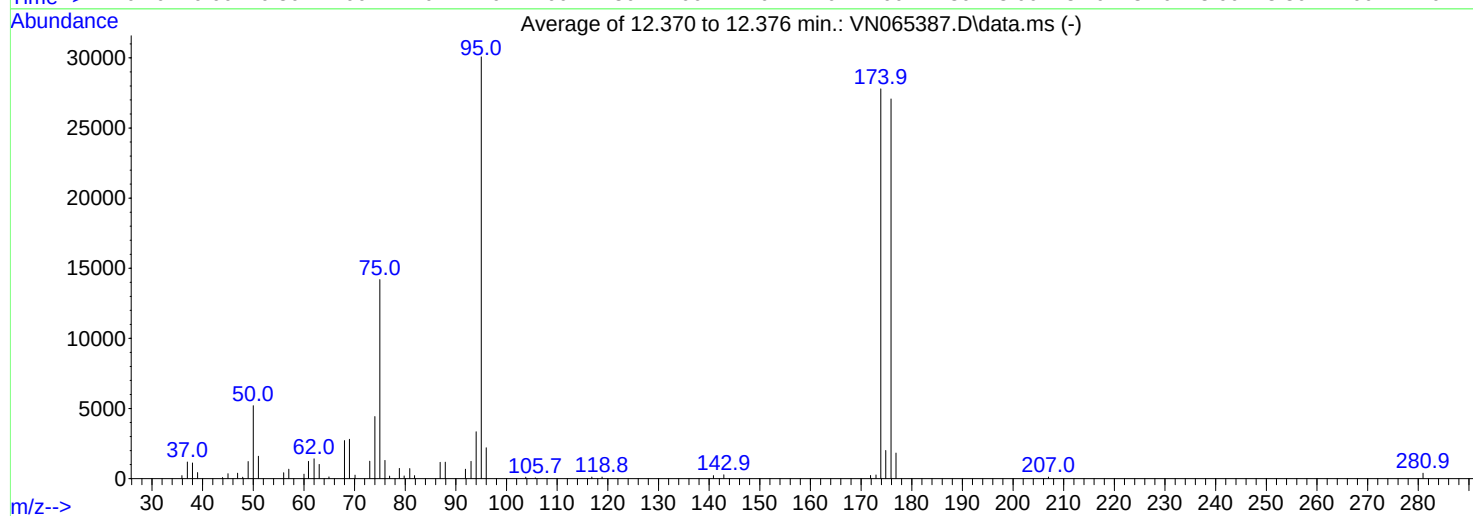


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010621\
 Data File : VN065387.D
 Acq On : 6 Jan 2021 8:55
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122120W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Dec 21 13:17:58 2020

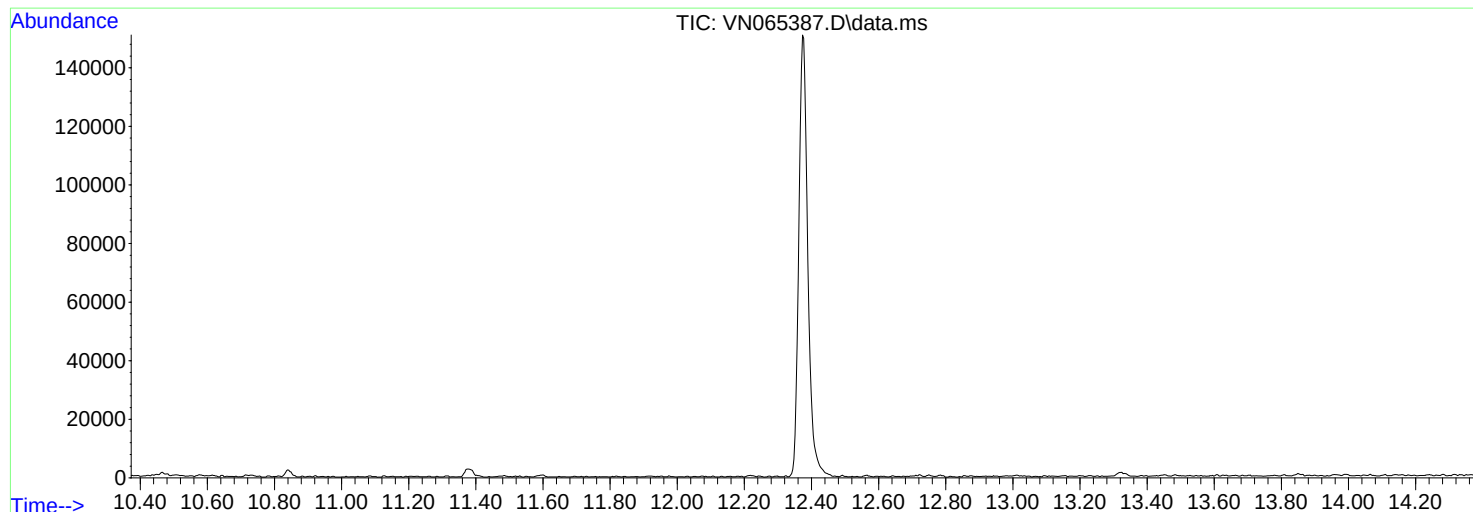

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	5203	PASS
75	95	30	60	47.2	14192	PASS
95	95	100	100	100.0	30075	PASS
96	95	5	9	7.3	2205	PASS
173	174	0.00	2	1.0	267	PASS
174	95	50	100	92.4	27795	PASS
175	174	5	9	7.2	2010	PASS
176	174	95	101	97.4	27069	PASS
177	176	5	9	6.8	1829	PASS