

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010622\
 Data File : VN070523.D
 Acq On : 6 Jan 2022 16:52
 Operator : JC/MD
 Sample : N1015-07 100X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 20986

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M

Title : SW846 8260

Signal : TIC: VN070523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.140	776	802	835	rBV	10380856	29824635	100.00%	46.327%
2	4.283	836	855	925	rVB	3266467	9825313	32.94%	15.262%
3	8.021	2226	2249	2260	rBV	627566	1514671	5.08%	2.353%
4	8.083	2260	2272	2310	rVB	1101715	2549117	8.55%	3.960%
5	8.434	2380	2403	2429	rBV	797233	1825711	6.12%	2.836%
6	8.965	2584	2601	2634	rVB	1702031	3505386	11.75%	5.445%
7	10.440	3132	3151	3190	rBV	2706798	5064871	16.98%	7.867%
8	11.744	3612	3637	3669	rBV	2224960	4045980	13.57%	6.285%
9	12.685	3972	3988	3993	rBV2	188670	303586	1.02%	0.472%
10	12.731	3993	4005	4036	rVB	1807101	3267275	10.95%	5.075%
11	13.675	4340	4357	4379	rBV	1501478	2652597	8.89%	4.120%




Sum of corrected areas: 64379142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010622\
Data File : VN070523.D
Acq On : 6 Jan 2022 16:52
Operator : JC/MD
Sample : N1015-07 100X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
20986

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

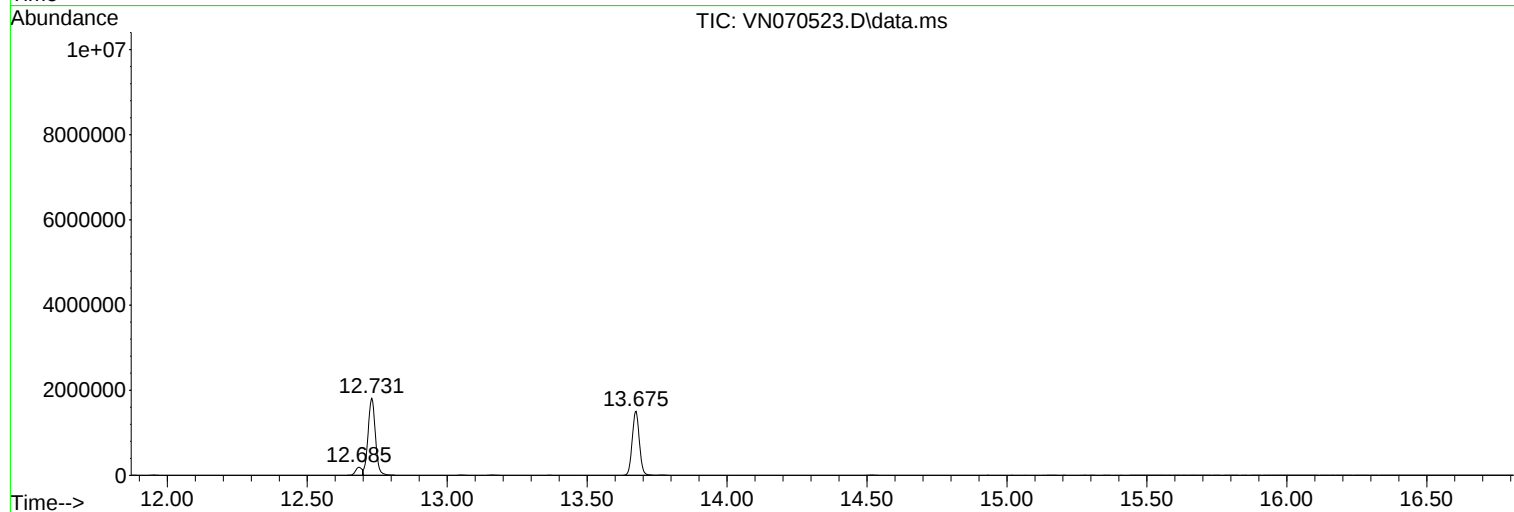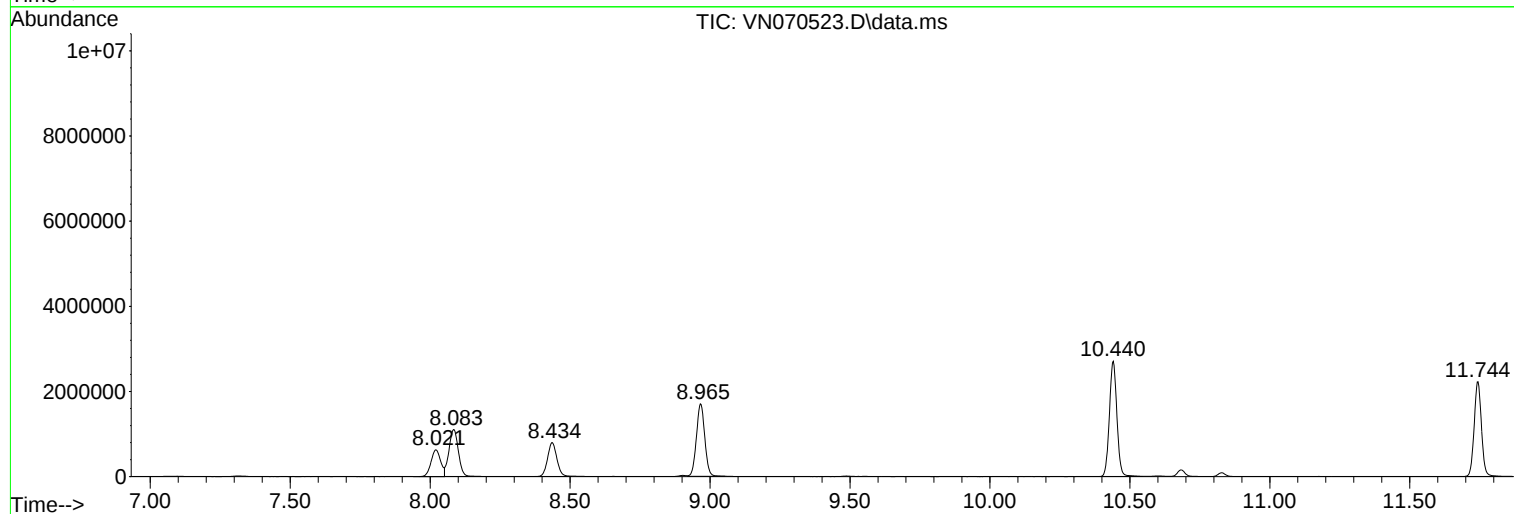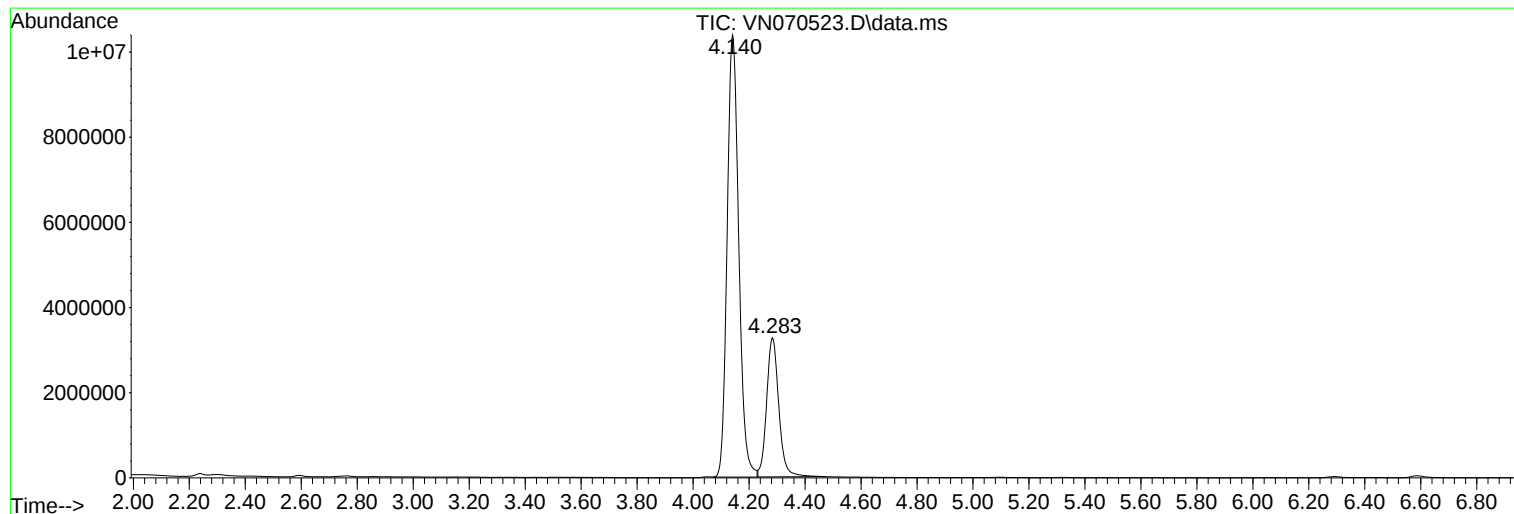

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010622\
Data File : VN070523.D
Acq On : 6 Jan 2022 16:52
Operator : JC/MD
Sample : N1015-07 100X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
20986










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propanal Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.140	585.00 ug/l	29824600	Pentafluorobenzene	8.086

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanal	58	C3H6O	000123-38-6	78
2			Trimethylene oxide	58	C3H6O	000503-30-0	56
3			2-(Aminomethyl)-4-methylpentanoic...	187	C10H21NO2	1891211-54-3	9
4			Quinolin-2(1H)-one, 3,4,5,6,7,8-...	208	C12H20N2O	1000259-95-6	9
5			Propylene oxide	58	C3H6O	000075-56-9	7

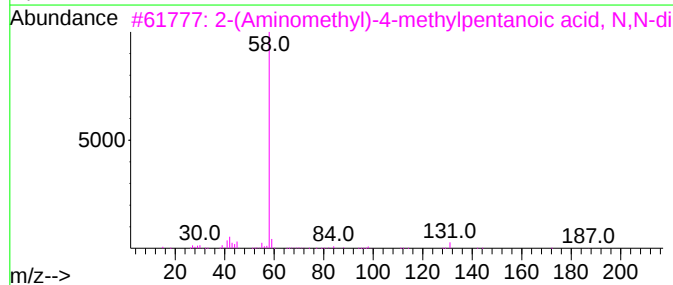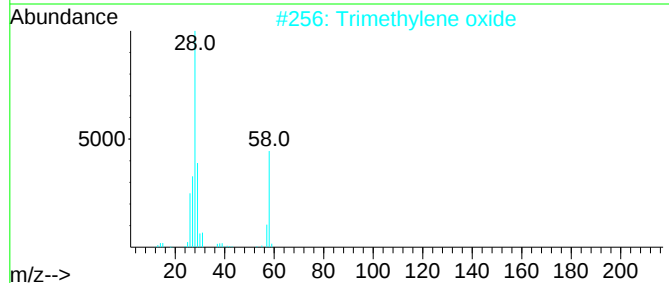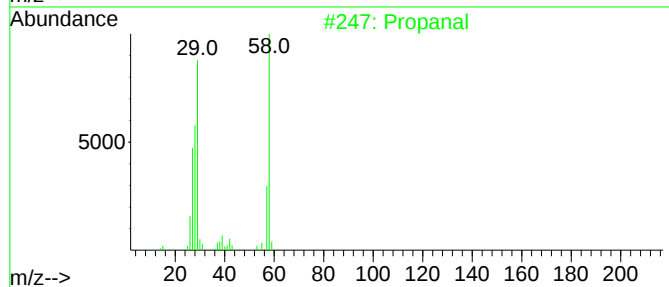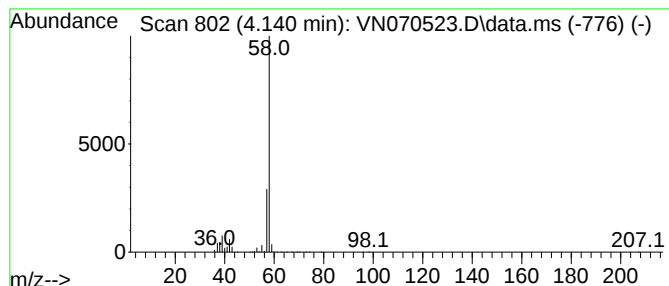

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010622\
Data File : VN070523.D
Acq On : 6 Jan 2022 16:52
Operator : JC/MD
Sample : N1015-07 100X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
20986

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propanal	4.140	585.0	ug/l	29824600	1	8.086	2549120	50.0