
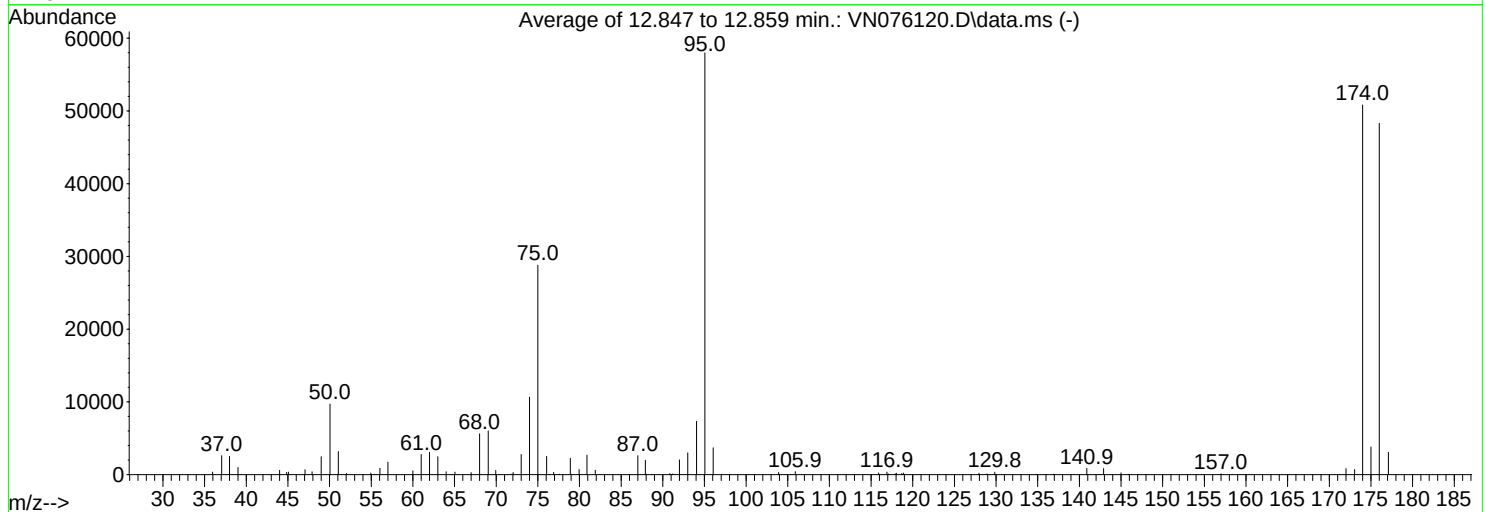


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010623\
 Data File : VN076120.D
 Acq On : 06 Jan 2023 09:17
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260
 Last Update : Wed Dec 14 13:03:41 2022

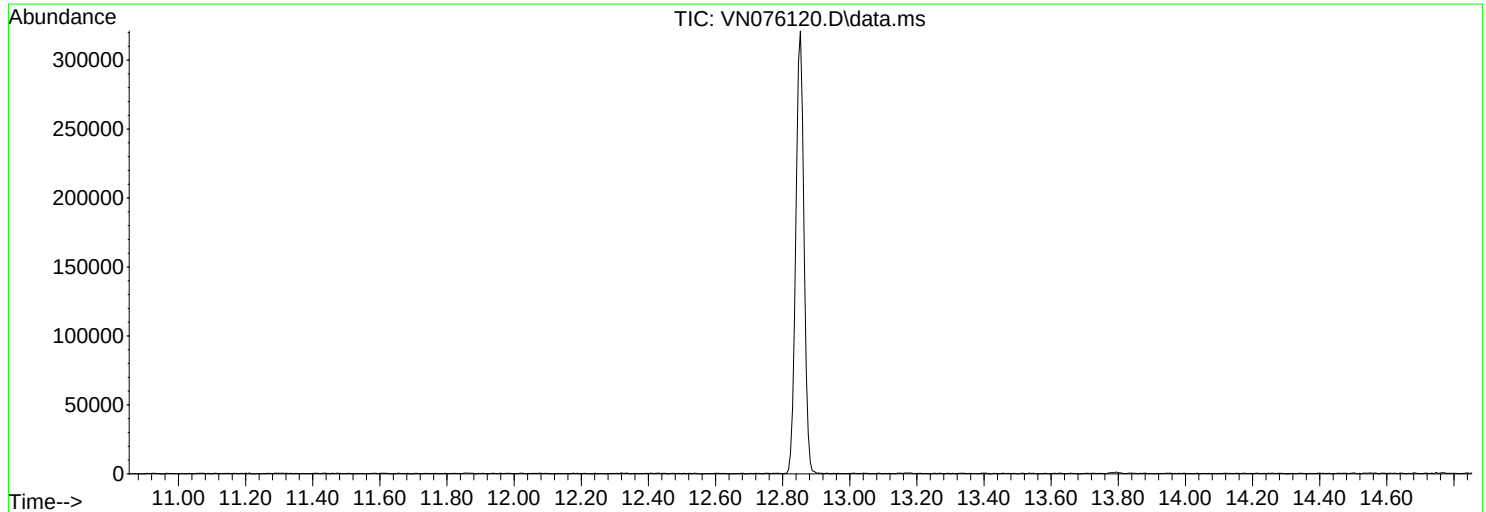

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	9710	PASS
75	95	30	60	49.7	28803	PASS
95	95	100	100	100.0	57987	PASS
96	95	5	9	6.4	3690	PASS
173	174	0.00	2	1.4	706	PASS
174	95	50	100	87.6	50821	PASS
175	174	5	9	7.5	3804	PASS
176	174	95	101	95.1	48309	PASS
177	176	5	9	6.4	3084	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	352	51.05	3200	67.00	280	77.60	64
37.05	2621	52.05	166	68.00	5606	78.90	225
38.00	2511	54.95	215	69.05	6010	79.95	69
39.00	994	56.05	876	69.95	565	80.90	269
44.00	599	57.00	1718	71.90	89	81.90	611
44.85	305	60.00	524	72.05	293	83.00	56
45.05	345	61.00	2782	73.00	2778	87.00	2624
47.05	691	62.00	3087	74.00	10653	87.90	1988
47.90	387	63.00	2460	75.00	28803	88.70	53
49.00	2466	64.00	393	76.05	2509	90.85	165
50.05	9710	65.05	360	76.90	304	91.20	102

Average of 12.847 to 12.859 min.: VN076120.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	2018	117.10	99	142.90	841		
93.00	2999	117.90	143	145.00	242		
94.05	7334	118.05	199	145.90	54		
95.05	57987	118.70	173	147.10	51		
96.05	3690	118.90	210	157.00	100		
97.10	64	127.95	188	172.00	829		
103.90	305	128.90	119	173.05	706		
104.80	53	129.85	336	174.00	50821		
105.90	416	134.80	62	175.00	3804		
115.90	249	136.90	59	176.00	48309		
116.90	347	140.90	856	177.10	3084		

Instrument :

MSVOA_N

ClientSampleId :

BFB