
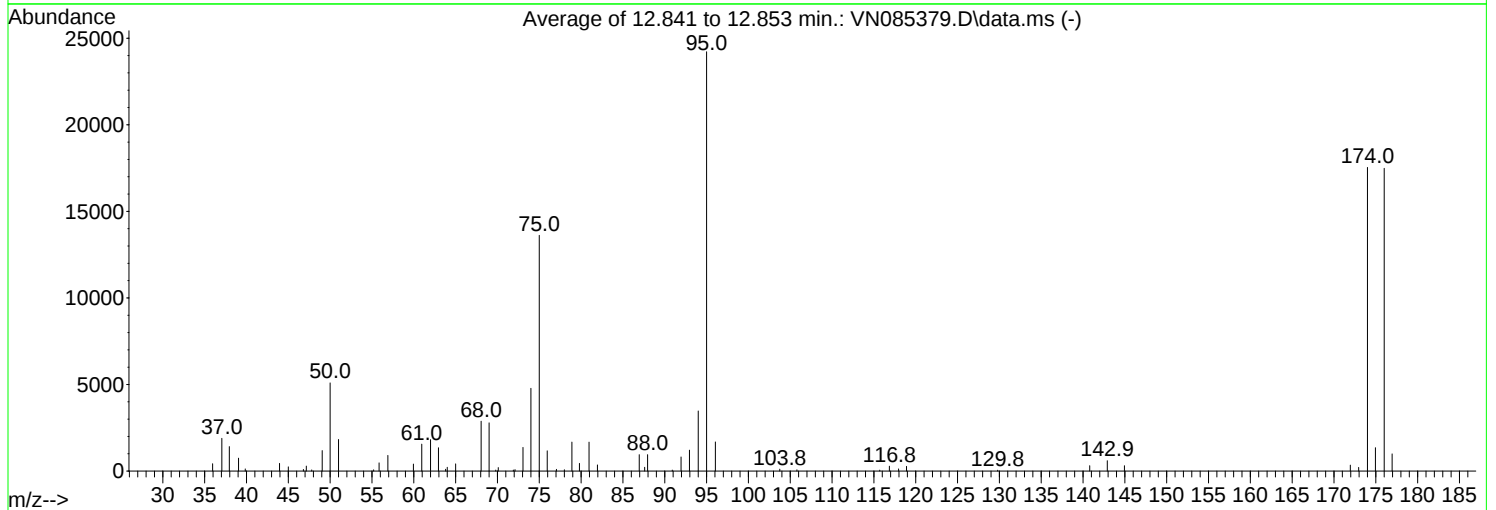


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010625\
Data File : VN085379.D
Acq On : 06 Jan 2025 10:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
Title : SW846 8260
Last Update : Sat Dec 28 01:36:16 2024

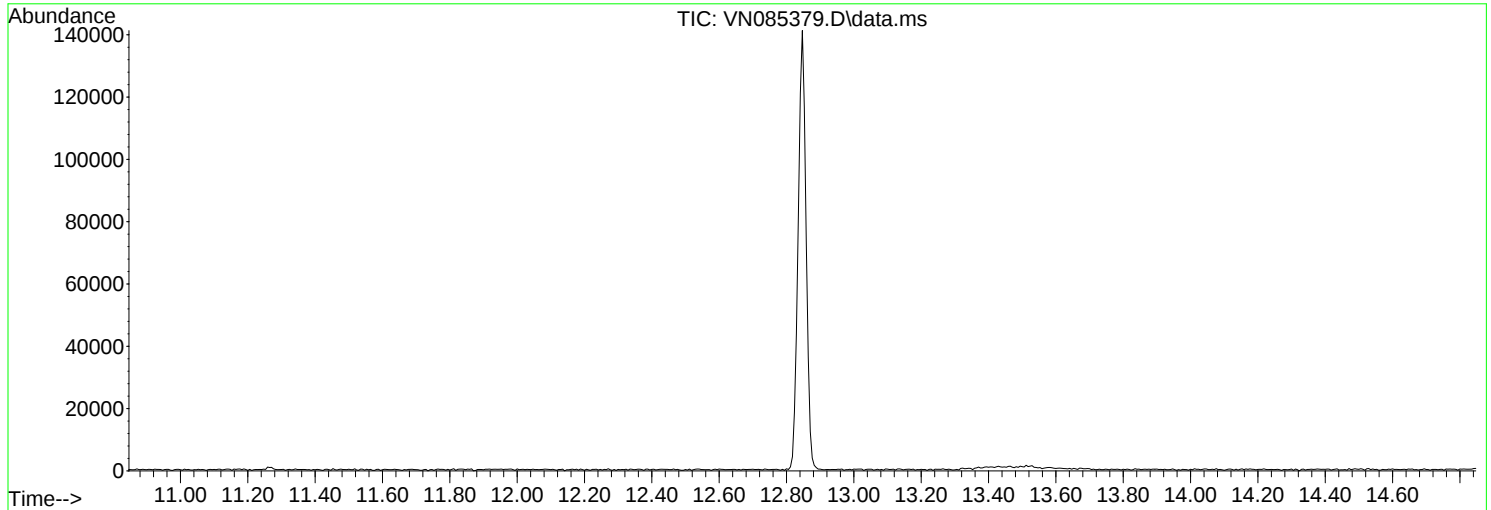

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	5093	PASS
75	95	30	60	56.2	13616	PASS
95	95	100	100	100.0	24221	PASS
96	95	5	9	6.9	1682	PASS
173	174	0.00	2	1.2	211	PASS
174	95	50	100	72.4	17539	PASS
175	174	5	9	7.7	1350	PASS
176	174	95	101	99.7	17487	PASS
177	176	5	9	5.7	992	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	423	50.00	5093	65.00	416	77.05	101
37.05	1892	51.00	1825	68.05	2880	78.00	79
37.95	1413	55.20	73	69.00	2787	78.90	1676
39.05	746	55.85	475	69.80	58	79.80	445
39.85	126	56.90	904	70.10	203	80.95	1672
43.95	443	59.95	405	71.90	62	81.95	356
45.00	243	60.95	1556	72.10	85	86.95	947
46.80	94	62.00	1816	73.05	1366	87.60	218
47.15	289	62.95	1347	74.00	4781	87.95	949
47.80	67	63.80	105	75.00	13616	90.90	58
49.05	1185	64.00	219	75.95	1169	91.95	814

Average of 12.841 to 12.853 min.: VN085379.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	1208	140.80	310				
94.00	3470	142.90	600				
95.00	24221	144.95	311				
96.05	1682	171.95	344				
103.75	110	172.95	211				
105.80	74	174.00	17539				
115.70	55	174.95	1350				
116.85	284	176.00	17487				
117.95	126	176.95	992				
118.90	273						
129.80	50						

Instrument :

MSVOA_N

ClientSampleId :

BFB