


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN010719\
 Data File : VN053292.D
 Acq On : 7 Jan 2019 8:32
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N010519W.M
 Title : SW846 8260
 Last Update : Mon Jan 07 09:34:27 2019

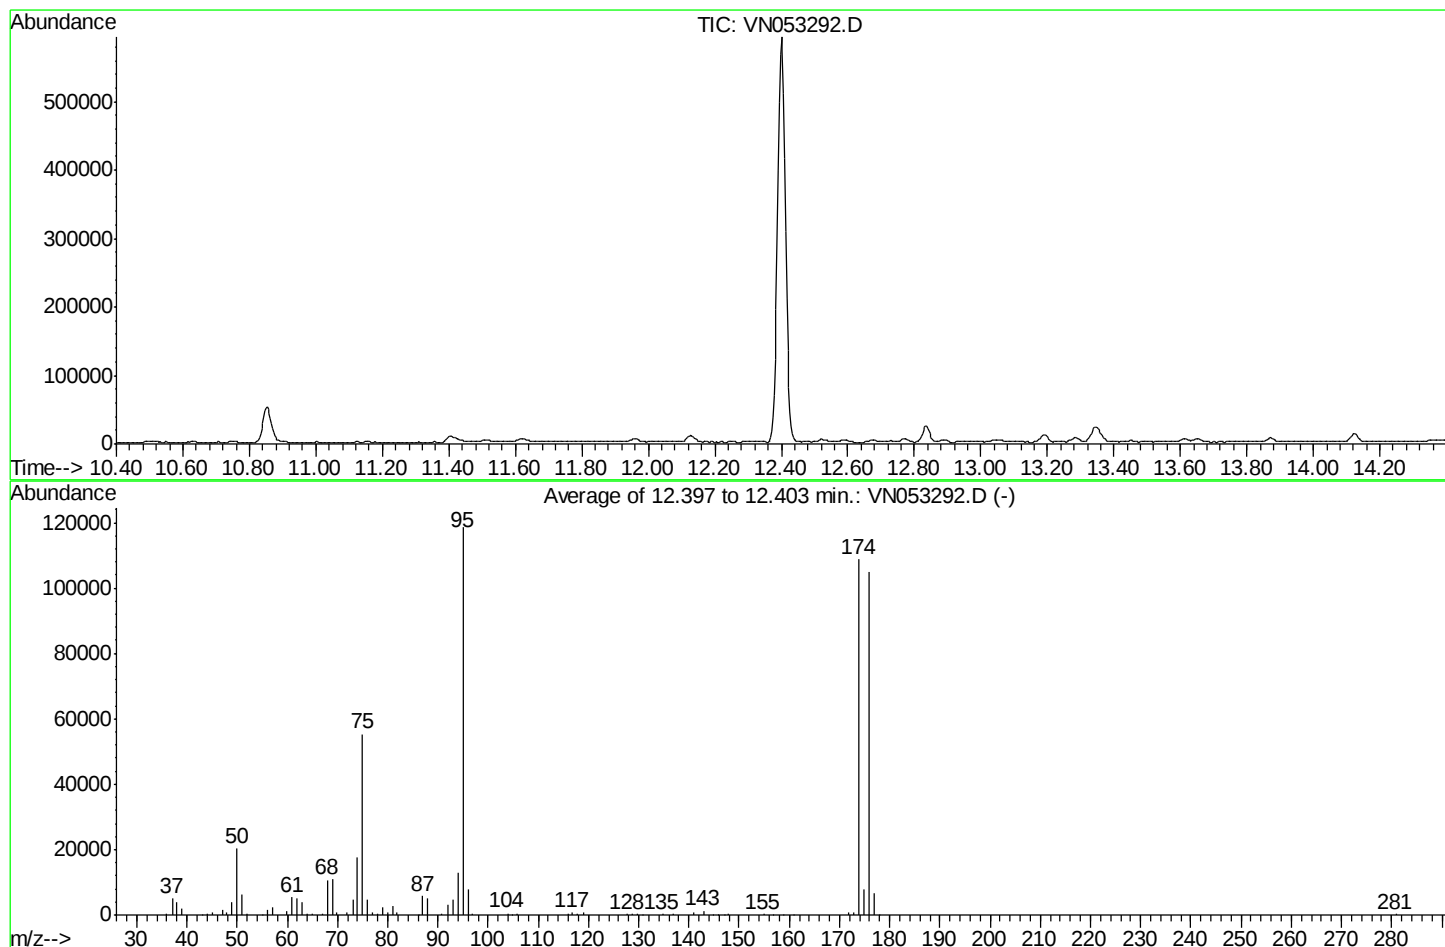

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	20325	PASS
75	95	30	60	46.6	55226	PASS
95	95	100	100	100.0	118581	PASS
96	95	5	9	6.7	7933	PASS
173	174	0.00	2	0.9	932	PASS
174	95	50	100	91.8	108802	PASS
175	174	5	9	7.2	7834	PASS
176	174	95	101	96.3	104813	PASS
177	176	5	9	6.5	6788	PASS