
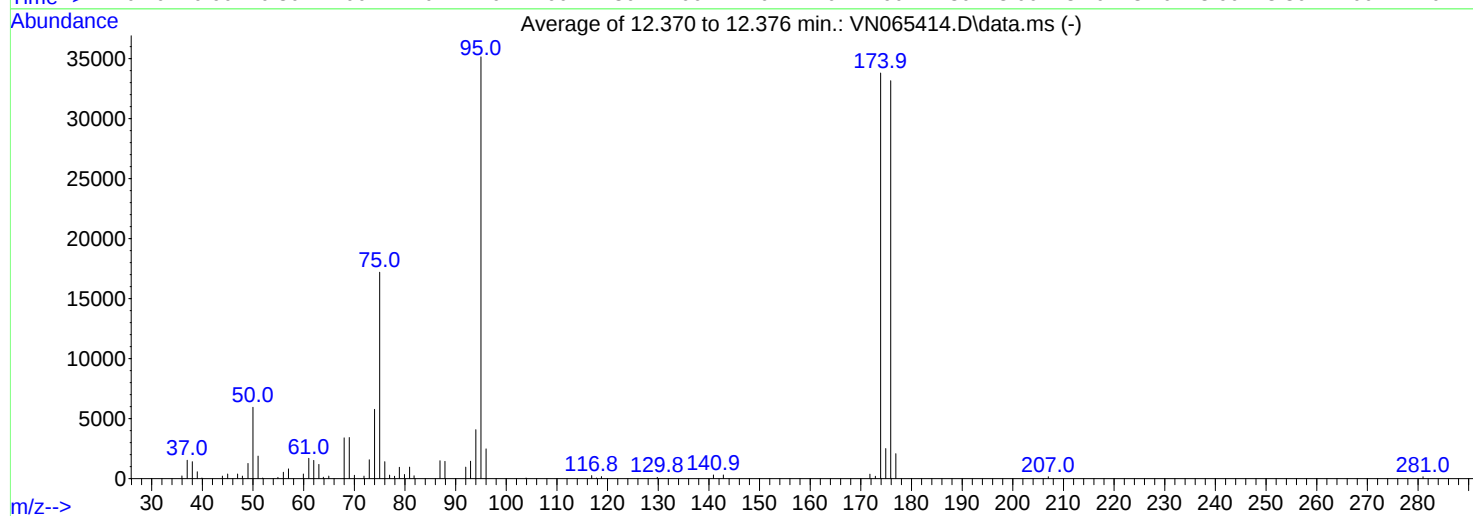


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010721\
Data File : VN065414.D
Acq On : 7 Jan 2021 8:54
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Title : SW846 8260
Last Update : Tue Dec 22 15:42:18 2020

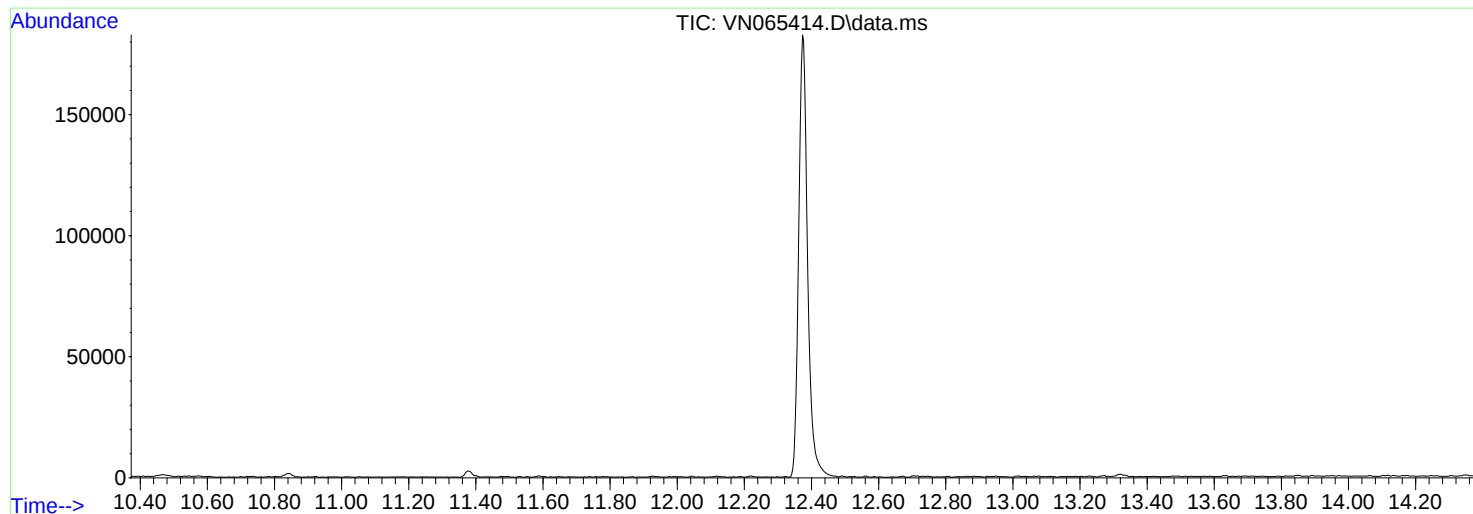

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	5951	PASS
75	95	30	60	49.0	17203	PASS
95	95	100	100	100.0	35144	PASS
96	95	5	9	7.1	2482	PASS
173	174	0.00	2	0.6	200	PASS
174	95	50	100	96.1	33789	PASS
175	174	5	9	7.4	2511	PASS
176	174	95	101	98.1	33155	PASS
177	176	5	9	6.3	2078	PASS