

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010725\
 Data File : VN085395.D
 Acq On : 07 Jan 2025 13:05
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Jan 08 04:17:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122024W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Sat Dec 21 02:03:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.806	128	25198	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.100	114	114812	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.865	117	107360	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.577	65	67351	30.384	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	101.267%
60) 4-Bromofluorobenzene	12.847	95	40514	23.296	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	77.667%
63) Toluene-d8	10.565	98	147012	28.043	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	93.467%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010725\
Data File : VN085395.D
Acq On : 07 Jan 2025 13:05
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Jan 08 04:17:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122024W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Sat Dec 21 02:03:07 2024
Response via : Initial Calibration




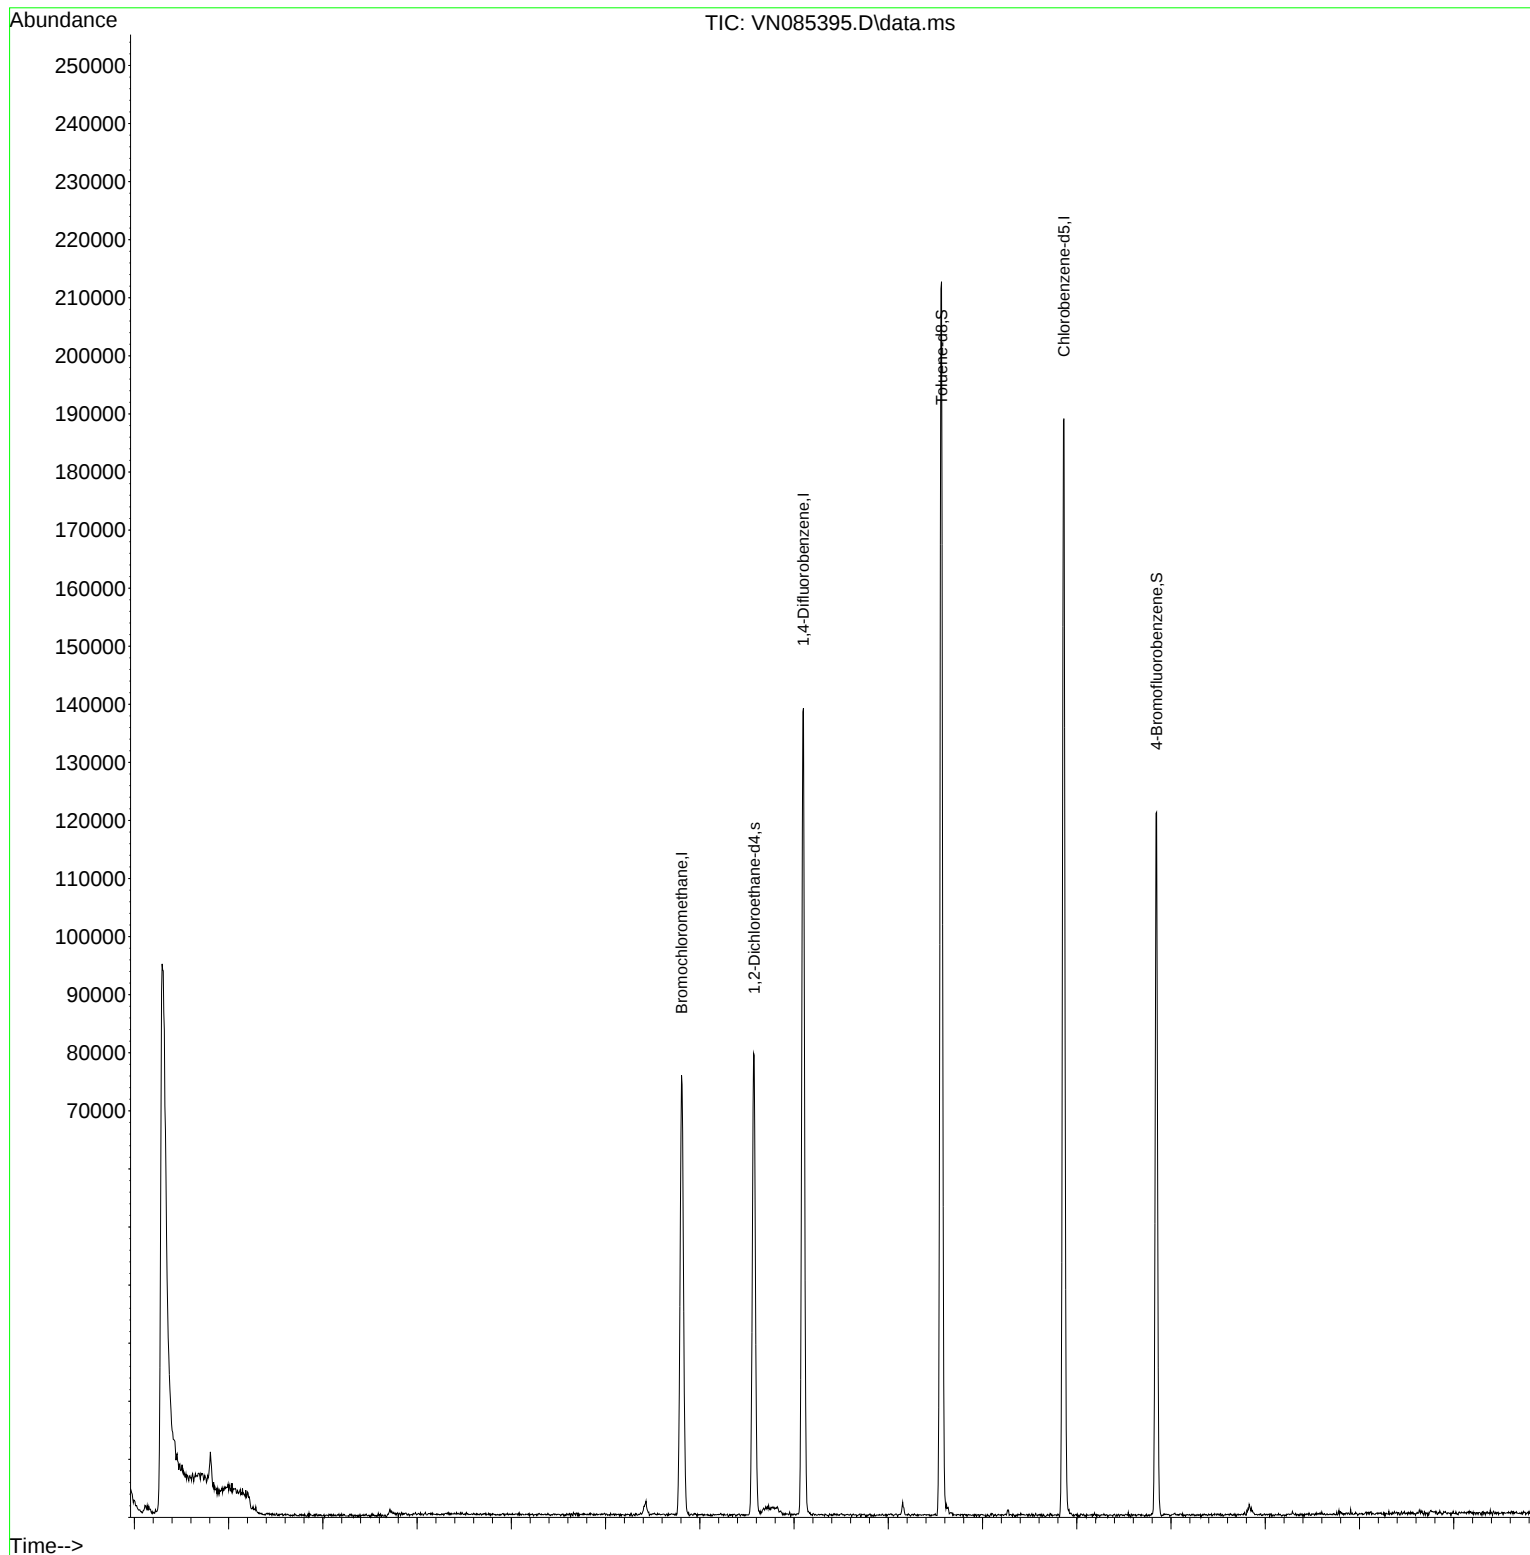


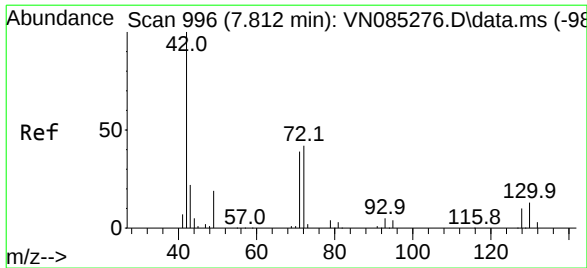

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.806 min Scan# 996
Delta R.T. -0.006 min
Lab File: VN085395.D
Acq: 07 Jan 2025 13:05




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion	Ratio	Lower	Upper
128	100		
49	190.8	0.0	497.8
130	130.0	0.0	328.5

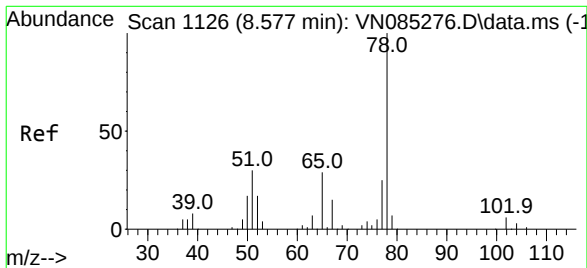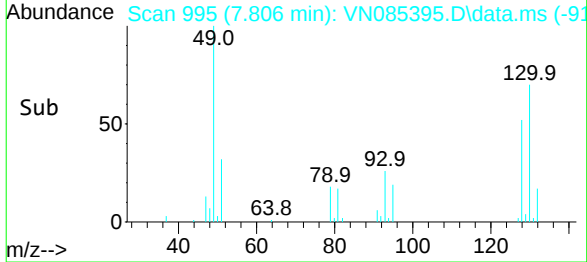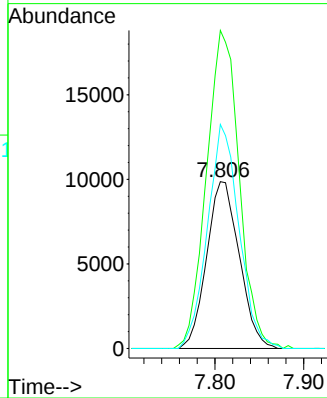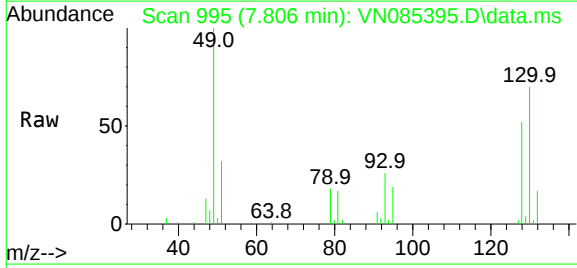

#27
1,2-Dichloroethane-d4
Concen: 30.384 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN085395.D
Acq: 07 Jan 2025 13:05

Tgt Ion	Ratio	Lower	Upper
65	100		
67	49.4	42.0	63.0


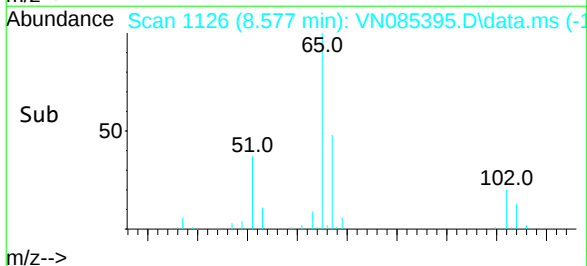
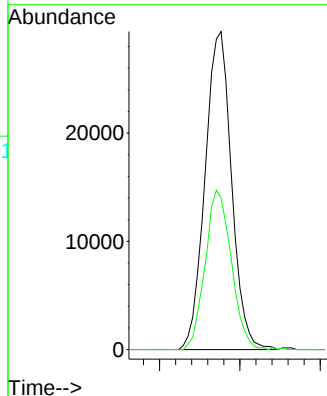
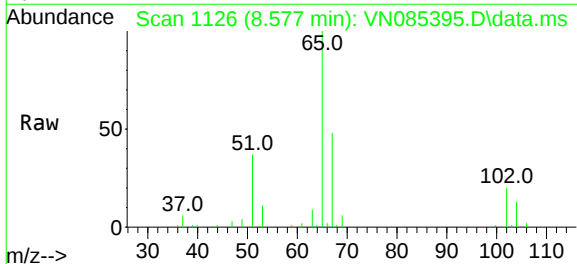


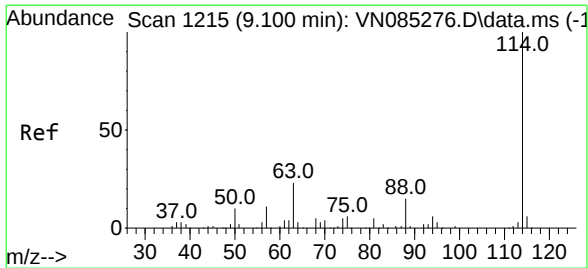

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.100 min Scan# 1215
Delta R.T. 0.000 min
Lab File: VN085395.D
Acq: 07 Jan 2025 13:05




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:	114	Resp:	114812
Ion Ratio	Lower	Upper	
114	100		
63	22.4	18.0	27.0
88	15.9	12.9	19.3

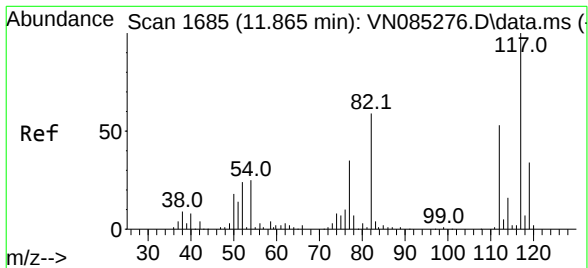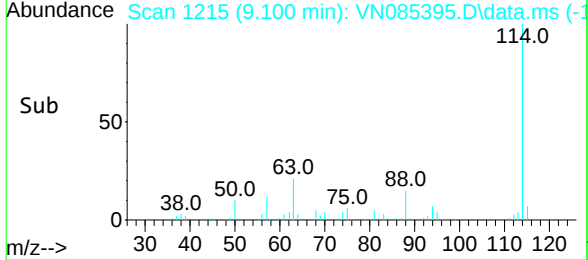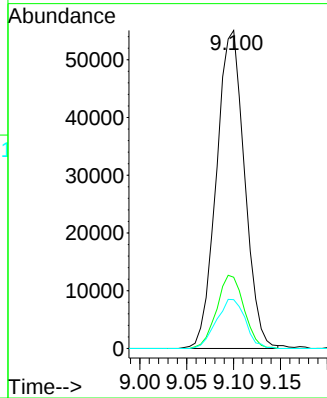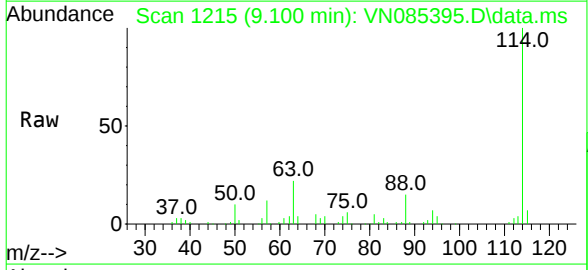

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VN085395.D
Acq: 07 Jan 2025 13:05

Tgt Ion:	117	Resp:	107360
Ion Ratio	Lower	Upper	
117	100		
82	58.1	47.4	71.0
119	31.5	25.3	37.9

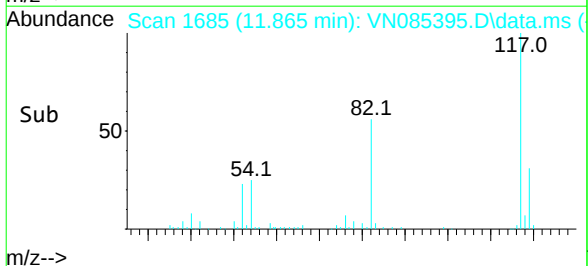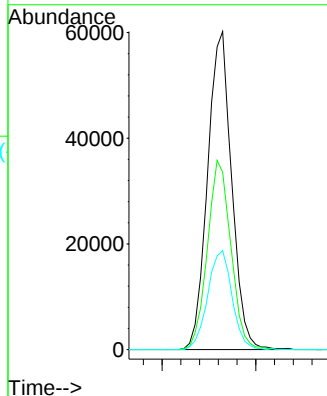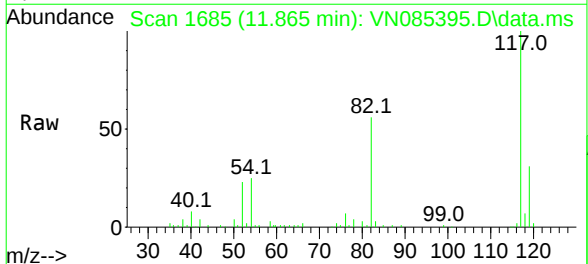

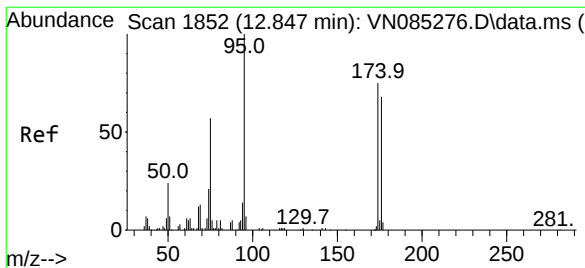

#60

4-Bromofluorobenzene

Concen: 23.296 ug/l

RT: 12.847 min Scan# 18

Delta R.T. 0.000 min

Lab File: VN085395.D

Acq: 07 Jan 2025 13:05

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion: 95 Resp: 40514

Ion Ratio Lower Upper

95 100

174 75.3 57.8 86.8

176 70.0 57.1 85.7

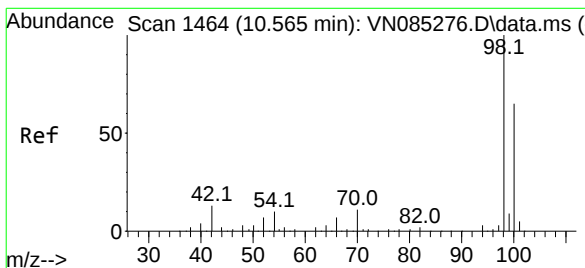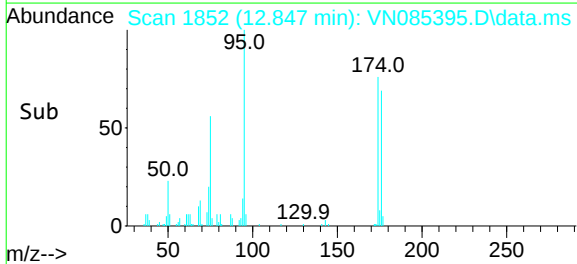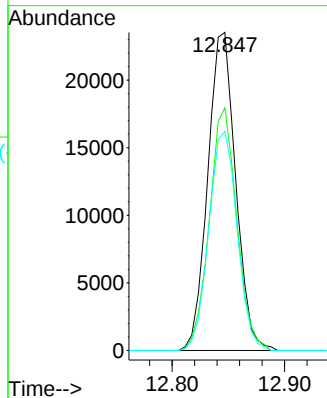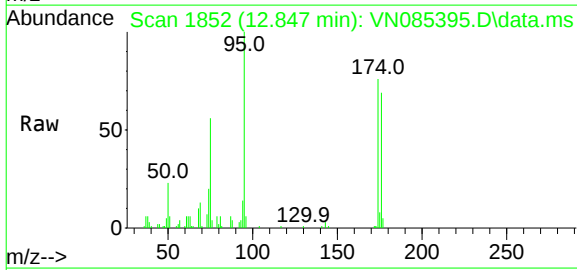

#63

Toluene-d8

Concen: 28.043 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. 0.000 min

Lab File: VN085395.D

Acq: 07 Jan 2025 13:05

Tgt Ion: 98 Resp: 147012

Ion Ratio Lower Upper

98 100

100 61.8 50.8 76.2

