
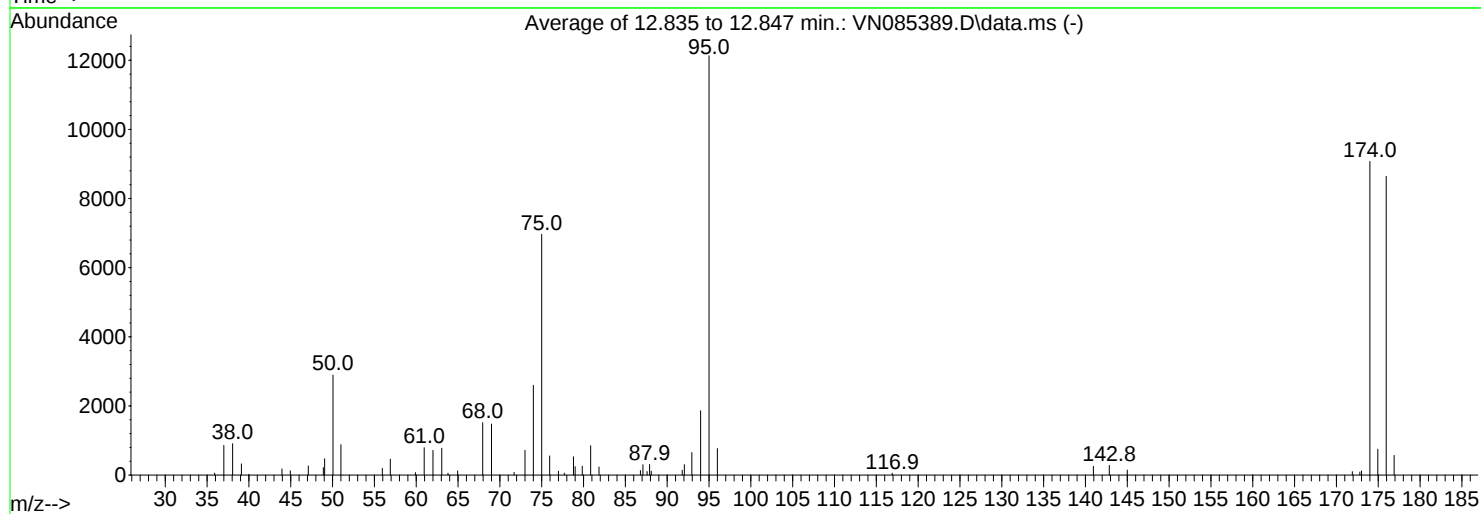


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010725\
Data File : VN085389.D
Acq On : 07 Jan 2025 09:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122024W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Dec 21 02:03:07 2024

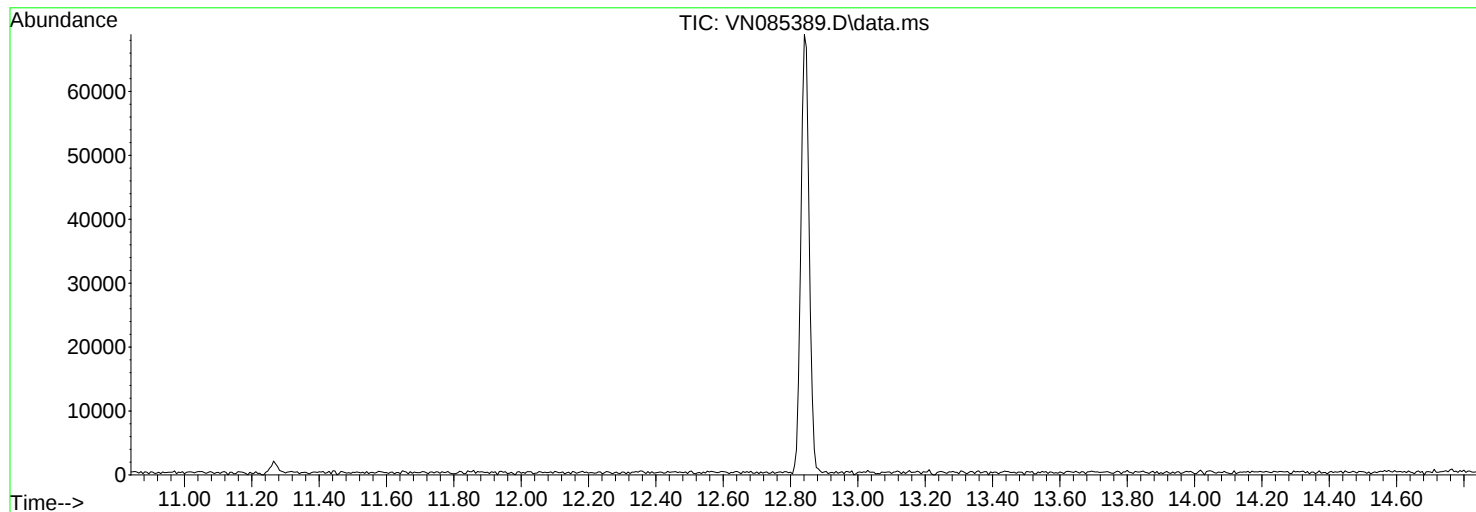

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	2894	PASS
75	95	30	60	57.4	6965	PASS
95	95	100	100	100.0	12131	PASS
96	95	5	9	6.3	768	PASS
173	174	0.00	2	1.3	120	PASS
174	95	50	100	74.8	9076	PASS
175	174	5	9	8.3	749	PASS
176	174	95	101	95.2	8644	PASS
177	176	5	9	6.6	571	PASS