

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010821\
 Data File : VN065438.D
 Acq On : 8 Jan 2021 12:51
 Operator : JC/MD
 Sample : VN0108MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0108MBL01

Quant Time: Jan 08 22:45:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 22 15:42:18 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.627	168	291887	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	479657	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.379	117	481479	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.318	152	180060	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.990	65	164575	49.94	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.88%
35) Dibromofluoromethane	7.553	113	147852	51.09	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	102.18%
50) Toluene-d8	10.058	98	581620	53.63	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	107.26%
62) 4-Bromofluorobenzene	12.376	95	215099	50.13	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	100.26%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010821\
Data File : VN065438.D
Acq On : 8 Jan 2021 12:51
Operator : JC/MD
Sample : VN0108MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0108MBL01

Quant Time: Jan 08 22:45:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 22 15:42:18 2020
Response via : Initial Calibration




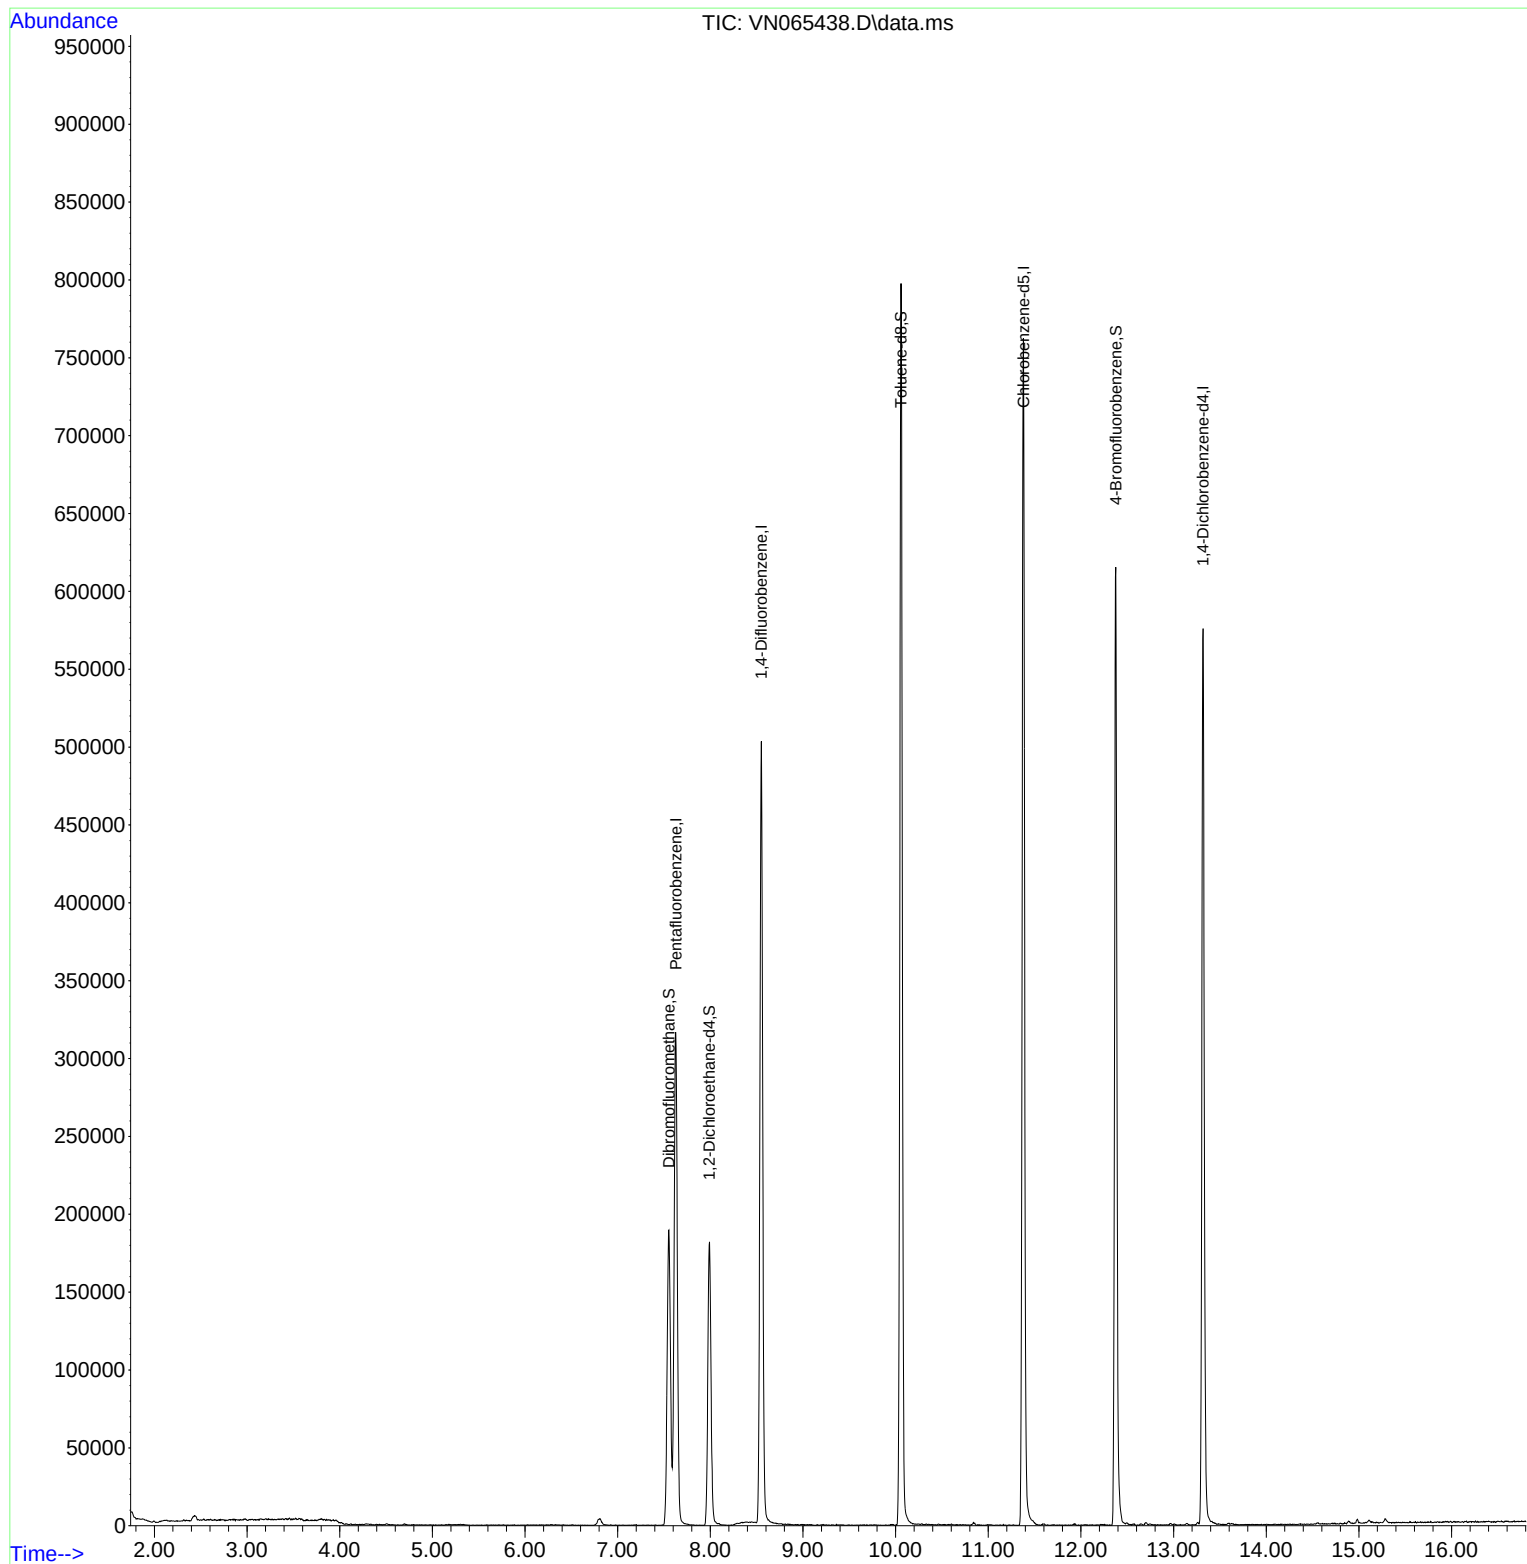


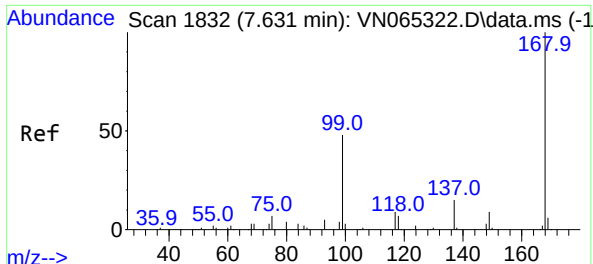

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. 0.000 min
Lab File: VN065438.D
Acq: 8 Jan 2021 12:51




Instrument :
MSVOA_N
ClientSampleId :
VN0108MBL01


Tgt Ion:168 Resp: 291887
Ion Ratio Lower Upper
168 100
99 48.9 43.0 64.4

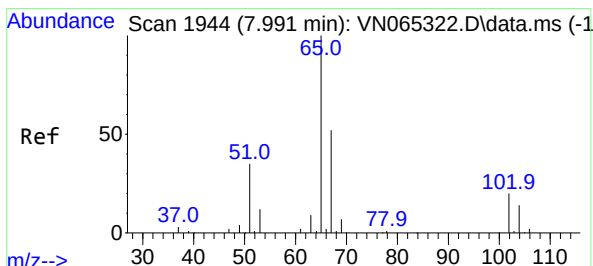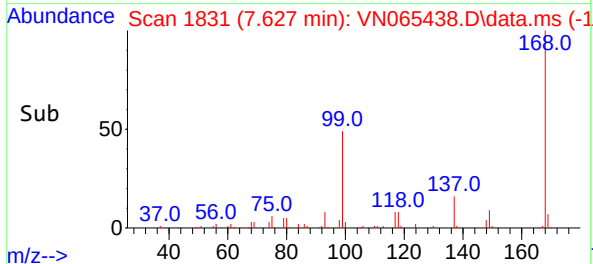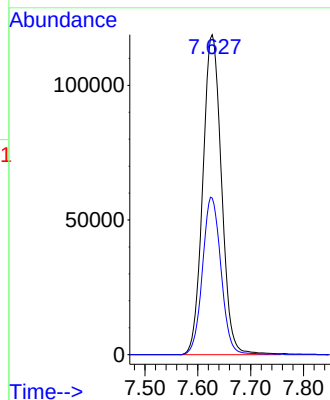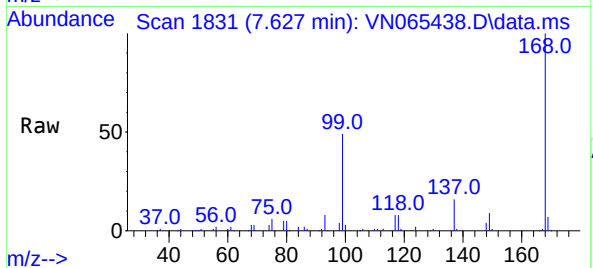

#33
1,2-Dichloroethane-d4
Concen: 49.94 ug/l
RT: 7.990 min Scan# 1944
Delta R.T. -0.000 min
Lab File: VN065438.D
Acq: 8 Jan 2021 12:51

Tgt Ion: 65 Resp: 164575
Ion Ratio Lower Upper
65 100
67 51.4 0.0 108.2

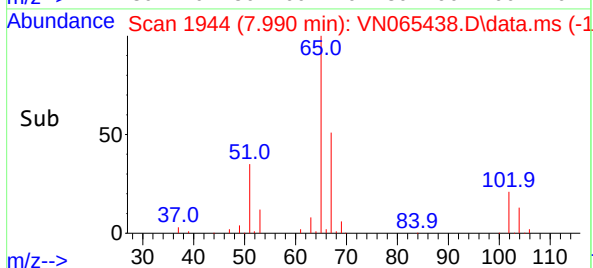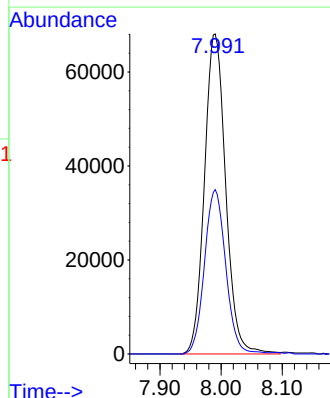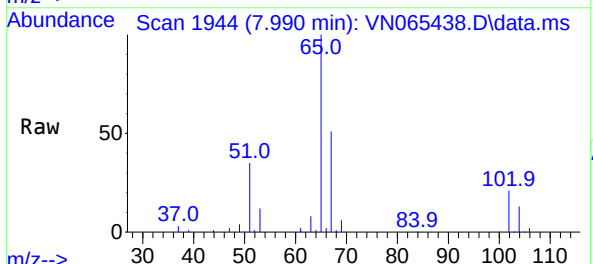




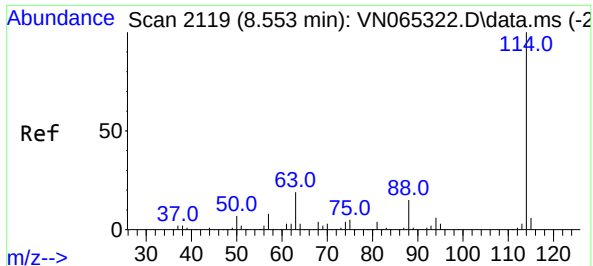


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. -0.000 min
Lab File: VN065438.D
Acq: 8 Jan 2021 12:51

Instrument :
MSVOA_N
ClientSampleId :
VN0108MBL01




Tgt Ion:114 Resp: 479657
Ion Ratio Lower Upper
114 100
63 18.9 0.0 38.6
88 14.9 0.0 32.6

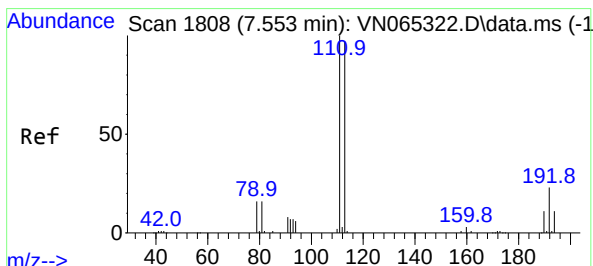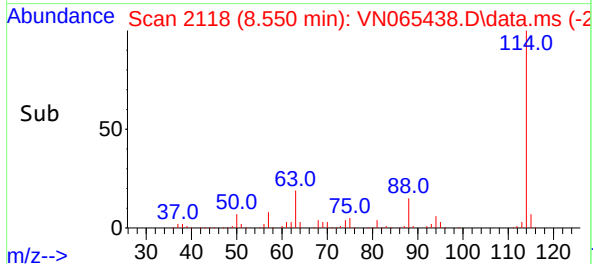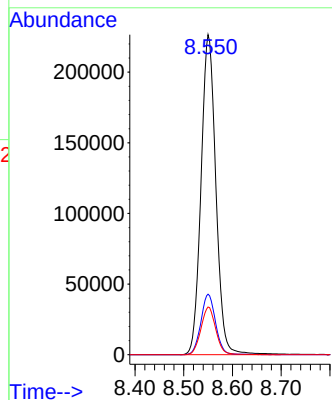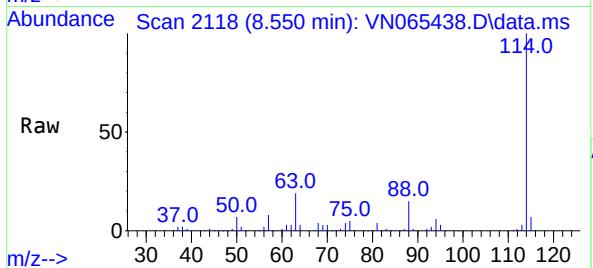


#35

Dibromofluoromethane
Concen: 51.09 ug/l
RT: 7.553 min Scan# 1808
Delta R.T. 0.003 min
Lab File: VN065438.D
Acq: 8 Jan 2021 12:51

Tgt Ion:113 Resp: 147852
Ion Ratio Lower Upper
113 100
111 102.4 81.6 122.4
192 23.2 16.2 24.2


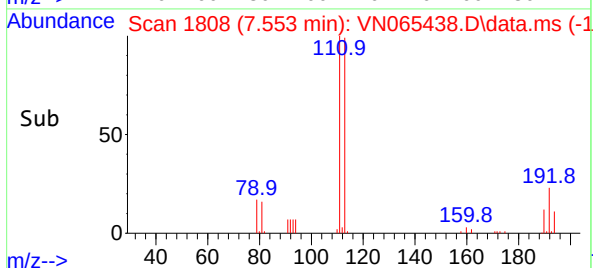
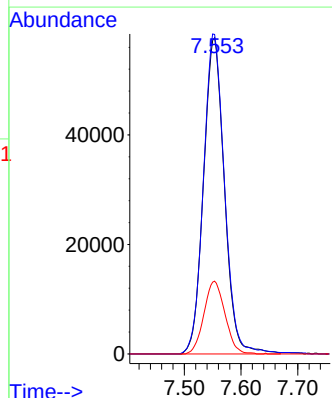
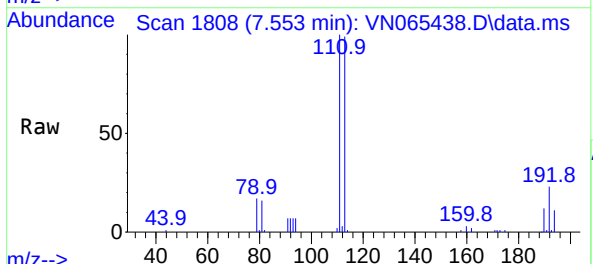


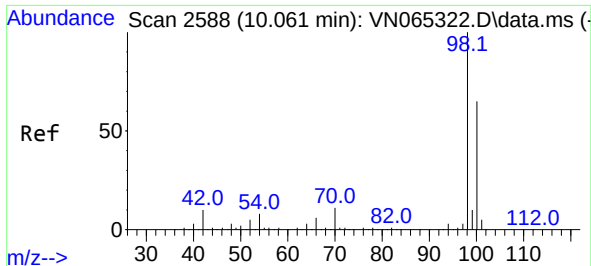

#50
Toluene-d8
Concen: 53.63 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. -0.000 min
Lab File: VN065438.D
Acq: 8 Jan 2021 12:51




Instrument :
MSVOA_N
ClientSampleId :
VN0108MBL01


Tgt Ion: 98 Resp: 581620
Ion Ratio Lower Upper
98 100
100 64.3 51.7 77.5

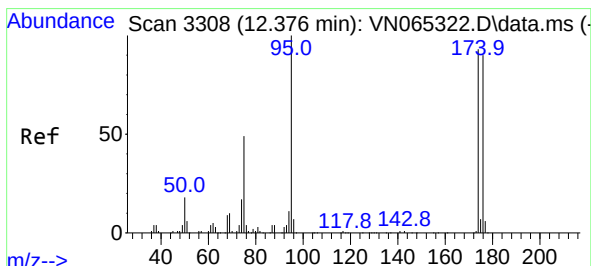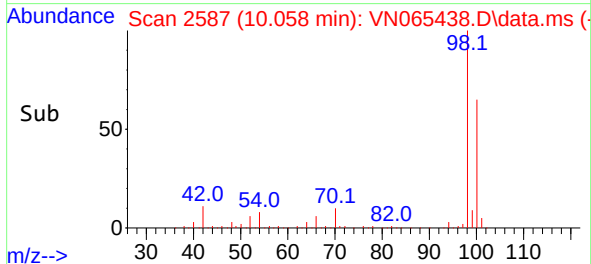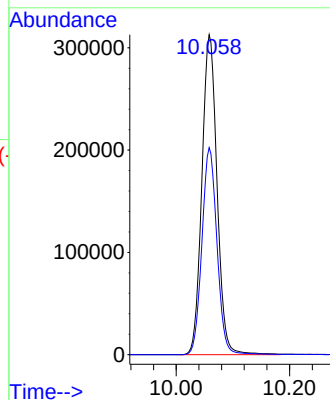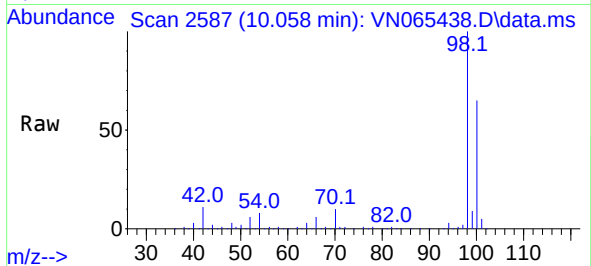

#62
4-Bromofluorobenzene
Concen: 50.13 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.000 min
Lab File: VN065438.D
Acq: 8 Jan 2021 12:51

Tgt Ion: 95 Resp: 215099
Ion Ratio Lower Upper
95 100
174 94.9 0.0 160.4
176 92.0 0.0 158.4


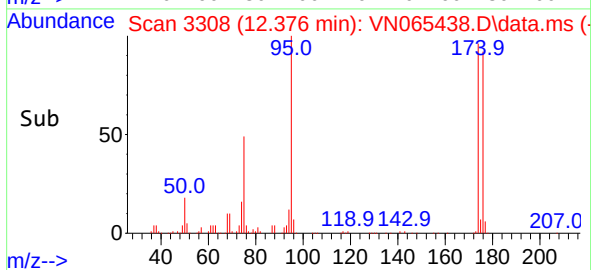
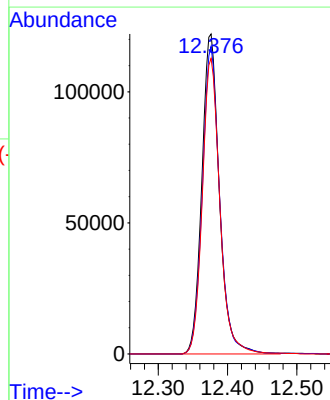
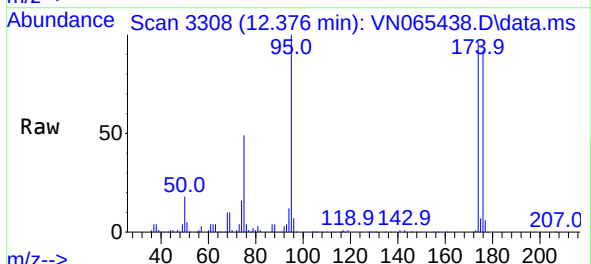


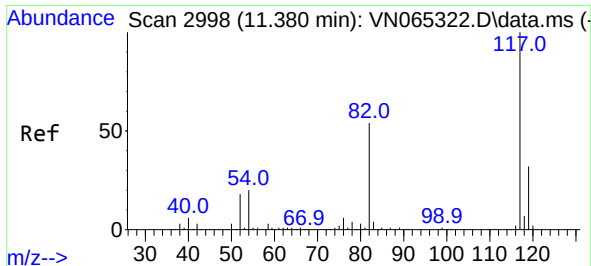

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.379 min Scan# 2998
Delta R.T. -0.001 min
Lab File: VN065438.D
Acq: 8 Jan 2021 12:51

Instrument :
MSVOA_N
ClientSampleId :
VN0108MBL01

Tgt Ion:117 Resp: 481479
Ion Ratio Lower Upper
117 100
82 52.9 44.2 66.2
119 32.6 25.8 38.6

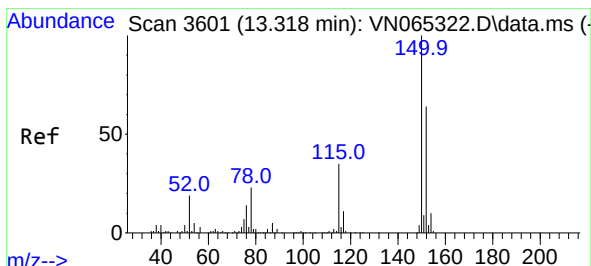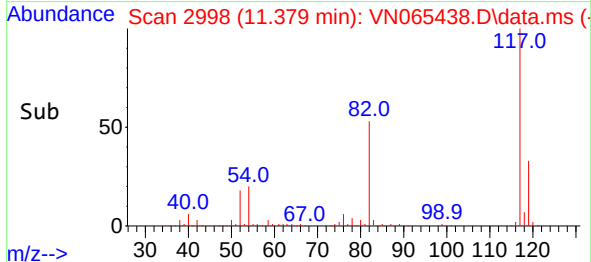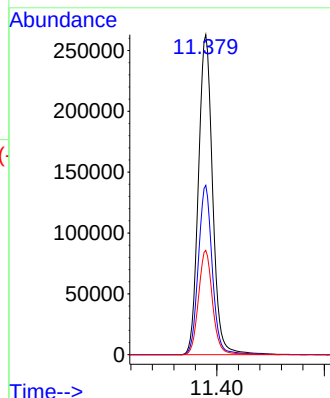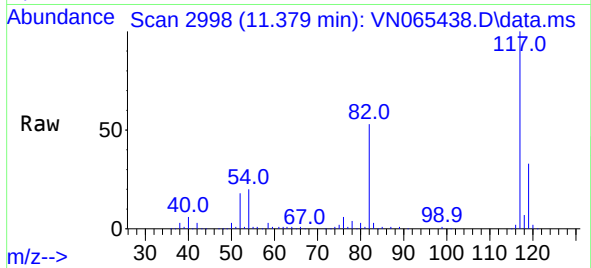

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.318 min Scan# 3601
Delta R.T. 0.000 min
Lab File: VN065438.D
Acq: 8 Jan 2021 12:51

Tgt Ion:152 Resp: 180060
Ion Ratio Lower Upper
152 100
115 55.6 29.7 89.1
150 156.9 0.0 350.6

