
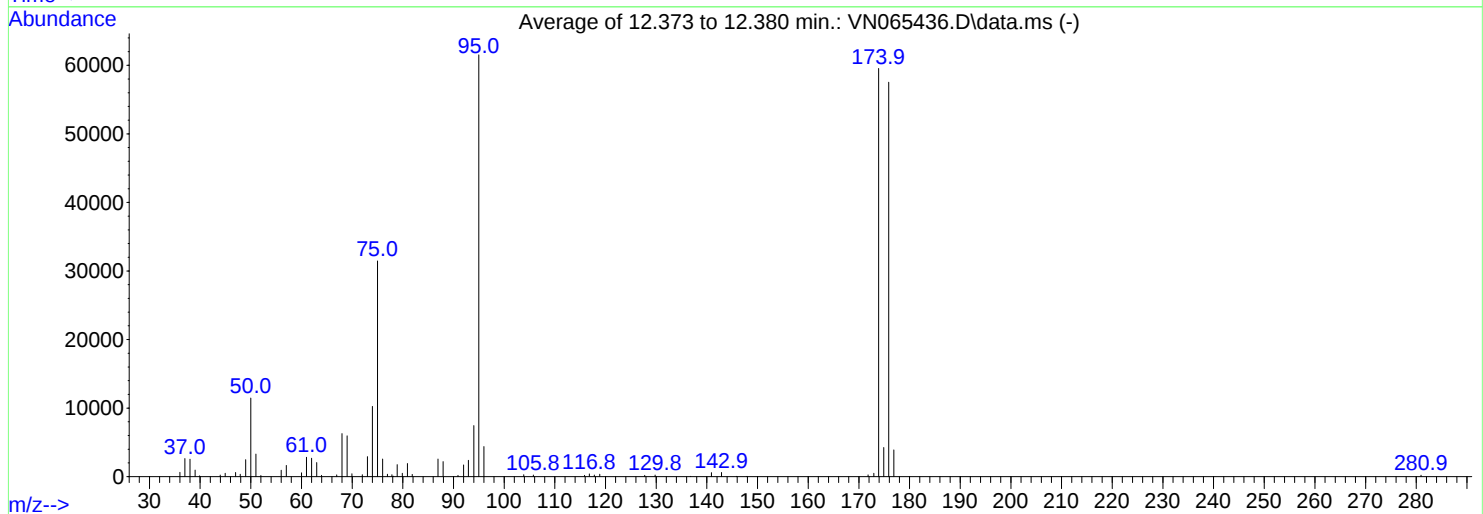


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010821\
 Data File : VN065436.D
 Acq On : 8 Jan 2021 11:46
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Title : SW846 8260
 Last Update : Tue Dec 22 15:42:18 2020

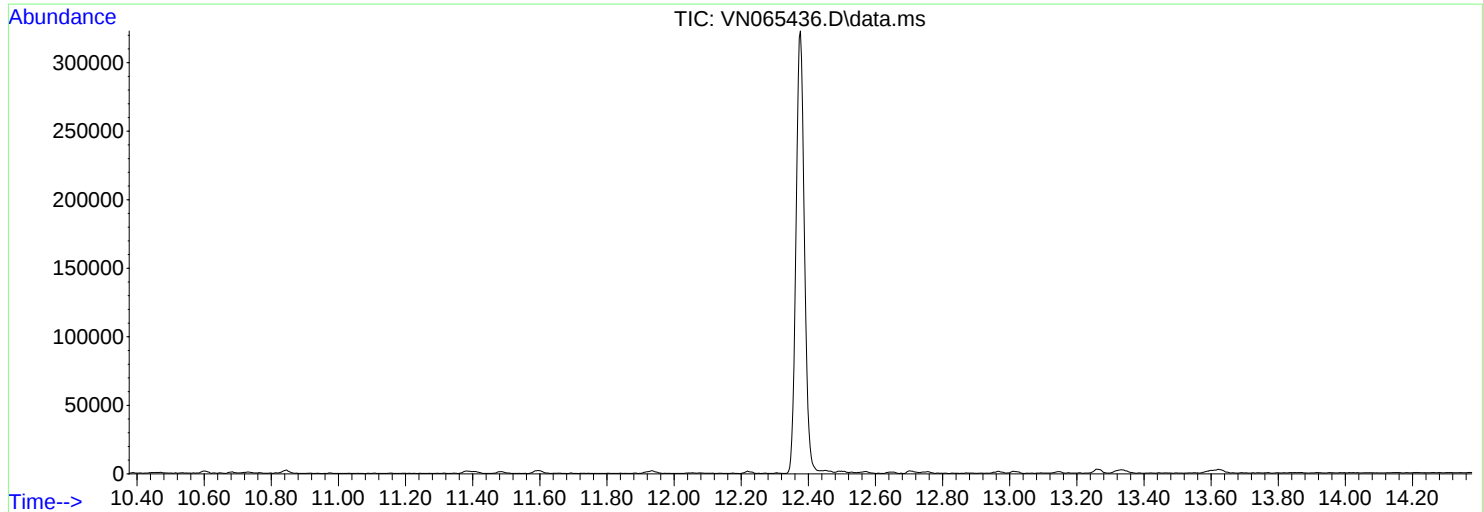

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	11463	PASS
75	95	30	60	51.2	31472	PASS
95	95	100	100	100.0	61528	PASS
96	95	5	9	7.1	4385	PASS
173	174	0.00	2	0.8	483	PASS
174	95	50	100	96.8	59549	PASS
175	174	5	9	7.1	4251	PASS
176	174	95	101	96.6	57525	PASS
177	176	5	9	6.8	3900	PASS