

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010923\
 Data File : VN076163.D
 Acq On : 09 Jan 2023 18:04
 Operator : JC\MD
 Sample : 01042-05 500X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 HYATT-SILICA

Quant Time: Jan 10 01:10:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	325736	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	518753	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	442008	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	181837	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	171045	48.267	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	96.540%
35) Dibromofluoromethane	8.177	113	156562	48.734	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.460%
50) Toluene-d8	10.571	98	593622	49.421	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.840%
62) 4-Bromofluorobenzene	12.853	95	184677	46.421	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.840%


Target Compounds				Qvalue		
6) Chloroethane	3.130	64	590	0.232	ug/l #	44
8) Diethyl Ether	3.983	74	429	0.226	ug/l	89
11) Tert butyl alcohol	5.536	59	4072	8.121	ug/l #	72
16) Acetone	4.459	43	7663	6.273	ug/l #	84
18) Methyl Acetate	5.053	43	2273	0.629	ug/l #	68
19) Methyl tert-butyl Ether	5.824	73	2262	0.238	ug/l #	84
20) Methylene Chloride	5.283	84	1765	Below Cal	#	76
22) Diisopropyl ether	6.694	45	24197	2.951	ug/l #	1
23) Vinyl Acetate	6.677	43	1631	0.296	ug/l #	65
25) 2-Butanone	7.500	43	3621	2.117	ug/l #	74
31) Cyclohexane	8.230	56	8710	1.716	ug/l #	24
36) 1,1-Dichloropropene	8.230	75	23346	5.471	ug/l #	49
37) Ethyl Acetate	7.577	43	2172	0.634	ug/l #	65
38) Carbon Tetrachloride	8.230	117	31799	6.658	ug/l #	17
39) Methylcyclohexane	9.606	83	2574	0.500	ug/l	95
40) Benzene	8.612	78	391479	29.732	ug/l	98
43) Isopropyl Acetate	8.718	43	6415	1.134	ug/l #	50
51) 4-Methyl-2-Pentanone	10.453	43	992	0.290	ug/l #	32
52) Toluene	10.635	92	302546	35.281	ug/l	99
59) 2-Hexanone	11.206	43	1730	0.694	ug/l	61
67) Ethyl Benzene	11.965	91	27447	1.793	ug/l	93
68) m/p-Xylenes	12.070	106	55532	9.163	ug/l	100
69) o-Xylene	12.400	106	19369	3.230	ug/l	100
71) Bromoform	12.853	173	1293	0.529	ug/l #	1
74) N-amyl acetate	12.465	43	1105	0.287	ug/l #	37
76) 1,2,3-Trichloropropane	12.853	75	95165	25.963	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.176	105	2601	0.237	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.853	75	95165	93.454	ug/l #	12
84) 1,2,4-Trimethylbenzene	13.488	105	5265	0.483	ug/l	95
85) sec-Butylbenzene	13.488	105	5265	0.393	ug/l #	56
92) 1,2-Dibromo-3-Chloropr...	14.770	75	339	0.470	ug/l #	1
95) Naphthalene	15.641	128	9614	3.107	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010923\
Data File : VN076163.D
Acq On : 09 Jan 2023 18:04
Operator : JC\MD
Sample : 01042-05 500X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA

Quant Time: Jan 10 01:10:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration




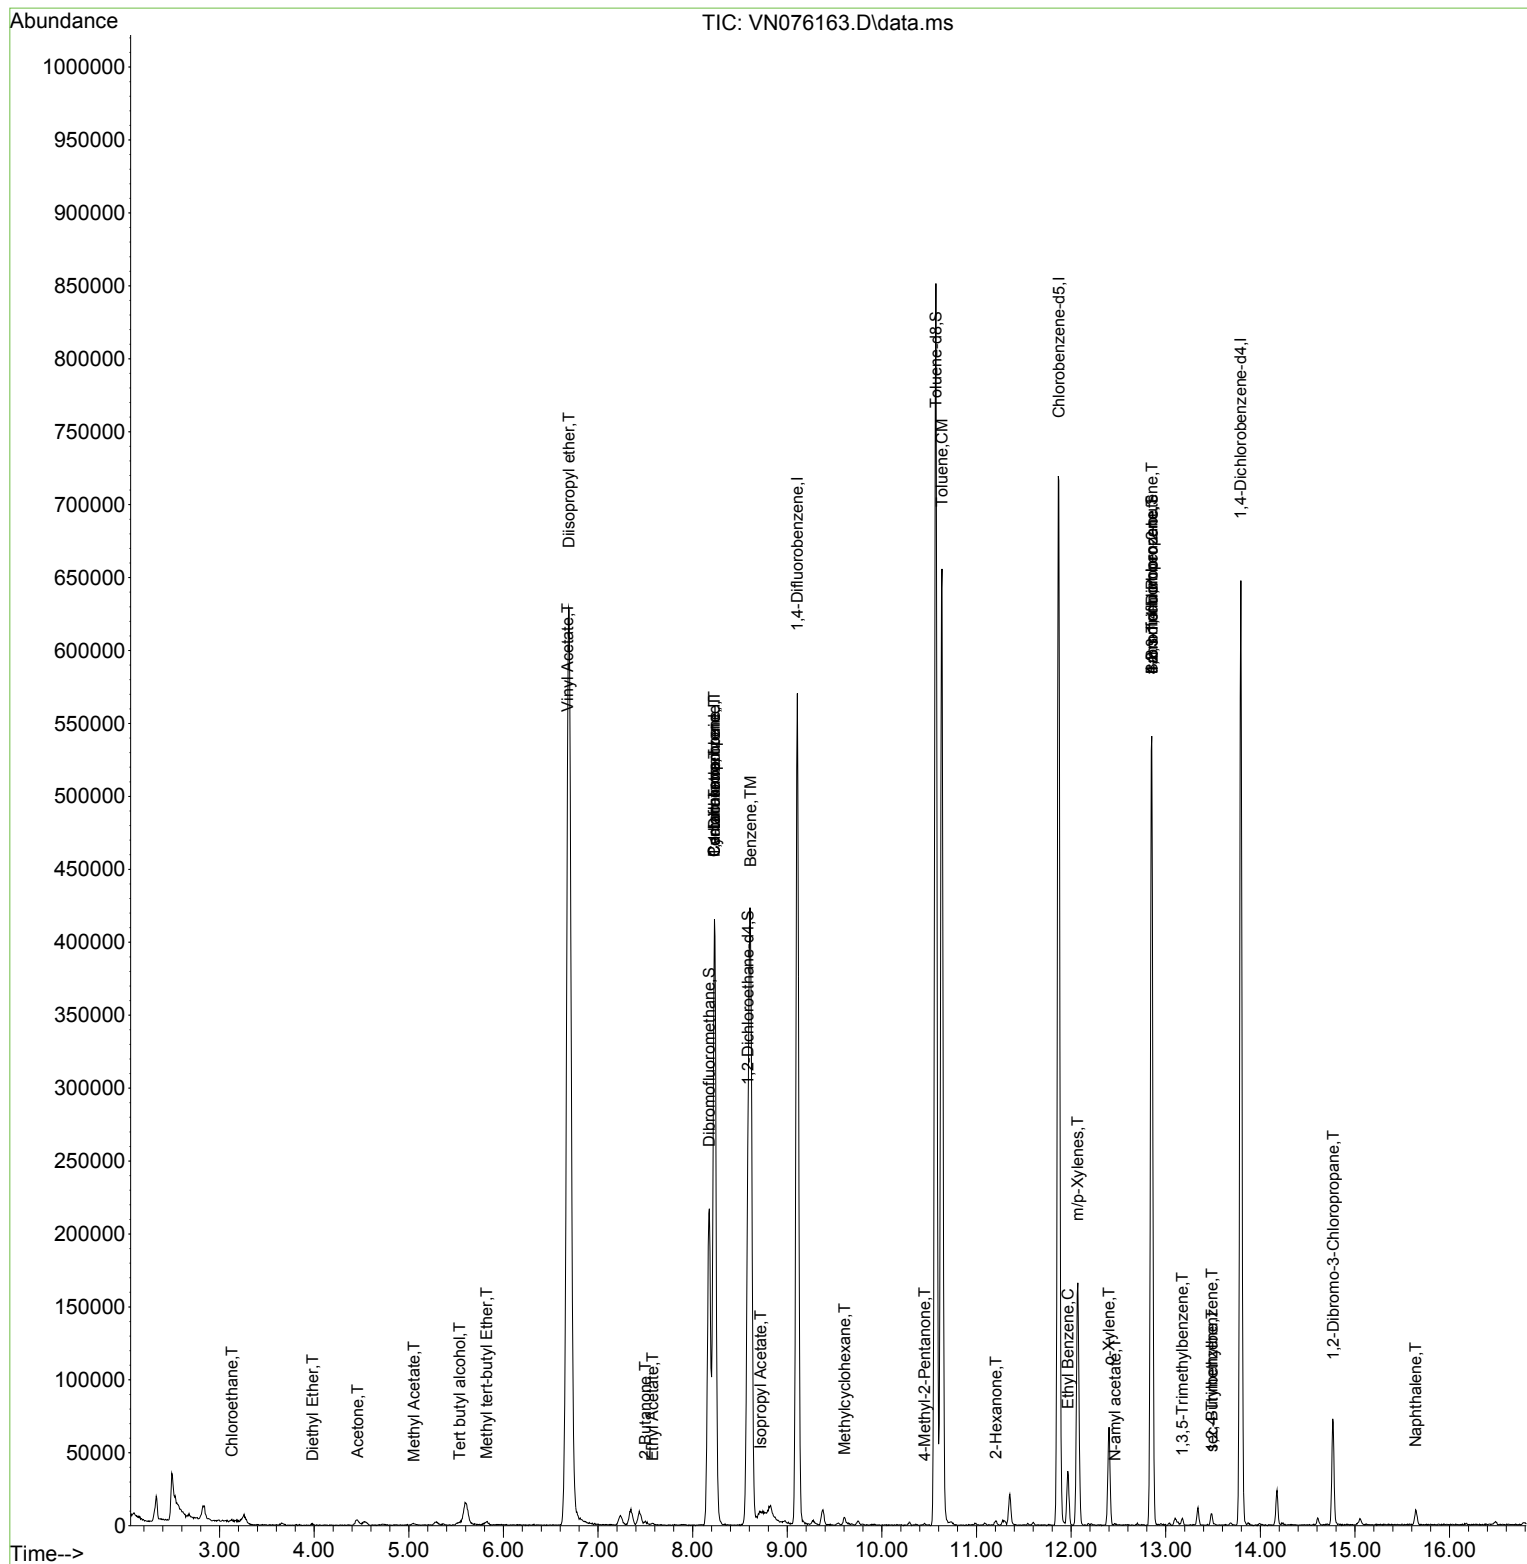




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion:168 Resp: 325736
Ion Ratio Lower Upper
168 100
99 52.0 44.2 66.4

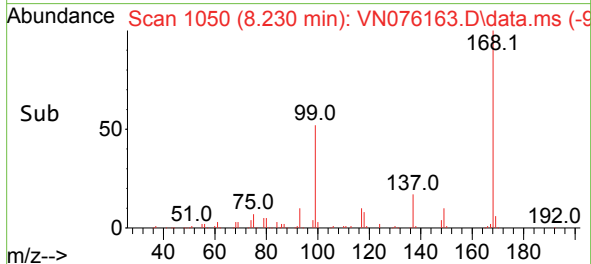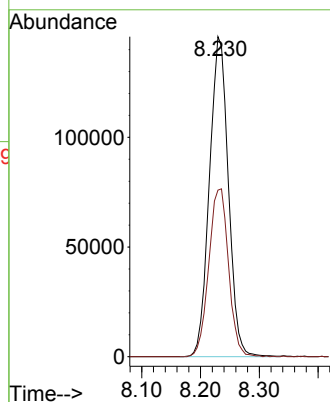

#6
Chloroethane
Concen: 0.232 ug/l
RT: 3.130 min Scan# 183
Delta R.T. 0.012 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 64 Resp: 590
Ion Ratio Lower Upper
64 100
66 0.0 24.6 36.8#

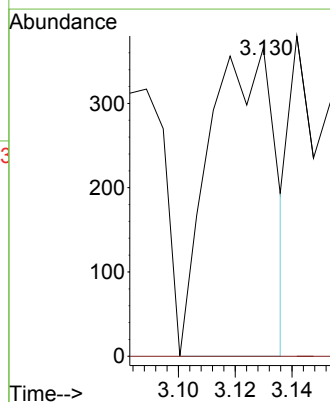



#8
Diethyl Ether

Concen: 0.226 ug/l

RT: 3.983 min Scan# 31

Delta R.T. 0.012 min

Lab File: VN076163.D

Acq: 09 Jan 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :





HYATT-SILICA

Tgt Ion: 74 Resp: 429

Ion Ratio Lower Upper

74 100

45 84.8 37.8 113.4

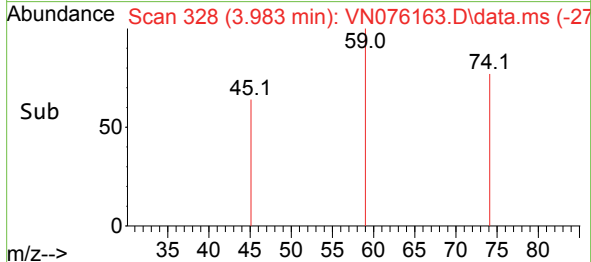

#11

Tert butyl alcohol

Concen: 8.121 ug/l

RT: 5.536 min Scan# 592

Delta R.T. -0.000 min

Lab File: VN076163.D




Acq: 09 Jan 2023 18:04


Tgt Ion: 59 Resp: 4072

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.4#




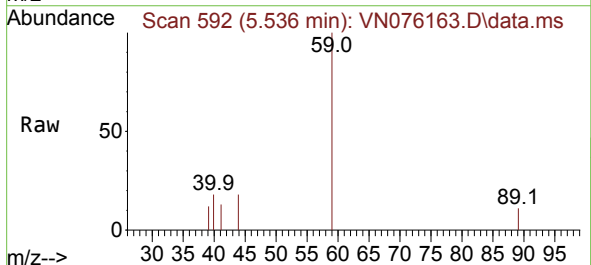




#16
Acetone
Concen: 6.273 ug/l
RT: 4.459 min Scan# 406
Delta R.T. 0.018 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion: 43 Resp: 7663
Ion Ratio Lower Upper
43 100
58 26.5 28.6 43.0#

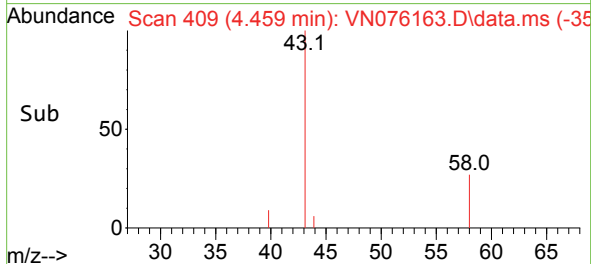

#18
Methyl Acetate
Concen: 0.629 ug/l
RT: 5.053 min Scan# 510
Delta R.T. 0.018 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 43 Resp: 2273
Ion Ratio Lower Upper
43 100
74 12.1 23.6 35.4#







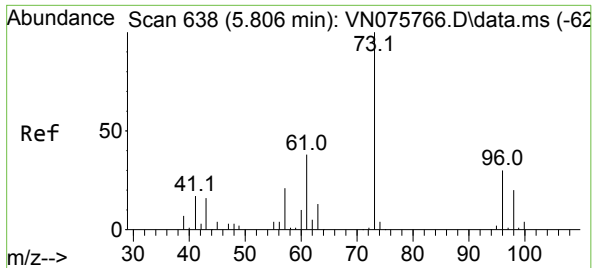

#19
Methyl tert-butyl Ether
Concen: 0.238 ug/l
RT: 5.824 min Scan# 641
Delta R.T. 0.018 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion: 73 Resp: 2262
Ion Ratio Lower Upper
73 100
57 29.0 17.1 25.7#

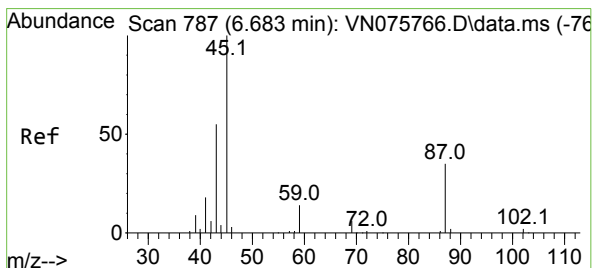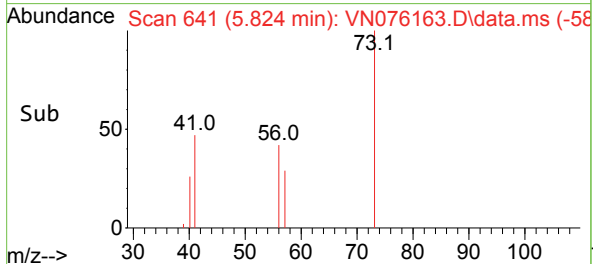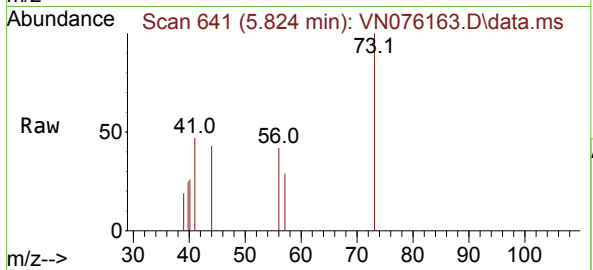

#22
Diisopropyl ether
Concen: 2.951 ug/l
RT: 6.694 min Scan# 789
Delta R.T. 0.012 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 45 Resp: 24197
Ion Ratio Lower Upper
45 100
43 5.5 44.2 66.4#
87 0.0 28.3 42.5#
59 217.9 11.1 16.7#


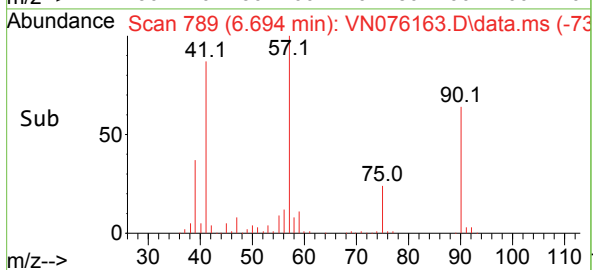

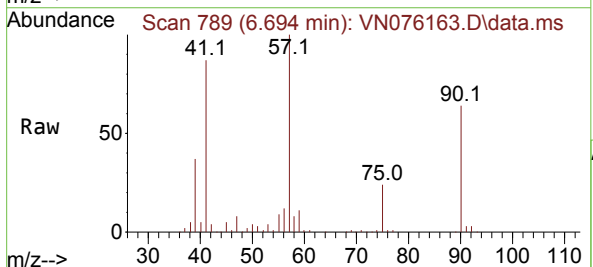




#23
 Vinyl Acetate
 Concen: 0.296 ug/l
 RT: 6.677 min Scan# 71
 Delta R.T. 0.065 min
 Lab File: VN076163.D
 Acq: 09 Jan 2023 18:04




Instrument :
 MSVOA_N
 ClientSampleId :
 HYATT-SILICA


Tgt Ion: 43 Resp: 1631
 Ion Ratio Lower Upper
 43 100
 86 0.0 11.4 17.2#

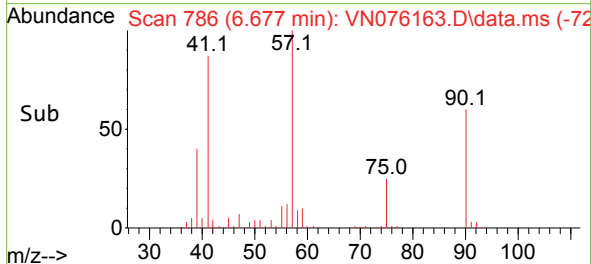

#25
 2-Butanone
 Concen: 2.117 ug/l
 RT: 7.500 min Scan# 926
 Delta R.T. 0.012 min
 Lab File: VN076163.D
 Acq: 09 Jan 2023 18:04

Tgt Ion: 43 Resp: 3621
 Ion Ratio Lower Upper
 43 100
 72 19.9 28.0 42.0#









#31
Cyclohexane
Concen: 1.716 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.035 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion: 56 Resp: 8710
Ion Ratio Lower Upper
56 100
69 145.2 24.7 37.1#
84 128.3 76.5 114.7#

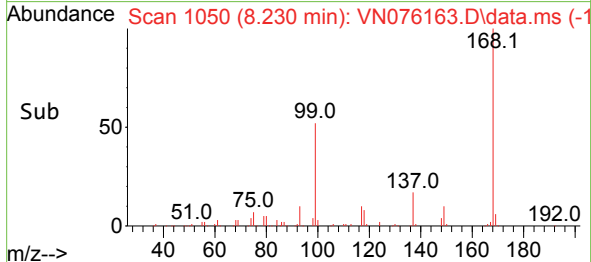

#33
1,2-Dichloroethane-d4
Concen: 48.267 ug/l
RT: 8.582 min Scan# 1110
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 65 Resp: 171045
Ion Ratio Lower Upper
65 100
67 53.4 0.0 103.4




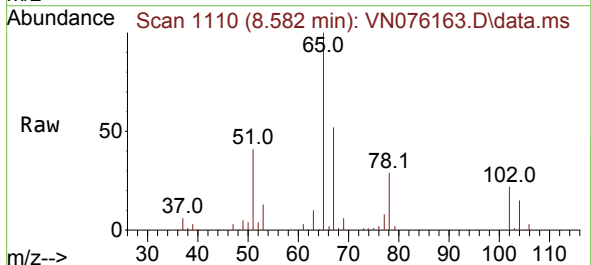




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion:114 Resp: 518753
Ion Ratio Lower Upper
114 100
63 17.2 0.0 34.4
88 14.0 0.0 28.8

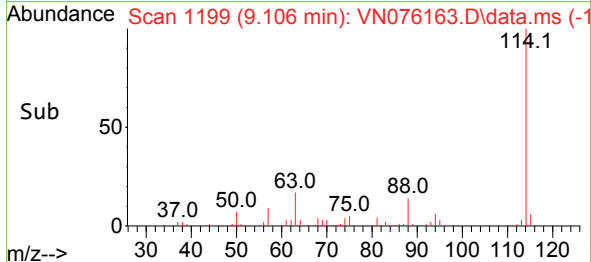

#35
Dibromofluoromethane
Concen: 48.734 ug/l
RT: 8.177 min Scan# 1041
Delta R.T. 0.006 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion:113 Resp: 156562
Ion Ratio Lower Upper
113 100
111 102.5 83.4 125.2
192 19.8 16.1 24.1

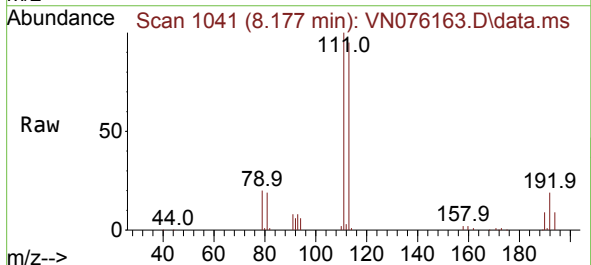



#36

1,1-Dichloropropene

Concen: 5.471 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.147 min

Lab File: VN076163.D

Acq: 09 Jan 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

HYATT-SILICA





Tgt Ion: 75 Resp: 23346

Ion Ratio Lower Upper

75 100

110 9.0 18.8 56.4#

77 0.0 24.1 36.1#

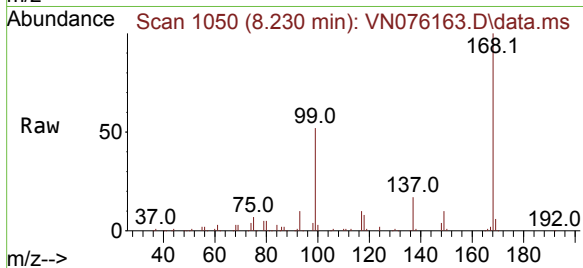

#37

Ethyl Acetate

Concen: 0.634 ug/l

RT: 7.577 min Scan# 939

Delta R.T. 0.012 min

Lab File: VN076163.D

Acq: 09 Jan 2023 18:04




Tgt Ion: 43 Resp: 2172


Ion Ratio Lower Upper

43 100

61 0.0 13.0 19.4#

70 0.0 9.4 14.0#




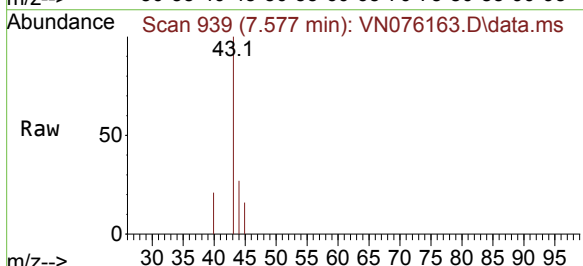




#38
Carbon Tetrachloride
Concen: 6.658 ug/l
RT: 8.230 min Scan# 1073
Delta R.T. -0.135 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion:117 Resp: 31799
Ion Ratio Lower Upper
117 100
119 5.4 76.1 114.1#
121 0.0 24.5 36.7#

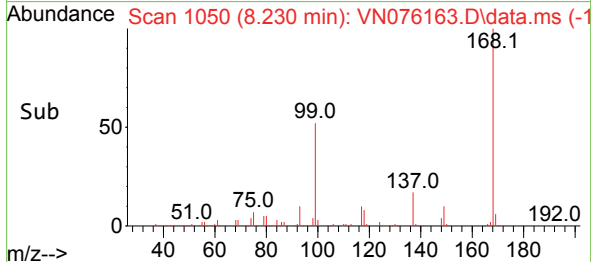

#39
Methylcyclohexane
Concen: 0.500 ug/l
RT: 9.606 min Scan# 1284
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 83 Resp: 2574
Ion Ratio Lower Upper
83 100
55 69.2 51.4 77.0
98 47.6 39.8 59.8




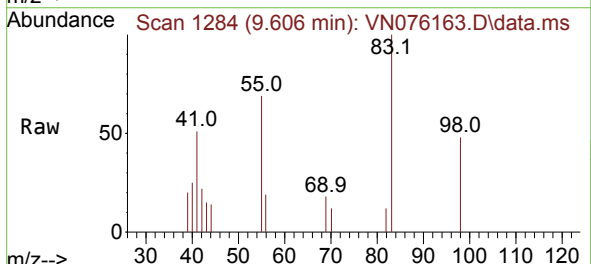




#40
Benzene
Concen: 29.732 ug/l
RT: 8.612 min Scan# 1115
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion: 78 Resp: 391479
Ion Ratio Lower Upper
78 100
77 23.9 18.5 27.7

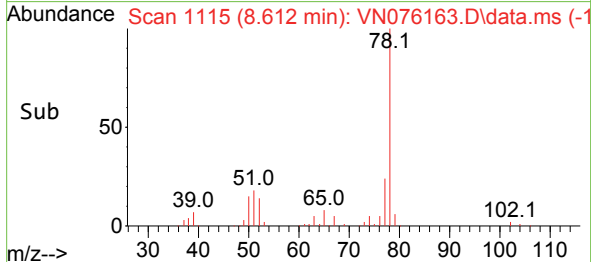

#43
Isopropyl Acetate
Concen: 1.134 ug/l
RT: 8.718 min Scan# 1133
Delta R.T. 0.024 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 43 Resp: 6415
Ion Ratio Lower Upper
43 100
61 0.0 24.2 36.4#
87 0.0 13.3 19.9#




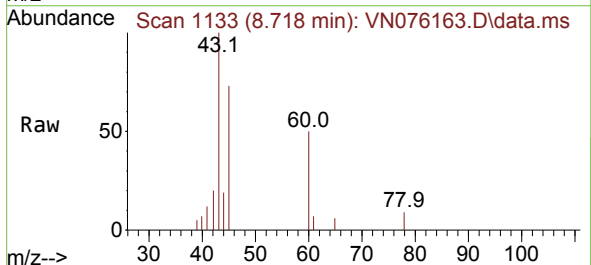




#50
Toluene-d8
Concen: 49.421 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion: 98 Resp: 593622
Ion Ratio Lower Upper
98 100
100 64.9 52.1 78.1

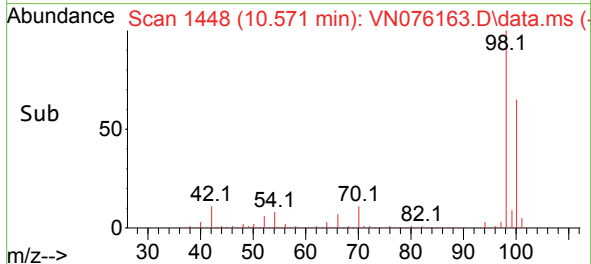

#51
4-Methyl-2-Pentanone
Concen: 0.290 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 43 Resp: 992
Ion Ratio Lower Upper
43 100
58 0.0 35.5 53.3#









#52
Toluene
Concen: 35.281 ug/l
RT: 10.635 min Scan# 1459
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion: 92 Resp: 302546
Ion Ratio Lower Upper
92 100
91 172.7 137.3 205.9

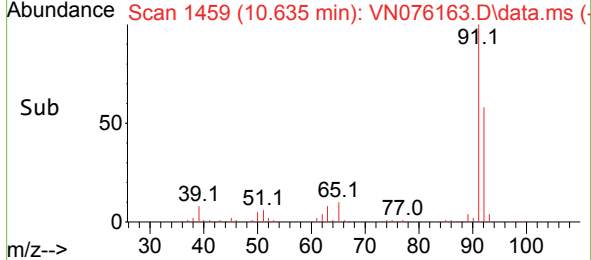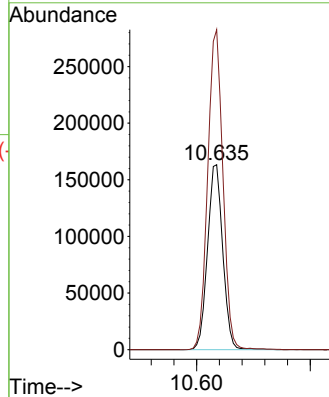

#59
2-Hexanone
Concen: 0.694 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.006 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 43 Resp: 1730
Ion Ratio Lower Upper
43 100
58 31.3 30.6 92.0


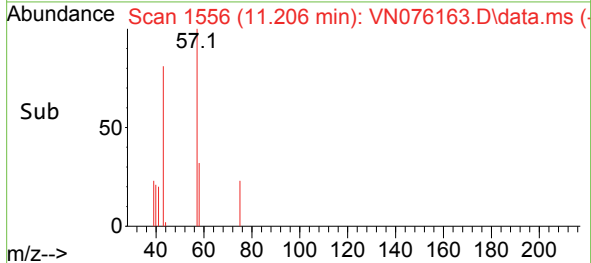
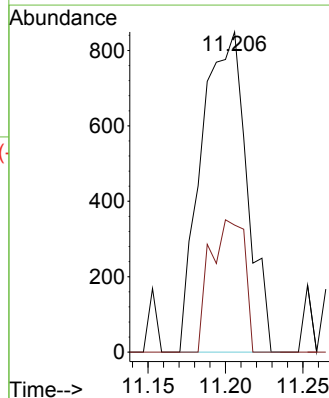





#62
4-Bromofluorobenzene
Concen: 46.421 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion: 95 Resp: 184677
Ion Ratio Lower Upper
95 100
174 86.4 0.0 171.6
176 82.7 0.0 169.2



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1669
Delta R.T. 0.006 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion: 117 Resp: 442008
Ion Ratio Lower Upper
117 100
82 53.9 41.3 61.9
119 32.0 24.6 37.0









#67
Ethyl Benzene
Concen: 1.793 ug/l
RT: 11.965 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion: 91 Resp: 27447
Ion Ratio Lower Upper
91 100
106 28.0 25.7 38.5

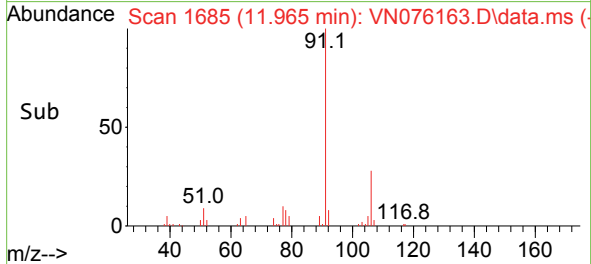

#68
m/p-Xylenes
Concen: 9.163 ug/l
RT: 12.070 min Scan# 1703
Delta R.T. -0.006 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion:106 Resp: 55532
Ion Ratio Lower Upper
106 100
91 196.4 156.6 235.0




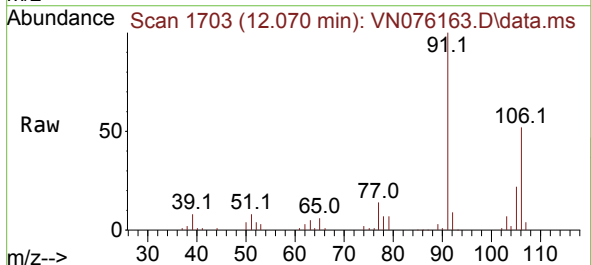




#69
o-Xylene
Concen: 3.230 ug/l
RT: 12.400 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA


Tgt Ion:106 Resp: 19369
Ion Ratio Lower Upper
106 100
91 208.2 103.8 311.6

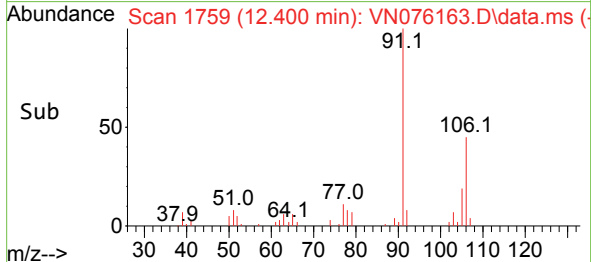

#71
Bromoform
Concen: 0.529 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.271 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Tgt Ion:173 Resp: 1293
Ion Ratio Lower Upper
173 100
175 779.1 24.3 72.8#
254 0.0 0.0 0.0




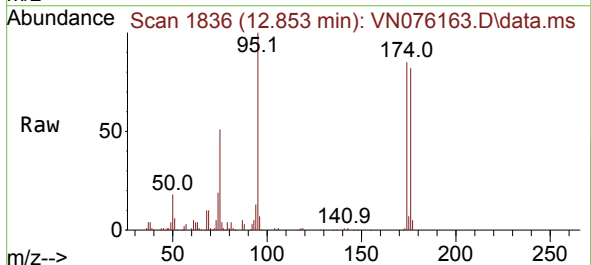




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 1996
 Delta R.T. -0.000 min
 Lab File: VN076163.D
 Acq: 09 Jan 2023 18:04




Instrument :
 MSVOA_N
 ClientSampleId :
 HYATT-SILICA


Tgt Ion:152 Resp: 181837
 Ion Ratio Lower Upper
 152 100
 115 56.7 29.1 87.4
 150 154.1 0.0 347.0

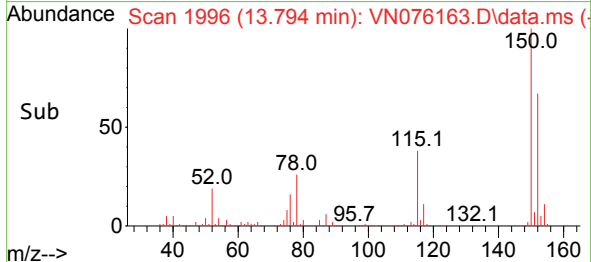

#74
 N-ethyl acetate
 Concen: 0.287 ug/l
 RT: 12.465 min Scan# 1770
 Delta R.T. -0.029 min
 Lab File: VN076163.D
 Acq: 09 Jan 2023 18:04

Tgt Ion: 43 Resp: 1105
 Ion Ratio Lower Upper
 43 100
 70 0.0 41.4 62.0#
 55 0.0 21.3 31.9#
 61 0.0 21.2 31.8#

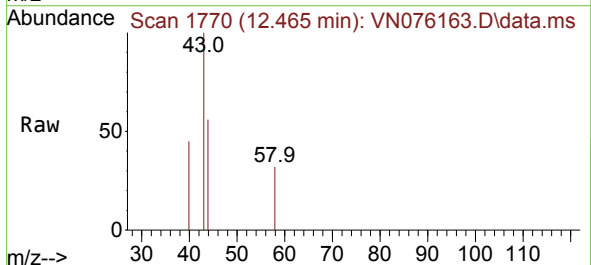



#76

1,2,3-Trichloropropane

Concen: 25.963 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. -0.141 min

Lab File: VN076163.D

Acq: 09 Jan 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :





HYATT-SILICA

Tgt Ion: 75 Resp: 95165

Ion Ratio Lower Upper

75 100

77 1.3 82.6 247.8#

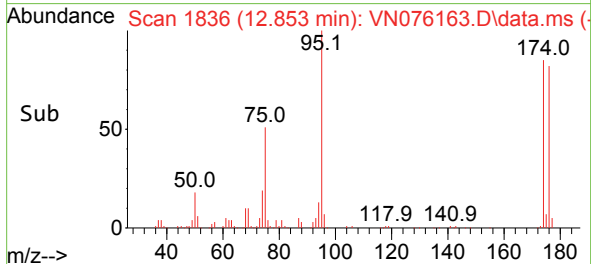

#80

1,3,5-Trimethylbenzene

Concen: 0.237 ug/l

RT: 13.176 min Scan# 1891

Delta R.T. -0.000 min

Lab File: VN076163.D




Acq: 09 Jan 2023 18:04


Tgt Ion:105 Resp: 2601

Ion Ratio Lower Upper

105 100

120 48.2 24.7 74.1









#81
 trans-1,4-Dichloro-2-butene
 Concen: 93.454 ug/l
 RT: 12.853 min Scan# 1836
 Delta R.T. 0.112 min
 Lab File: VN076163.D
 Acq: 09 Jan 2023 18:04




Instrument :
 MSVOA_N
 ClientSampleId :
 HYATT-SILICA


Tgt Ion: 75 Resp: 95165
 Ion Ratio Lower Upper
 75 100
 53 0.0 73.8 110.6#
 89 0.0 39.5 59.3#



#84
 1,2,4-Trimethylbenzene
 Concen: 0.483 ug/l
 RT: 13.488 min Scan# 1944
 Delta R.T. 0.006 min
 Lab File: VN076163.D
 Acq: 09 Jan 2023 18:04

Tgt Ion: 105 Resp: 5265
 Ion Ratio Lower Upper
 105 100
 120 49.9 23.3 69.8









#85
 sec-Butylbenzene
 Concen: 0.393 ug/l
 RT: 13.488 min Scan# 1966
 Delta R.T. -0.129 min
 Lab File: VN076163.D
 Acq: 09 Jan 2023 18:04




Instrument :
 MSVOA_N
 ClientSampleId :
 HYATT-SILICA


Tgt Ion:105 Resp: 5265
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.1 30.1#

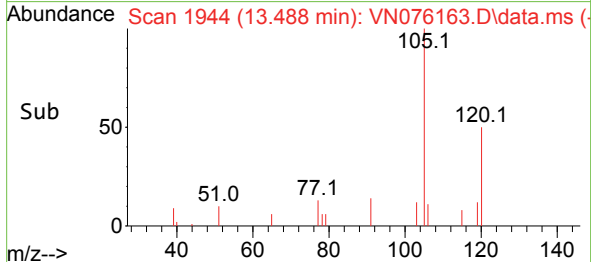

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.470 ug/l
 RT: 14.770 min Scan# 2162
 Delta R.T. 0.047 min
 Lab File: VN076163.D
 Acq: 09 Jan 2023 18:04


Tgt Ion: 75 Resp: 339
 Ion Ratio Lower Upper
 75 100
 155 0.0 49.3 147.8#
 157 0.0 63.7 191.3#

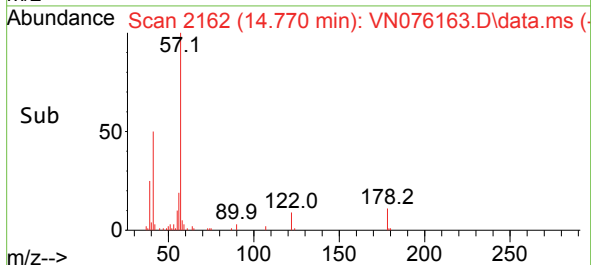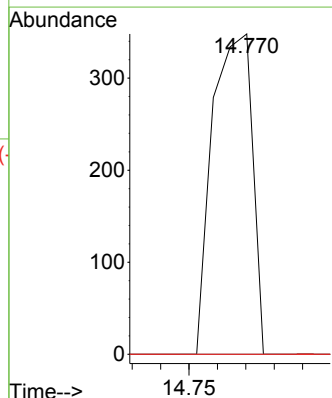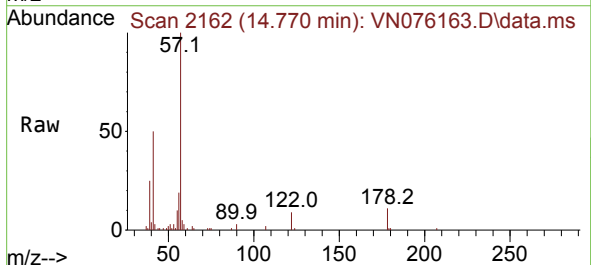

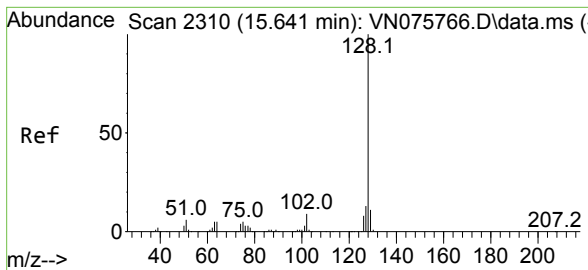

#95
Naphthalene
Concen: 3.107 ug/l
RT: 15.641 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN076163.D
Acq: 09 Jan 2023 18:04

Instrument :
MSVOA_N
ClientSampleId :
HYATT-SILICA

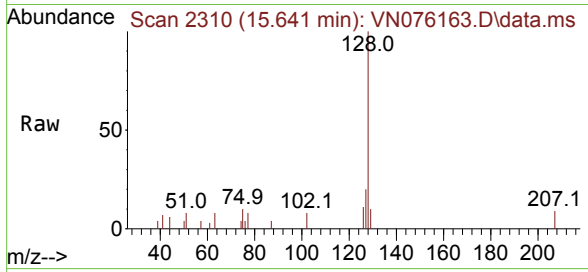

Tgt Ion:	128	Resp:	9614
Ion	Ratio	Lower	Upper
128	100		
127	14.1	10.4	15.6
129	9.9	8.7	13.1

