

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010923\
 Data File : VN076153.D
 Acq On : 09 Jan 2023 14:04
 Operator : JC\MD
 Sample : 01078-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Jan 10 01:06:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	307024	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	488446	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	416808	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	168098	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	163310	48.893	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.780%
35) Dibromofluoromethane	8.171	113	145490	48.098	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.200%
50) Toluene-d8	10.571	98	565300	49.984	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.960%
62) 4-Bromofluorobenzene	12.853	95	169593	45.274	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010923\
Data File : VN076153.D
Acq On : 09 Jan 2023 14:04
Operator : JC\MD
Sample : 01078-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Jan 10 01:06:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration




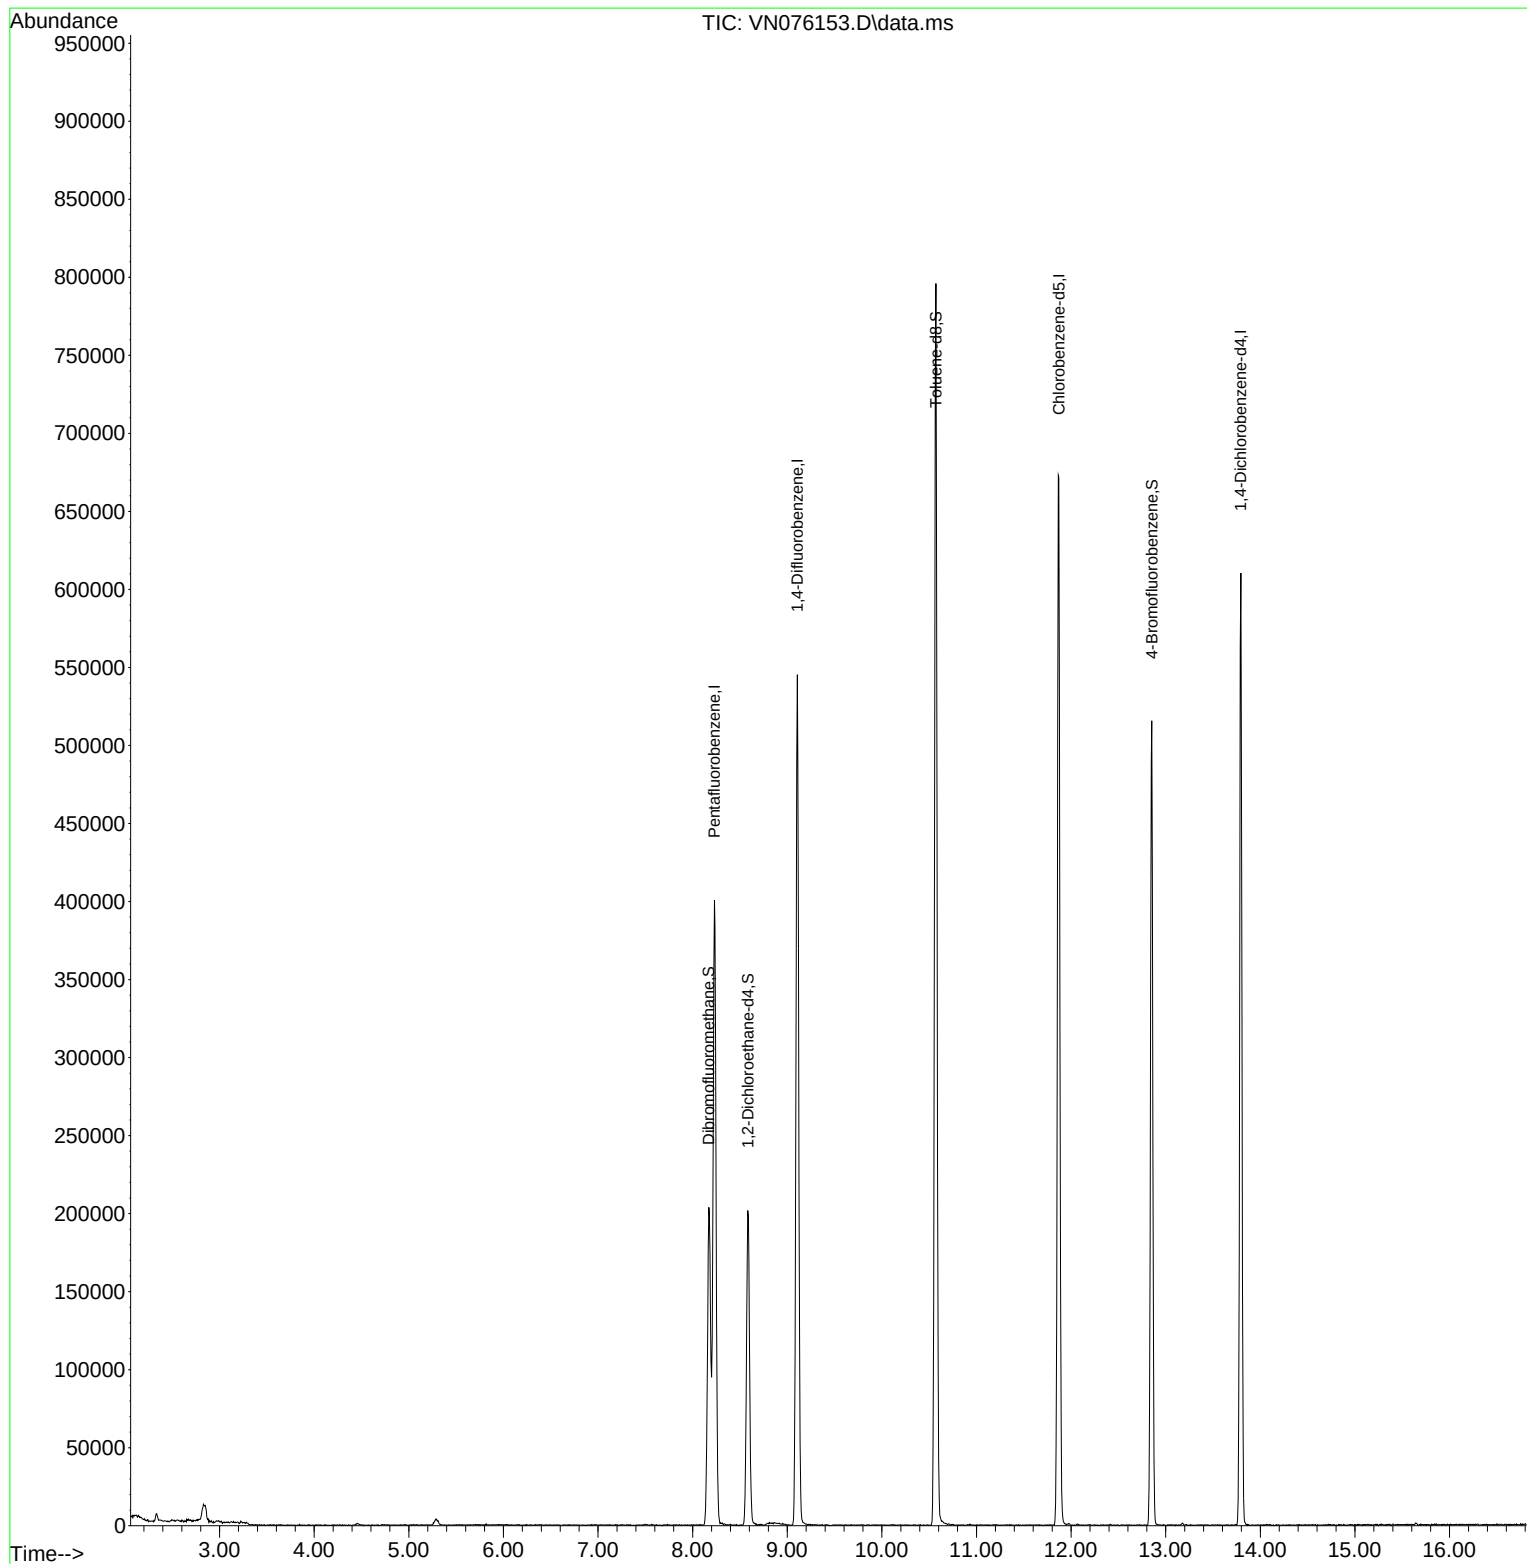


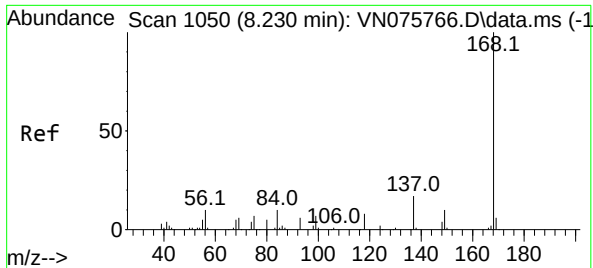

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1105
Delta R.T. -0.000 min
Lab File: VN076153.D
Acq: 09 Jan 2023 14:04




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 307024
Ion Ratio Lower Upper
168 100
99 56.8 44.2 66.4

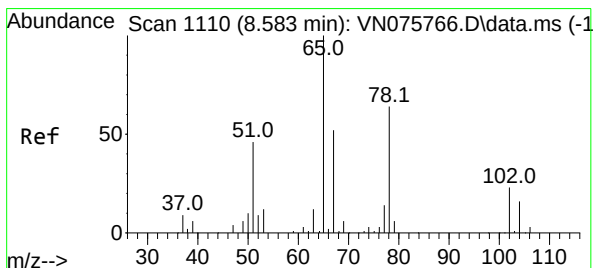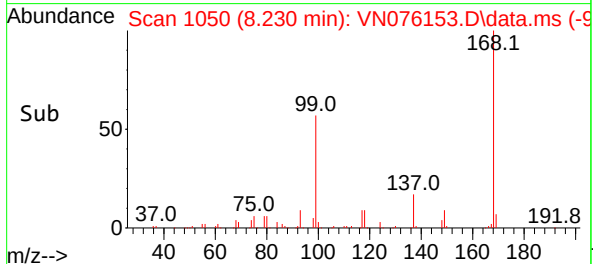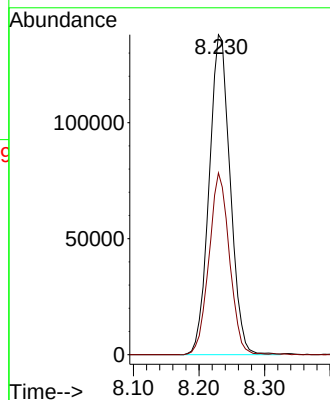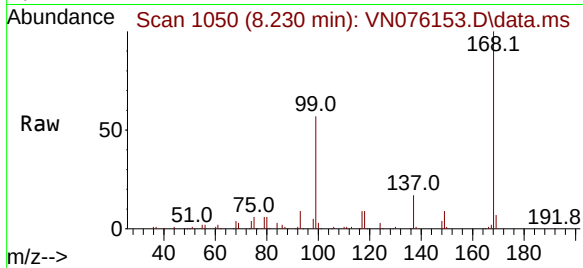

#33
1,2-Dichloroethane-d4
Concen: 48.893 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.000 min
Lab File: VN076153.D
Acq: 09 Jan 2023 14:04

Tgt Ion: 65 Resp: 163310
Ion Ratio Lower Upper
65 100
67 53.3 0.0 103.4

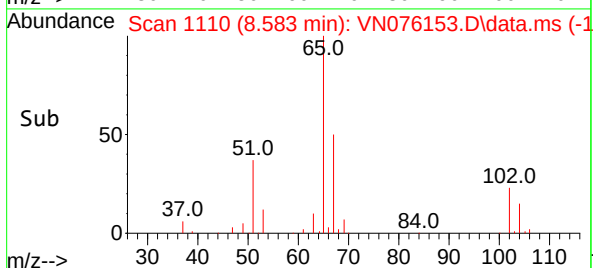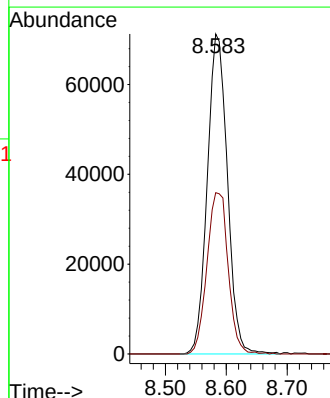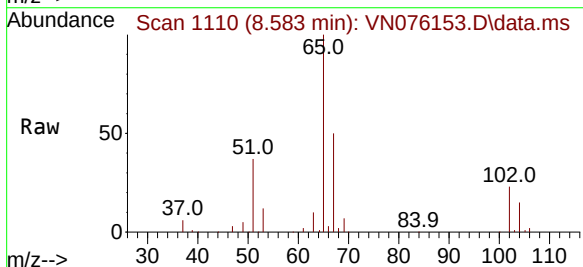

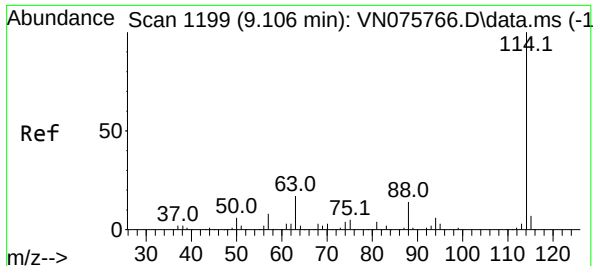

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN076153.D

Acq: 09 Jan 2023 14:04

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-WATER-REF-4





Tgt Ion:114 Resp: 488446

Ion Ratio Lower Upper

114 100

63 18.2 0.0 34.4

88 14.5 0.0 28.8

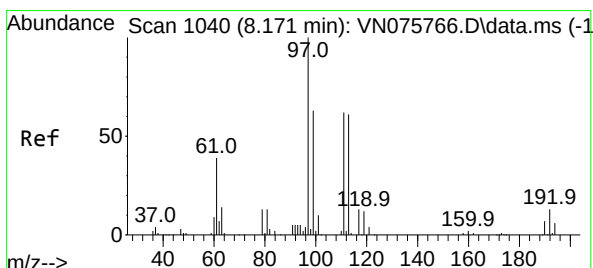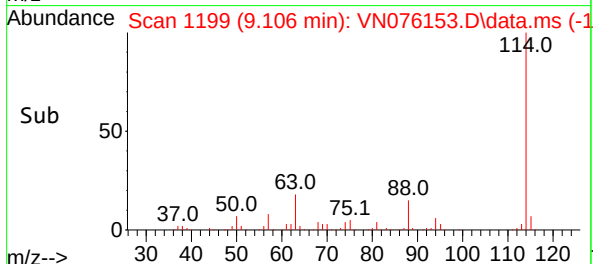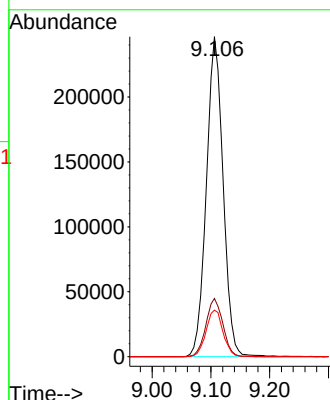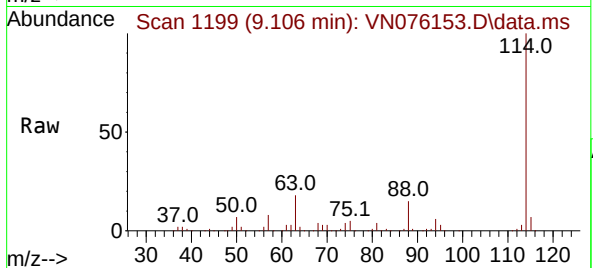

#35

Dibromofluoromethane

Concen: 48.098 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VN076153.D

Acq: 09 Jan 2023 14:04




Tgt Ion:113 Resp: 145490


Ion Ratio Lower Upper

113 100

111 103.4 83.4 125.2

192 20.2 16.1 24.1


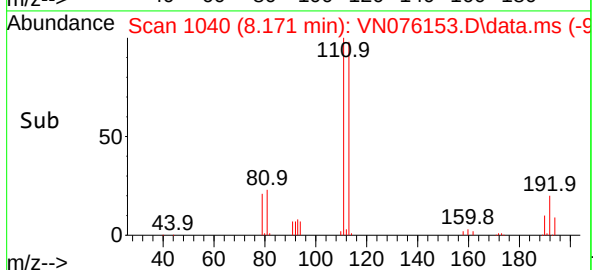
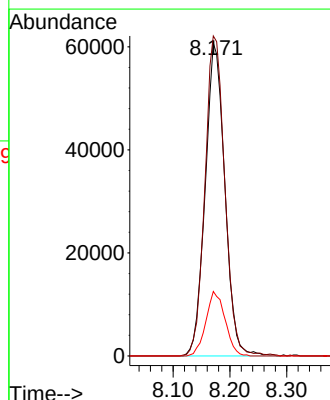
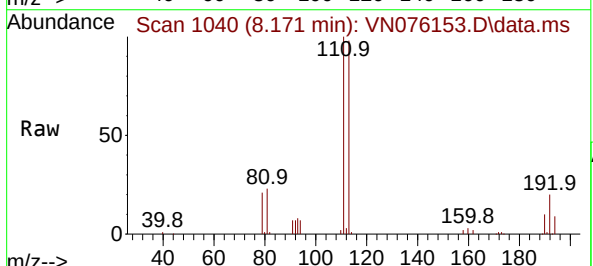


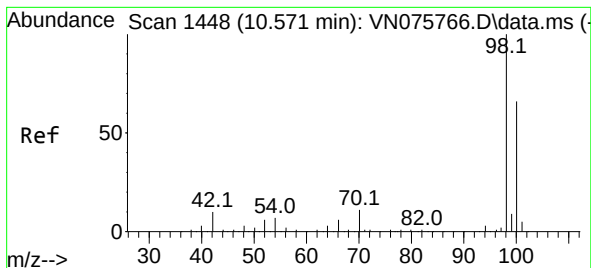

#50
Toluene-d8
Concen: 49.984 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. 0.000 min
Lab File: VN076153.D
Acq: 09 Jan 2023 14:04




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 565300
Ion Ratio Lower Upper
98 100
100 65.5 52.1 78.1

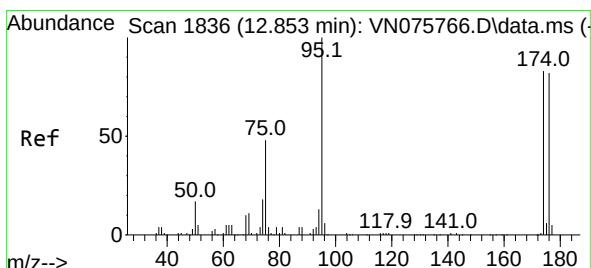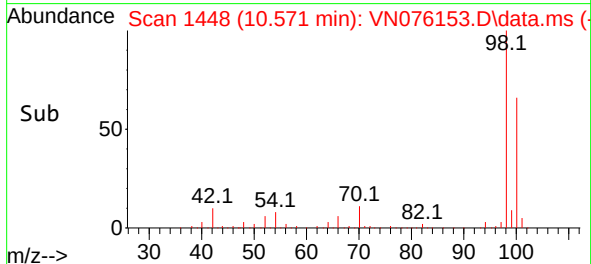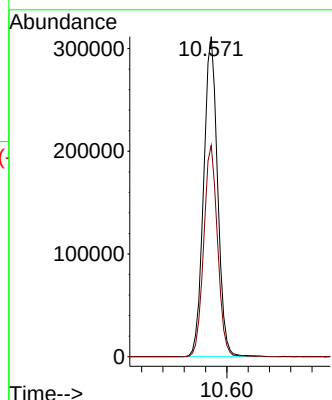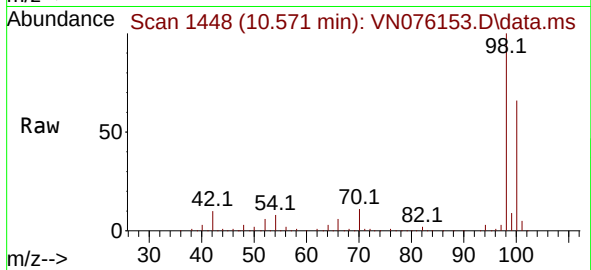

#62
4-Bromofluorobenzene
Concen: 45.274 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.000 min
Lab File: VN076153.D
Acq: 09 Jan 2023 14:04

Tgt Ion: 95 Resp: 169593
Ion Ratio Lower Upper
95 100
174 86.9 0.0 171.6
176 84.1 0.0 169.2


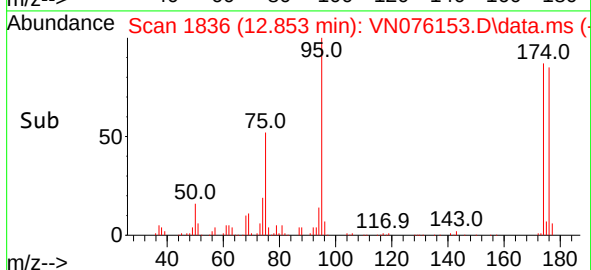
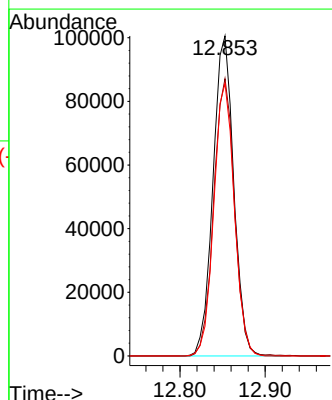
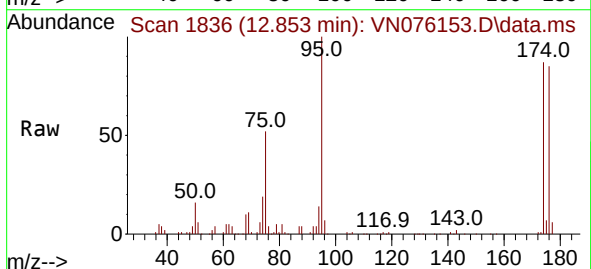


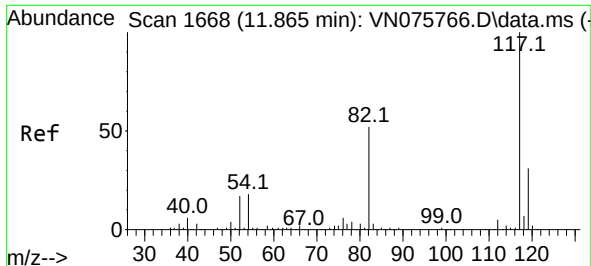

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1669
Delta R.T. 0.006 min
Lab File: VN076153.D
Acq: 09 Jan 2023 14:04

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 416808
Ion Ratio Lower Upper
117 100
82 52.4 41.3 61.9
119 31.3 24.6 37.0

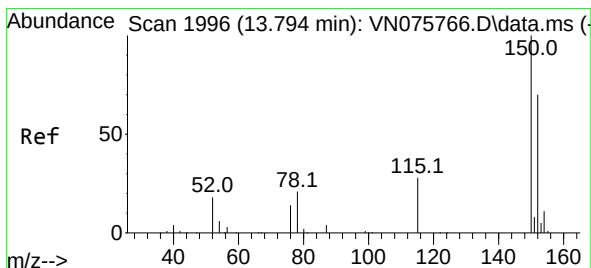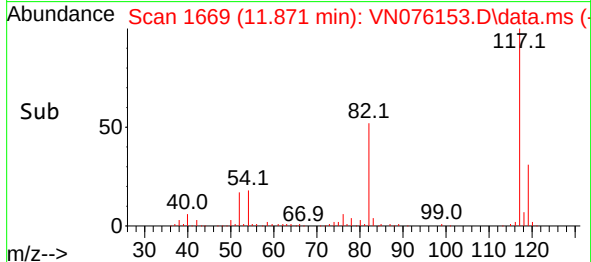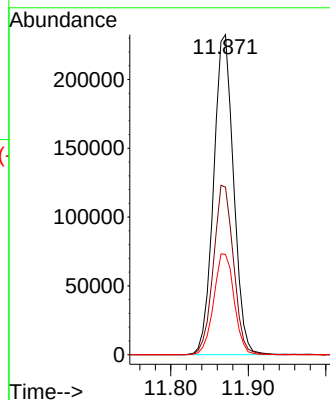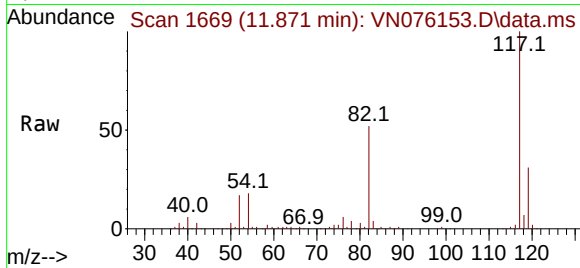

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN076153.D
Acq: 09 Jan 2023 14:04

Tgt Ion:152 Resp: 168098
Ion Ratio Lower Upper
152 100
115 59.2 29.1 87.4
150 158.3 0.0 347.0

