
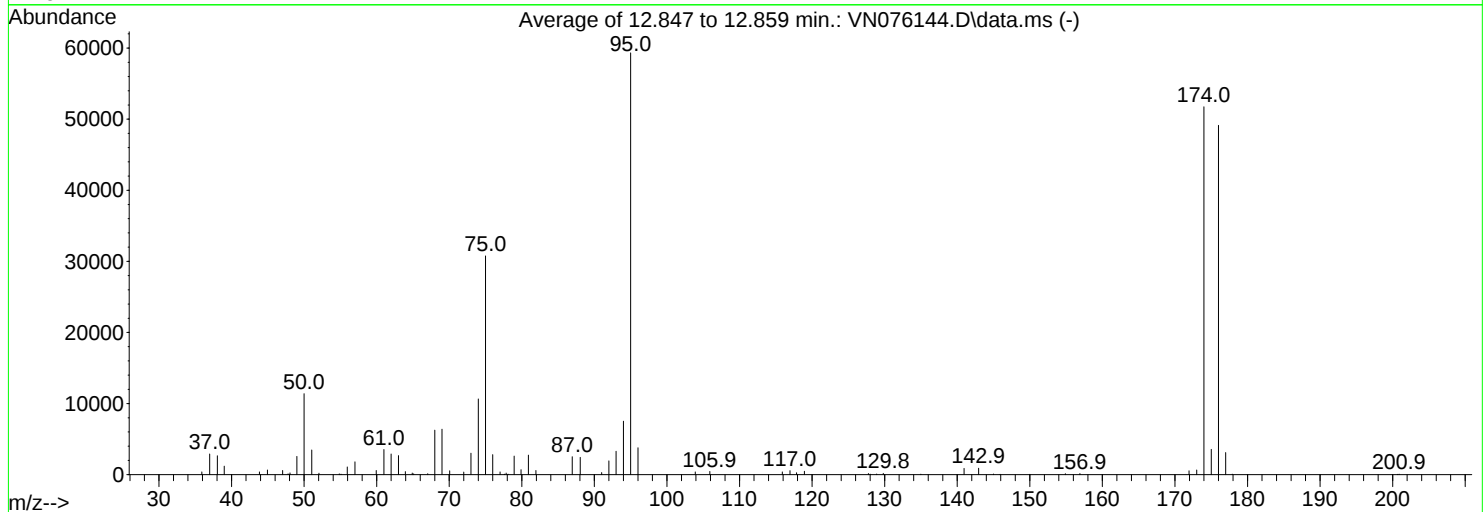


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010923\
Data File : VN076144.D
Acq On : 09 Jan 2023 09:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

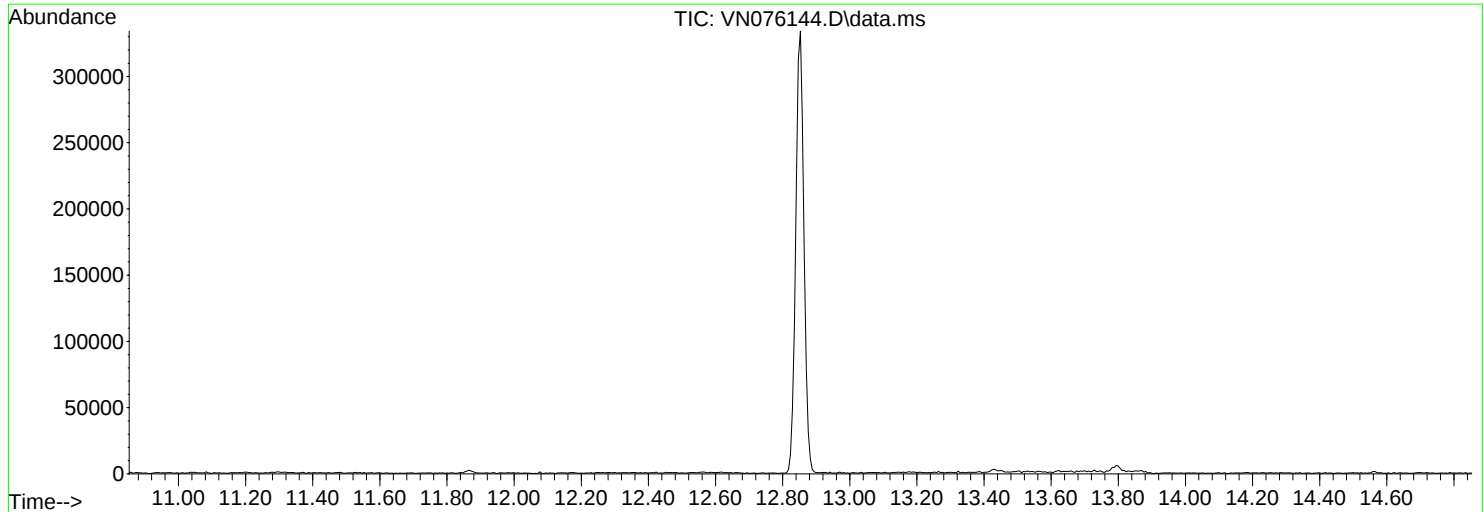

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	11394	PASS
75	95	30	60	51.9	30768	PASS
95	95	100	100	100.0	59331	PASS
96	95	5	9	6.4	3787	PASS
173	174	0.00	2	1.3	665	PASS
174	95	50	100	87.2	51755	PASS
175	174	5	9	6.9	3551	PASS
176	174	95	101	94.9	49133	PASS
177	176	5	9	6.3	3112	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	393	51.05	3475	64.90	237	77.00	390
37.00	2911	52.05	214	65.10	116	77.60	61
38.05	2659	54.85	121	67.05	144	77.85	23
39.00	1186	55.10	60	68.00	6265	78.10	6
43.85	388	55.95	1071	69.00	6388	78.95	2613
44.95	651	57.00	1793	70.05	532	79.90	706
47.05	591	59.95	580	72.00	364	80.90	2755
47.80	105	61.00	3545	73.00	3006	81.95	596
48.05	241	62.00	2899	74.00	10643	86.95	2522
49.00	2571	63.00	2679	75.00	30768	88.05	2441
50.00	11394	63.95	420	76.00	2805	91.00	295

Average of 12.847 to 12.859 min.: VN076144.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	1931	127.75	151	156.90	150		
93.00	3284	128.00	62	171.95	550		
94.00	7525	128.90	82	173.00	665		
95.00	59331	129.80	184	174.00	51755		
96.00	3787	135.00	64	175.00	3551		
103.90	394	140.95	884	176.00	49133		
105.90	451	142.95	897	177.00	3112		
115.90	391	145.00	93	177.90	61		
116.95	562	145.90	51	200.70	55		
117.85	261	150.00	55	200.90	79		
118.95	478	154.90	145				

Instrument :
MSVOA_N
ClientSampleId :
BFB