

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010925\
 Data File : VN085409.D
 Acq On : 09 Jan 2025 15:15
 Operator : JC\MD
 Sample : Q1038-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jan 10 00:21:48 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
 Quant Title : SW846 8260
 QLast Update : Sat Dec 28 01:36:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	180603	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	323361	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.859	117	281455	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	115636	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.571	65	137659	53.441	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 106.880%			
35) Dibromofluoromethane	8.159	113	107472	53.275	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 106.560%			
50) Toluene-d8	10.565	98	385402	52.063	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 104.120%			
62) 4-Bromofluorobenzene	12.847	95	120764	49.122	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 98.240%			
Target Compounds						Qvalue
5) Bromomethane	2.971	94	440	0.232	ug/l	94
6) Chloroethane	3.124	64	535	0.291	ug/l #	45
8) Diethyl Ether	3.953	74	10141	8.025	ug/l	98
11) Tert butyl alcohol	5.512	59	57744	179.019	ug/l	100
16) Acetone	4.424	43	1250	1.476	ug/l #	44
19) Methyl tert-butyl Ether	5.795	73	2357	0.361	ug/l #	80
20) Methylene Chloride	5.265	84	567	0.249	ug/l #	87
26) 2,2-Dichloropropane	7.424	77	6678	1.828	ug/l #	55
29) Tetrahydrofuran	7.836	42	90386	106.781	ug/l	96
31) Cyclohexane	8.218	56	5263	1.382	ug/l #	12
36) 1,1-Dichloropropene	8.218	75	17330	5.867	ug/l #	49
38) Carbon Tetrachloride	8.218	117	20306	6.307	ug/l #	16
40) Benzene	8.600	78	3893	0.436	ug/l	95
41) Methacrylonitrile	7.836	41	54793	36.443	ug/l #	48
49) 1,4-Dioxane	9.694	88	4283	135.334	ug/l #	94
51) 4-Methyl-2-Pentanone	10.430	43	1512	0.557	ug/l #	37
59) 2-Hexanone	11.059	43	3144	1.668	ug/l	67
65) Chlorobenzene	11.888	112	24292	3.994	ug/l	98
68) m/p-Xylenes	12.071	106	1019	0.275	ug/l #	70
69) o-Xylene	12.394	106	1215	0.339	ug/l	83
76) 1,2,3-Trichloropropane	12.847	75	69381	32.130	ug/l #	1
79) 2-Chlorotoluene	13.118	91	1231	0.202	ug/l	75
81) trans-1,4-Dichloro-2-b...	12.847	75	69381	76.947	ug/l #	10
82) 4-Chlorotoluene	13.118	91	1231	0.200	ug/l	73
86) p-Isopropyltoluene	13.729	119	299	0.236	ug/l #	51
87) 1,3-Dichlorobenzene	13.806	146	18257	4.888	ug/l	95
88) 1,4-Dichlorobenzene	13.806	146	18257	4.759	ug/l	95
90) Hexachloroethane	14.441	117	428	0.323	ug/l #	20
91) 1,2-Dichlorobenzene	14.106	146	1264	0.355	ug/l	77
95) Naphthalene	15.635	128	5788	0.961	ug/l #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010925\
Data File : VN085409.D
Acq On : 09 Jan 2025 15:15
Operator : JC\MD
Sample : Q1038-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Jan 10 00:21:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
Quant Title : SW846 8260
QLast Update : Sat Dec 28 01:36:16 2024
Response via : Initial Calibration

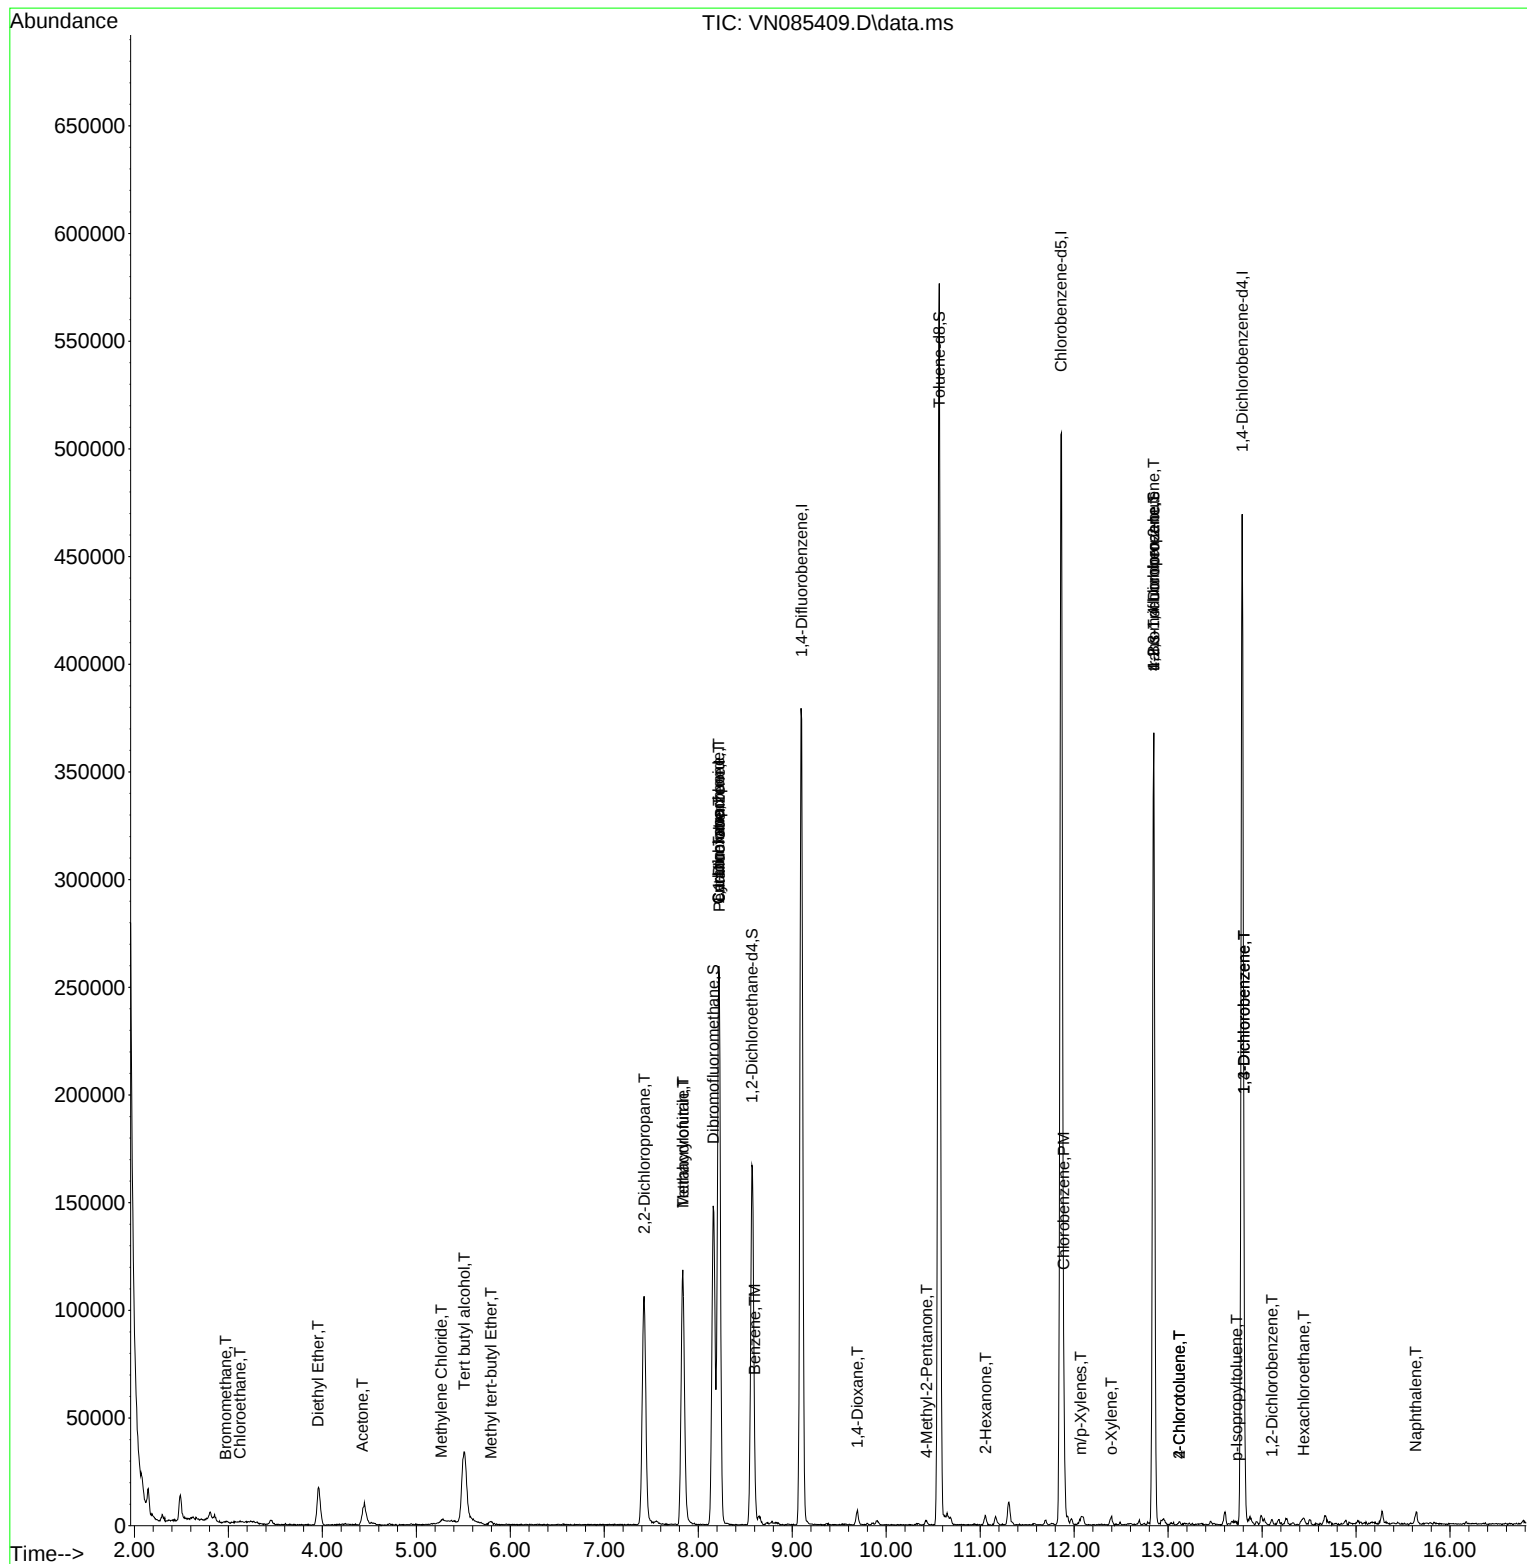






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 180603
Ion Ratio Lower Upper
168 100
99 62.4 51.0 76.4

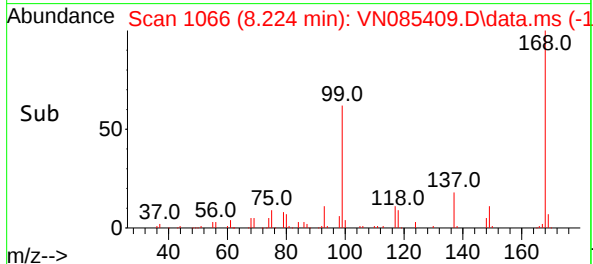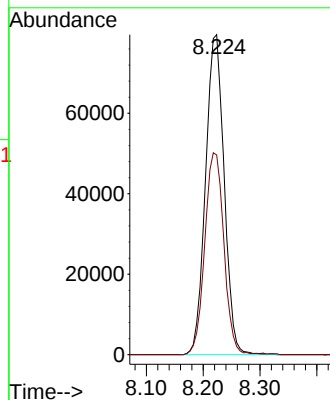

#5
Bromomethane
Concen: 0.232 ug/l
RT: 2.971 min Scan# 173
Delta R.T. 0.012 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15


Tgt Ion: 94 Resp: 440
Ion Ratio Lower Upper
94 100
96 87.9 75.2 112.8

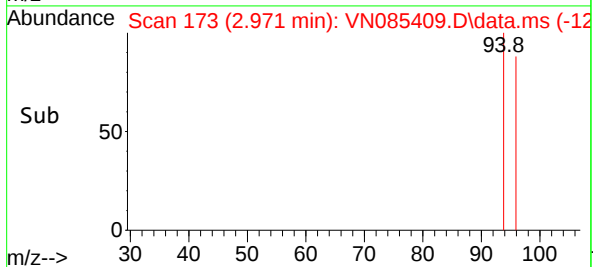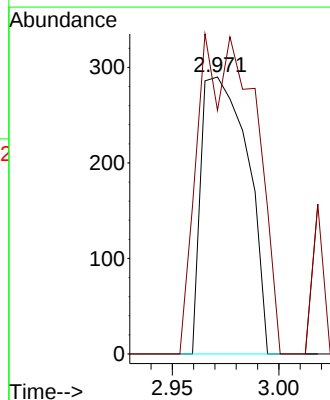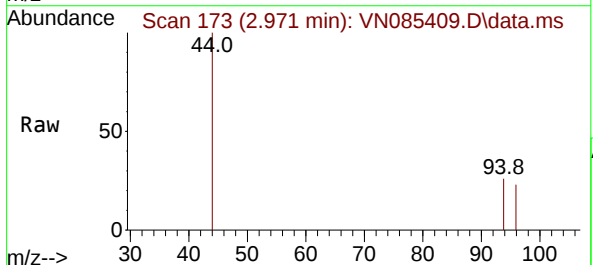






#6
Chloroethane
Concen: 0.291 ug/l
RT: 3.124 min Scan# 199
Delta R.T. 0.000 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 64 Resp: 535
Ion Ratio Lower Upper
64 100
66 0.0 24.1 36.1#

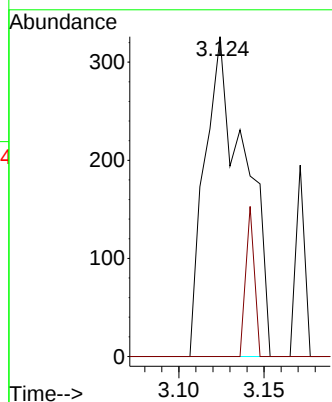

#8
Diethyl Ether
Concen: 8.025 ug/l
RT: 3.953 min Scan# 340
Delta R.T. -0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 74 Resp: 10141
Ion Ratio Lower Upper
74 100
45 92.7 47.5 142.6


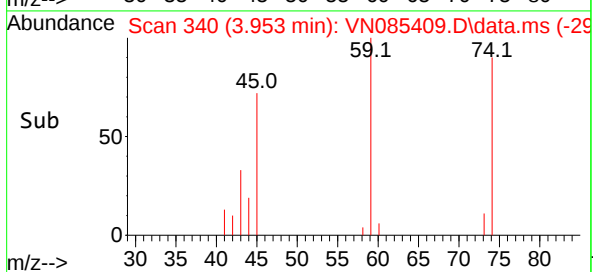
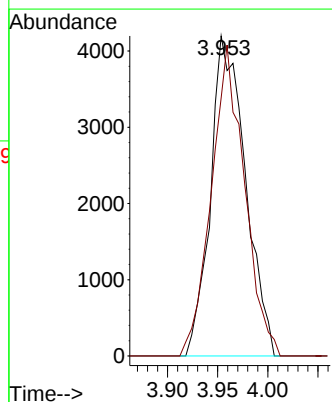





#11
Tert butyl alcohol
Concen: 179.019 ug/l
RT: 5.512 min Scan# 605
Delta R.T. 0.000 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 57744
Ion Ratio Lower Upper
59 100
57 10.0 8.1 12.1

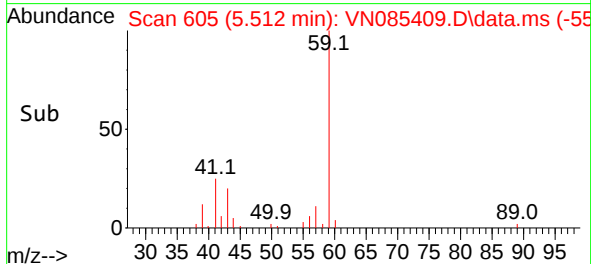

#16
Acetone
Concen: 1.476 ug/l
RT: 4.424 min Scan# 420
Delta R.T. 0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 43 Resp: 1250
Ion Ratio Lower Upper
43 100
58 0.0 24.5 36.7#


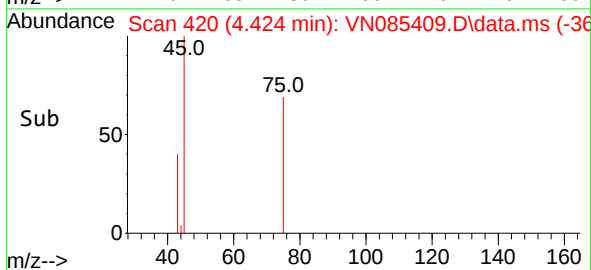

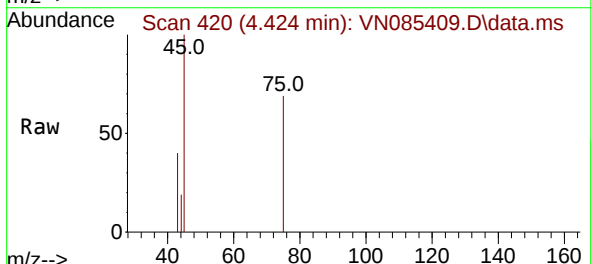




#19
Methyl tert-butyl Ether
Concen: 0.361 ug/l
RT: 5.795 min Scan# 61
Delta R.T. 0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 73 Resp: 2357
Ion Ratio Lower Upper
73 100
57 30.5 17.0 25.6#

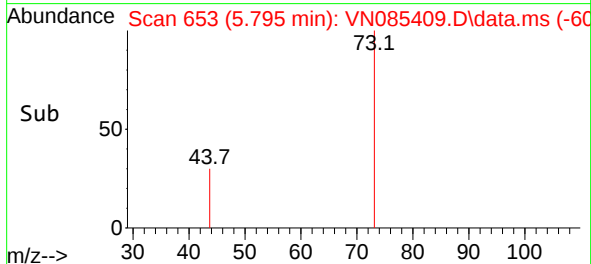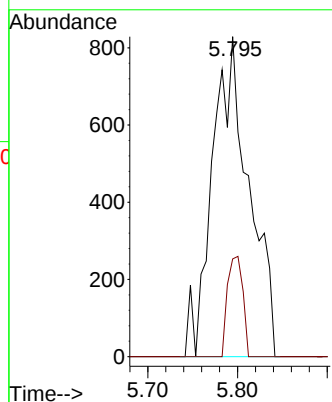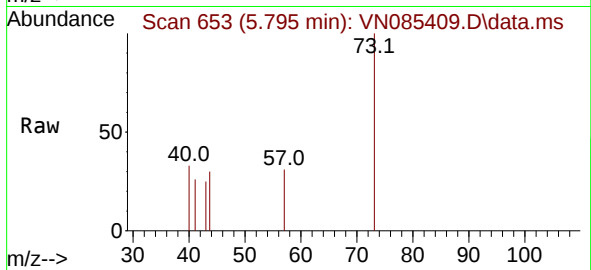

#20
Methylene Chloride
Concen: 0.249 ug/l
RT: 5.265 min Scan# 563
Delta R.T. -0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 84 Resp: 567
Ion Ratio Lower Upper
84 100
49 111.0 97.6 146.4
51 38.2 29.1 43.7
86 43.1 49.3 73.9#


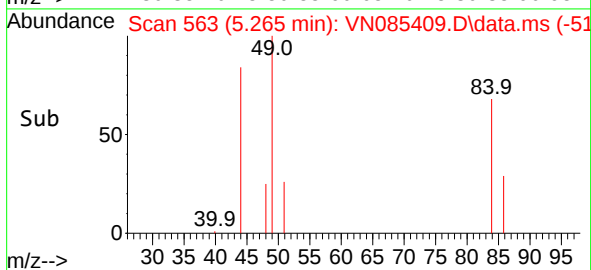






#26
2,2-Dichloropropane
Concen: 1.828 ug/l
RT: 7.424 min Scan# 91
Delta R.T. -0.059 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 77 Resp: 6678
Ion Ratio Lower Upper
77 100
97 0.0 10.6 31.8#

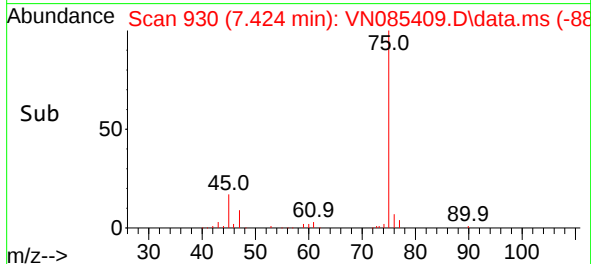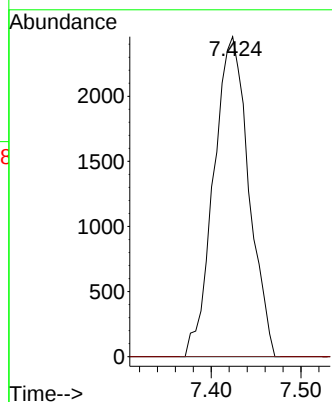

#29
Tetrahydrofuran
Concen: 106.781 ug/l
RT: 7.836 min Scan# 1000
Delta R.T. 0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15


Tgt Ion: 42 Resp: 90386
Ion Ratio Lower Upper
42 100
72 41.9 35.1 52.7
71 39.1 33.4 50.0








#31
Cyclohexane
Concen: 1.382 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.035 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Instrument :
MSVOA_N
ClientSampleId :



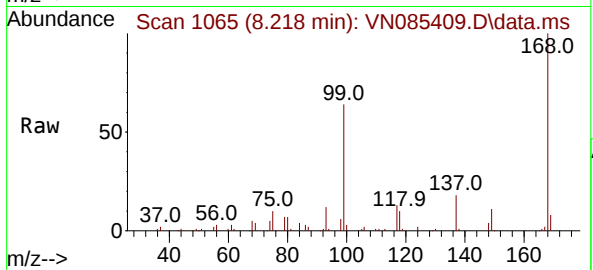



Tgt Ion: 56 Resp: 5263
Ion Ratio Lower Upper
56 100
69 143.7 23.4 35.0#
84 132.2 71.0 106.6#

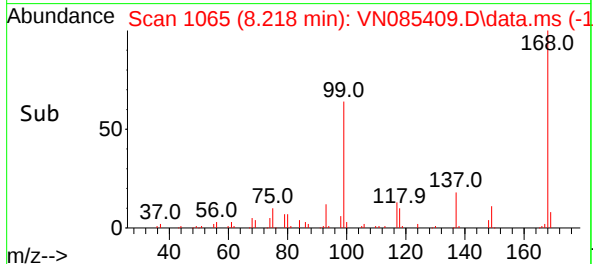

#33
1,2-Dichloroethane-d4
Concen: 53.441 ug/l
RT: 8.571 min Scan# 1125
Delta R.T. -0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 65 Resp: 137659
Ion Ratio Lower Upper
65 100
67 52.5 0.0 104.0

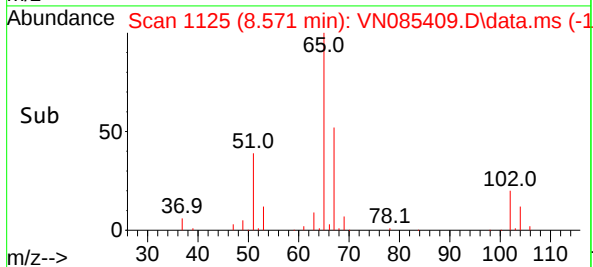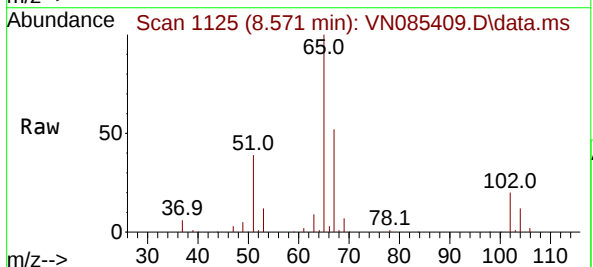



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN085409.D

Acq: 09 Jan 2025 15:15

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 323361

Ion Ratio Lower Upper

114 100

63 20.5 0.0 43.4

88 15.7 0.0 33.6

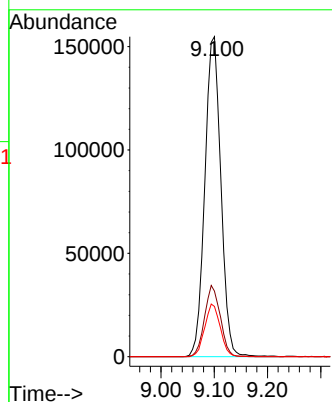

#35

Dibromofluoromethane

Concen: 53.275 ug/l

RT: 8.159 min Scan# 1055

Delta R.T. 0.000 min

Lab File: VN085409.D

Acq: 09 Jan 2025 15:15




Tgt Ion:113 Resp: 107472


Ion Ratio Lower Upper

113 100

111 102.6 80.5 120.7

192 16.5 12.9 19.3

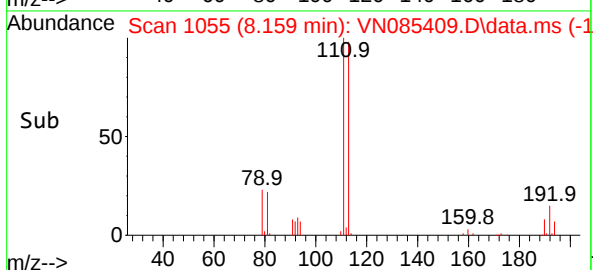



#36

1,1-Dichloropropene

Concen: 5.867 ug/l

RT: 8.218 min Scan# 1065

Delta R.T. -0.147 min

Lab File: VN085409.D





Acq: 09 Jan 2025 15:15

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion: 75	Resp: 17330
Ion Ratio	Lower Upper
75	100
110	7.3 16.6 49.8#
77	0.0 24.3 36.5#

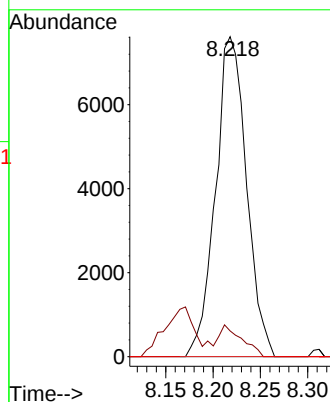

#38

Carbon Tetrachloride

Concen: 6.307 ug/l




RT: 8.218 min Scan# 1065


Delta R.T. -0.141 min

Lab File: VN085409.D

Acq: 09 Jan 2025 15:15

Tgt Ion: 117	Resp: 20306
Ion Ratio	Lower Upper
117	100
119	5.7 77.8 116.6#
121	0.0 22.5 33.7#


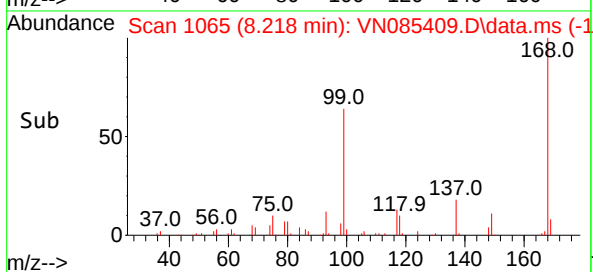
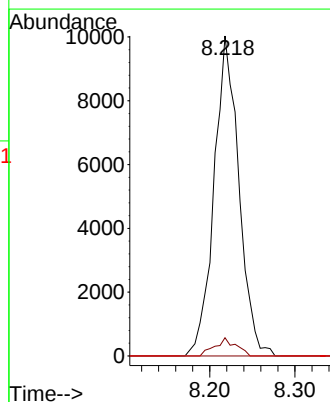





#40
Benzene
Concen: 0.436 ug/l
RT: 8.600 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 78 Resp: 3893
Ion Ratio Lower Upper
78 100
77 21.5 19.0 28.4

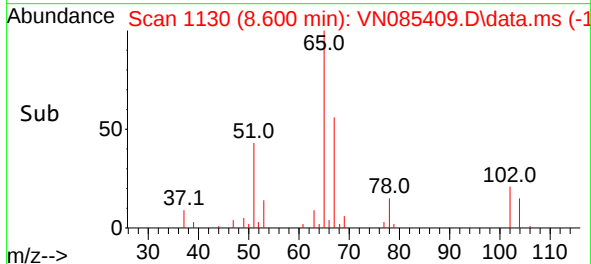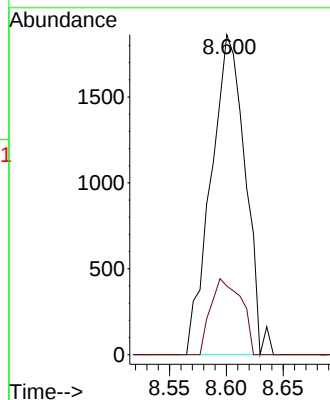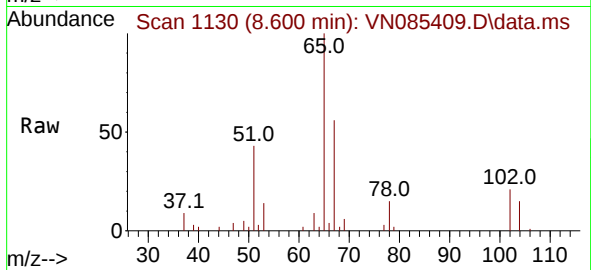

#41
Methacrylonitrile
Concen: 36.443 ug/l
RT: 7.836 min Scan# 1000
Delta R.T. 0.059 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 41 Resp: 54793
Ion Ratio Lower Upper
41 100
39 52.0 45.8 68.8
67 0.0 57.1 85.7#
52 0.0 25.1 37.7#

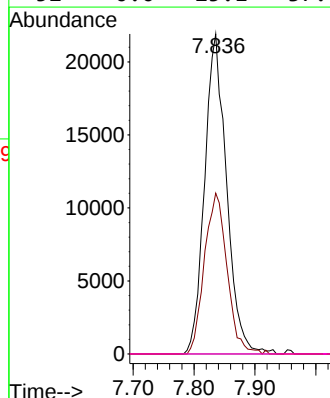



#49

1,4-Dioxane

Concen: 135.334 ug/l

RT: 9.694 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN085409.D

Acq: 09 Jan 2025 15:15

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 88 Resp: 4283

Ion Ratio Lower Upper

88 100

43 33.9 22.1 33.1#

58 74.1 56.7 85.1

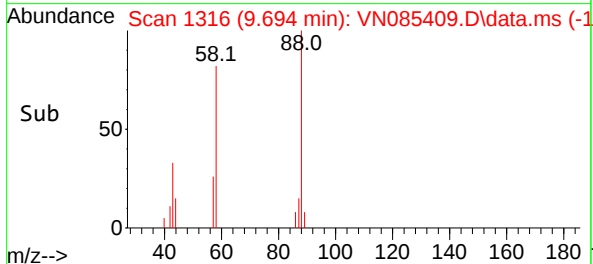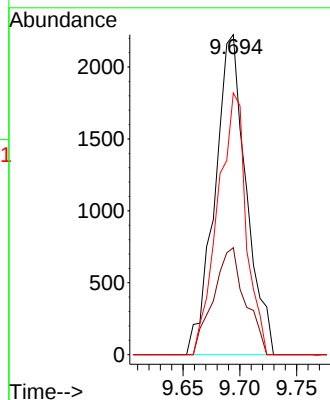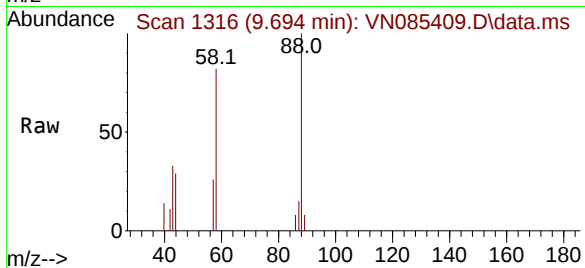

#50

Toluene-d8

Concen: 52.063 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. 0.006 min

Lab File: VN085409.D




Acq: 09 Jan 2025 15:15


Tgt Ion: 98 Resp: 385402

Ion Ratio Lower Upper

98 100

100 64.2 51.5 77.3


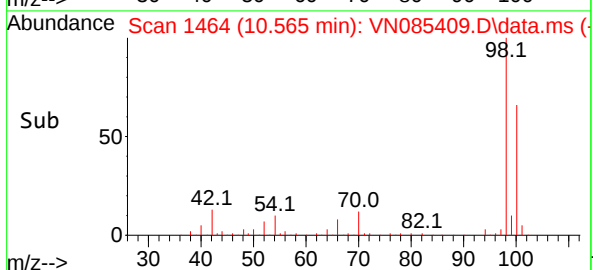
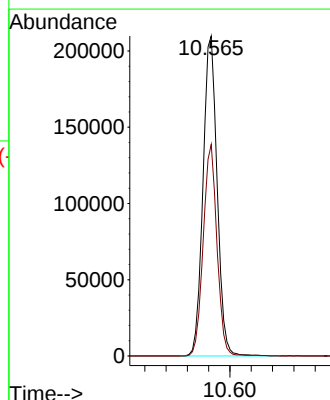
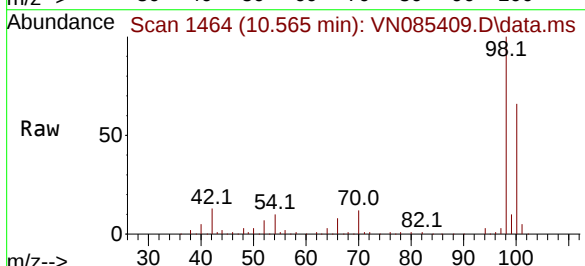




#51
4-Methyl-2-Pentanone
Concen: 0.557 ug/l
RT: 10.430 min Scan# 1443
Delta R.T. -0.012 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1512
Ion Ratio Lower Upper
43 100
58 0.0 30.3 45.5#

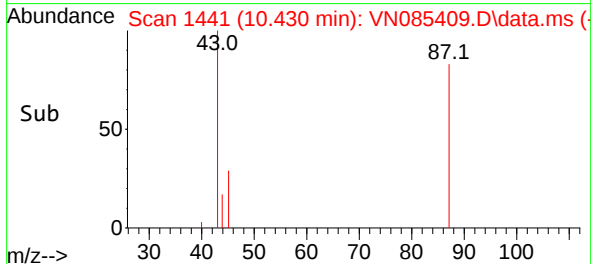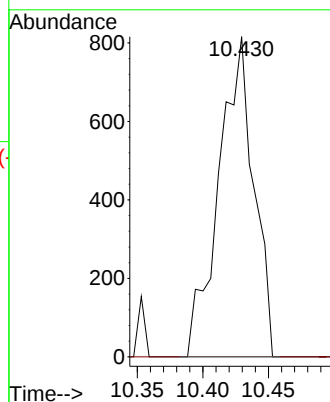

#59
2-Hexanone
Concen: 1.668 ug/l
RT: 11.059 min Scan# 1548
Delta R.T. -0.135 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 43 Resp: 3144
Ion Ratio Lower Upper
43 100
58 29.8 26.5 79.5



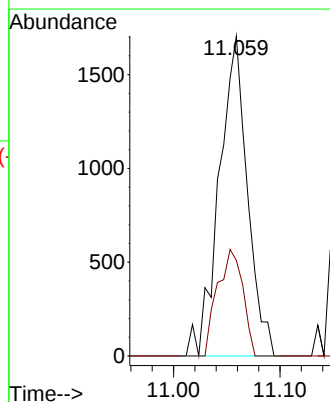





#62
4-Bromofluorobenzene
Concen: 49.122 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 120764
Ion Ratio Lower Upper
95 100
174 72.5 0.0 143.2
176 69.4 0.0 135.8

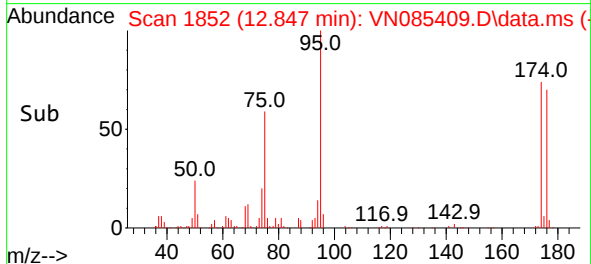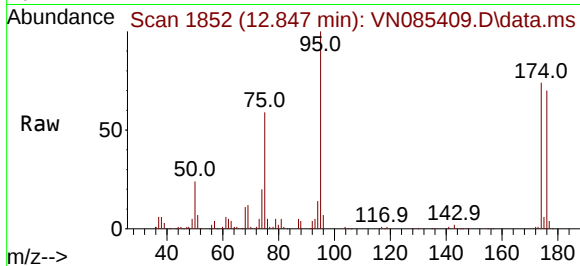

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.859 min Scan# 1684
Delta R.T. 0.000 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 117 Resp: 281455
Ion Ratio Lower Upper
117 100
82 58.9 45.7 68.5
119 31.0 25.8 38.8



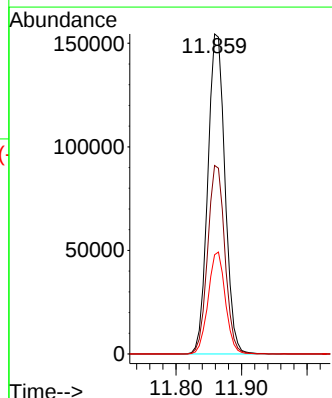
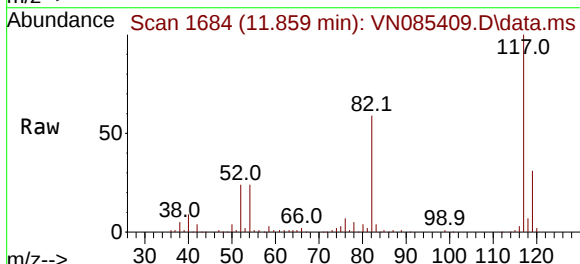




#65
Chlorobenzene
Concen: 3.994 ug/l
RT: 11.888 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:112 Resp: 24292
Ion Ratio Lower Upper
112 100
114 30.5 25.2 37.8

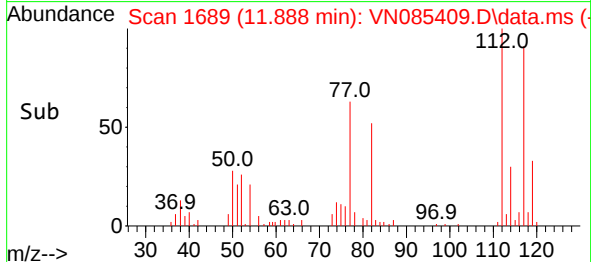

#68
m/p-Xylenes
Concen: 0.275 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion:106 Resp: 1019
Ion Ratio Lower Upper
106 100
91 253.2 165.2 247.8#




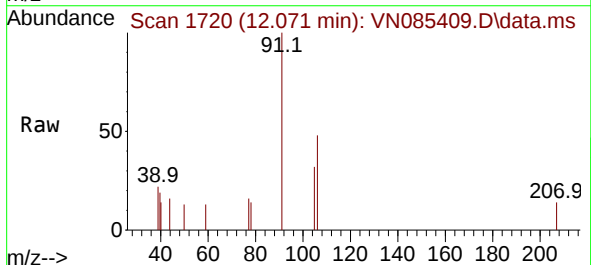




#69
o-Xylene
Concen: 0.339 ug/l
RT: 12.394 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 1215
Ion Ratio Lower Upper
106 100
91 187.7 107.3 321.8

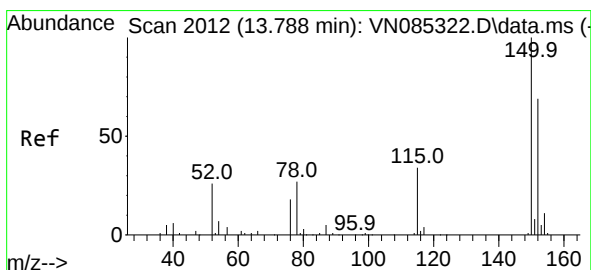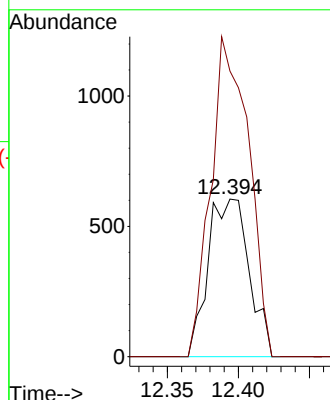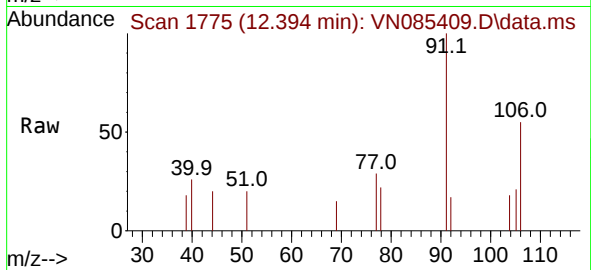

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion:152 Resp: 115636
Ion Ratio Lower Upper
152 100
115 62.2 30.4 91.3
150 158.5 0.0 345.0


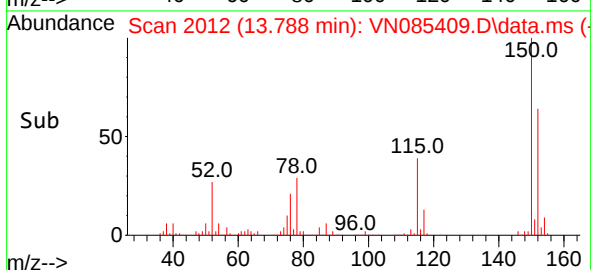
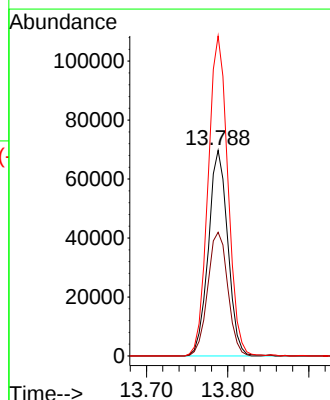
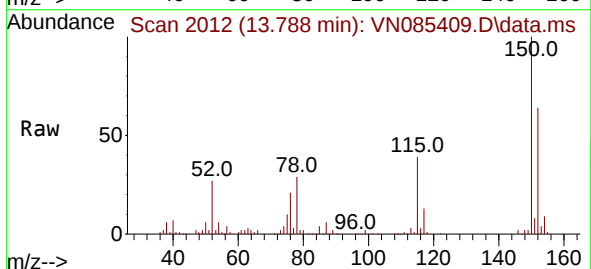




#76
1,2,3-Trichloropropane
Concen: 32.130 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 69381
Ion Ratio Lower Upper
75 100
77 1.0 98.1 294.3#

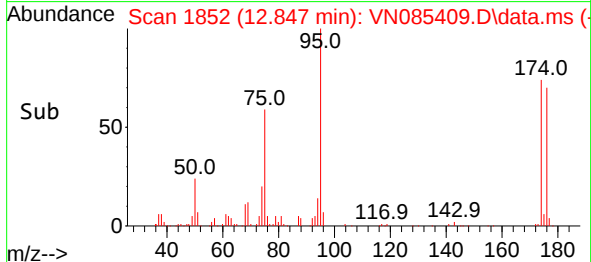

#79
2-Chlorotoluene
Concen: 0.202 ug/l
RT: 13.118 min Scan# 1898
Delta R.T. -0.006 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 91 Resp: 1231
Ion Ratio Lower Upper
91 100
126 17.8 16.0 48.0




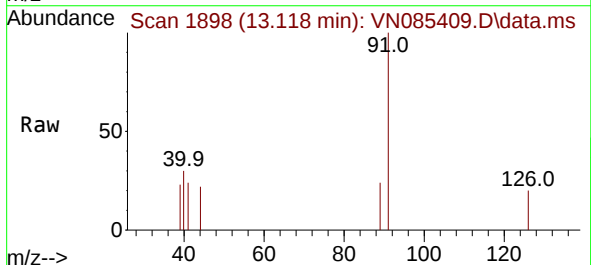




#81
trans-1,4-Dichloro-2-butene
Concen: 76.947 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.118 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 69381
Ion Ratio Lower Upper
75 100
53 0.1 80.0 120.0#
89 0.0 35.8 53.8#

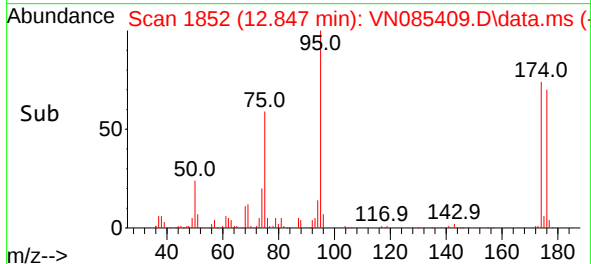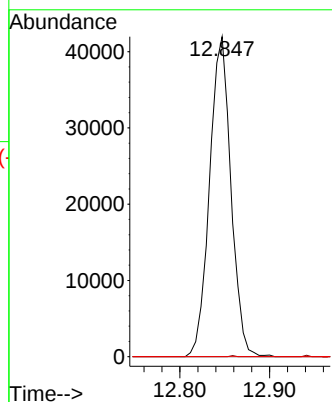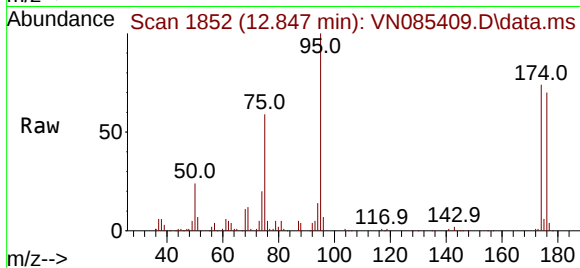

#82
4-Chlorotoluene
Concen: 0.200 ug/l
RT: 13.118 min Scan# 1898
Delta R.T. -0.100 min
Lab File: VN085409.D
Acq: 09 Jan 2025 15:15

Tgt Ion: 91 Resp: 1231
Ion Ratio Lower Upper
91 100
126 17.8 16.4 49.4

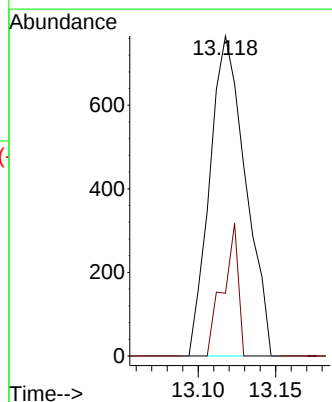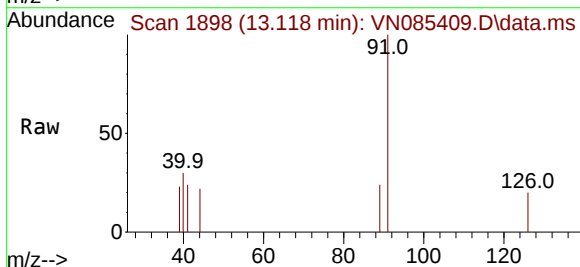



#86

p-Isopropyltoluene

Concen: 0.236 ug/l

RT: 13.729 min Scan# 2001

Delta R.T. 0.006 min

Lab File: VN085409.D

Acq: 09 Jan 2025 15:15

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:119 Resp: 299

Ion Ratio Lower Upper

119 100

134 0.0 12.5 37.5#

91 0.0 12.2 36.4#

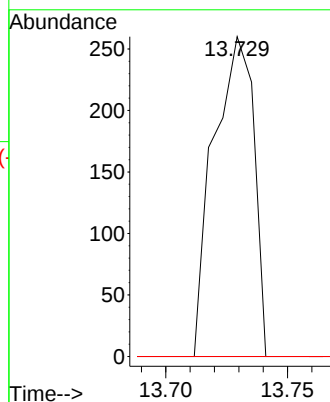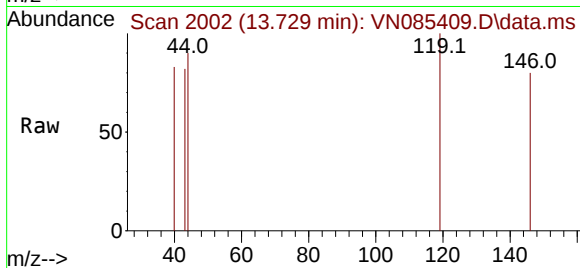

#87

1,3-Dichlorobenzene

Concen: 4.888 ug/l

RT: 13.806 min Scan# 2015

Delta R.T. 0.077 min

Lab File: VN085409.D

Acq: 09 Jan 2025 15:15




Tgt Ion:146 Resp: 18257


Ion Ratio Lower Upper

146 100

111 50.3 21.3 63.9

148 63.5 31.5 94.5


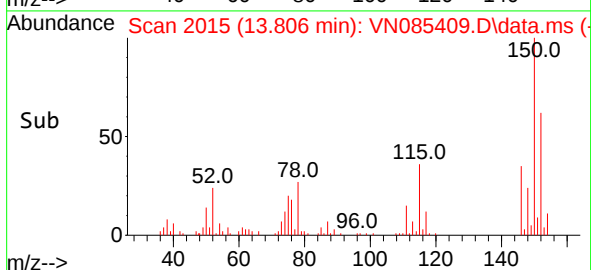
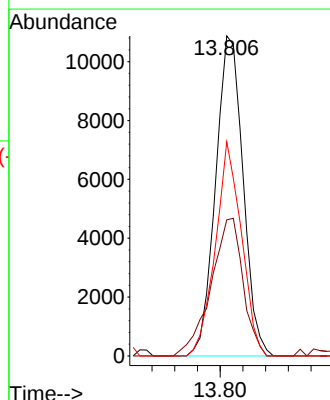
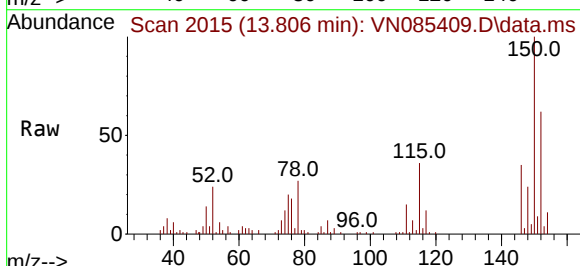




#88
 1,4-Dichlorobenzene
 Concen: 4.759 ug/l
 RT: 13.806 min Scan# 2015
 Delta R.T. 0.000 min
 Lab File: VN085409.D
 Acq: 09 Jan 2025 15:15




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:146 Resp: 18257
 Ion Ratio Lower Upper
 146 100
 111 50.3 20.8 62.5
 148 63.5 31.7 95.1

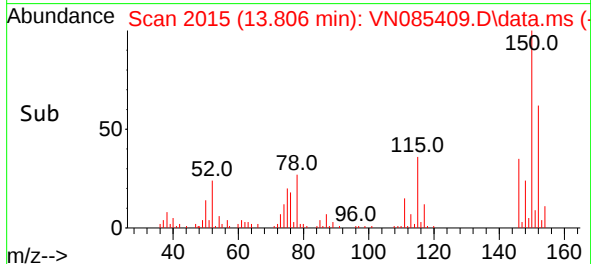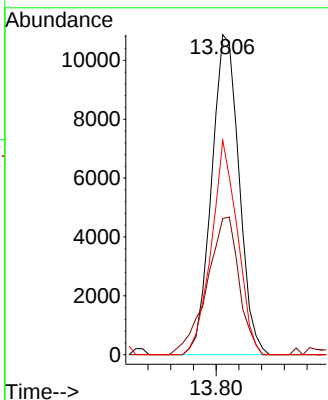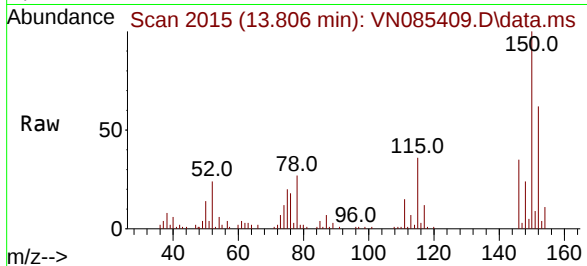

#90
 Hexachloroethane
 Concen: 0.323 ug/l
 RT: 14.441 min Scan# 2123
 Delta R.T. 0.112 min
 Lab File: VN085409.D
 Acq: 09 Jan 2025 15:15

Tgt Ion:117 Resp: 428
 Ion Ratio Lower Upper
 117 100
 201 0.0 30.7 92.1#

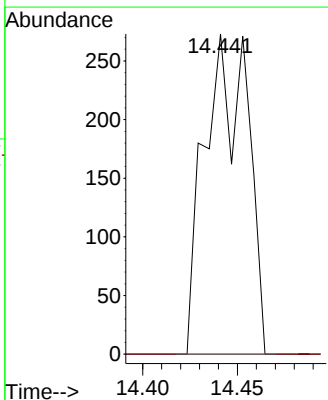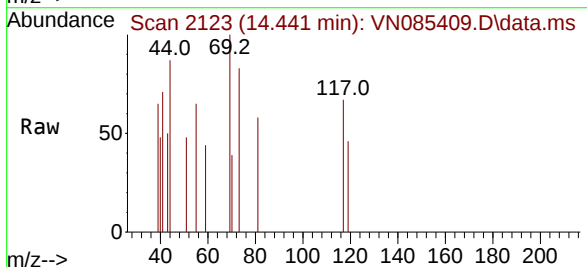



#91

1,2-Dichlorobenzene

Concen: 0.355 ug/l

RT: 14.106 min Scan# 2066

Delta R.T. 0.006 min

Lab File: VN085409.D

Acq: 09 Jan 2025 15:15

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:146 Resp: 1264

Ion Ratio Lower Upper

146 100

111 28.5 21.8 65.3

148 44.9 31.4 94.2



#95

Naphthalene

Concen: 0.961 ug/l

RT: 15.635 min Scan# 2326

Delta R.T. 0.000 min

Lab File: VN085409.D

Acq: 09 Jan 2025 15:15

Tgt Ion:128 Resp: 5788

Ion Ratio Lower Upper

128 100

127 9.4 10.6 16.0#

129 7.3 8.5 12.7#

