
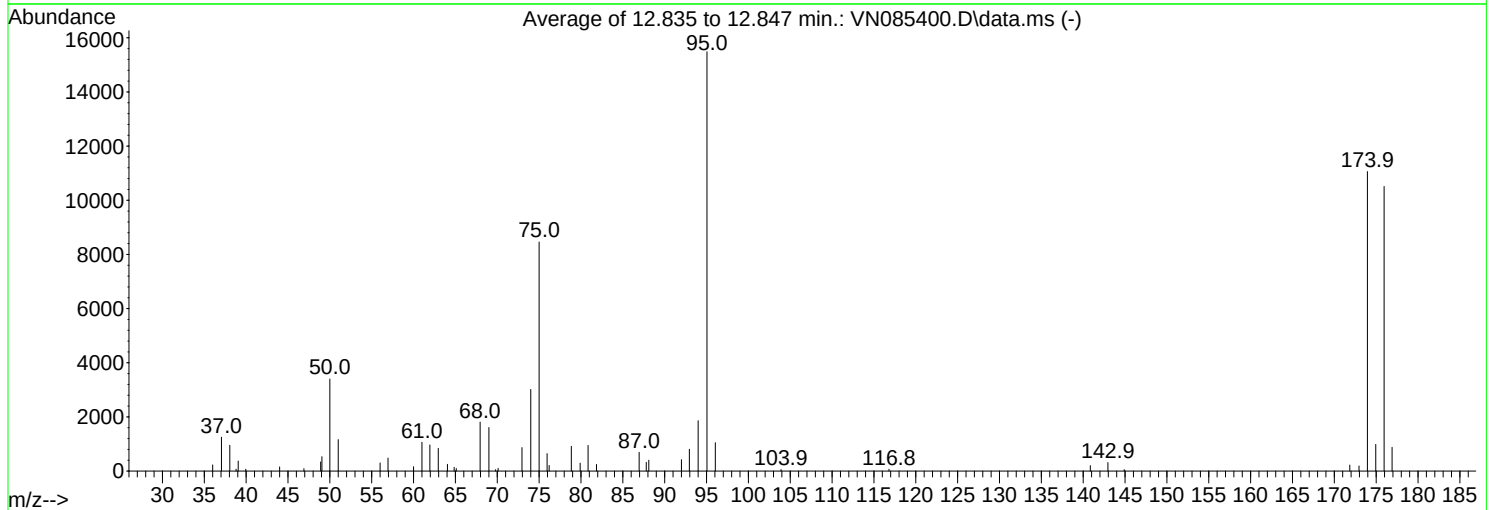


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN010925\
Data File : VN085400.D
Acq On : 09 Jan 2025 09:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
Title : SW846 8260
Last Update : Sat Dec 28 01:36:16 2024

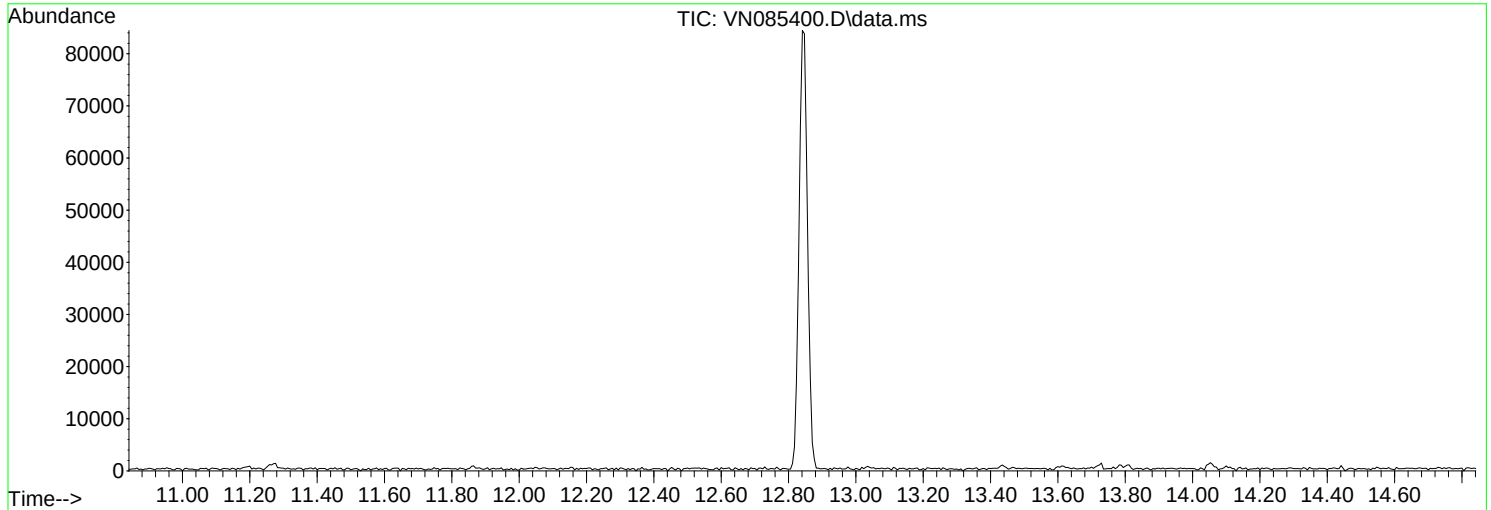

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	3399	PASS
75	95	30	60	54.6	8459	PASS
95	95	100	100	100.0	15485	PASS
96	95	5	9	6.8	1049	PASS
173	174	0.00	2	1.7	190	PASS
174	95	50	100	71.4	11061	PASS
175	174	5	9	8.9	984	PASS
176	174	95	101	95.0	10511	PASS
177	176	5	9	8.3	877	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	228	51.00	1163	69.00	1609	81.85	244
37.05	1252	56.00	302	69.80	52	86.95	695
38.05	952	56.95	483	70.10	101	87.80	325
38.80	71	60.00	161	72.95	869	88.10	405
39.05	373	61.00	1066	74.00	3015	92.00	422
39.95	68	61.95	966	75.00	8459	92.95	806
44.00	155	62.95	841	75.95	645	94.00	1859
46.90	91	64.05	250	76.20	208	95.05	15485
48.90	338	64.85	139	78.85	914	96.05	1049
49.05	532	65.10	94	79.90	295	103.90	56
50.00	3399	67.95	1810	80.85	947	116.80	69

Average of 12.835 to 12.847 min.: VN085400.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
140.85	202						
142.95	316						
144.90	54						
171.85	224						
172.95	190						
173.95	11061						
174.95	984						
175.95	10511						
176.90	877						

Instrument :

MSVOA_N

ClientSampleId :

BFB